


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
 Data File : BF126714.D
 Acq On : 28 Jan 2022 13:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 27 03:09:40 2022

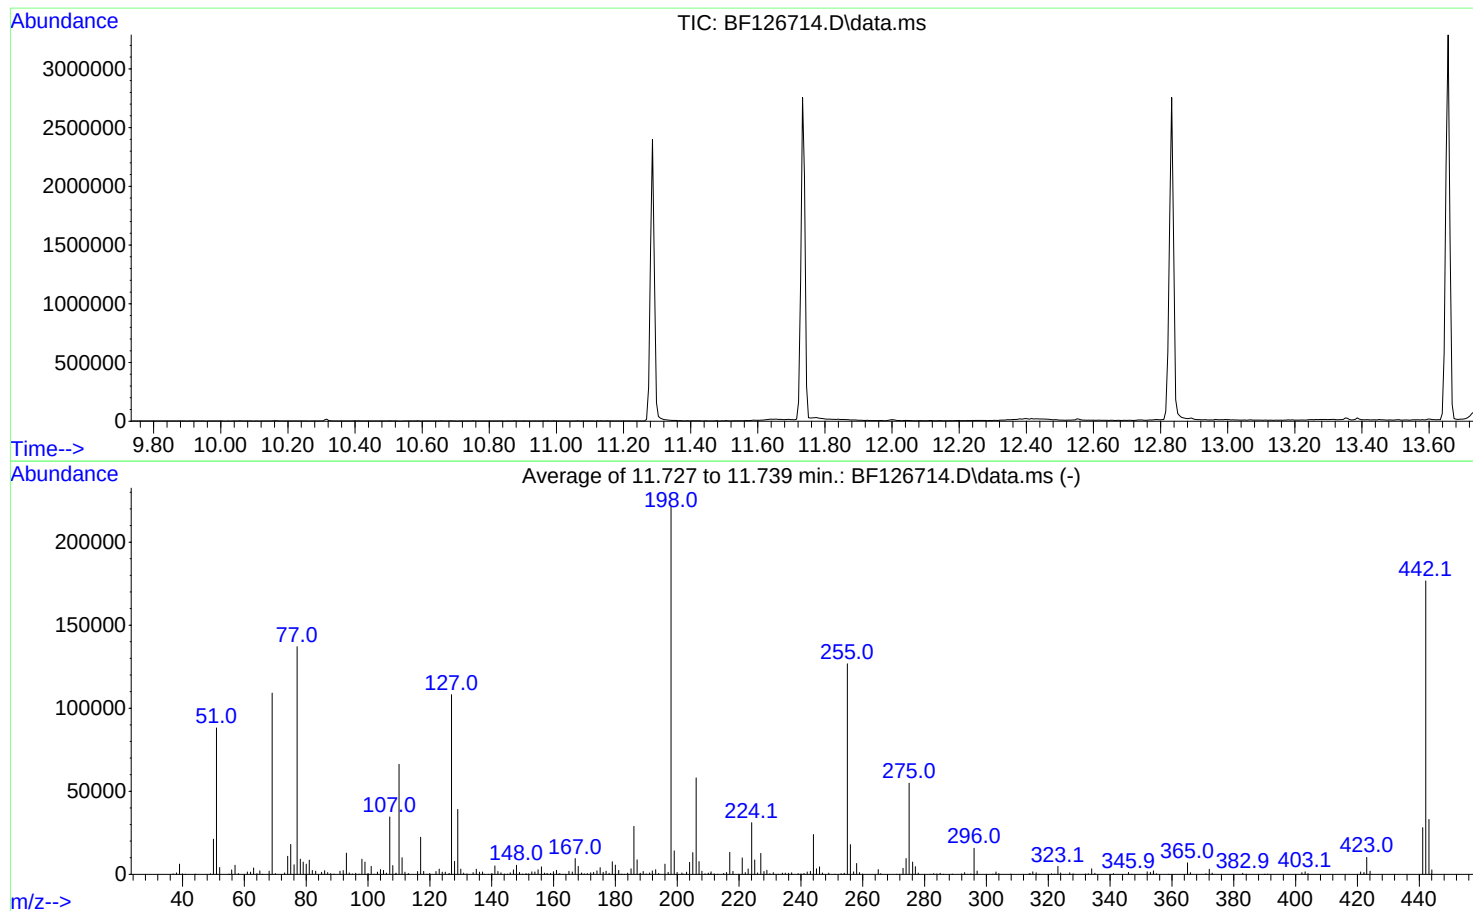




AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	88133	PASS
68	69	0.00	2	1.8	1937	PASS
69	198	0.00	100	49.3	109139	PASS
70	69	0.00	2	0.4	480	PASS
127	198	10	80	48.8	108136	PASS
197	198	0.00	2	0.6	1221	PASS
198	198	100	100	100.0	221432	PASS
199	198	5	9	6.4	14149	PASS
275	198	10	60	24.8	54947	PASS
365	198	1	100	3.1	6898	PASS
441	198	0.01	100	12.7	28138	PASS
442	442	50	100	100.0	176635	PASS
443	442	15	24	18.7	33072	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
 Data File : BF126714.D
 Acq On : 28 Jan 2022 13:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 29 04:02:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 27 03:09:40 2022
 Response via : Initial Calibration

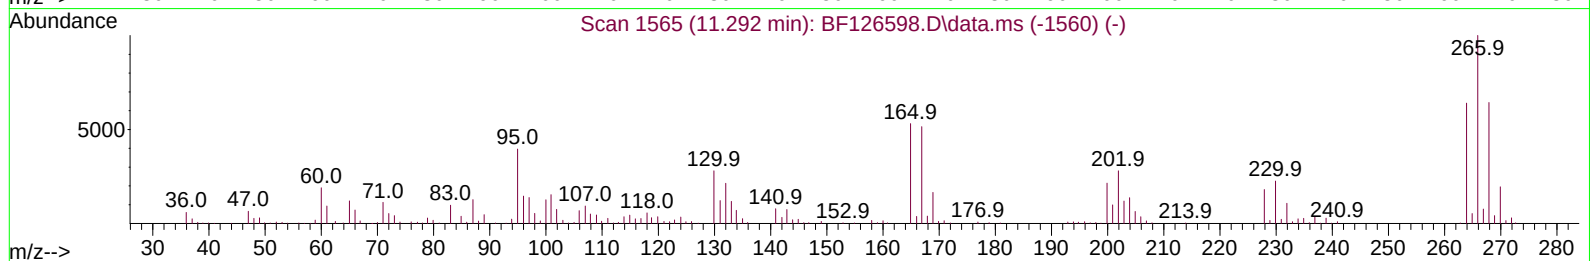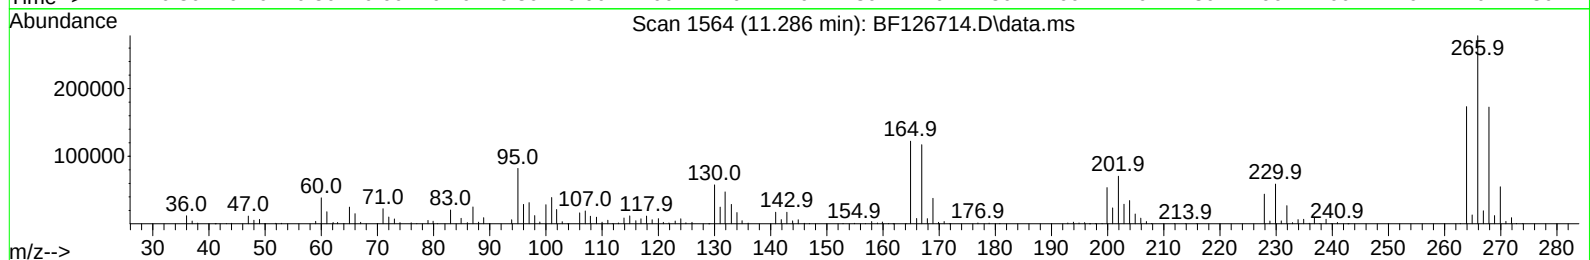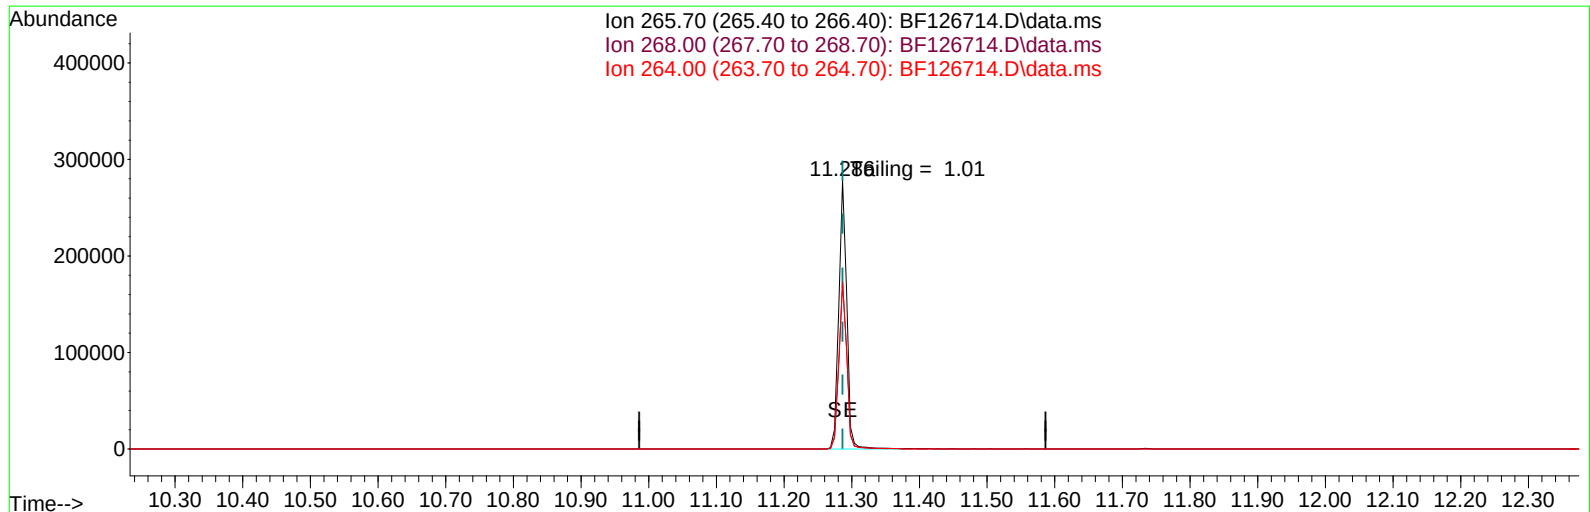

TIC: BF126714.D\data.ms

(70) Pentachlorophenol (C)

11.286min (+ 0.000) 35096.41 ng




response 228365

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.09
264.00	63.00	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012822\
Data File : BF126714.D
Acq On : 28 Jan 2022 13:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 29 04:02:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration

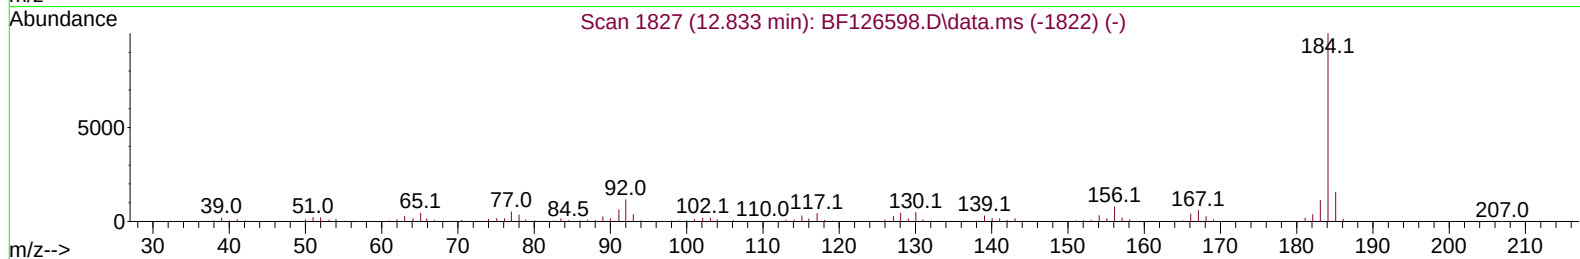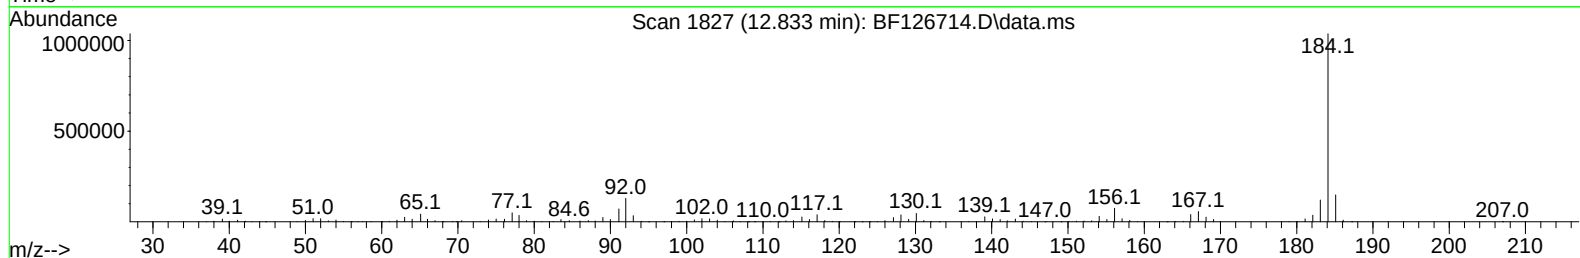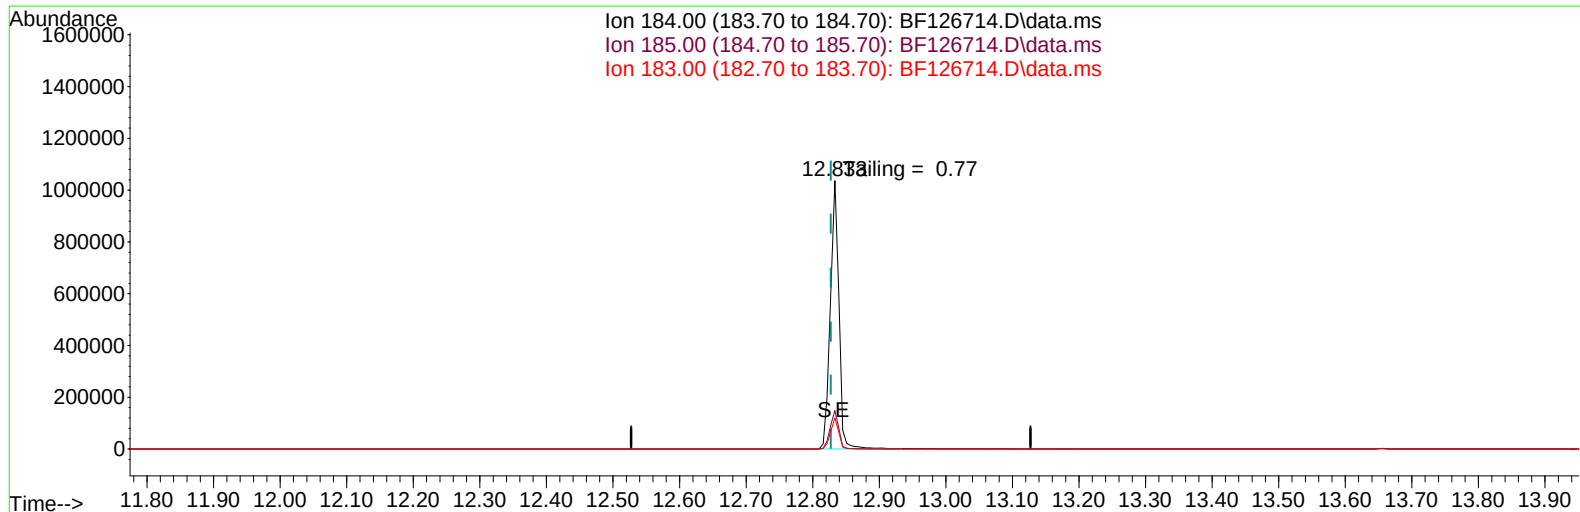

TIC: BF126714.D\data.ms

(77) Benzidine

12.833min (+ 0.006) 0.00 ng

response 940708

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.30
183.00	10.20	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/28/2022	BNA_F	<u>BF126714.D</u>
Compound Name	Response	Retention Time
DDT	531277	13.657
DDD	5311	13.351
DDE	278	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5589	536866	1.04

Instrument :
BNA_F
ClientSampleId :
DFTPP