
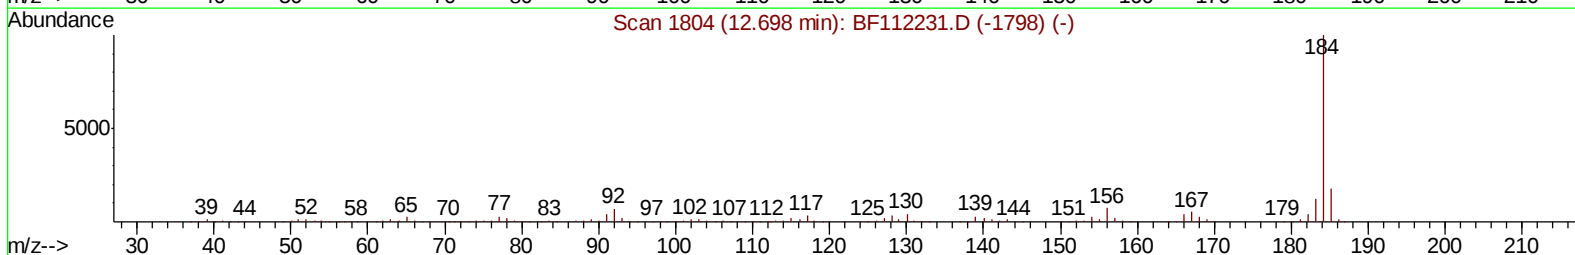
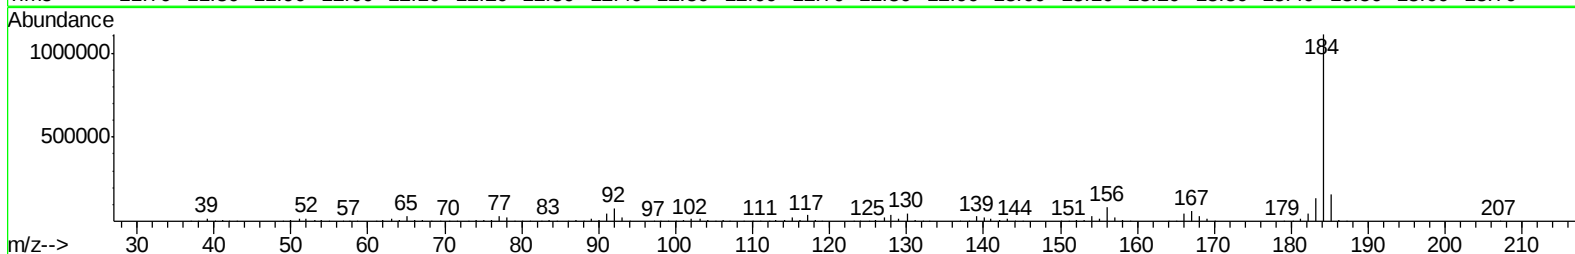


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012919\
 Data File : BF112287.D
 Acq On : 29 Jan 2019 10:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 05:57:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

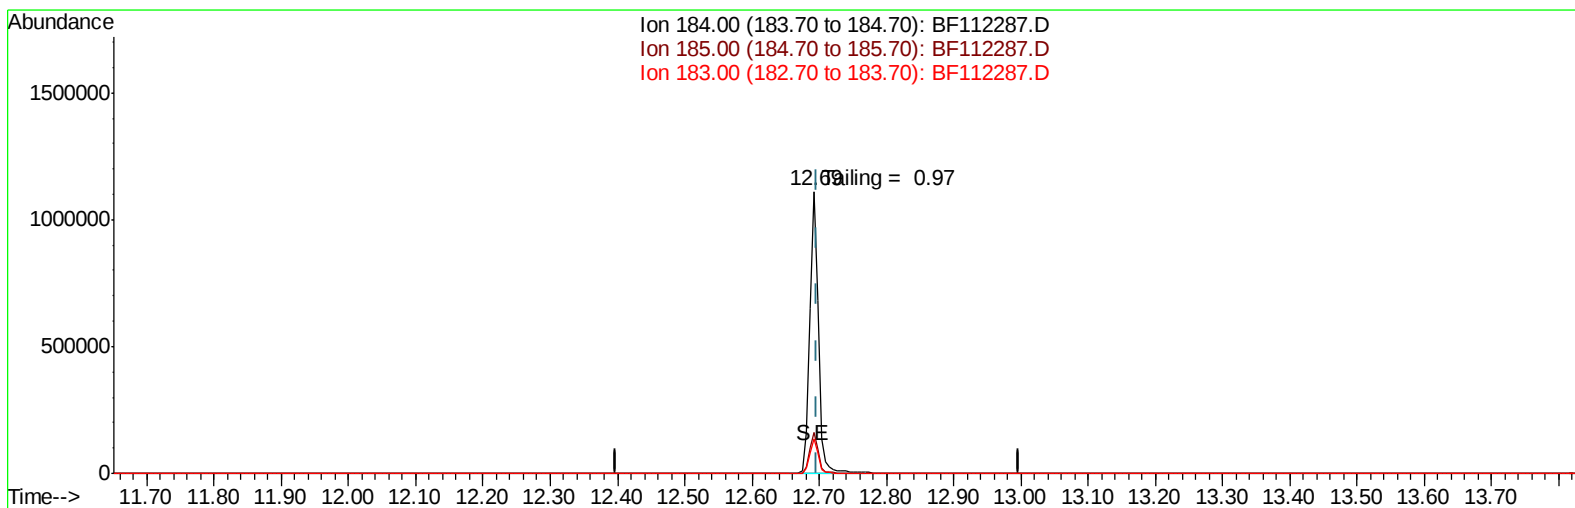

TIC: BF112287.D

(77) Benzidine




12.692min (-0.006) 0.00ng

response 1027671

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.48
183.00	12.50	12.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012919\
Data File : BF112287.D
Acq On : 29 Jan 2019 10:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 05:57:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

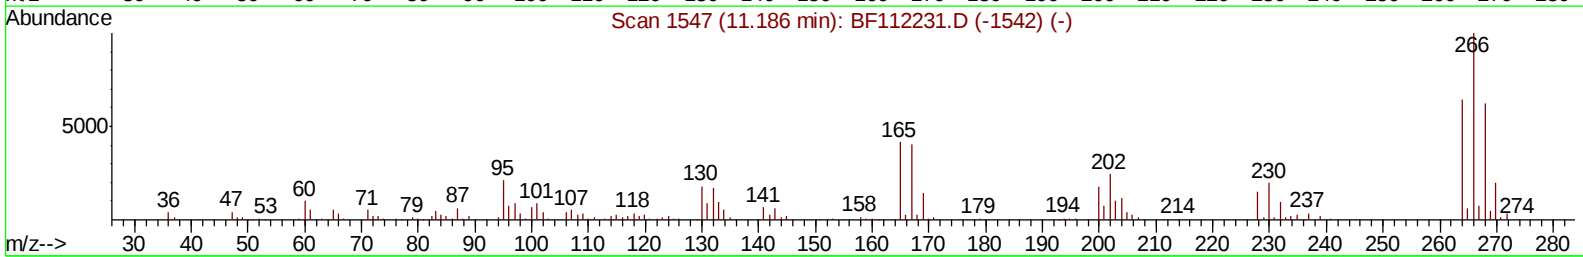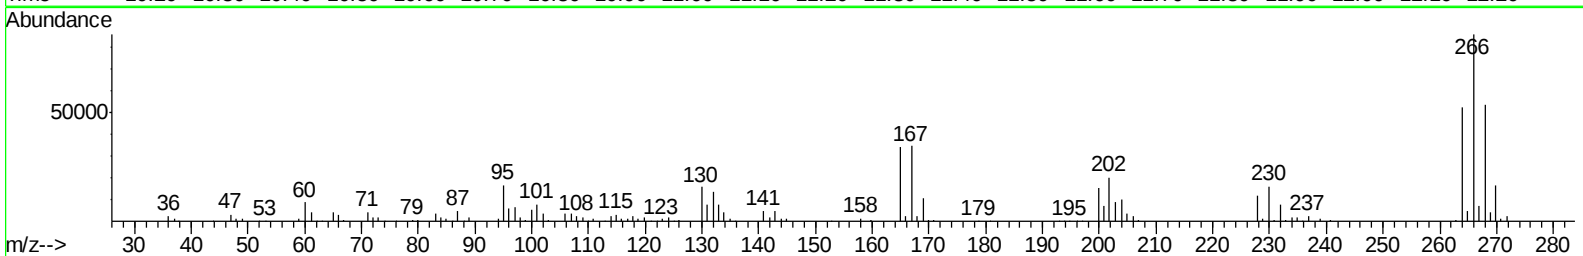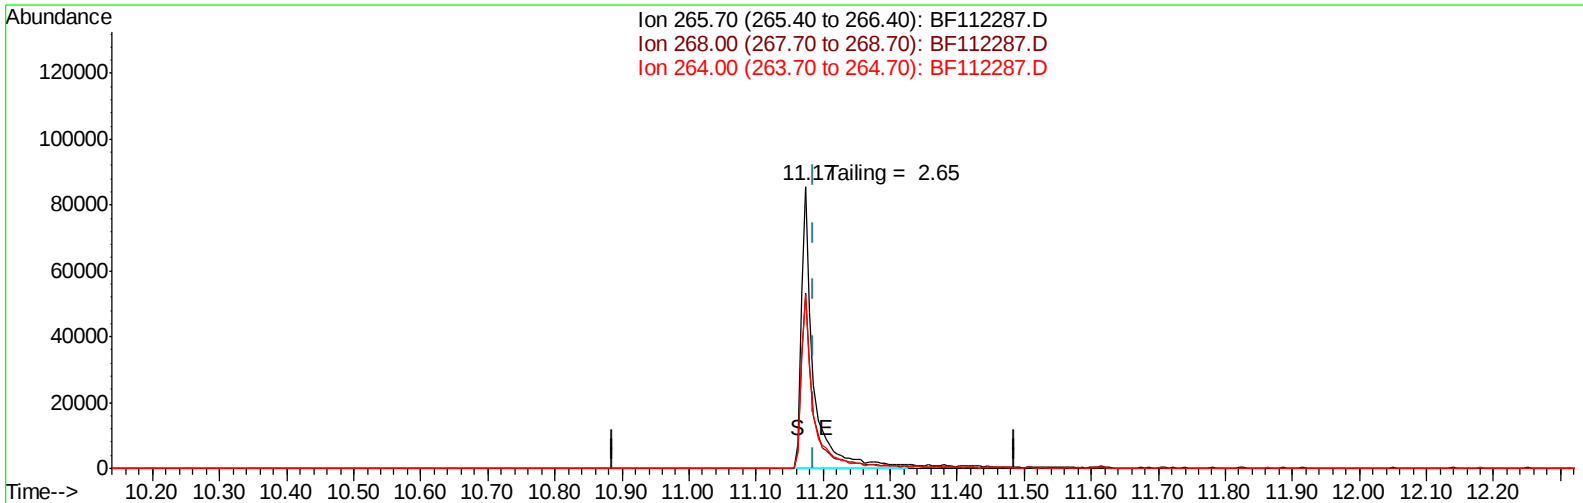

TIC: BF112287.D

(70) Pentachlorophenol (C)

11.174min (-0.012) 23669.42ng

response 107500

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.14
264.00	63.60	61.24
0.00	0.00	0.00