

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012919\
 Data File : BF112289.D
 Acq On : 29 Jan 2019 11:27
 Operator : JU/SJ
 Sample : K1015-16
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-012419-B

Quant Time: Jan 29 13:12:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	154505	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	600413	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	290287	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	539997	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	366585	20.00	ng	-0.01
87) Perylene-d12	15.46	264	332560	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	384438	52.85	ng	0.00
7) Phenol-d6	6.48	99	470030	46.50	ng	-0.01
23) Nitrobenzene-d5	7.39	82	385503	37.00	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	151784	44.92	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	836145	40.74	ng	-0.01
79) Terphenyl-d14	12.94	244	822336	42.25	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF012919\
Data File : BF112289.D
Acq On : 29 Jan 2019 11:27
Operator : JU/SJ
Sample : K1015-16
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-04-012419-B

Quant Time: Jan 29 13:12:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

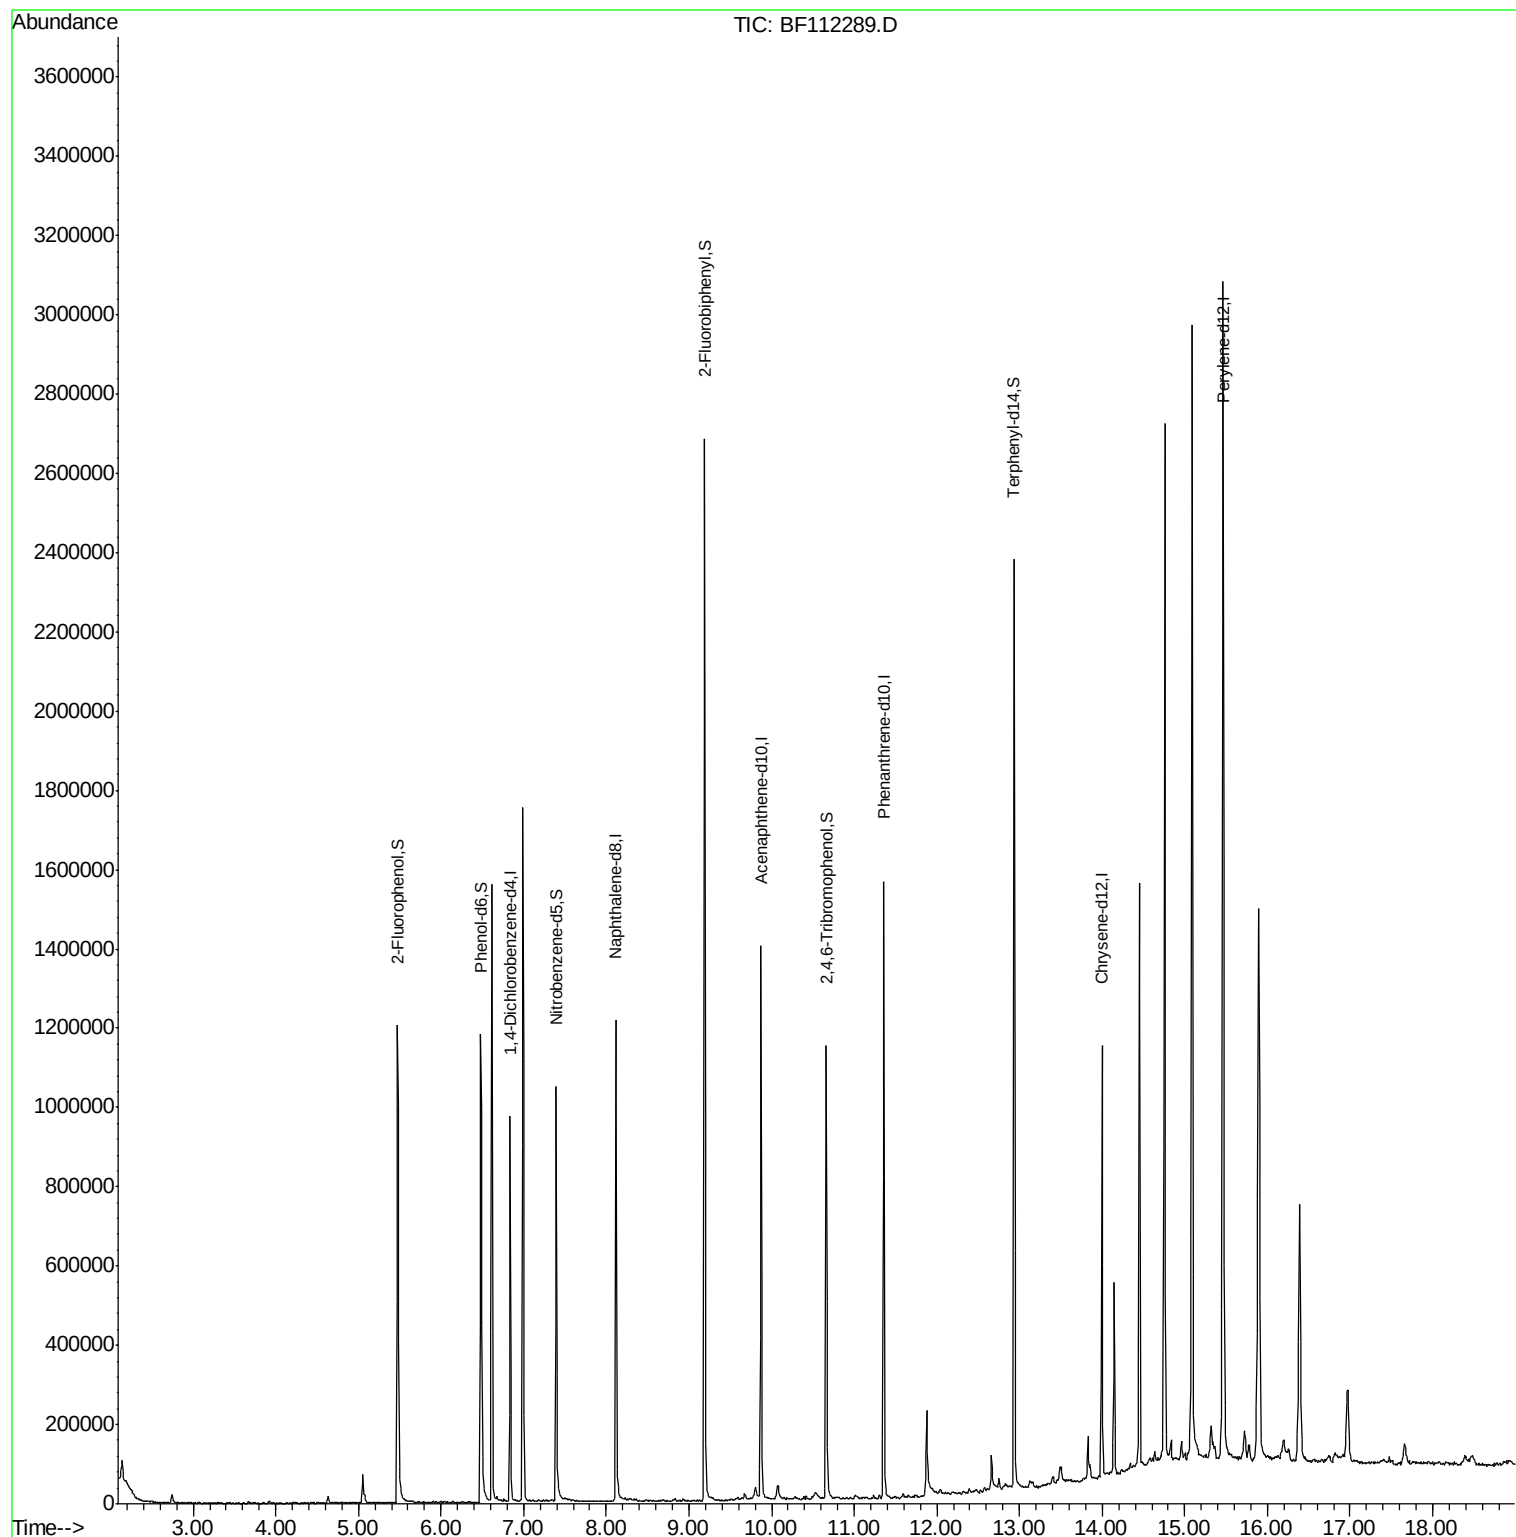

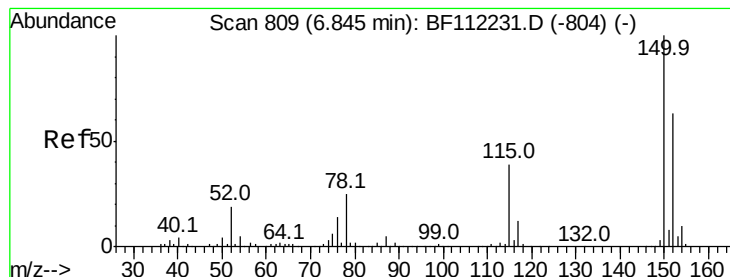


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.84 min Scan# 808
Delta R.T. -0.01 min
Lab File: BF112289.D
Acq: 29 Jan 2019 11:27

Instrument :
BNA_F
ClientSampleId :
SU-04-012419-B

Tot Ion:152 Resp: 154505
Ion Ratio Lower Upper
152 100
150 155.3 127.4 191.0
115 56.0 45.5 68.3

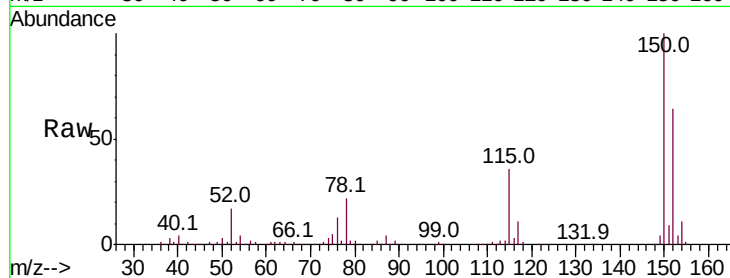


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

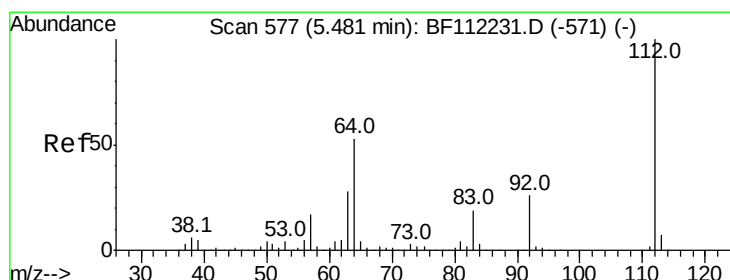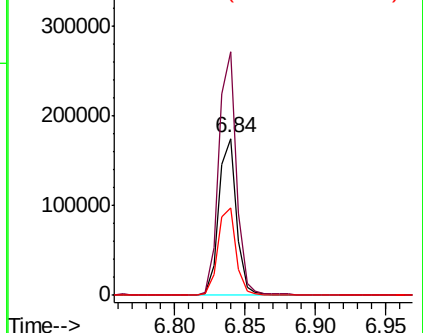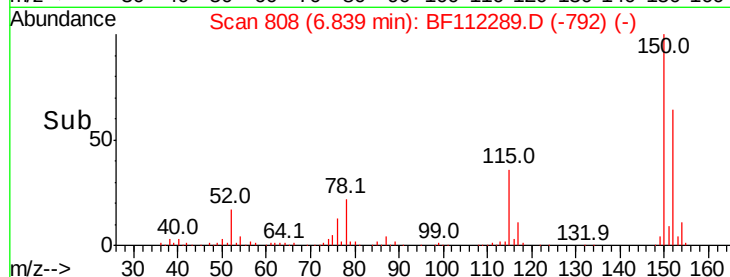



#5


2-Fluorophenol
Concen: 52.851 ng
RT: 5.47 min Scan# 576
Delta R.T. -0.01 min
Lab File: BF112289.D
Acq: 29 Jan 2019 11:27

Tgt Ion:112 Resp: 384438
Ion Ratio Lower Upper
112 100
64 56.5 45.7 68.5
63 30.2 23.6 35.4

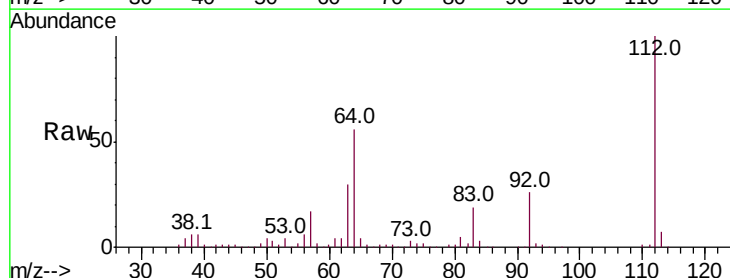

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

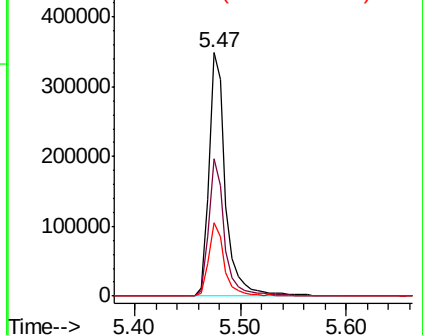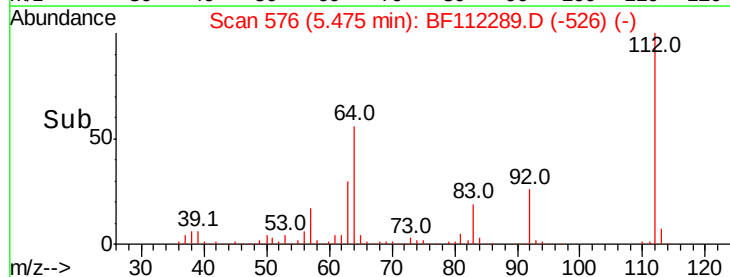

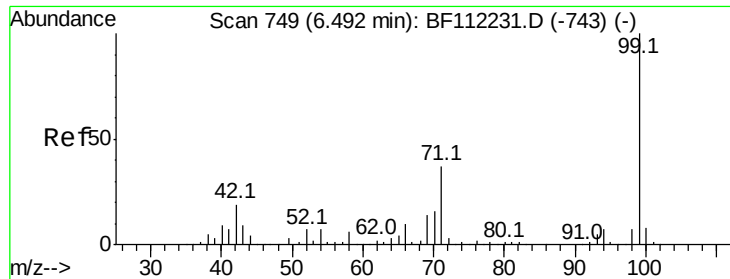

#7

Phenol-d6

Concen: 46.503 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF112289.D

Acq: 29 Jan 2019 11:27

Instrument :

BNA_F

ClientSampleId :

SU-04-012419-B


Tot Ion: 99 Resp: 470030

Ion Ratio Lower Upper




99 100

42 18.5 15.1 22.7

71 36.2 26.9 40.3

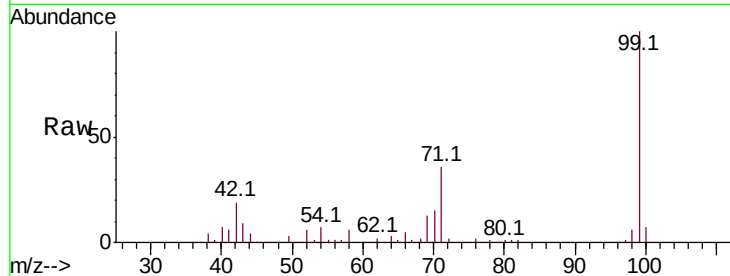

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

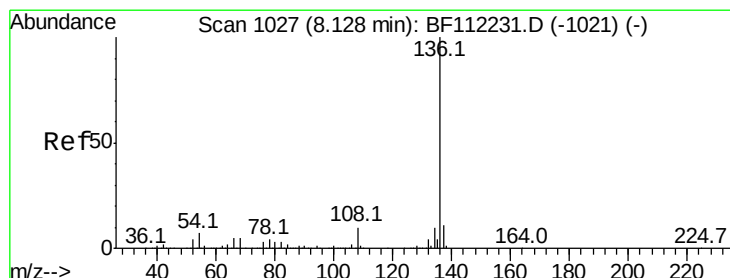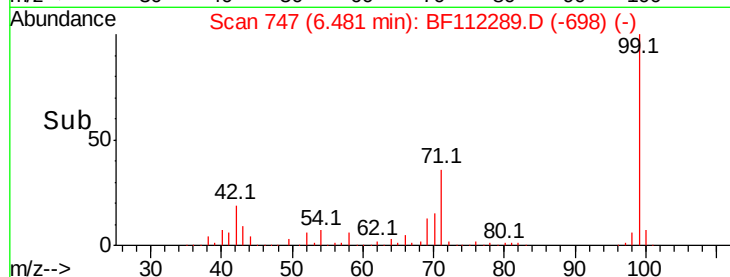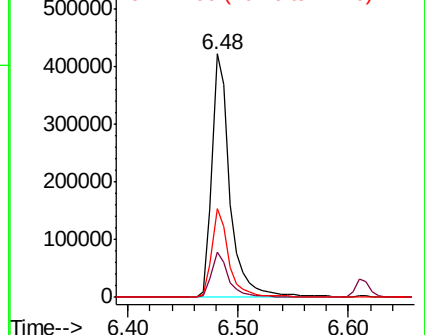

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112289.D

Acq: 29 Jan 2019 11:27

Tgt Ion: 136 Resp: 600413


Ion Ratio Lower Upper

136 100



137 10.9 9.1 13.7


54 6.4 5.9 8.9

68 5.2 5.1 7.7

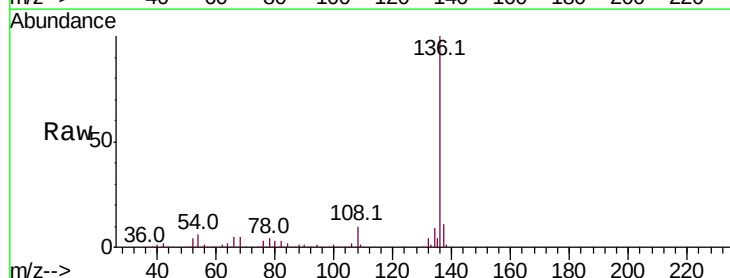

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

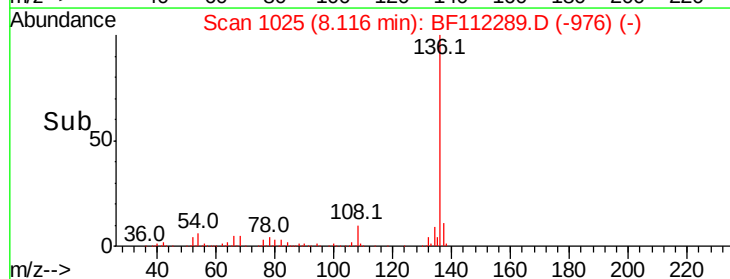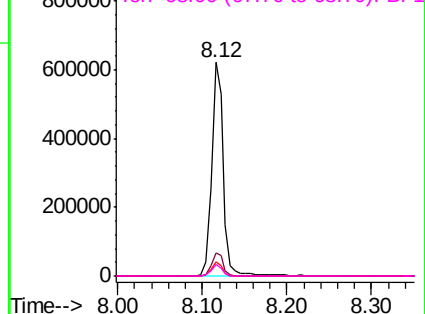


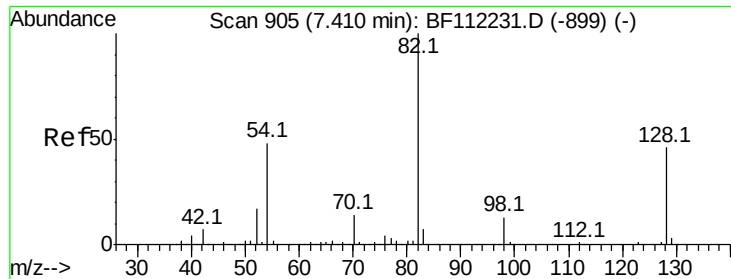




#23
 Nitrobenzene-d5
 Concen: 36.996 ng
 RT: 7.39 min Scan# 902
 Delta R.T. -0.02 min
 Lab File: BF112289.D
 Acq: 29 Jan 2019 11:27

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-012419-B

Tot Ion	82	Resp	385503
Ion Ratio	Lower	Upper	
82	100		
128	43.7	37.8	56.8
54	48.6	39.7	59.5

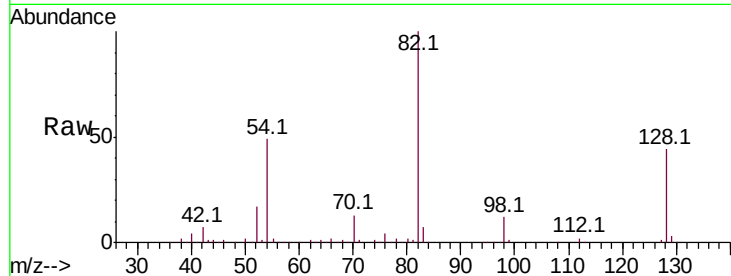


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

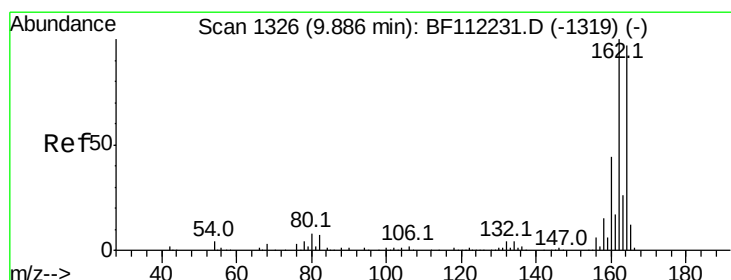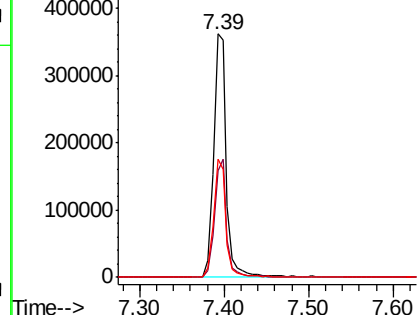
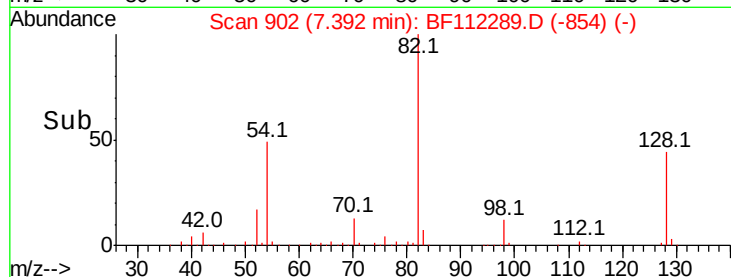



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1324
 Delta R.T. -0.01 min
 Lab File: BF112289.D
 Acq: 29 Jan 2019 11:27

Tgt Ion	164	Resp	290287
Ion Ratio	Lower	Upper	
164	100		
162	103.5	82.2	123.4
160	47.7	36.2	54.4

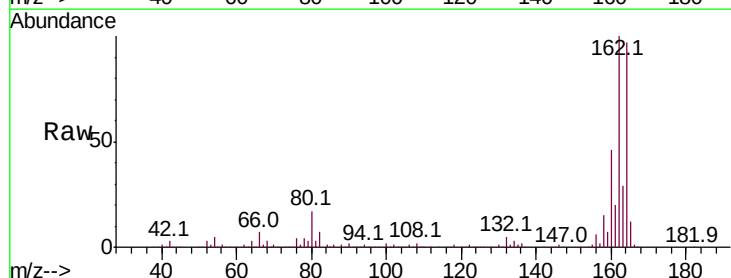

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

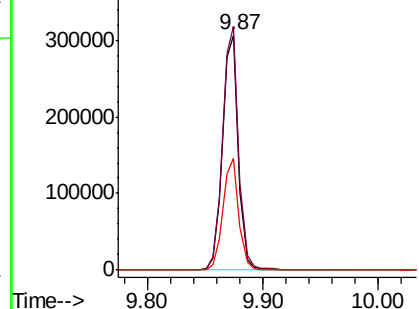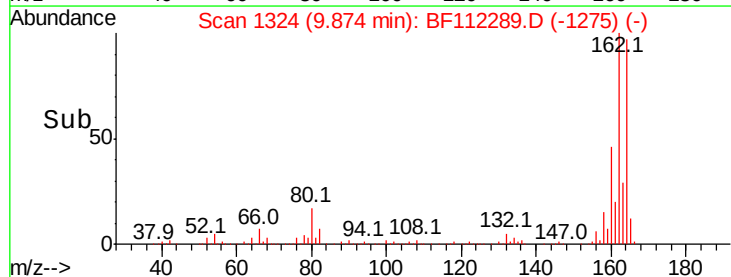


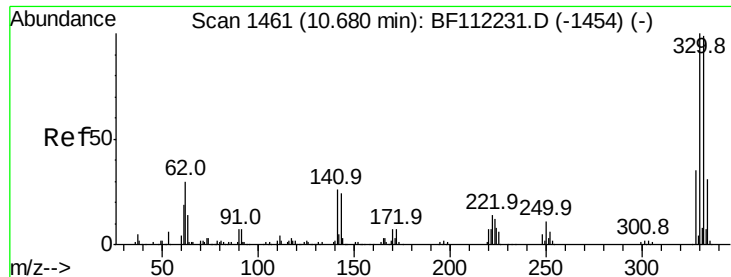




#42
 2,4,6-Tribromophenol
 Concen: 44.922 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.02 min
 Lab File: BF112289.D
 Acq: 29 Jan 2019 11:27

Instrument :
 BNA_F
 ClientSampleId :
 SU-04-012419-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	76.6	114.8
141	32.3	24.3	36.5

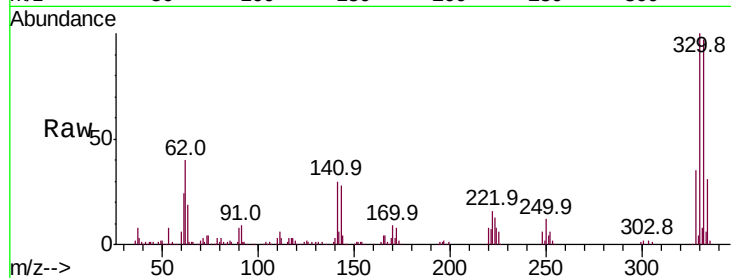


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

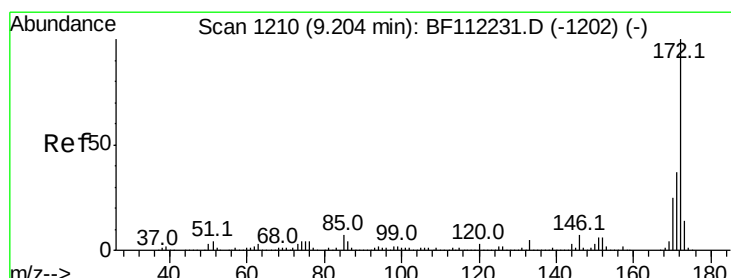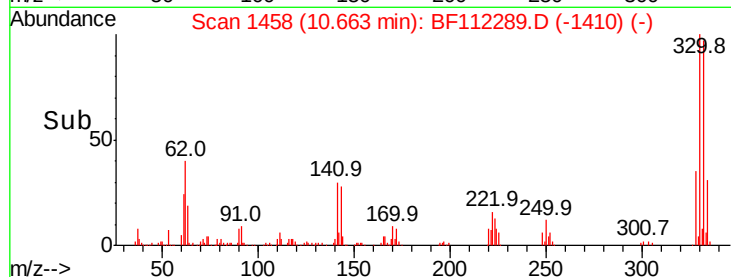
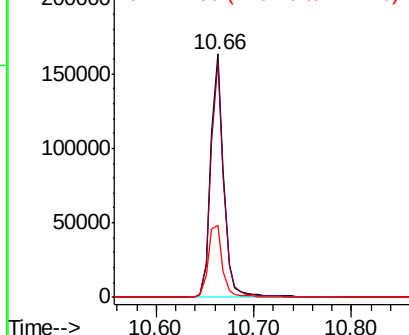



#45
 2-Fluorobiphenyl
 Concen: 40.739 ng
 RT: 9.19 min Scan# 1208
 Delta R.T. -0.01 min
 Lab File: BF112289.D
 Acq: 29 Jan 2019 11:27

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	30.5	45.7
170	23.5	20.2	30.4

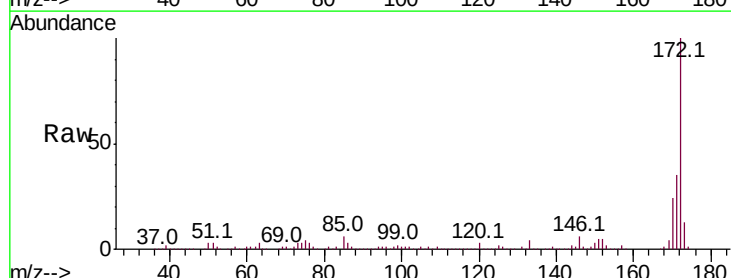

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



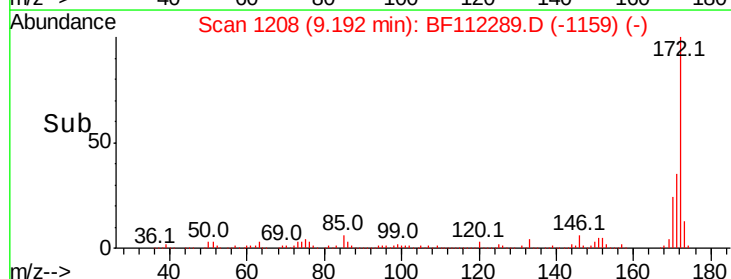
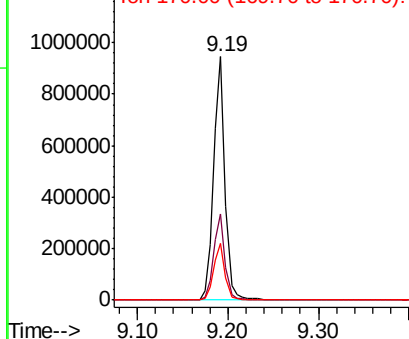


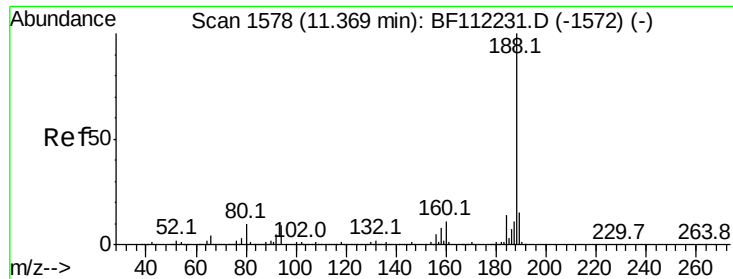

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112289.D
Acq: 29 Jan 2019 11:27




Instrument :
BNA_F
ClientSampleId :
SU-04-012419-B


Tot Ion	Ratio	Lower	Upper
188	100		
94	9.0	8.2	12.2
80	9.8	8.9	13.3

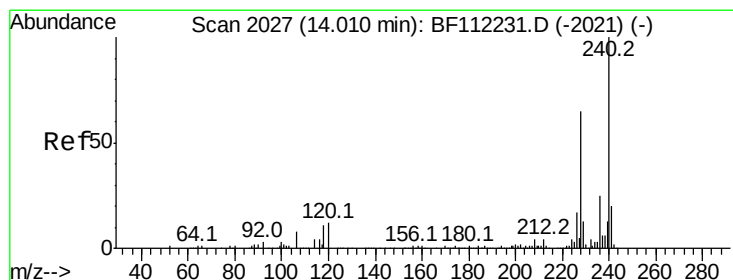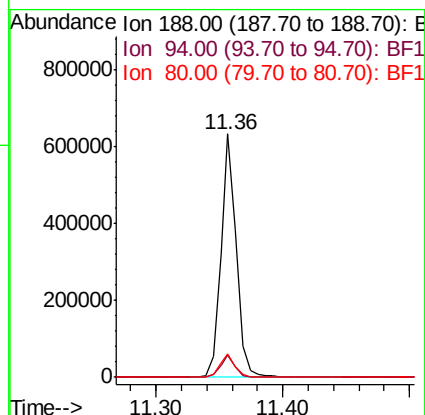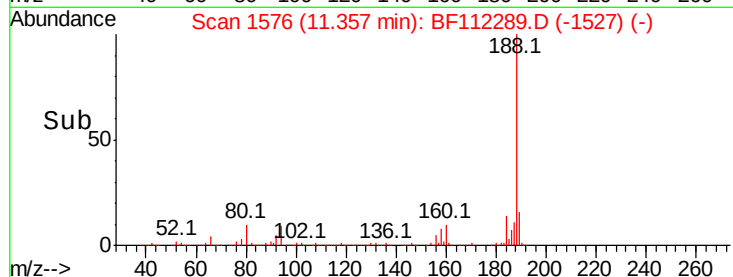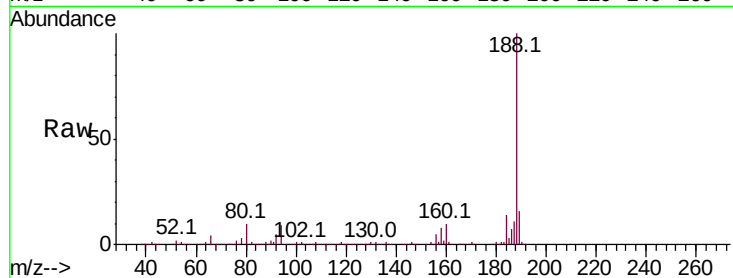

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112289.D
Acq: 29 Jan 2019 11:27

Tgt Ion	Ratio	Lower	Upper
240	100		
120	10.5	9.0	13.6
236	25.7	20.7	31.1

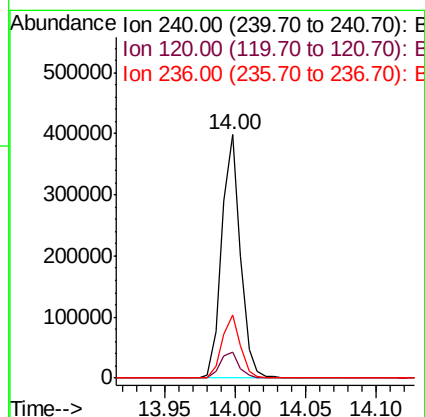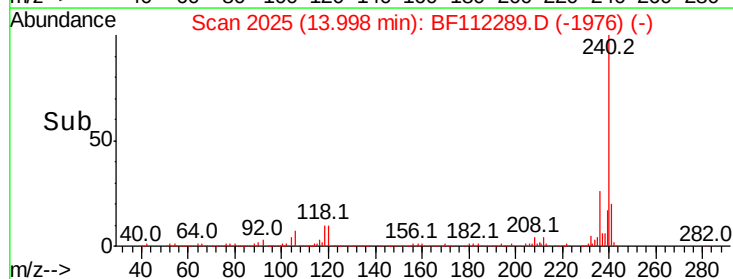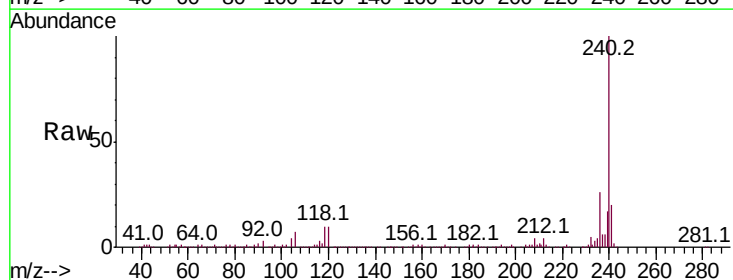

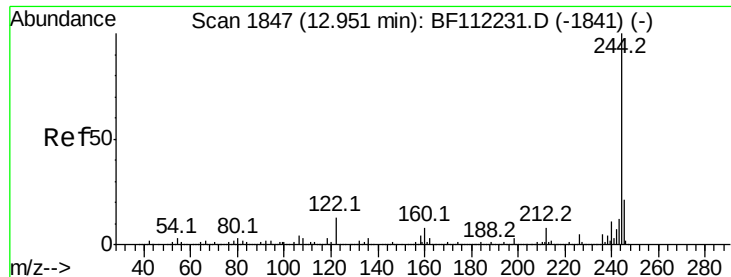

#79

Terphenyl-d14

Concen: 42.250 ng

RT: 12.94 min Scan# 1845

Delta R.T. -0.01 min

Lab File: BF112289.D

Acq: 29 Jan 2019 11:27

Instrument :

BNA_F

ClientSampleId :

SU-04-012419-B


Tot Ion:244 Resp: 822336

Ion Ratio Lower Upper

244 100

212 6.6 5.9 8.9




122 10.3 9.8 14.6

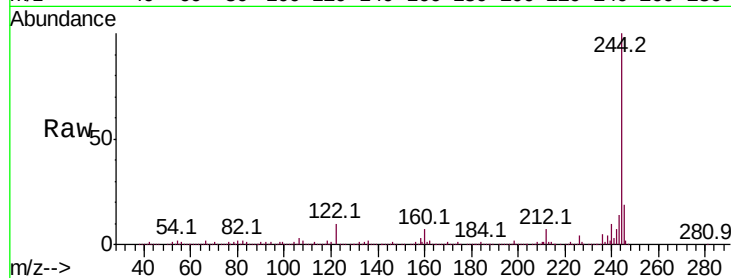

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

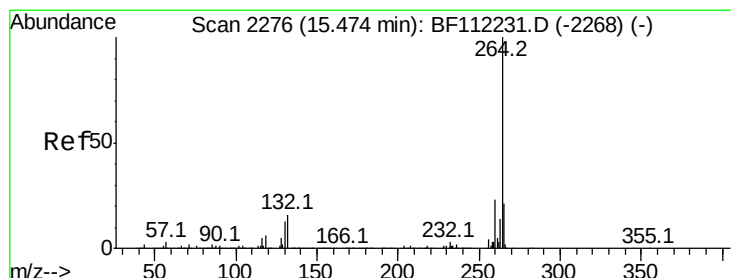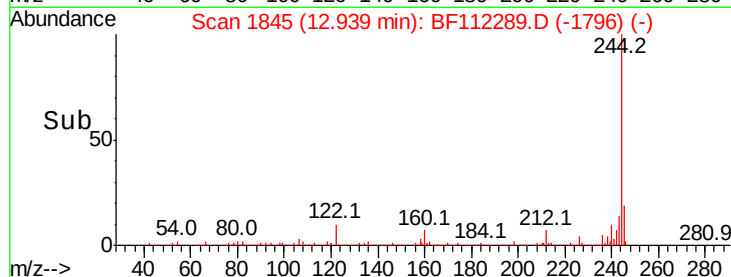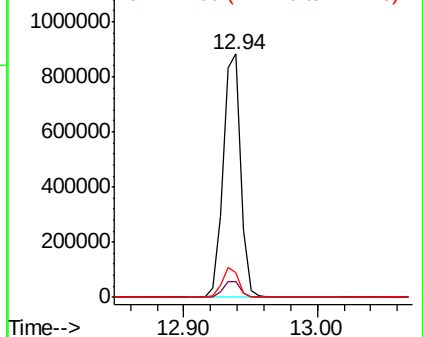

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2274

Delta R.T. -0.01 min

Lab File: BF112289.D

Acq: 29 Jan 2019 11:27


Tgt Ion:264 Resp: 332560

Ion Ratio Lower Upper

264 100

260 23.0 18.2 27.2

265 20.8 17.0 25.4

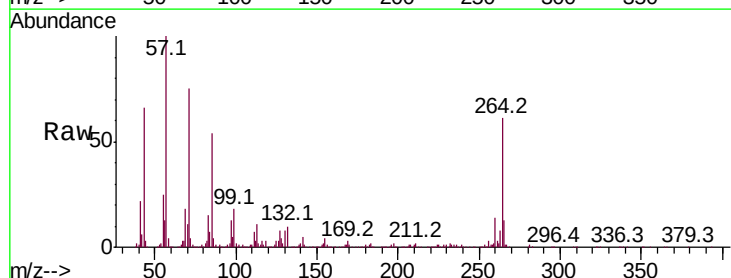

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

