
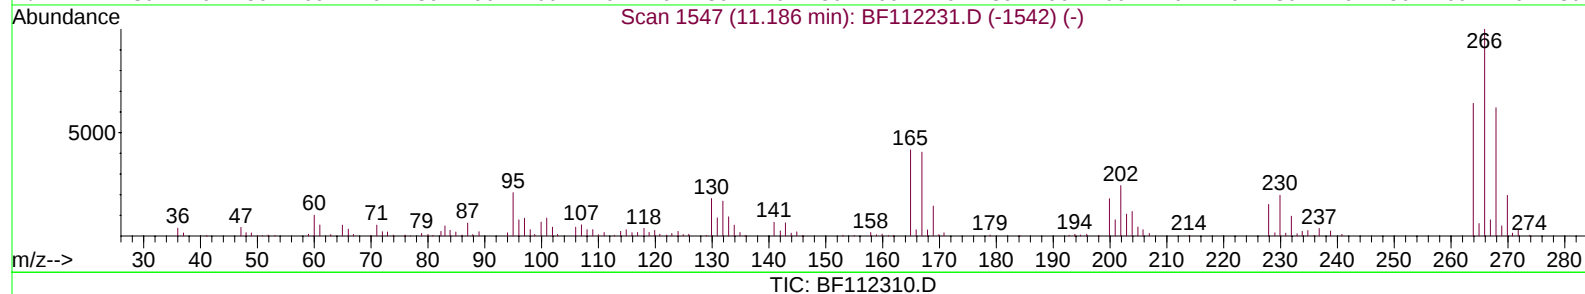
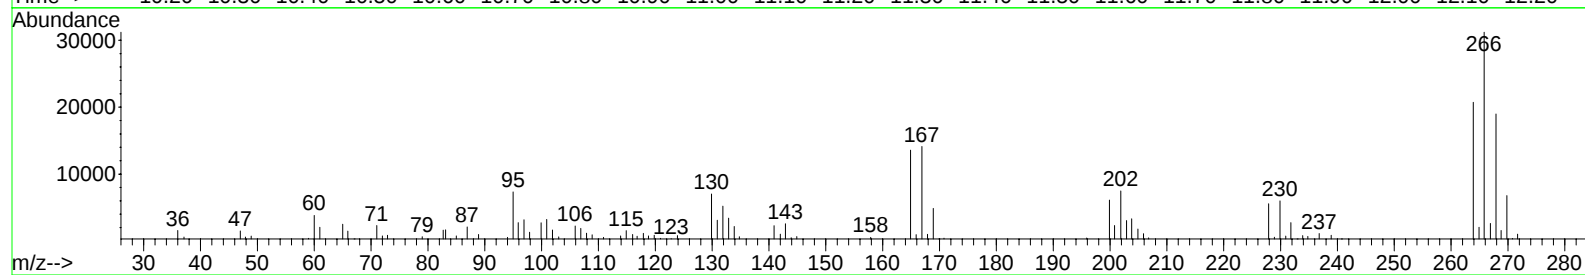


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF013019\
Data File : BF112310.D
Acq On : 30 Jan 2019 8:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 11:16:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

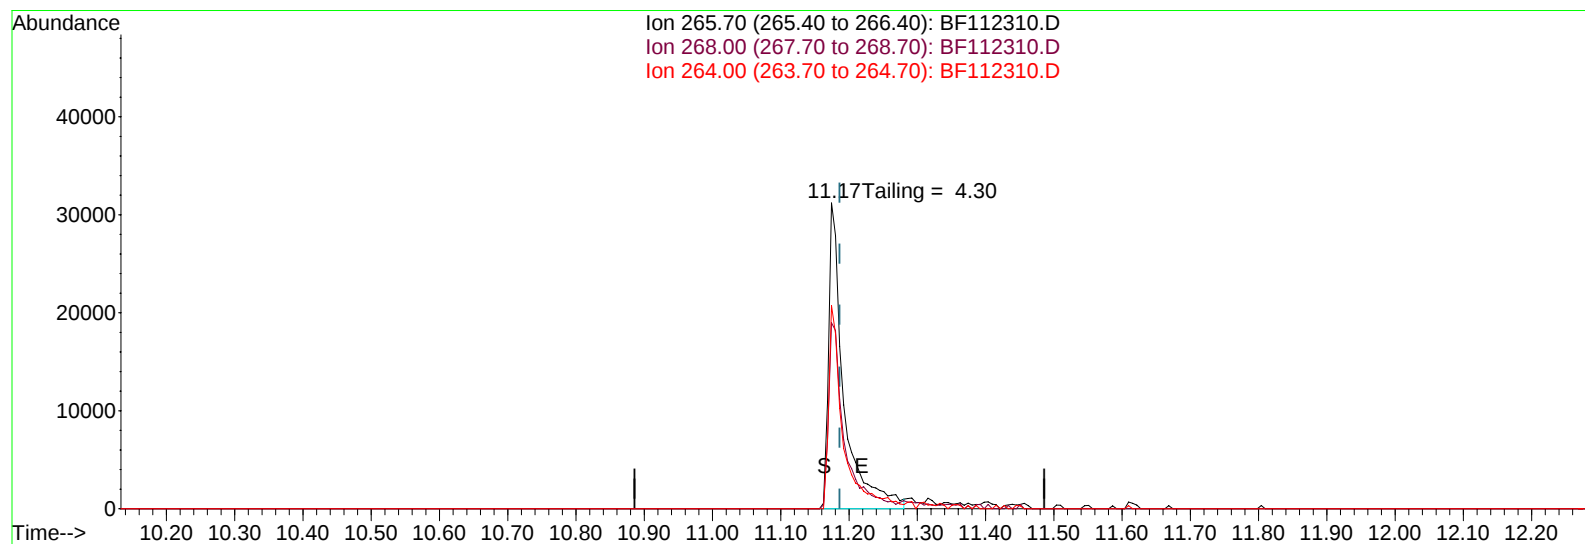

(70) Pentachlorophenol (C)




11.174min (-0.012) 20493.79ng

response 48702

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	60.82
264.00	63.60	66.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF013019\
Data File : BF112310.D
Acq On : 30 Jan 2019 8:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 11:16:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

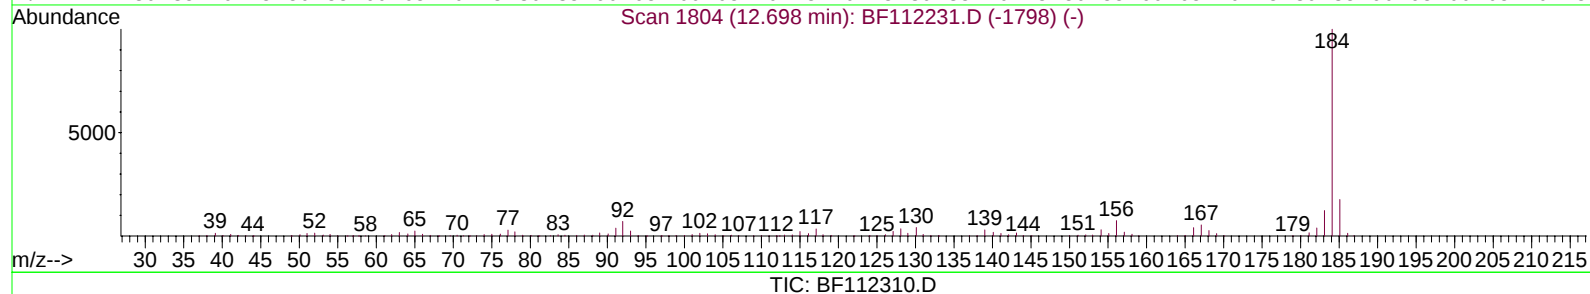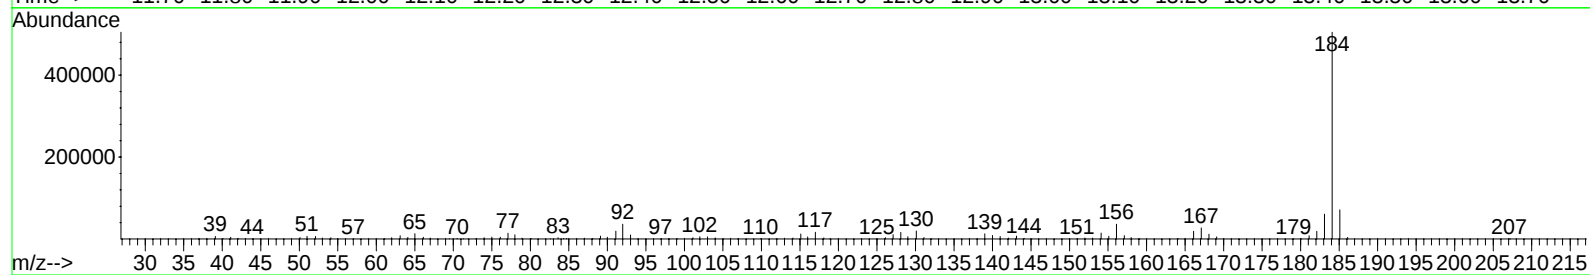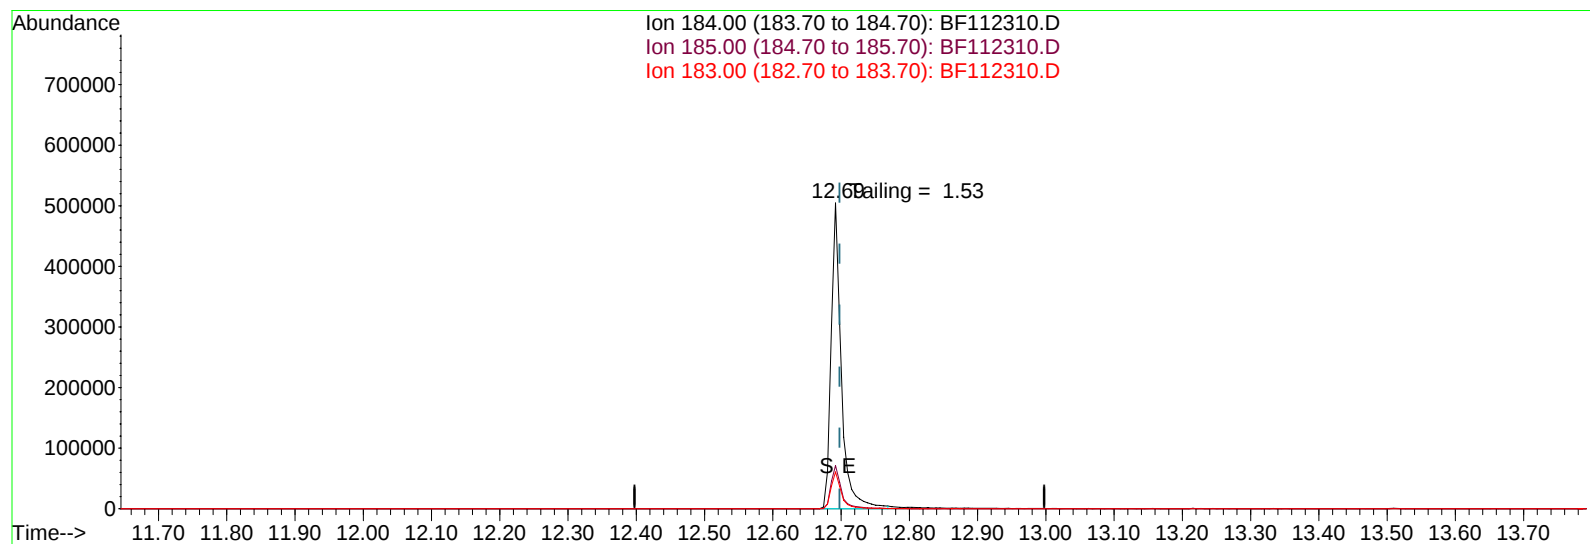

(77) Benzidine

12.692min (-0.006) 0.00ng

response 523856

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.14
183.00	12.50	12.04
0.00	0.00	0.00