

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013019\
 Data File : BF112320.D
 Acq On : 30 Jan 2019 14:31
 Operator : JU/SJ
 Sample : K1250-04 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DRUM-1-3

Quant Time: Jan 30 15:40:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	97792	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	363433	20.00	ng	0.00
39) Acenaphthene-d10	9.87	164	153552	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	258189	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	215206	20.00	ng	0.00
87) Perylene-d12	15.48	264	253596	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	60309	13.10	ng	0.00
7) Phenol-d6	6.49	99	46735	7.31	ng	0.00
23) Nitrobenzene-d5	7.40	82	110245	17.48	ng	-0.01
42) 2,4,6-Tribromophenol	10.67	330	39152	21.91	ng	-0.01
45) 2-Fluorobiphenyl	9.19	172	224144	20.65	ng	-0.01
79) Terphenyl-d14	12.94	244	166750	14.59	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF013019\
Data File : BF112320.D
Acq On : 30 Jan 2019 14:31
Operator : JU/SJ
Sample : K1250-04 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DRUM-1-3

Quant Time: Jan 30 15:40:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

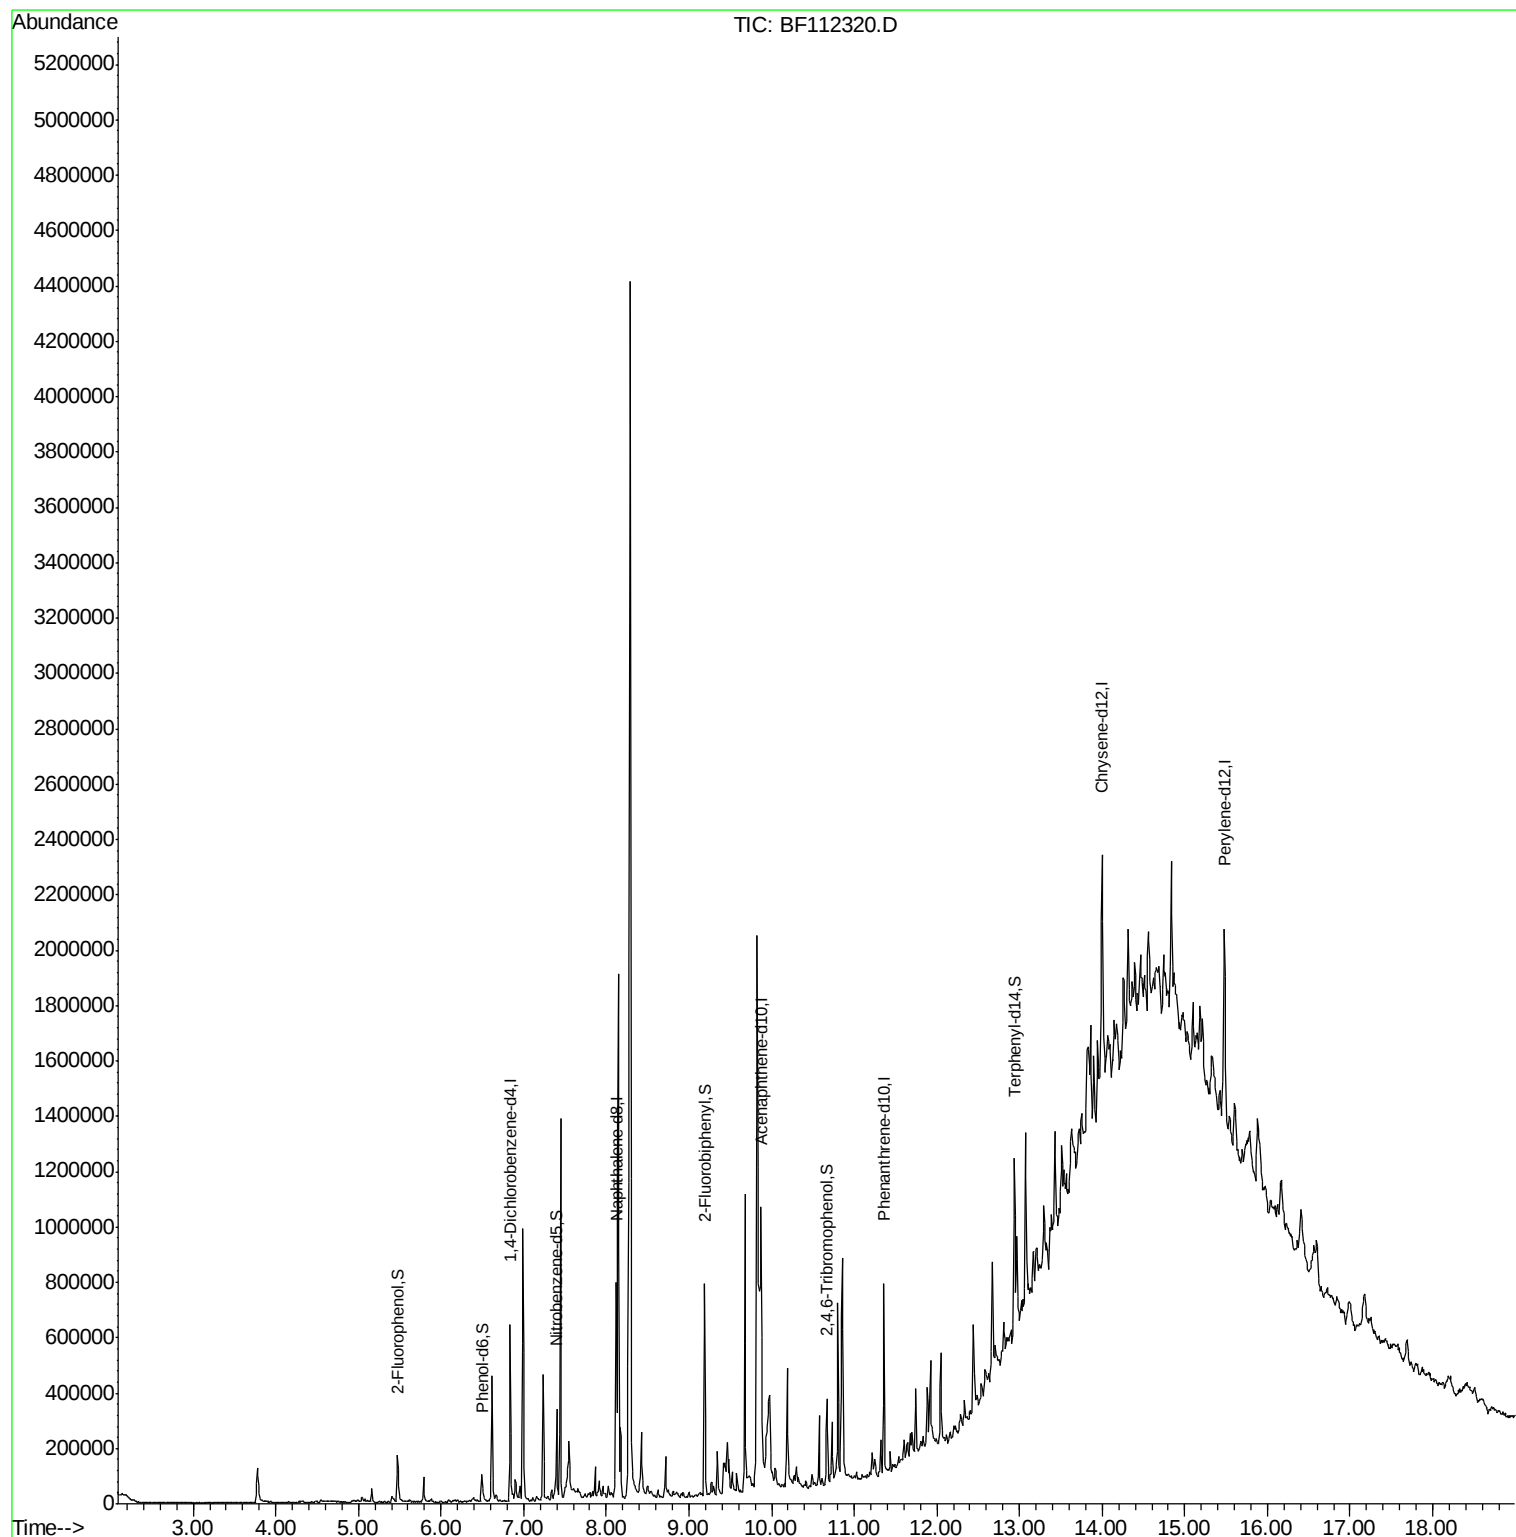

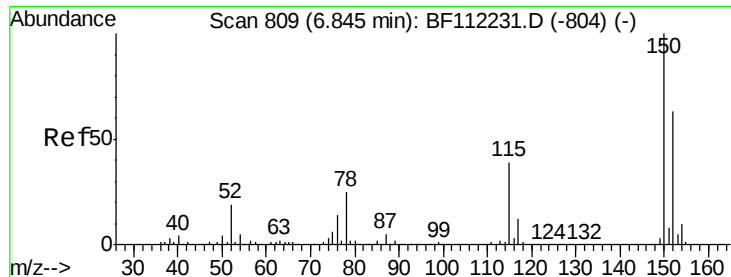


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.84 min Scan# 808
Delta R.T. -0.01 min
Lab File: BF112320.D
Acq: 30 Jan 2019 14:31

Instrument :
BNA_F
ClientSampleId :
DRUM-1-3

Tot Ion:152 Resp: 97792
Ion Ratio Lower Upper
152 100
150 154.5 127.4 191.0
115 59.0 45.5 68.3

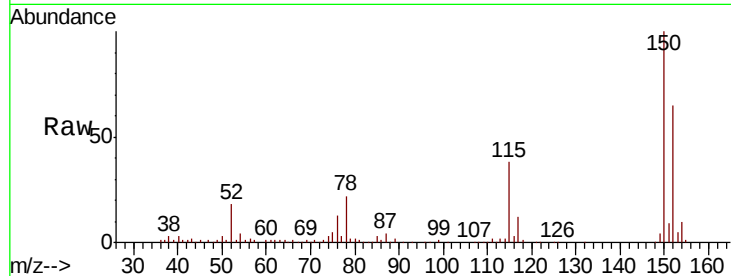


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

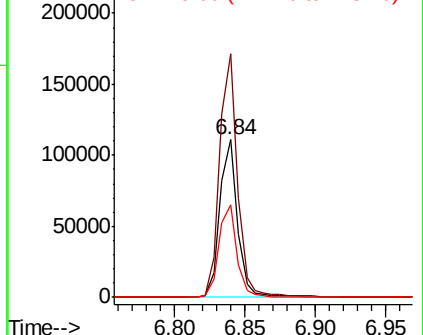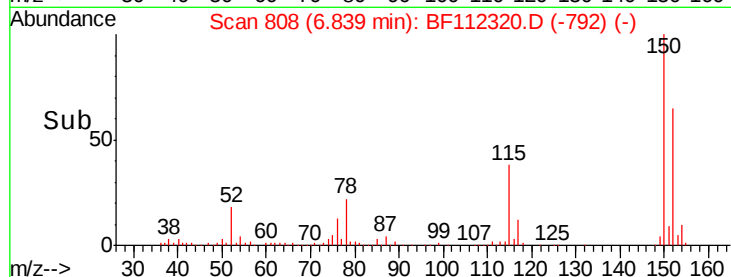



#5

2-Fluorophenol
Concen: 13.099 ng
RT: 5.47 min Scan# 576
Delta R.T. -0.01 min
Lab File: BF112320.D
Acq: 30 Jan 2019 14:31

Tgt Ion:112 Resp: 60309
Ion Ratio Lower Upper
112 100
64 53.6 45.7 68.5
63 29.1 23.6 35.4

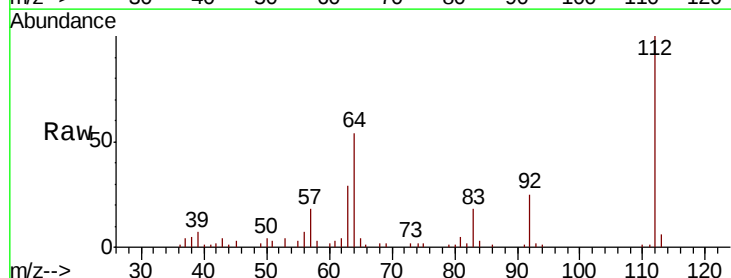

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

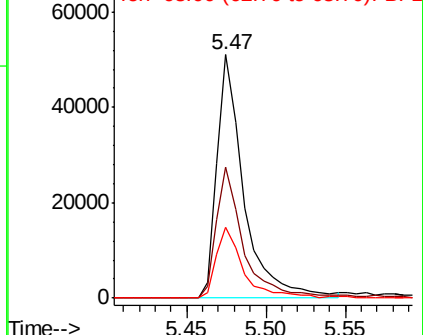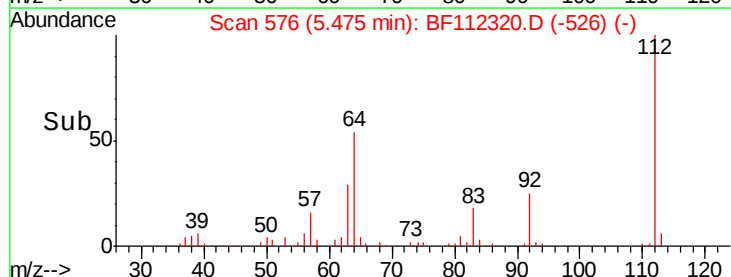



#7

Phenol-d6

Concen: 7.305 ng

RT: 6.49 min Scan# 749

Delta R.T. 0.00 min

Lab File: BF112320.D

Acq: 30 Jan 2019 14:31

Instrument :

BNA_F

ClientSampleId :

DRUM-1-3


Tot Ion: 99 Resp: 46735

Ion Ratio Lower Upper




99 100

42 19.1 15.1 22.7

71 33.0 26.9 40.3

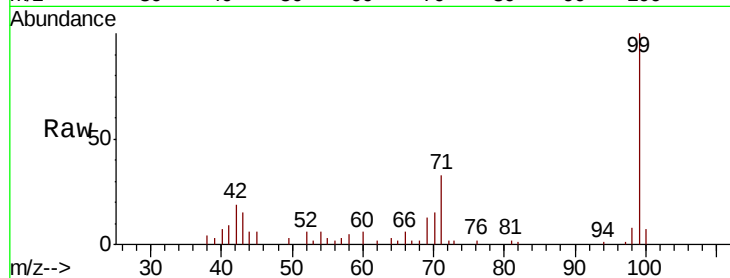

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

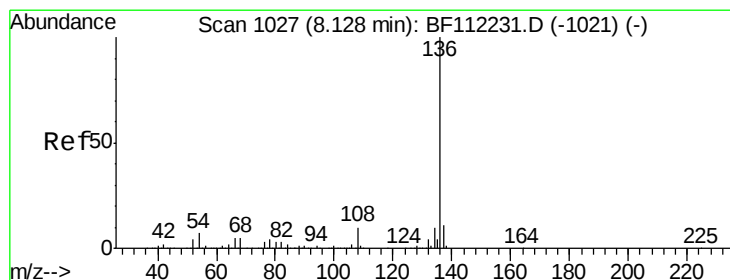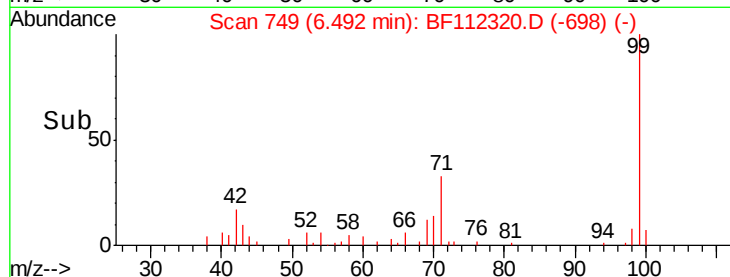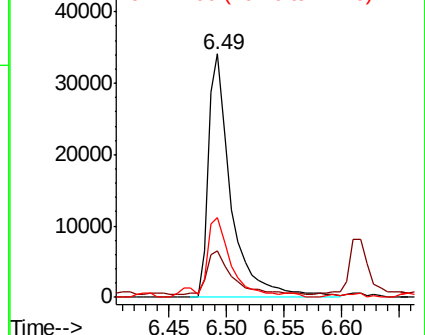

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1026

Delta R.T. -0.01 min

Lab File: BF112320.D

Acq: 30 Jan 2019 14:31

Tgt Ion: 136 Resp: 363433


Ion Ratio Lower Upper

136 100



137 10.6 9.1 13.7


54 5.9 5.9 8.9#

68 4.8 5.1 7.7#

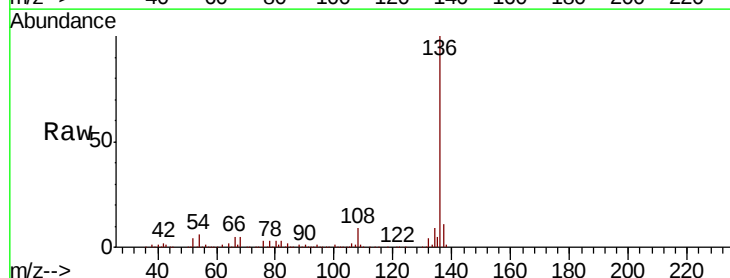

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



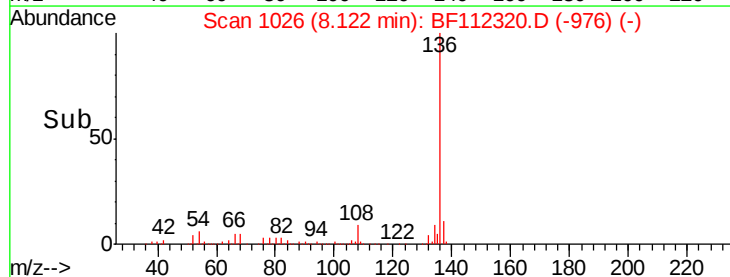
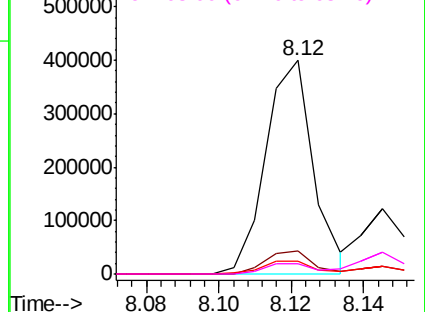


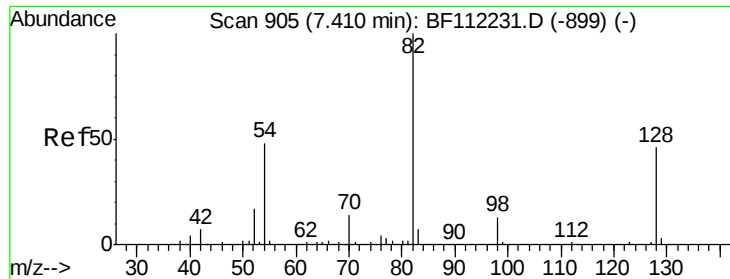

#23
Nitrobenzene-d5
Concen: 17.479 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.01 min
Lab File: BF112320.D
Acq: 30 Jan 2019 14:31




Instrument :
BNA_F
ClientSampled :
DRUM-1-3

Tot Ion: 82 Resp: 110245
Ion Ratio Lower Upper
82 100
128 47.1 37.8 56.8
54 46.0 39.7 59.5

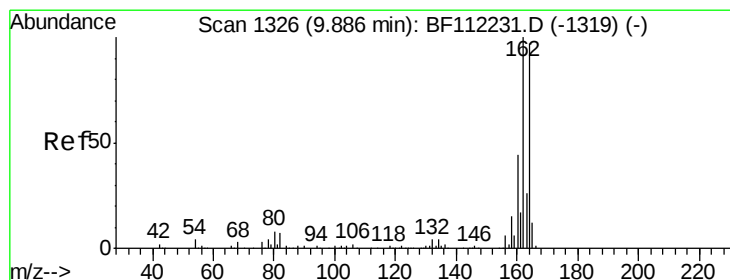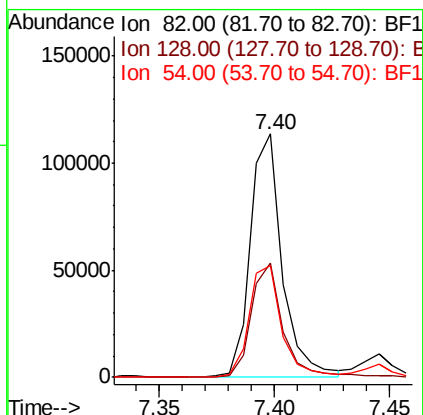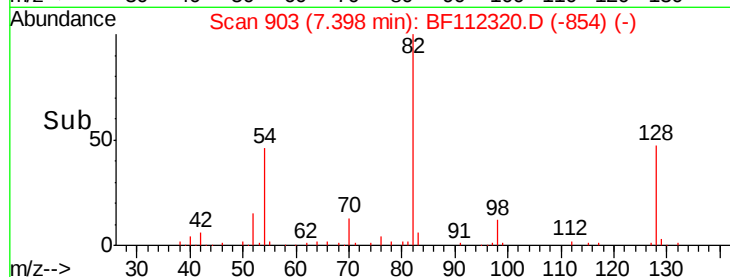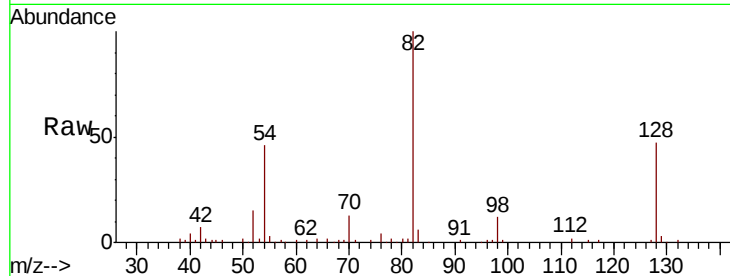

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.87 min Scan# 1324
Delta R.T. -0.01 min
Lab File: BF112320.D
Acq: 30 Jan 2019 14:31

Tgt Ion:164 Resp: 153552
Ion Ratio Lower Upper
164 100
162 104.6 82.2 123.4
160 46.4 36.2 54.4

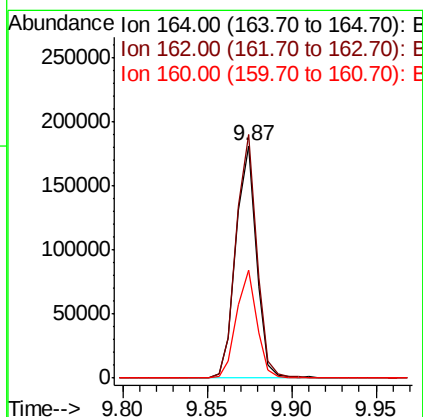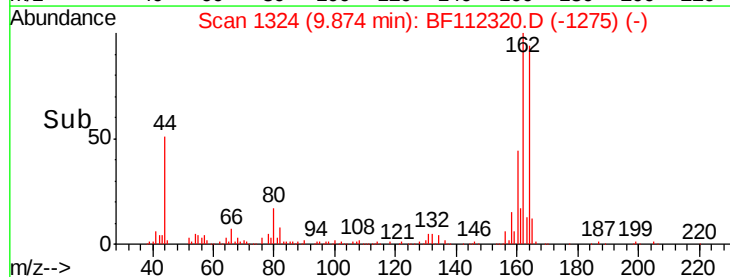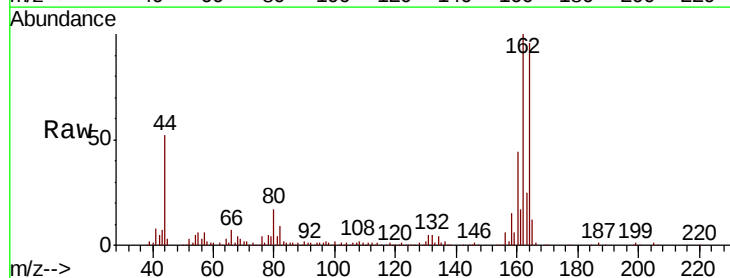



#42

2,4,6-Tribromophenol

Concen: 21.906 ng

RT: 10.67 min Scan# 1459

Delta R.T. -0.01 min

Lab File: BF112320.D

Acq: 30 Jan 2019 14:31

Instrument :

BNA_F

ClientSampled :

DRUM-1-3


Tot Ion:330 Resp: 39152

Ion Ratio Lower Upper




330 100

332 96.5 76.6 114.8

141 36.5 24.3 36.5#

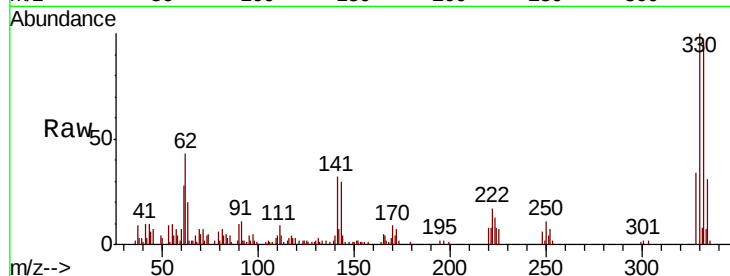

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

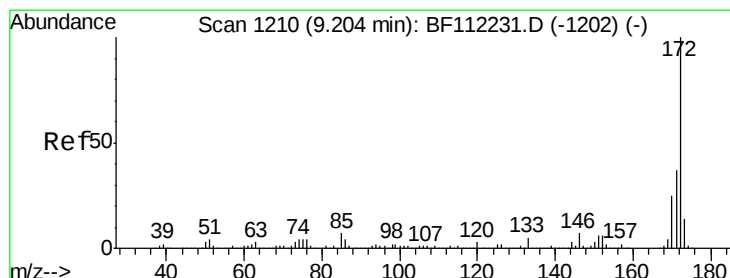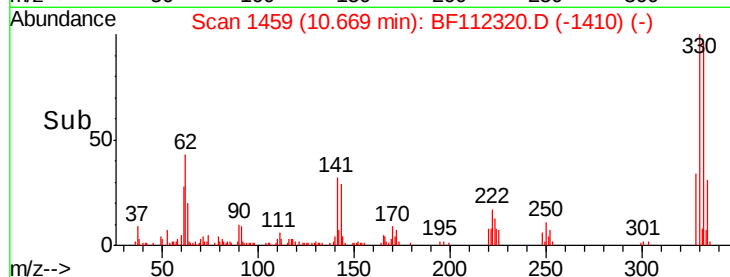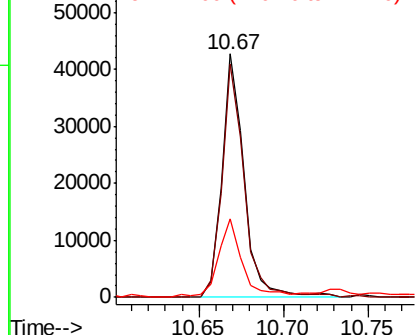

#45

2-Fluorobiphenyl

Concen: 20.645 ng

RT: 9.19 min Scan# 1208

Delta R.T. -0.01 min

Lab File: BF112320.D

Acq: 30 Jan 2019 14:31


Tgt Ion:172 Resp: 224144

Ion Ratio Lower Upper



172 100

171 35.8 30.5 45.7

170 23.5 20.2 30.4

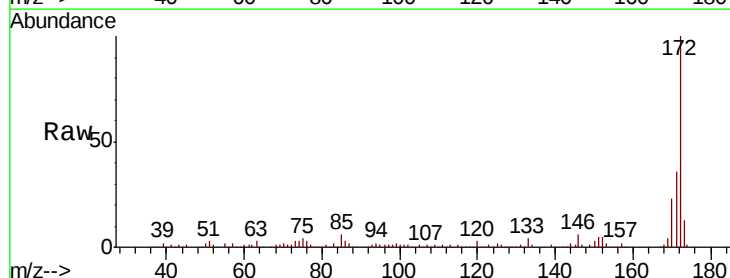

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



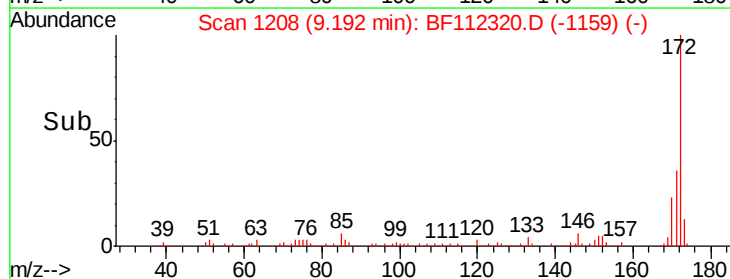
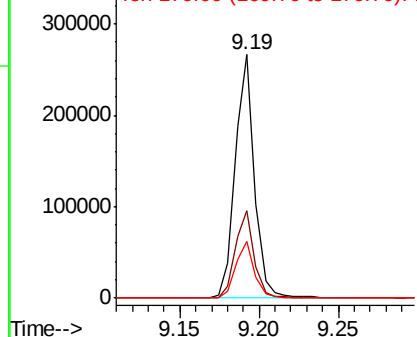




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112320.D
Acq: 30 Jan 2019 14:31




Instrument :
BNA_F
ClientSampleId :
DRUM-1-3


Tot Ion:188 Resp: 258189
Ion Ratio Lower Upper
188 100
94 8.6 8.2 12.2
80 9.4 8.9 13.3

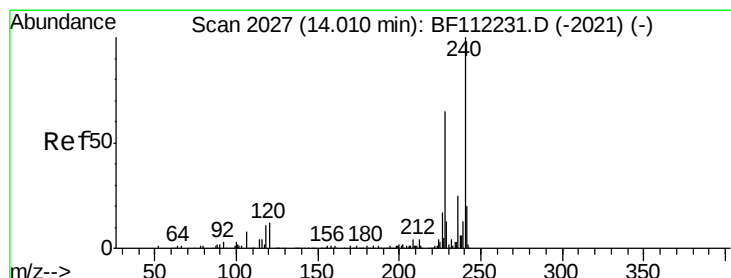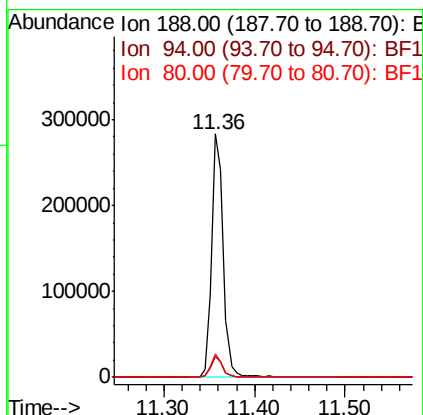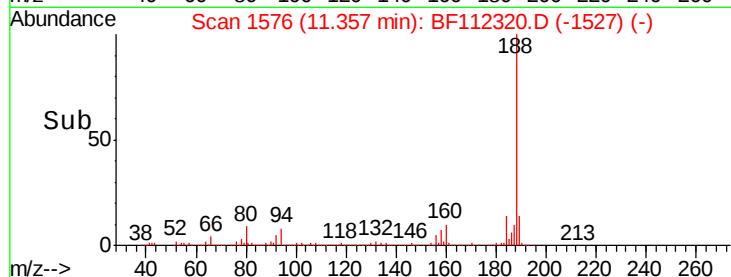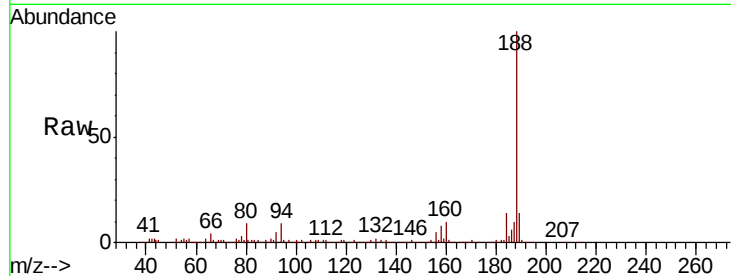

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.01 min
Lab File: BF112320.D
Acq: 30 Jan 2019 14:31

Tgt Ion:240 Resp: 215206
Ion Ratio Lower Upper
240 100
120 13.4 9.0 13.6
236 25.9 20.7 31.1


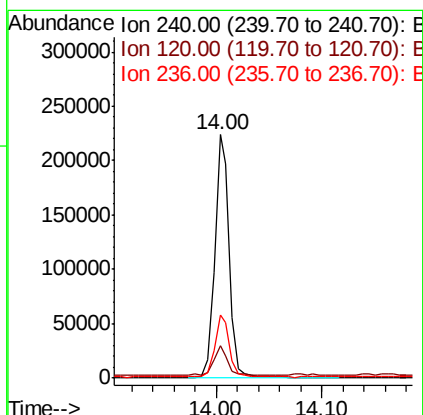
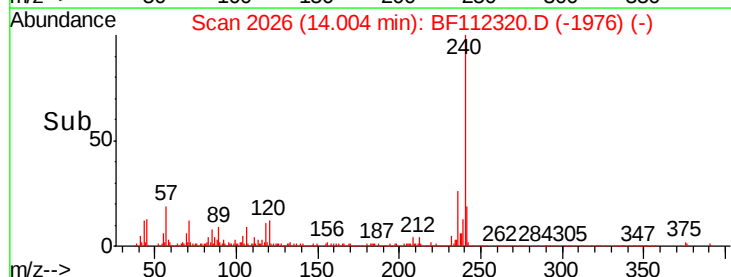
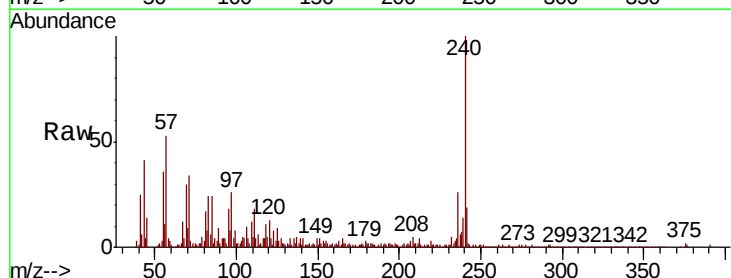


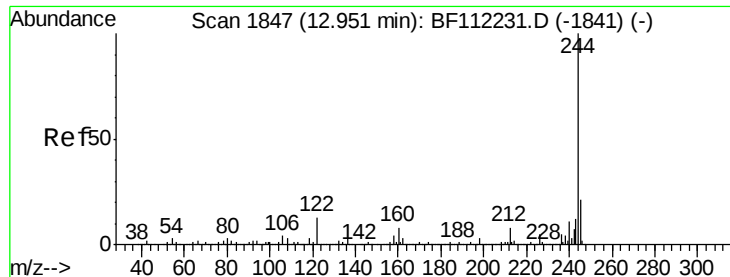

#79
 Terphenyl-d14
 Concen: 14.594 ng
 RT: 12.94 min Scan# 1845
 Delta R.T. -0.01 min
 Lab File: BF112320.D
 Acq: 30 Jan 2019 14:31

Instrument :
 BNA_F
 ClientSampleId :
 DRUM-1-3

Tot Ion:244 Resp: 166750
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.9 8.9
 122 11.1 9.8 14.6

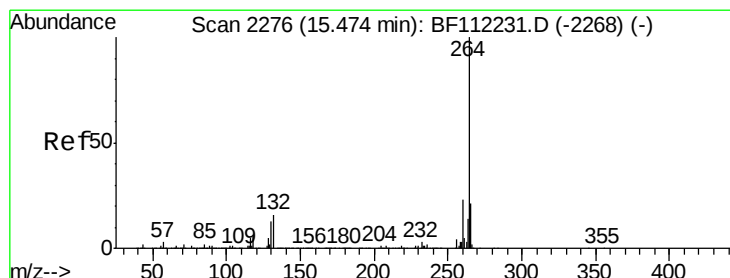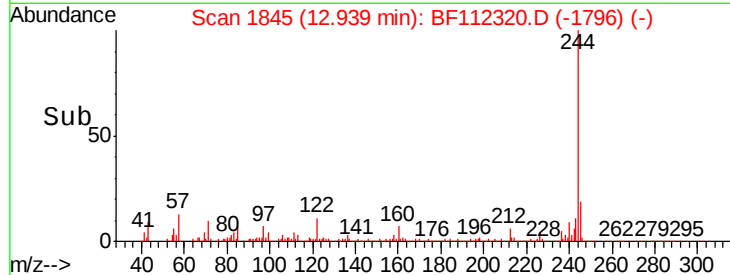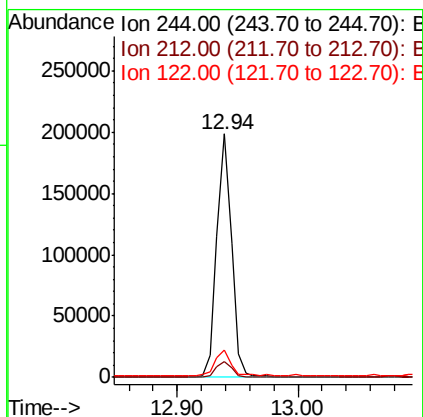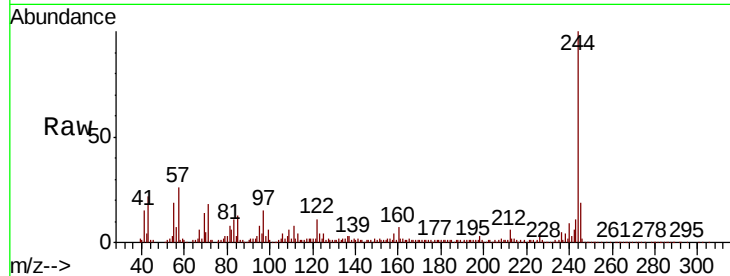

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.48 min Scan# 2277
 Delta R.T. 0.01 min
 Lab File: BF112320.D
 Acq: 30 Jan 2019 14:31

Tgt Ion:264 Resp: 253596
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.2 27.2
 265 21.6 17.0 25.4

