


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF013019\
 Data File : BF112310.D
 Acq On : 30 Jan 2019 8:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

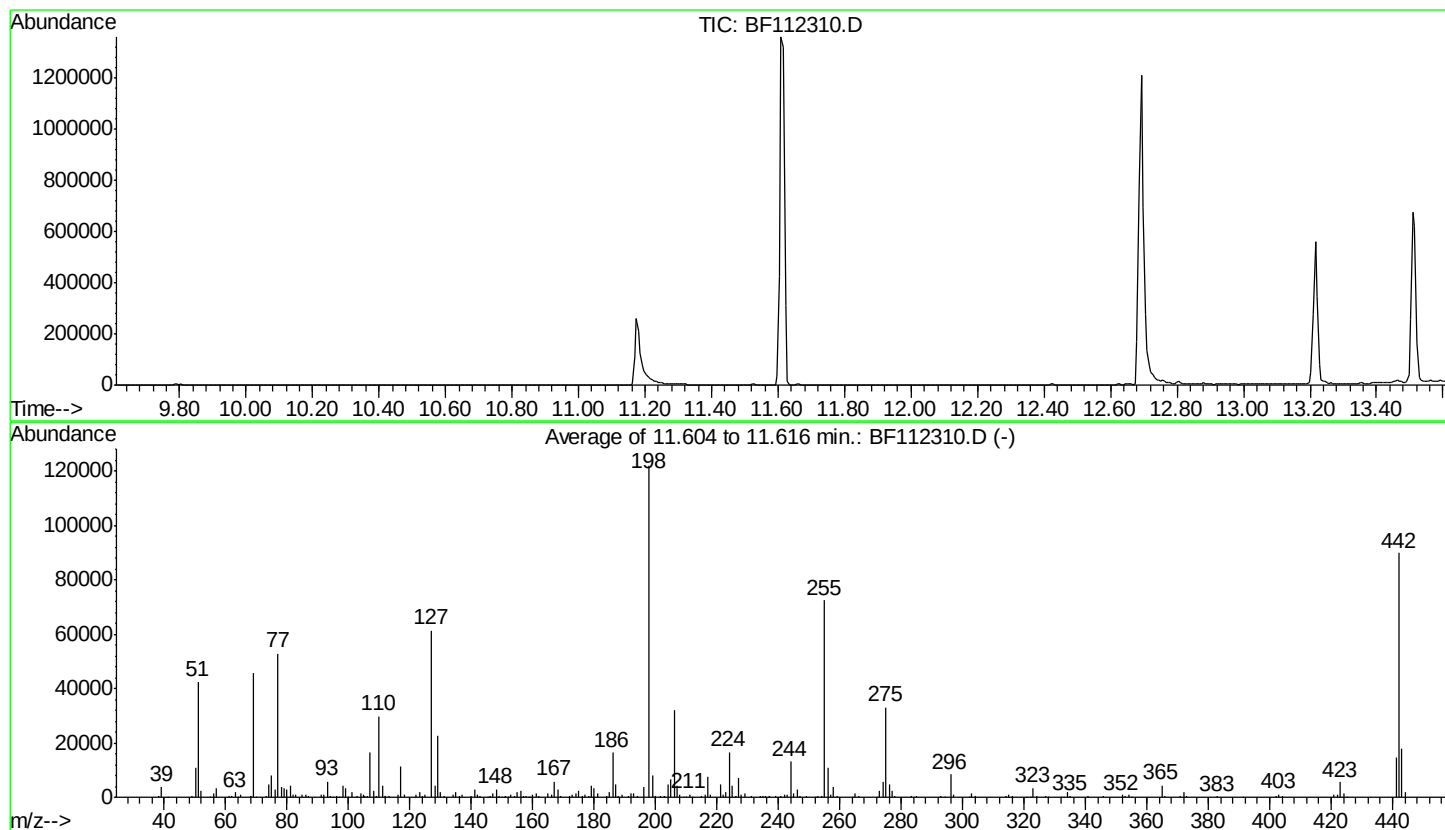

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	42509	PASS
68	69	0.00	2	1.0	476	PASS
69	198	0.00	100	37.5	45765	PASS
70	69	0.00	2	0.5	236	PASS
127	198	10	80	50.3	61309	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121938	PASS
199	198	5	9	6.6	8039	PASS
275	198	10	60	27.0	32958	PASS
365	198	1	100	3.5	4315	PASS
441	198	0.01	100	12.0	14595	PASS
442	198	50	100	73.6	89706	PASS
443	442	15	24	20.0	17953	PASS