


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF013019\
 Data File : BF112318.D
 Acq On : 30 Jan 2019 13:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

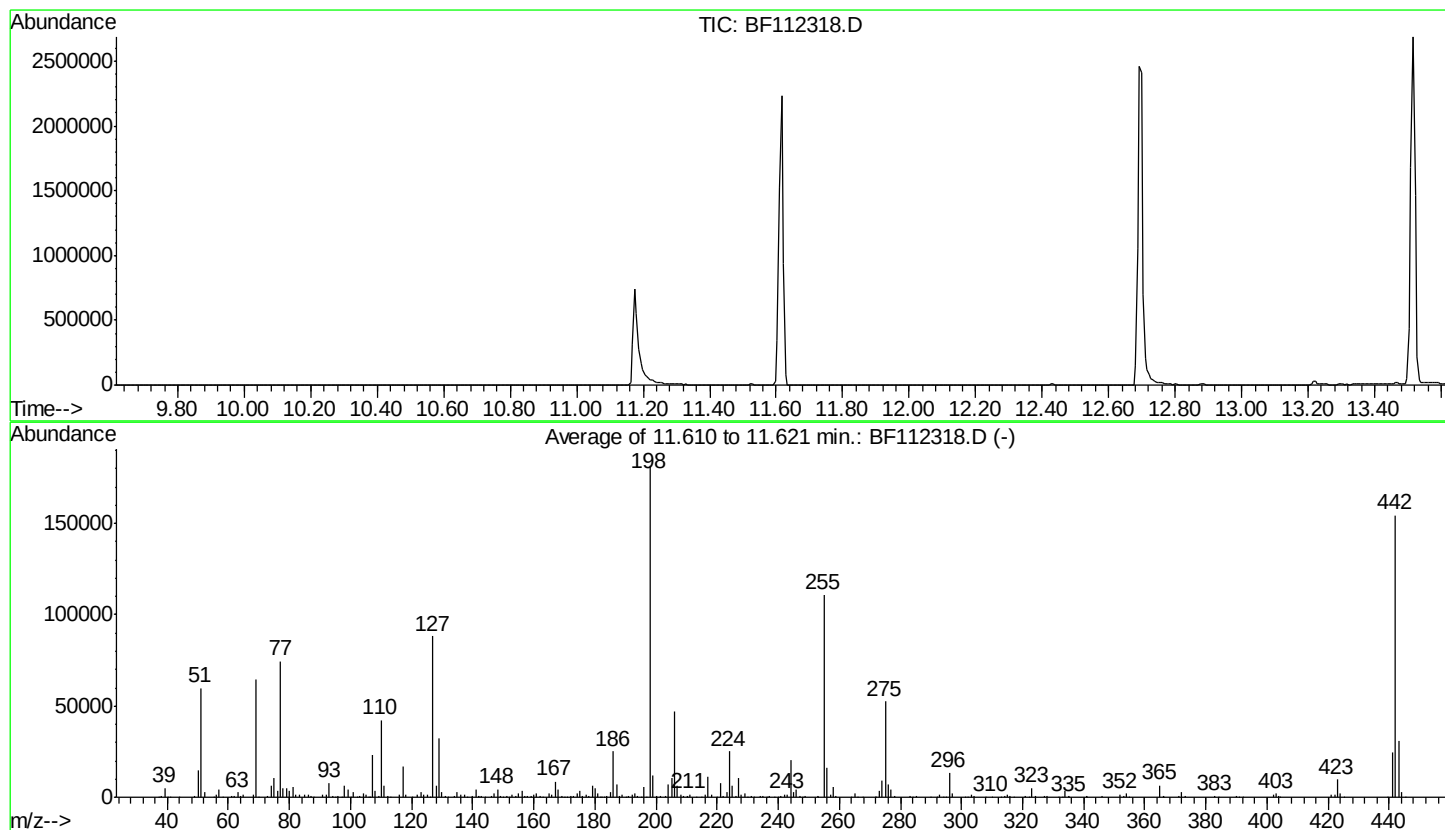

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	59706	PASS
68	69	0.00	2	1.8	1177	PASS
69	198	0.00	100	35.6	64608	PASS
70	69	0.00	2	0.5	339	PASS
127	198	10	80	48.6	88344	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	181738	PASS
199	198	5	9	6.8	12268	PASS
275	198	10	60	28.9	52602	PASS
365	198	1	100	3.6	6467	PASS
441	198	0.01	100	13.5	24547	PASS
442	198	50	100	85.0	154410	PASS
443	442	15	24	19.8	30597	PASS