

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
 Data File : BF132213.D
 Acq On : 30 Jan 2023 16:14
 Operator : CG\JU
 Sample : PB150541BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB150541BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.343	419	426	441	rVB	1624387	2358543	29.68%	4.815%
2	5.713	483	489	492	rBV	4910599	6040340	76.02%	12.332%
3	6.696	649	656	659	rBV	4548984	6046719	76.10%	12.345%
4	7.078	718	721	725	rVB	1735857	1427937	17.97%	2.915%
5	7.648	811	818	821	rBV	3712525	4041593	50.87%	8.251%
6	8.366	935	940	943	rBV	2376464	1871648	23.56%	3.821%
7	9.448	1117	1124	1127	rBV	7814219	7528379	94.75%	15.370%
8	10.131	1236	1240	1243	rBV	2777677	2184562	27.49%	4.460%
9	10.925	1370	1375	1378	rBV	4921104	4564328	57.44%	9.319%
10	11.630	1491	1495	1498	rBV	2696694	2242481	28.22%	4.578%
11	13.224	1761	1766	1769	rBV	7555964	7945683	100.00%	16.222%
12	14.289	1943	1947	1955	rBV	1782030	1508185	18.98%	3.079%
13	15.877	2211	2217	2233	rBV	845573	1127483	14.19%	2.302%
14	18.459	2650	2656	2672	rVB5	24721	92468	1.16%	0.189%




Sum of corrected areas: 48980349

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
Data File : BF132213.D
Acq On : 30 Jan 2023 16:14
Operator : CG\JU
Sample : PB150541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150541BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

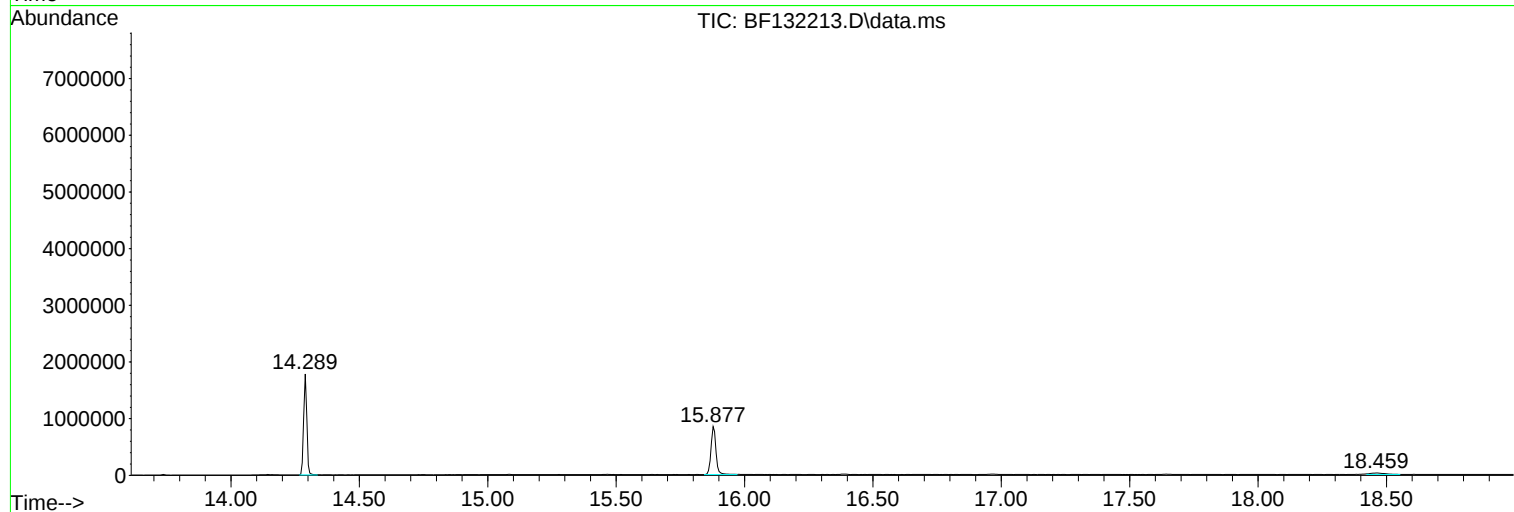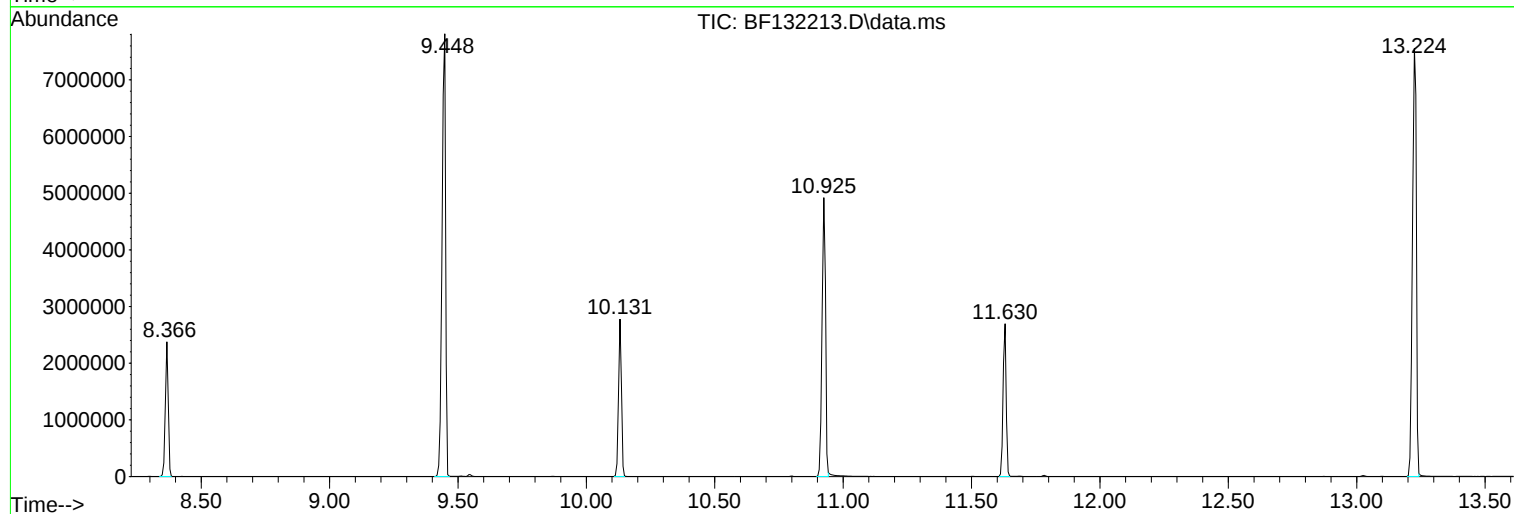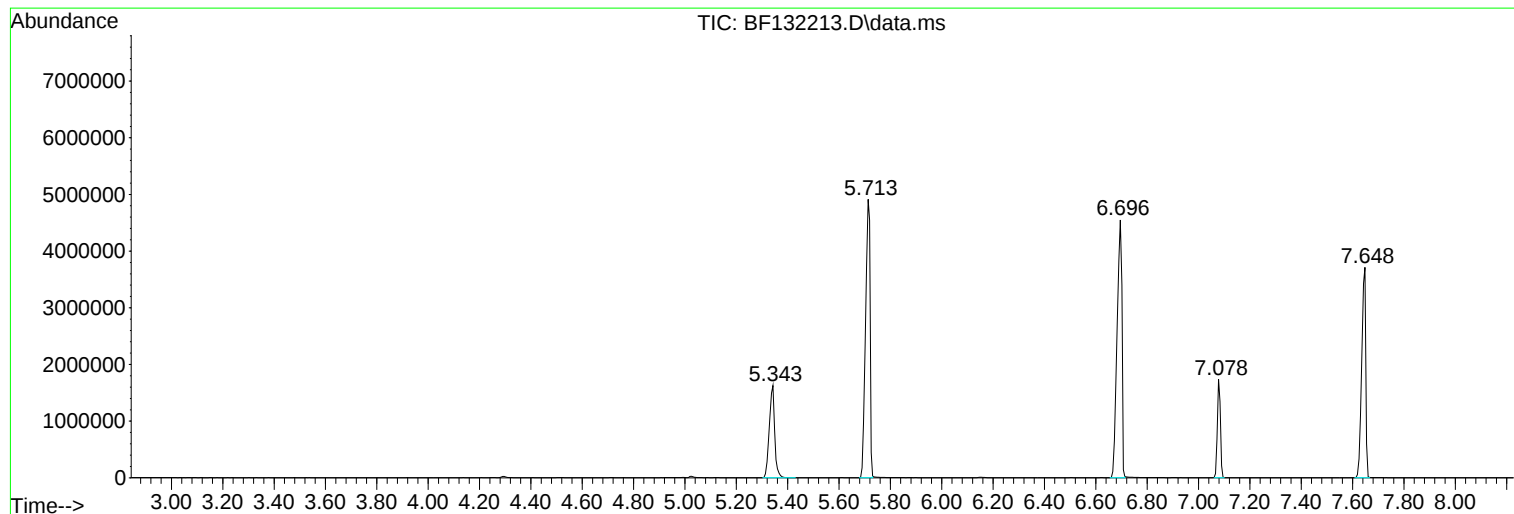

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
Data File : BF132213.D
Acq On : 30 Jan 2023 16:14
Operator : CG\JU
Sample : PB150541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB150541BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.343	33.03 ng	2358540	1,4-Dichlorobenzene-d4			7.078
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83	
2	5-Hexen-2-one	98	C6H10O	000109-49-9	9	
3	Acetone	58	C3H6O	000067-64-1	9	
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	
5	Formamide, N,N-diethyl-	101	C5H11NO	000617-84-5	9	

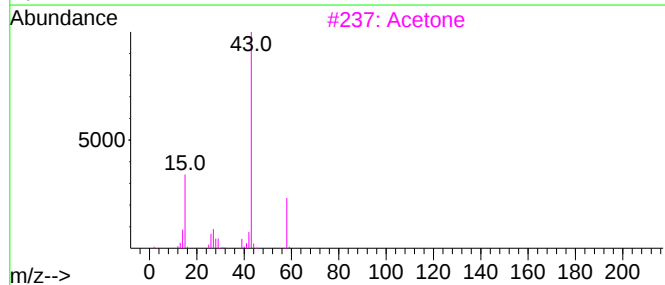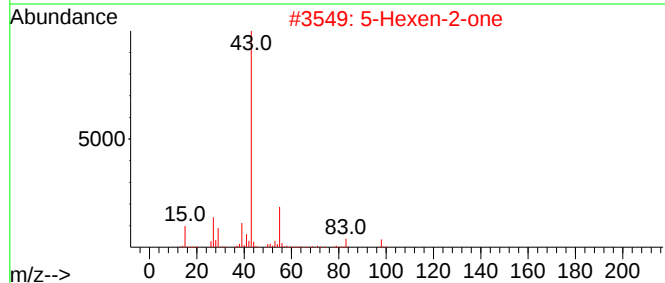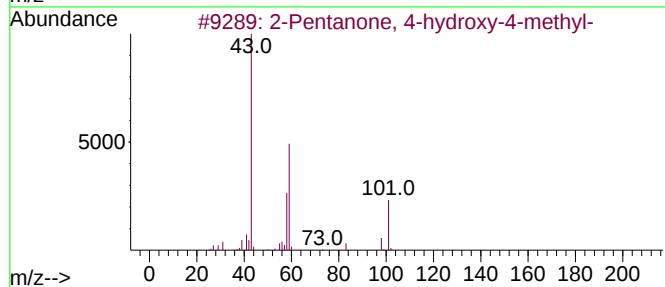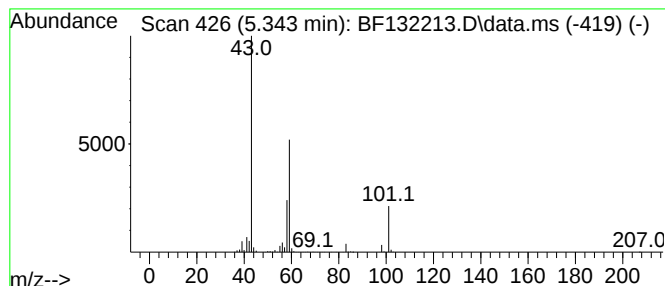

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
Data File : BF132213.D
Acq On : 30 Jan 2023 16:14
Operator : CG\JU
Sample : PB150541BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150541BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.343	33.0	ng	2358540	1	7.078	1427940	20.0