


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
Data File : BF132211.D
Acq On : 30 Jan 2023 15:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 28 02:25:45 2023

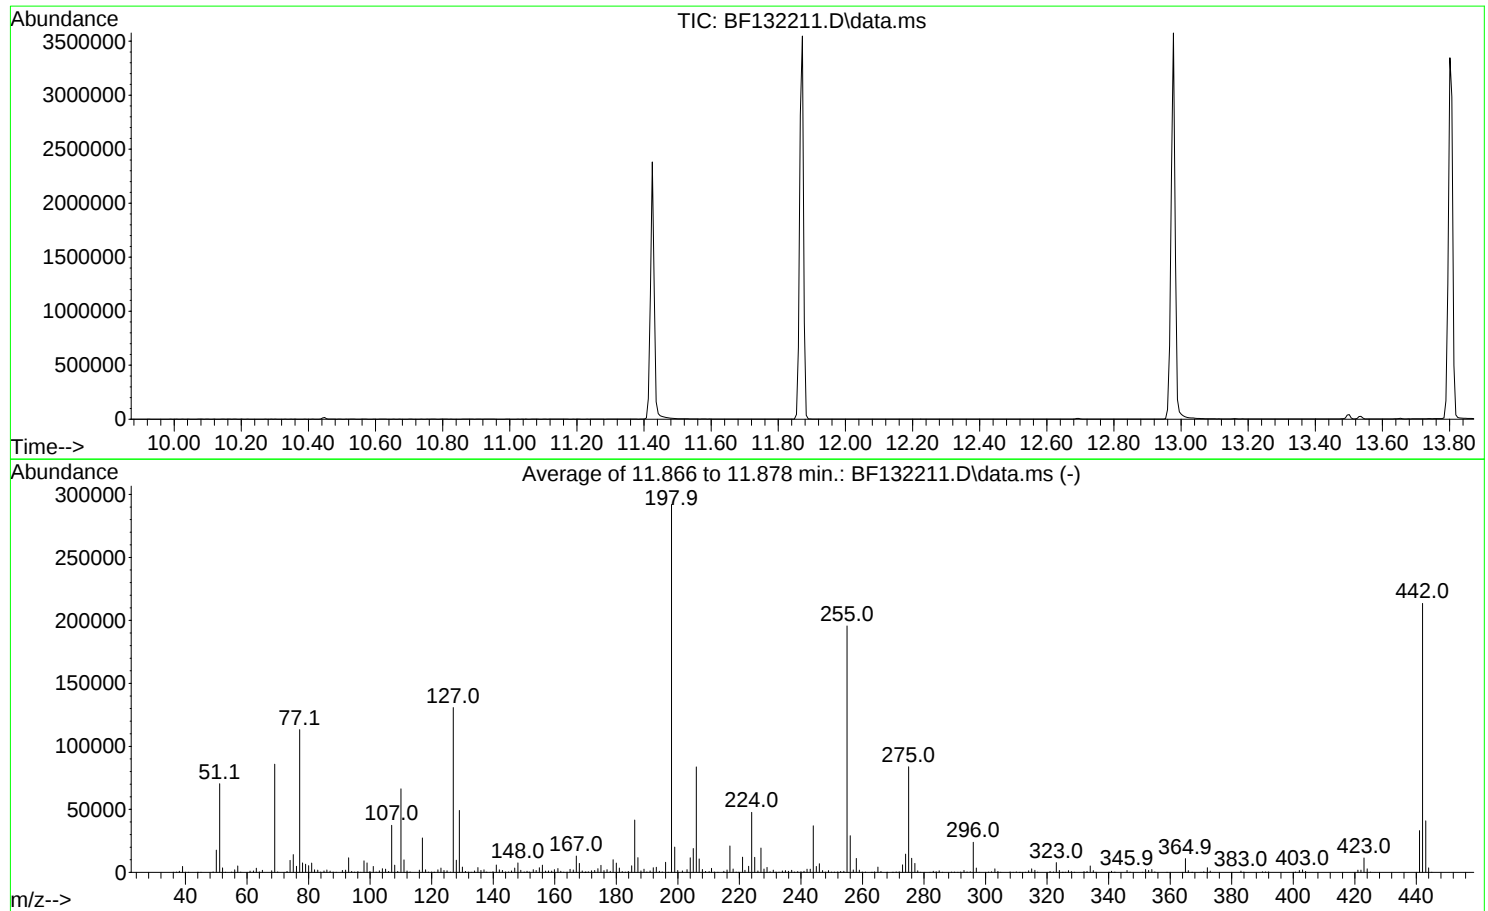




AutoFind: Scans 1535, 1536, 1537; Background Corrected with Scan 1530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.1	70315	PASS
68	69	0.00	2	1.4	1230	PASS
69	198	0.00	100	29.4	85931	PASS
70	69	0.00	2	0.5	418	PASS
127	198	10	80	44.8	130872	PASS
197	198	0.00	2	0.0	101	PASS
198	198	100	100	100.0	292005	PASS
199	198	5	9	6.9	20110	PASS
275	198	10	60	28.7	83864	PASS
365	198	1	100	3.7	10937	PASS
441	198	0.01	100	11.4	33168	PASS
442	442	50	100	100.0	213525	PASS
443	442	15	24	19.1	40867	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
 Data File : BF132211.D
 Acq On : 30 Jan 2023 15:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 31 03:33:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 28 02:25:45 2023
 Response via : Initial Calibration

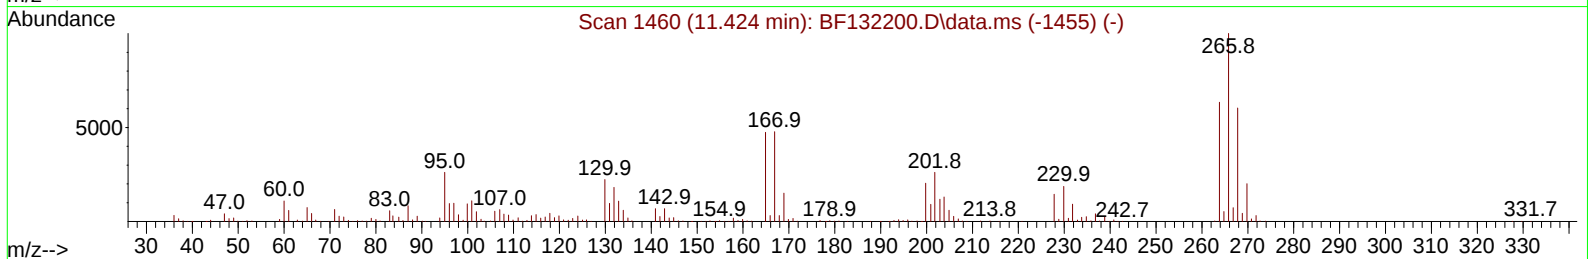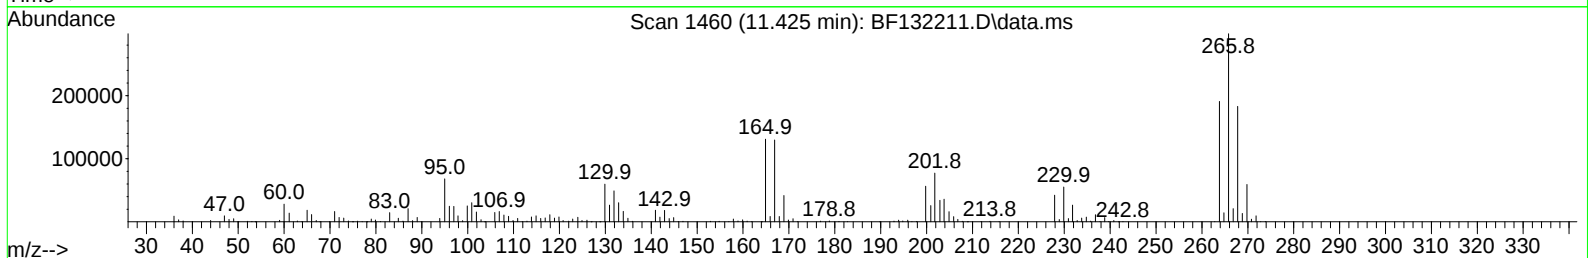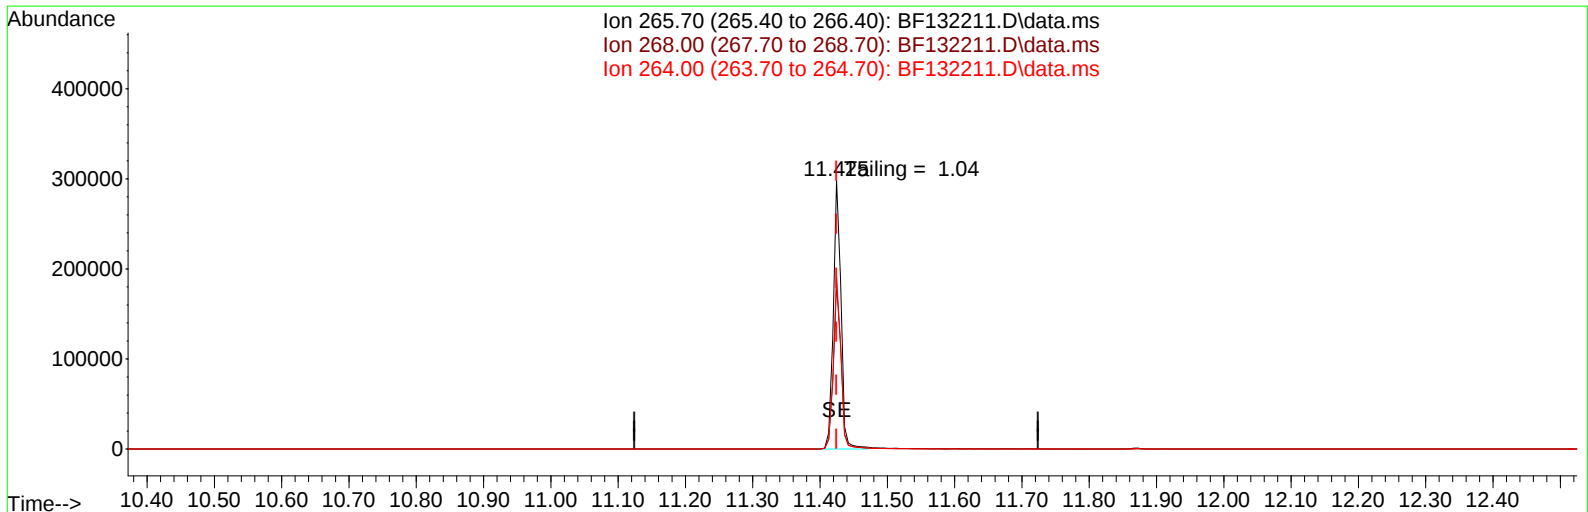

TIC: BF132211.D\data.ms

(70) Pentachlorophenol (C)

11.425min (+ 0.001) 23070.54 ng




response 240228

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.30	61.39
264.00	63.40	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013023\
Data File : BF132211.D
Acq On : 30 Jan 2023 15:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 31 03:33:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 28 02:25:45 2023
Response via : Initial Calibration

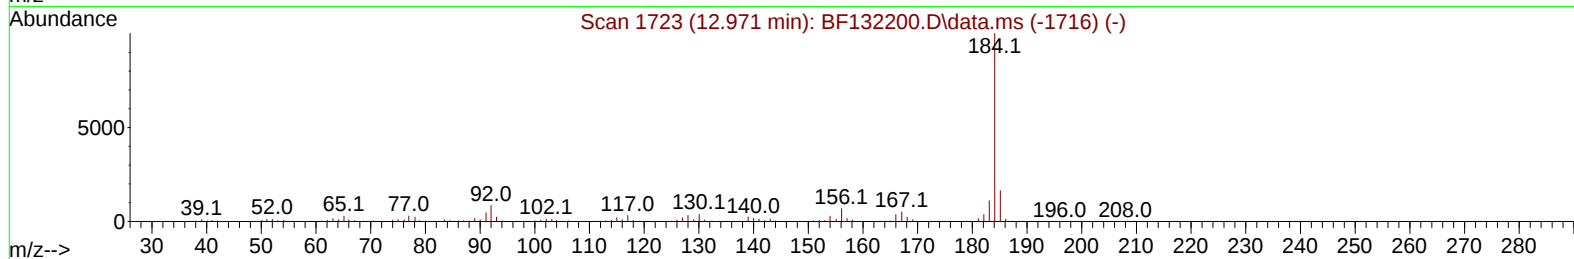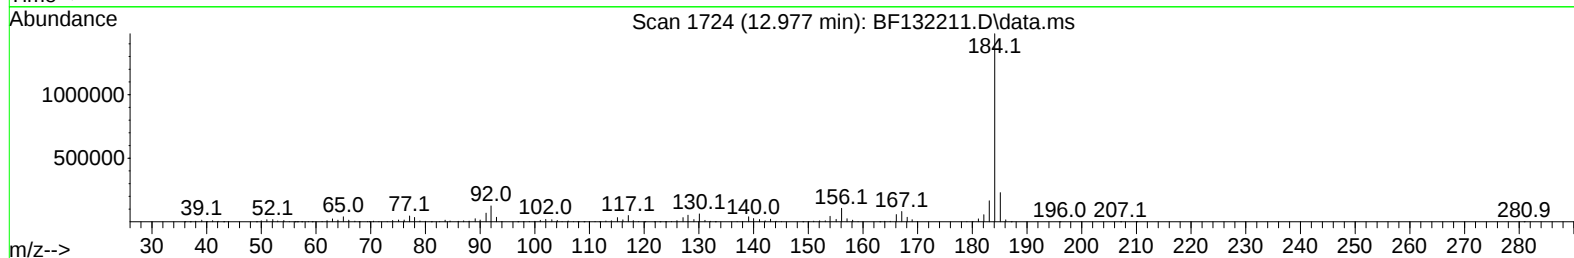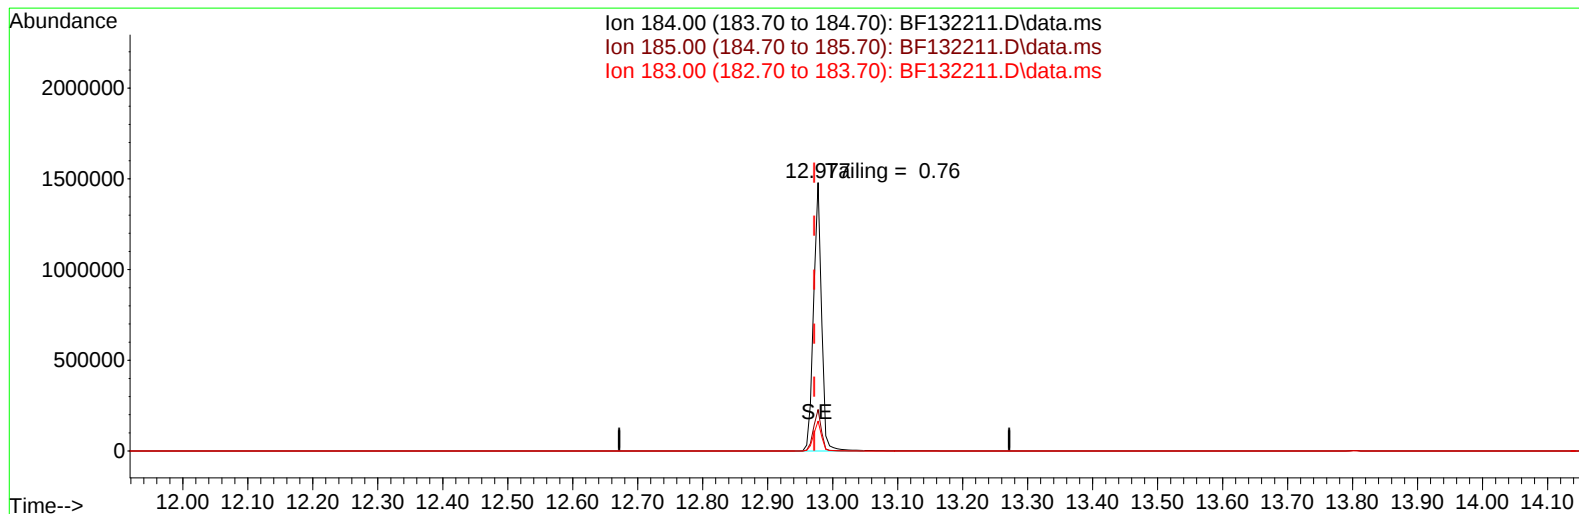

TIC: BF132211.D\data.ms

(77) Benzidine

12.977min (+ 0.006) 0.00 ng

response 1270909

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	15.48
183.00	11.00	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/30/2023	BNA_F	<u>BF132211.D</u>
Compound Name	Response	Retention Time
DDT	519184	13.801
DDD	11097	13.501
DDE	584	13.16
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11681	530865	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP