


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020119\
 Data File : BF112347.D
 Acq On : 1 Feb 2019 13:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

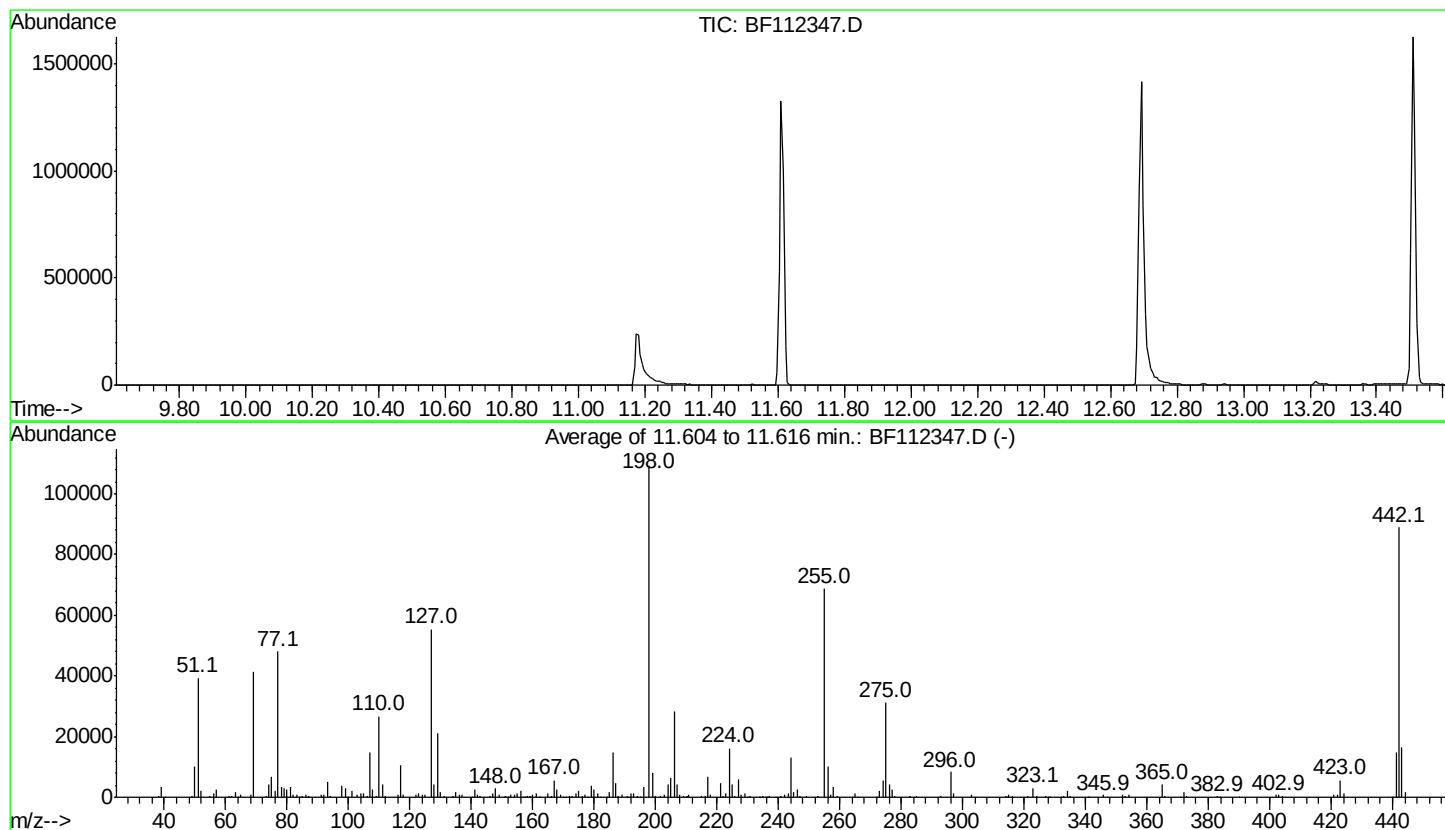

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	39264	PASS
68	69	0.00	2	1.7	698	PASS
69	198	0.00	100	37.7	41258	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	55485	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109296	PASS
199	198	5	9	7.2	7847	PASS
275	198	10	60	28.4	31028	PASS
365	198	1	100	3.8	4144	PASS
441	198	0.01	100	13.4	14621	PASS
442	198	50	100	81.3	88864	PASS
443	442	15	24	18.4	16342	PASS