

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020419\
 Data File : BF112382.D
 Acq On : 4 Feb 2019 16:12
 Operator : JU/SJ
 Sample : K1362-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-03-005-ABCD

Quant Time: Feb 04 23:46:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	149081	20.00	ng	-0.02
21) Naphthalene-d8	8.11	136	580955	20.00	ng	-0.02
39) Acenaphthene-d10	9.87	164	281354	20.00	ng	-0.02
64) Phenanthrene-d10	11.35	188	563697	20.00	ng	-0.02
76) Chrysene-d12	14.00	240	525811	20.00	ng	-0.01
87) Perylene-d12	15.46	264	395314	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	759863	108.26	ng	-0.01
7) Phenol-d6	6.47	99	952658	97.68	ng	-0.02
23) Nitrobenzene-d5	7.39	82	584779	58.00	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	289689	88.46	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	1192917	59.97	ng	-0.02
79) Terphenyl-d14	12.94	244	1388042	49.72	ng	-0.01
Target Compounds						
10) Phenol	6.49	94	24439	2.284	ng	95
19) n-Nitroso-di-n-propylamine	7.39	70	80120	11.914	ng	# 76
25) Isophorone	7.39	82	584773	36.970	ng	# 63
50) Dimethylphthalate	9.58	163	86356	3.950	ng	98
51) 2,6-Dinitrotoluene	9.86	165	35941	7.341	ng	# 34
57) 2,4-Dinitrotoluene	9.86	165	35941	5.767	ng	# 32
67) 4-Bromophenyl-phenylether	10.66	248	16574	2.500	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020419\
Data File : BF112382.D
Acq On : 4 Feb 2019 16:12
Operator : JU/SJ
Sample : K1362-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Quant Time: Feb 04 23:46:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

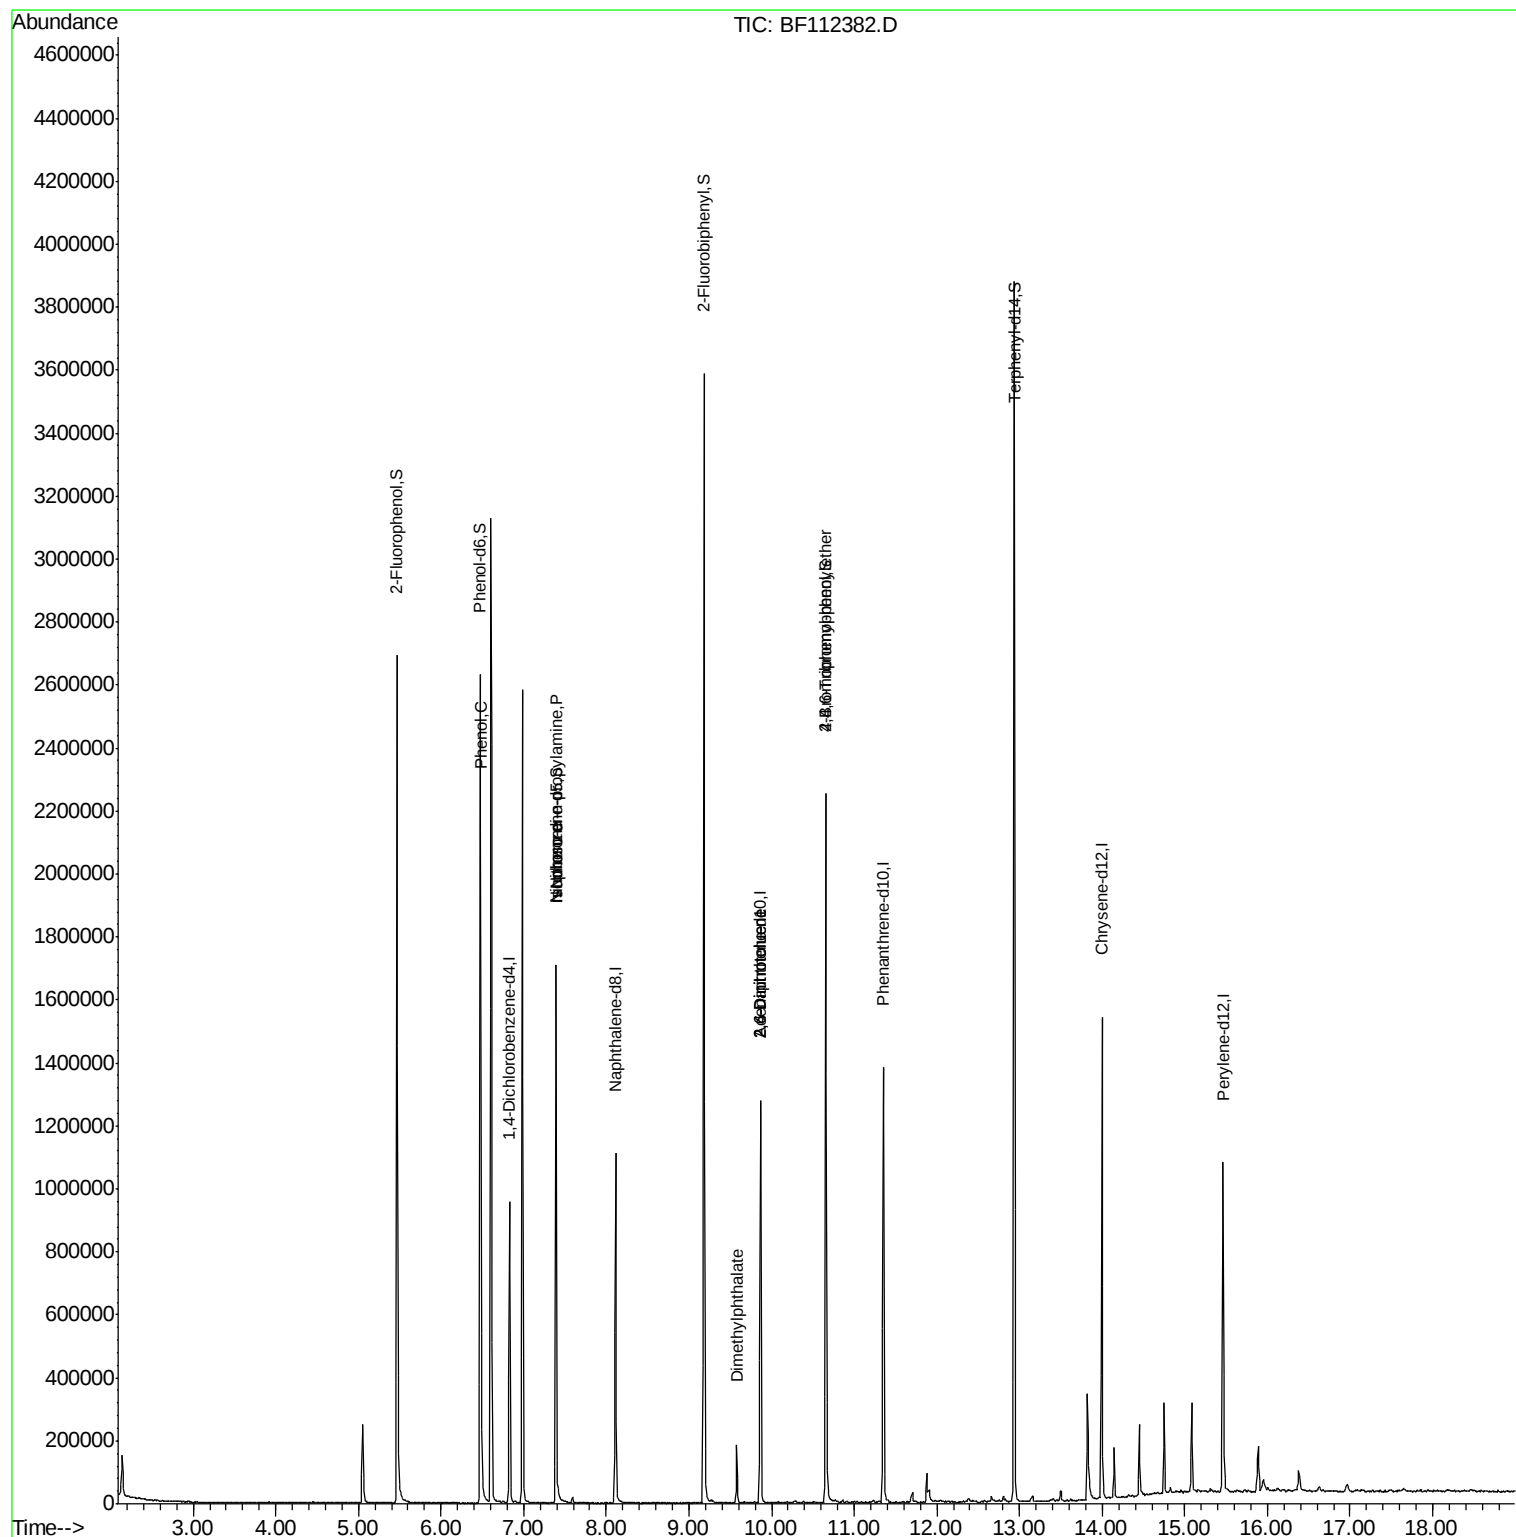

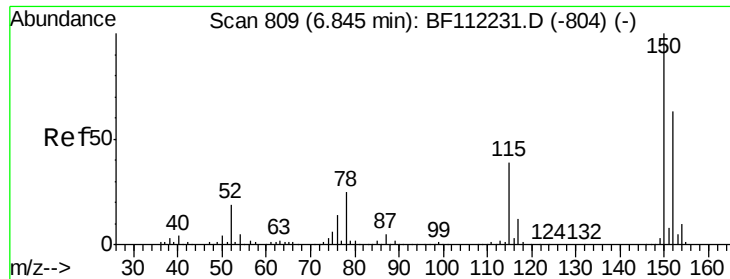


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 806
Delta R.T. -0.02 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Tgt Ion:152 Resp: 149081
Ion Ratio Lower Upper
152 100
150 159.7 127.4 191.0
115 60.0 45.5 68.3

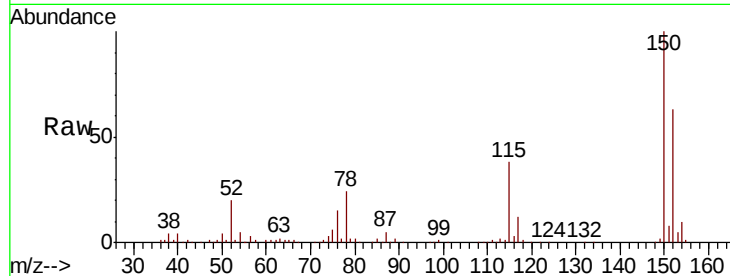


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

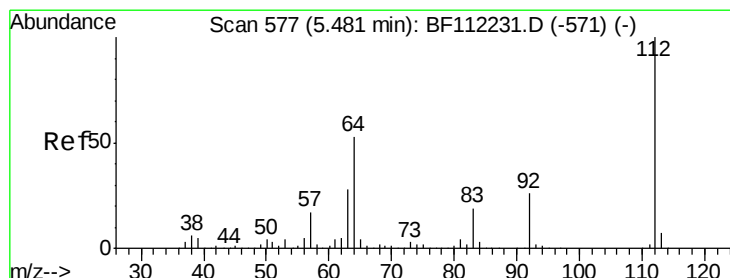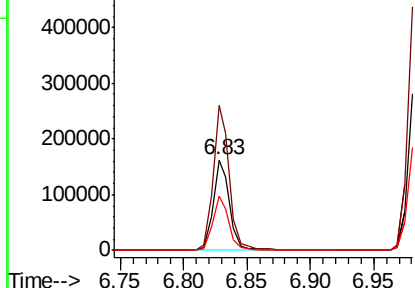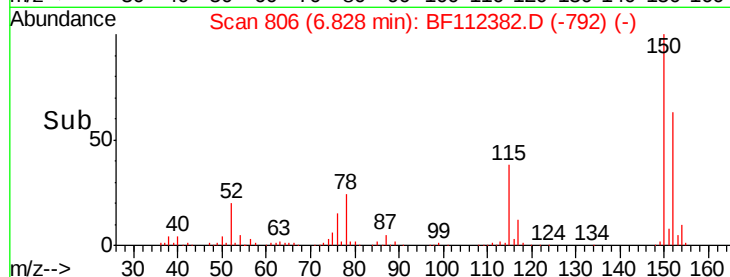



#5

2-Fluorophenol
Concen: 108.263 ng
RT: 5.47 min Scan# 575
Delta R.T. -0.01 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Tgt Ion:112 Resp: 759863
Ion Ratio Lower Upper
112 100
64 55.5 45.7 68.5
63 30.0 23.6 35.4

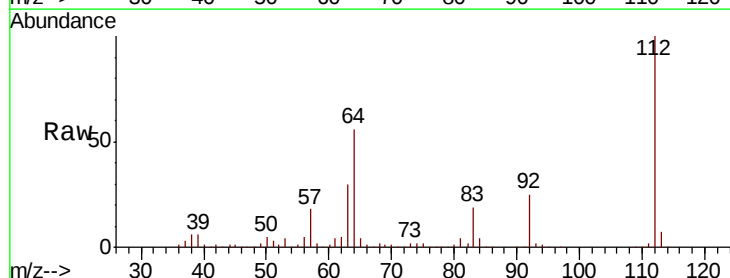

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

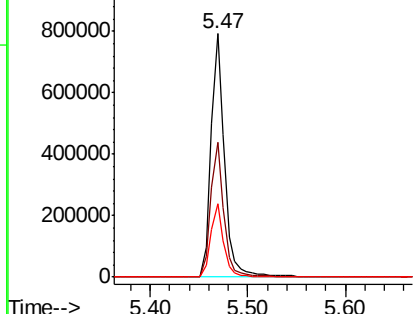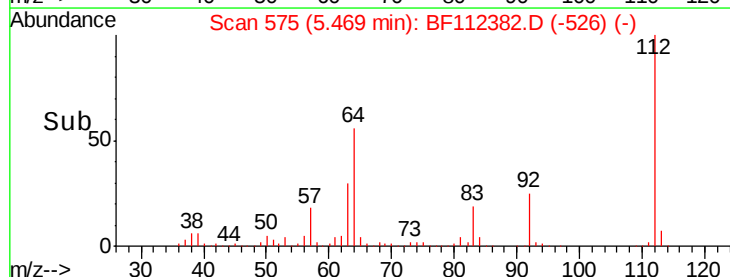



#7

Phenol-d6

Concen: 97.681 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.02 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12

Instrument :

BNA_F

ClientSampleId :

FK-BPM-03-005-ABCD


Tgt Ion: 99 Resp: 952658

Ion Ratio Lower Upper




99 100

42 19.6 15.1 22.7

71 36.5 26.9 40.3

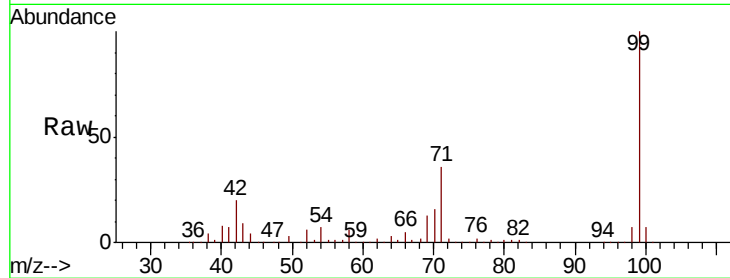

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

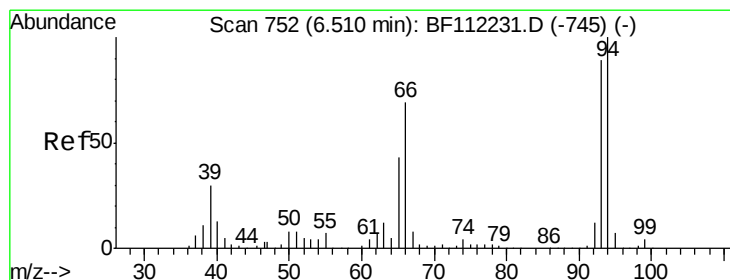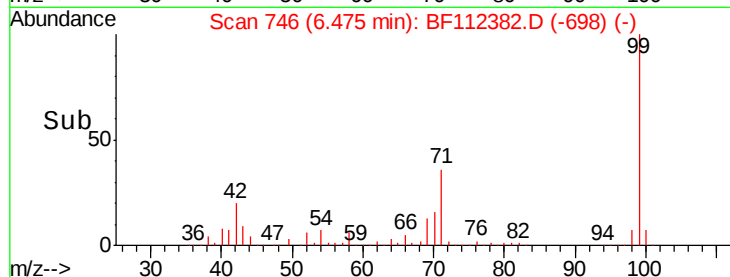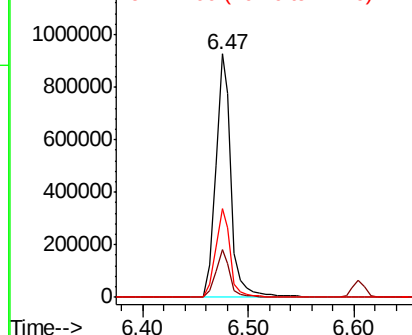

#10

Phenol

Concen: 2.284 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.02 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12


Tgt Ion: 94 Resp: 24439

Ion Ratio Lower Upper



94 100

65 39.1 20.3 60.3

66 67.7 42.4 82.4

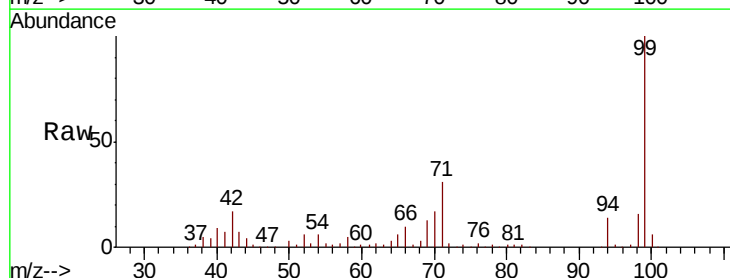

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1


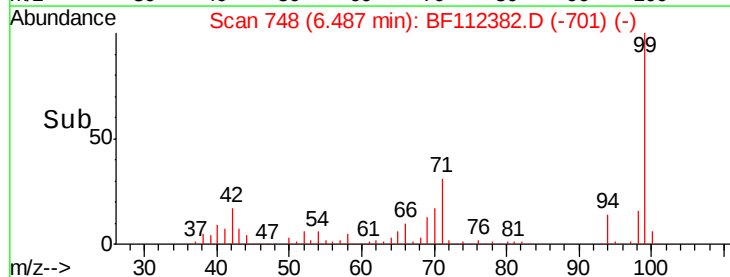
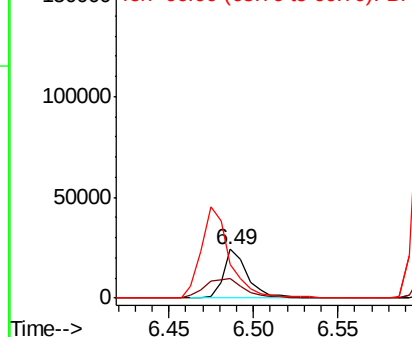




#19
n-Nitroso-di-n-propylamine
Concen: 11.914 ng
RT: 7.39 min Scan# 902
Delta R.T. 0.13 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12




Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Tgt Ion:	70	Resp:	80120
Ion	Ratio	Lower	Upper
70	100		
42	46.8	47.6	71.4#
101	0.0	7.9	11.9#
130	2.2	18.4	27.6#

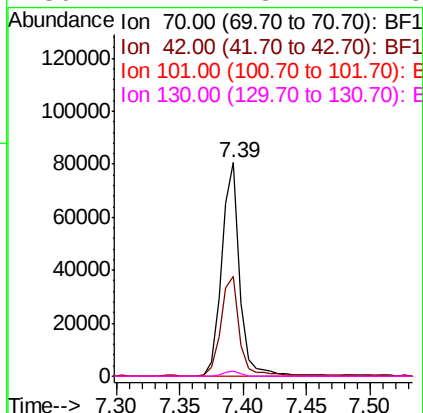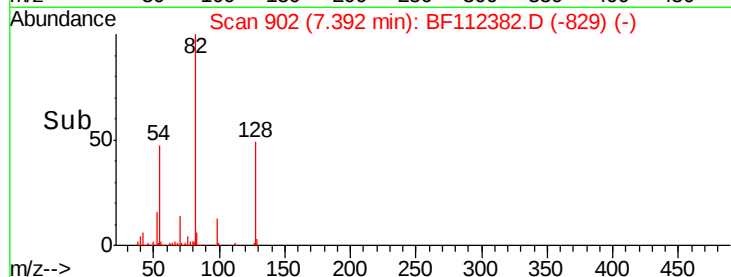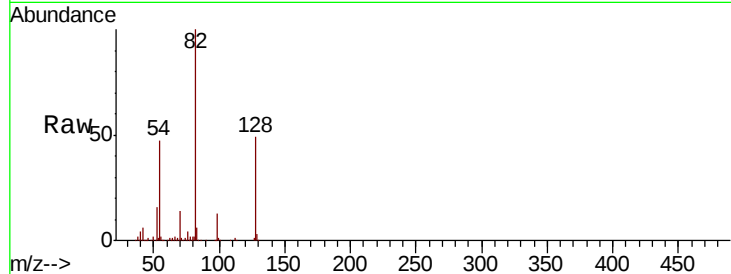

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.11 min Scan# 1024
Delta R.T. -0.02 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Tgt Ion:	136	Resp:	580955
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.1	13.7
54	6.7	5.9	8.9
68	5.0	5.1	7.7#

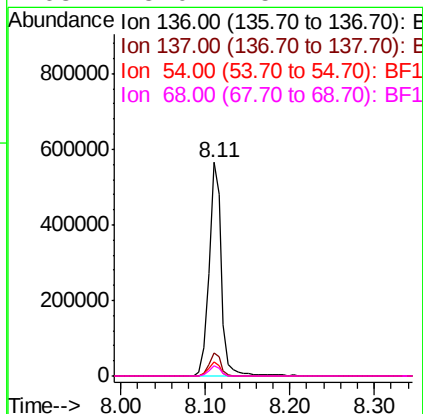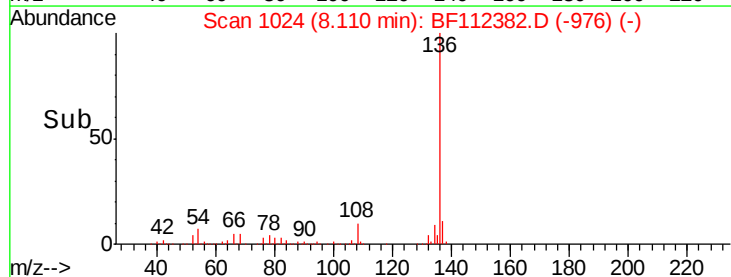







#23
Nitrobenzene-d5
Concen: 57.999 ng
RT: 7.39 min Scan# 902
Delta R.T. -0.02 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Tgt Ion: 82 Resp: 584779
Ion Ratio Lower Upper
82 100
128 48.6 37.8 56.8
54 47.2 39.7 59.5

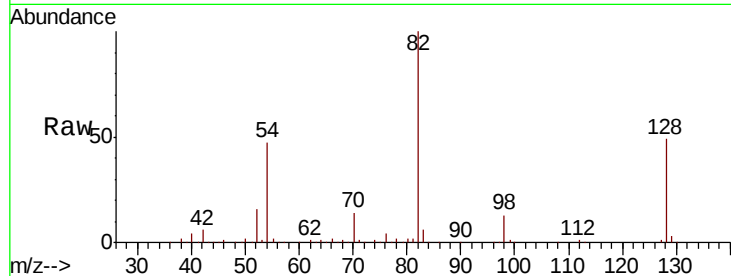


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

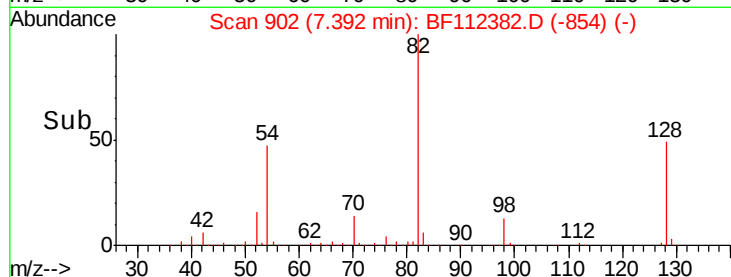
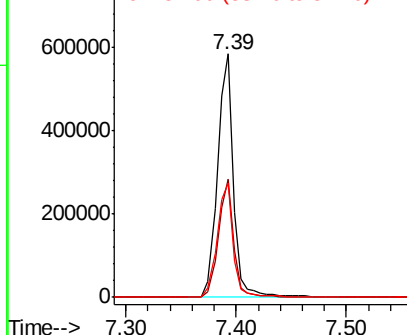



#25
Isophorone
Concen: 36.970 ng
RT: 7.39 min Scan# 902
Delta R.T. -0.28 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Tgt Ion: 82 Resp: 584773
Ion Ratio Lower Upper
82 100
95 0.0 5.7 8.5#
138 0.0 15.4 23.0#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

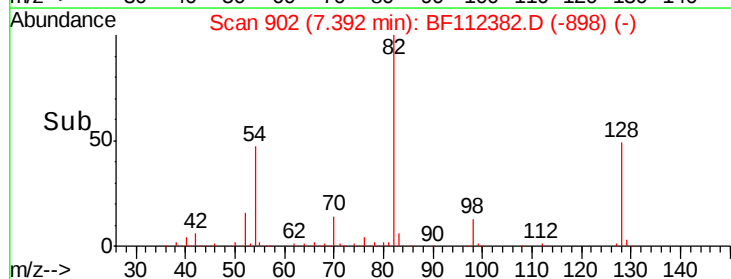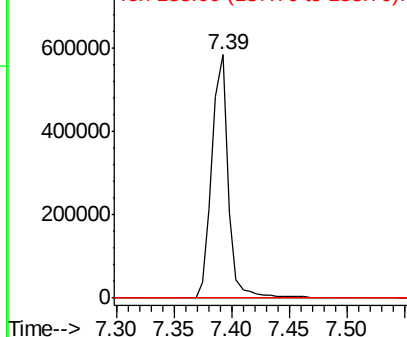

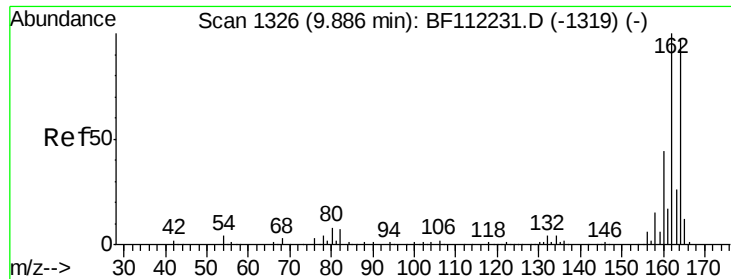

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12

Instrument :

BNA_F

ClientSampleId :

FK-BPM-03-005-ABCD


Tgt Ion:164 Resp: 281354

Ion Ratio Lower Upper

164 100

162 105.7 82.2 123.4




160 47.1 36.2 54.4

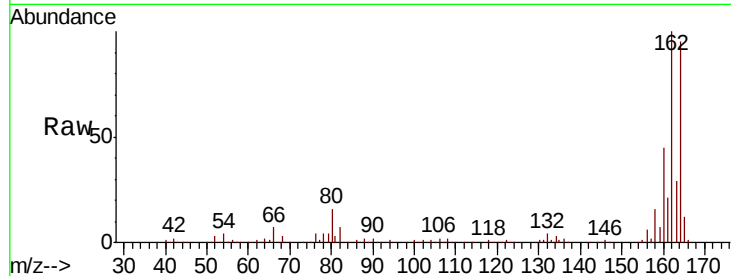

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

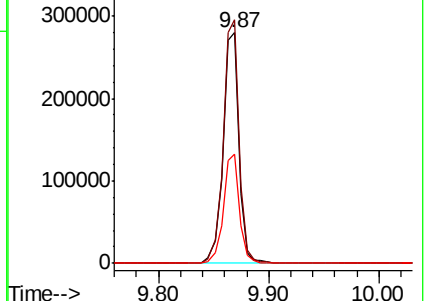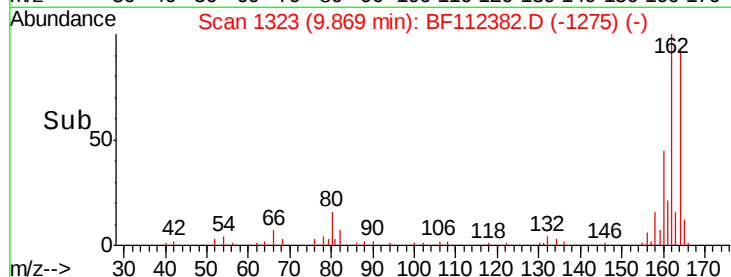

#42

2,4,6-Tribromophenol

Concen: 88.458 ng

RT: 10.66 min Scan# 1457

Delta R.T. -0.02 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12


Tgt Ion:330 Resp: 289689

Ion Ratio Lower Upper

330 100

332 95.7 76.6 114.8



141 32.2 24.3 36.5



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

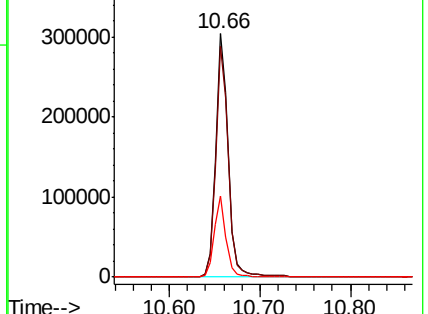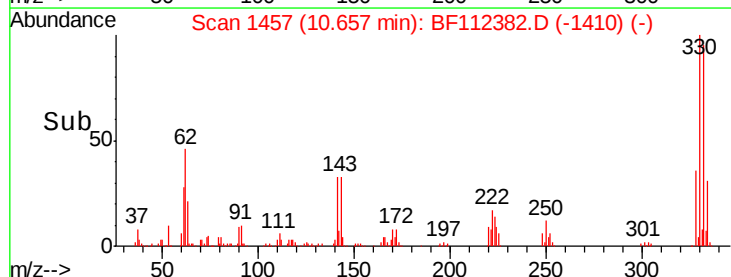







#45
2-Fluorobiphenyl
Concen: 59.967 ng
RT: 9.19 min Scan# 1207
Delta R.T. -0.02 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Tgt Ion:172 Resp: 1192917
Ion Ratio Lower Upper
172 100
171 36.3 30.5 45.7
170 23.5 20.2 30.4




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

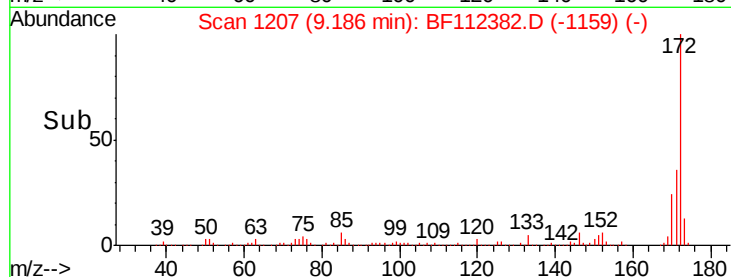
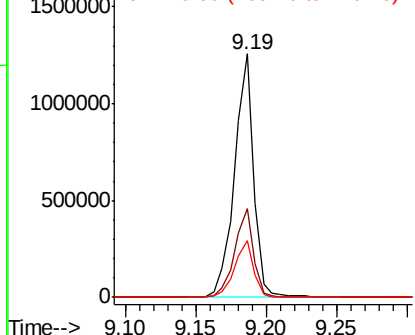



#50
Dimethylphthalate
Concen: 3.950 ng
RT: 9.58 min Scan# 1274
Delta R.T. -0.02 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Tgt Ion:163 Resp: 86356
Ion Ratio Lower Upper
163 100
194 3.4 3.3 4.9
164 9.8 8.5 12.7



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

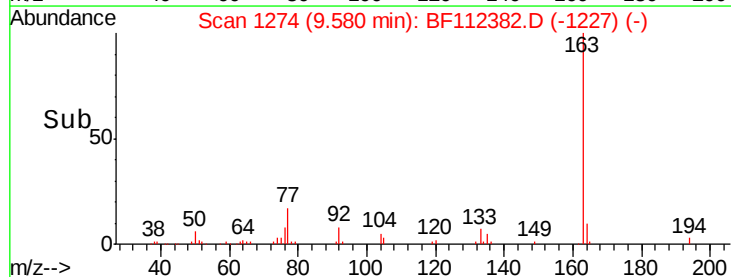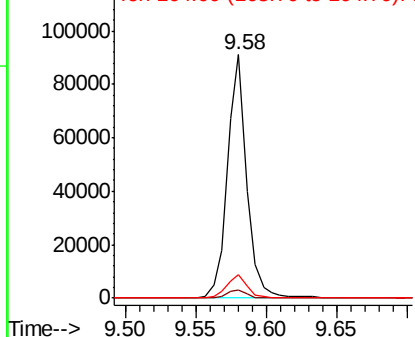

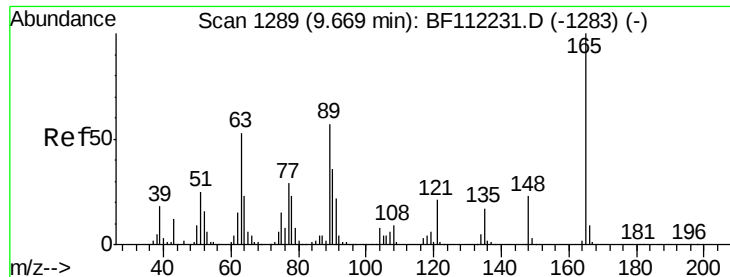

#51

2,6-Dinitrotoluene

Concen: 7.341 ng

RT: 9.86 min Scan# 1322

Delta R.T. 0.19 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12

Instrument :

BNA_F

ClientSampleId :

FK-BPM-03-005-ABCD


Tgt Ion:165 Resp: 35941

Ion Ratio Lower Upper

165 100

63 1.2 33.8 50.8#




89 2.1 36.9 55.3#

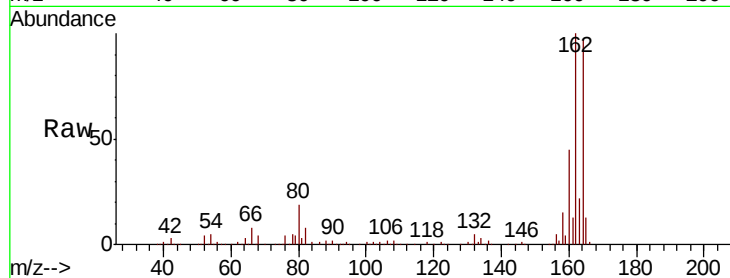

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

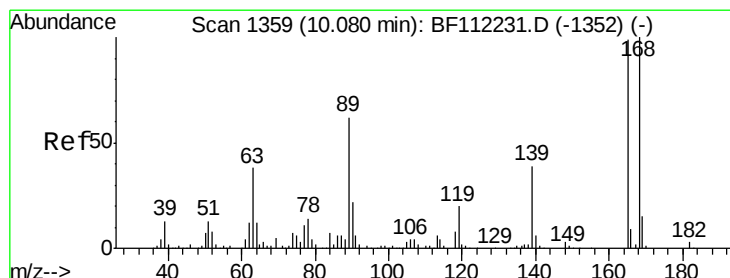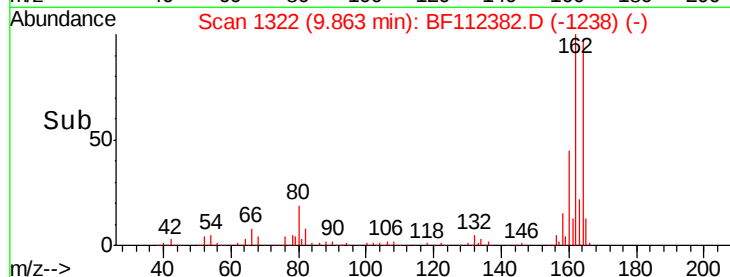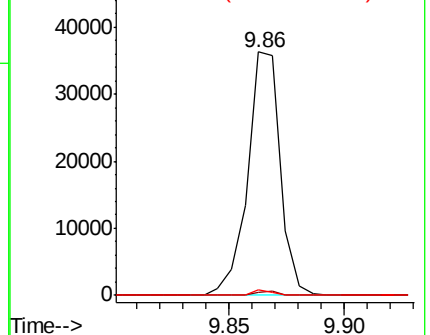

#57

2,4-Dinitrotoluene

Concen: 5.767 ng

RT: 9.86 min Scan# 1322

Delta R.T. -0.22 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12

Tgt Ion:165 Resp: 35941


Ion Ratio Lower Upper

165 100

63 1.2 27.9 41.9#

89 2.1 47.9 71.9#

182 0.0 2.2 3.4#


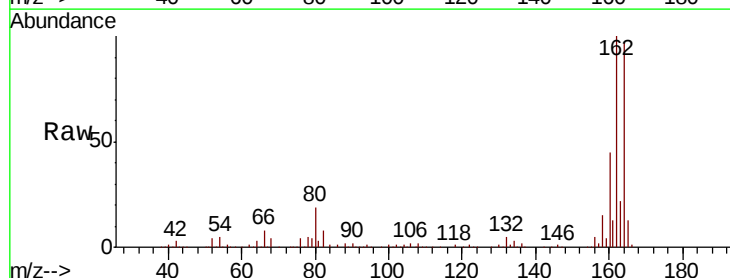



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

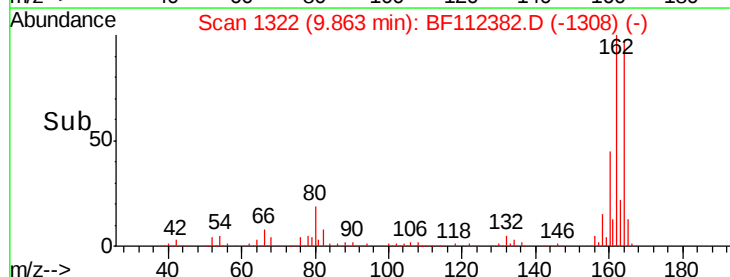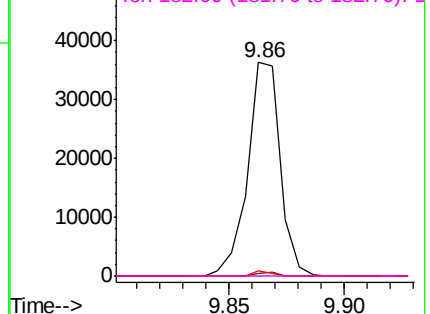

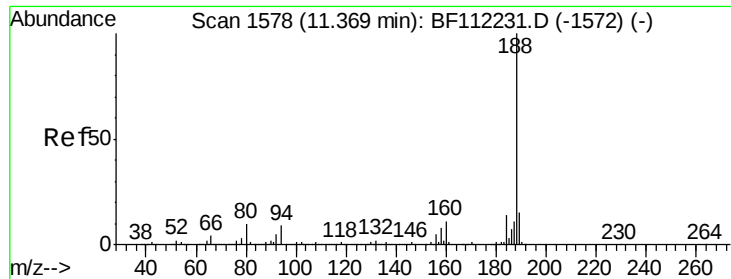

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.35 min Scan# 1575

Delta R.T. -0.02 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12

Instrument :

BNA_F

ClientSampleId :

FK-BPM-03-005-ABCD


Tgt Ion:188 Resp: 563697

Ion Ratio Lower Upper

188 100

94 9.2 8.2 12.2




80 9.8 8.9 13.3



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

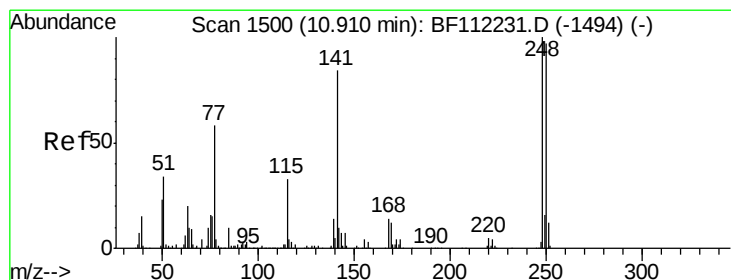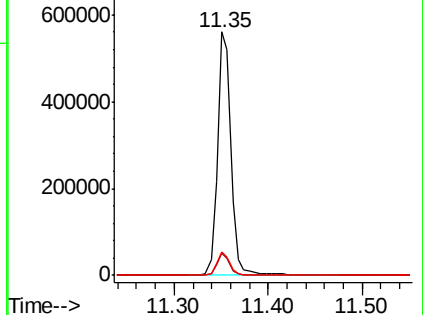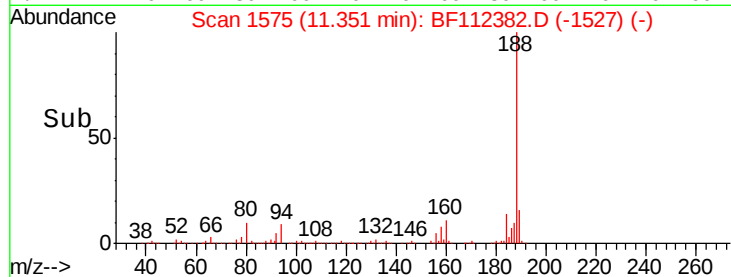

#67

4-Bromophenyl-phenylether

Concen: 2.500 ng

RT: 10.66 min Scan# 1457

Delta R.T. -0.25 min

Lab File: BF112382.D

Acq: 4 Feb 2019 16:12


Tgt Ion:248 Resp: 16574

Ion Ratio Lower Upper

248 100

250 211.6 79.7 119.5#



141 570.6 60.3 90.5#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

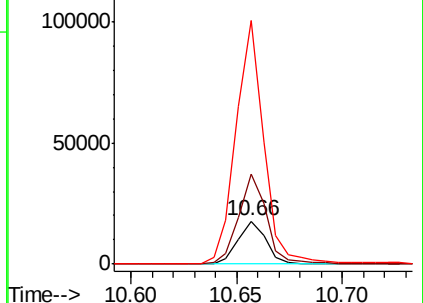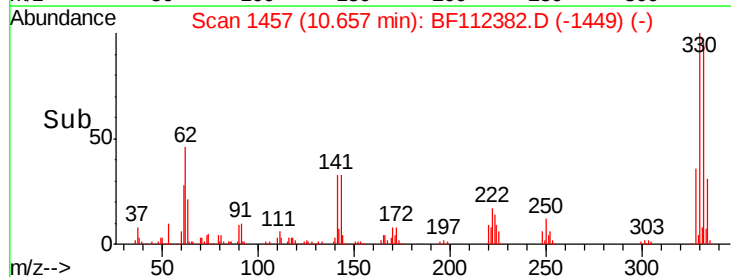


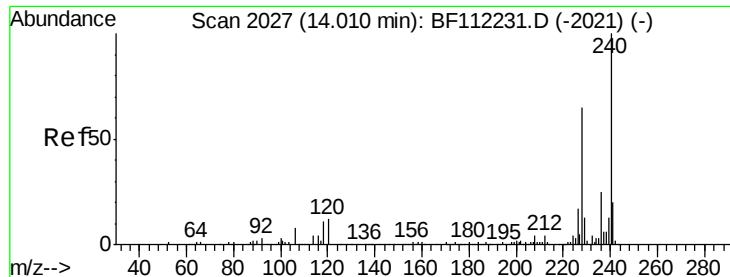




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Tgt Ion:240 Resp: 525811
Ion Ratio Lower Upper
240 100
120 10.0 9.0 13.6
236 25.2 20.7 31.1

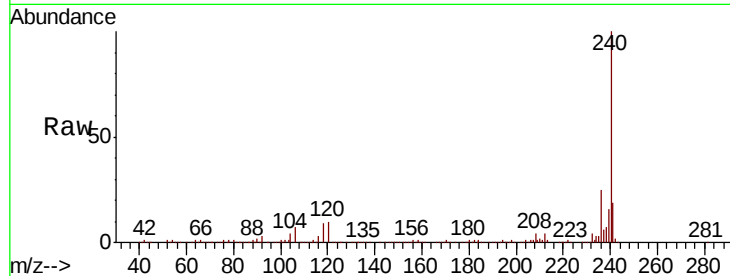


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

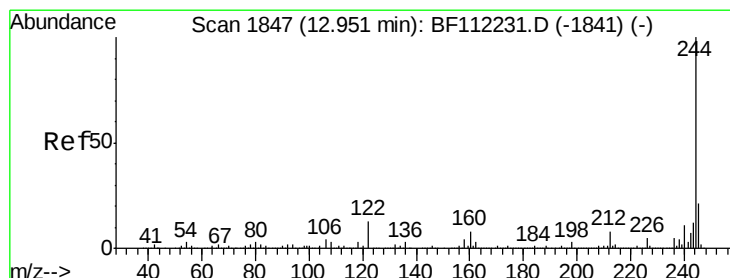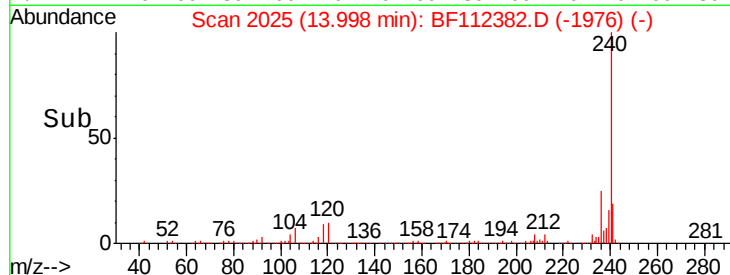
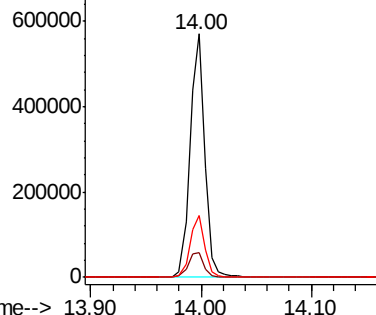



#79
Terphenyl-d14
Concen: 49.719 ng
RT: 12.94 min Scan# 1845
Delta R.T. -0.01 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Tgt Ion:244 Resp: 1388042
Ion Ratio Lower Upper
244 100
212 6.7 5.9 8.9
122 10.2 9.8 14.6

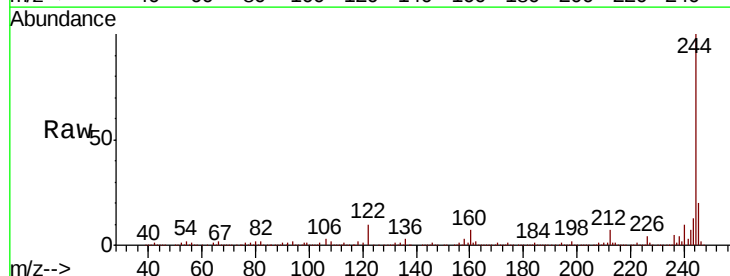

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

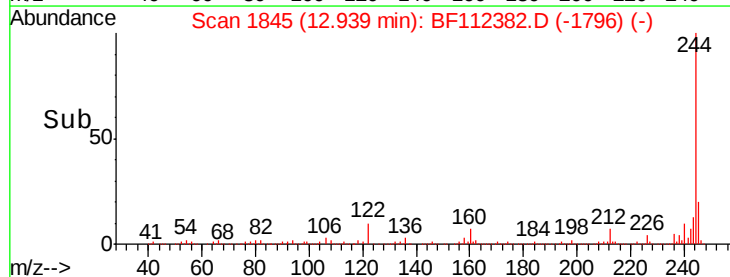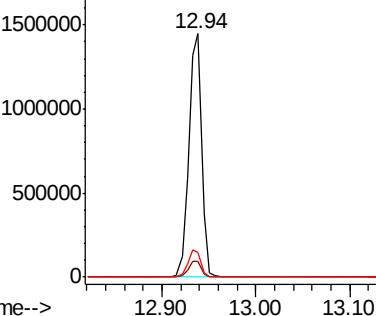

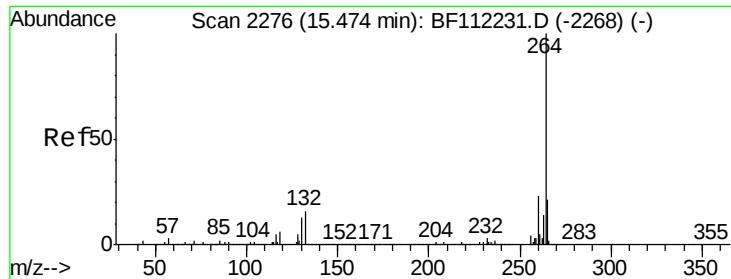

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.46 min Scan# 2274
Delta R.T. -0.01 min
Lab File: BF112382.D
Acq: 4 Feb 2019 16:12

Instrument :
BNA_F
ClientSampleId :
FK-BPM-03-005-ABCD

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.8	18.2	27.2
265	21.5	17.0	25.4

