
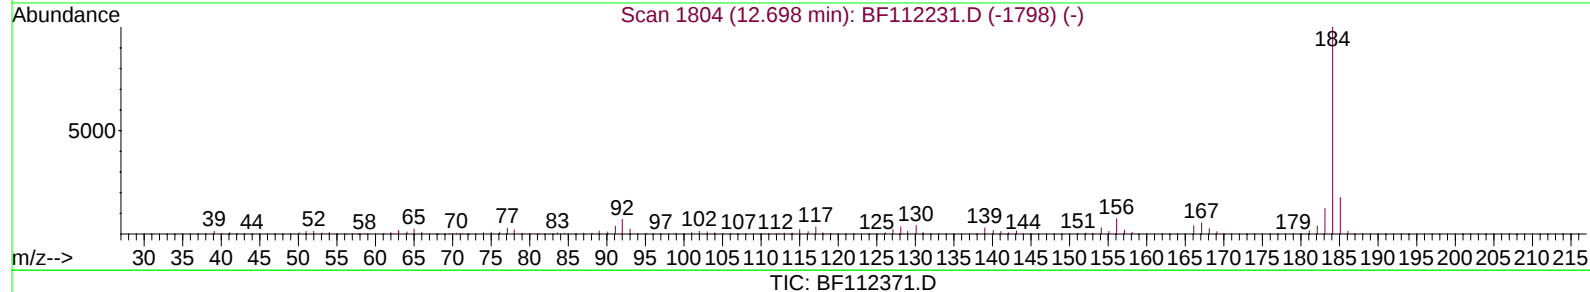
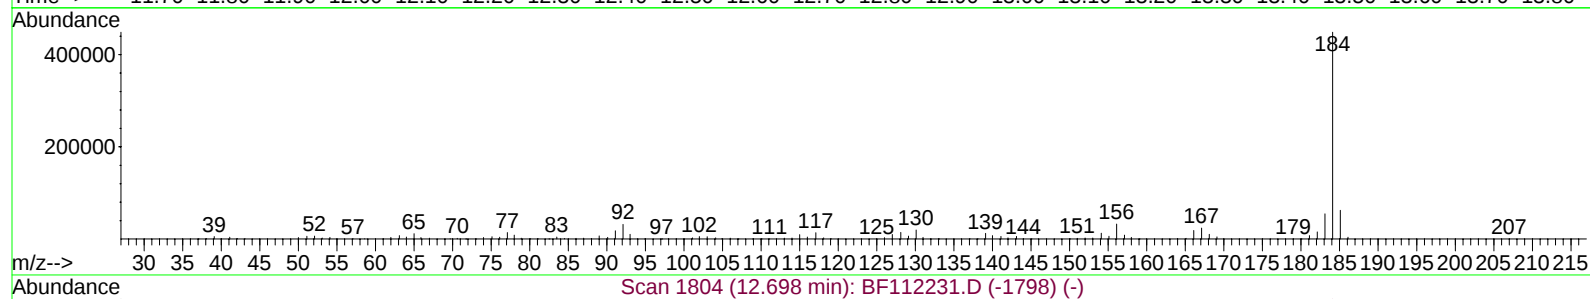


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020419\
Data File : BF112371.D
Acq On : 4 Feb 2019 9:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 17:30:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

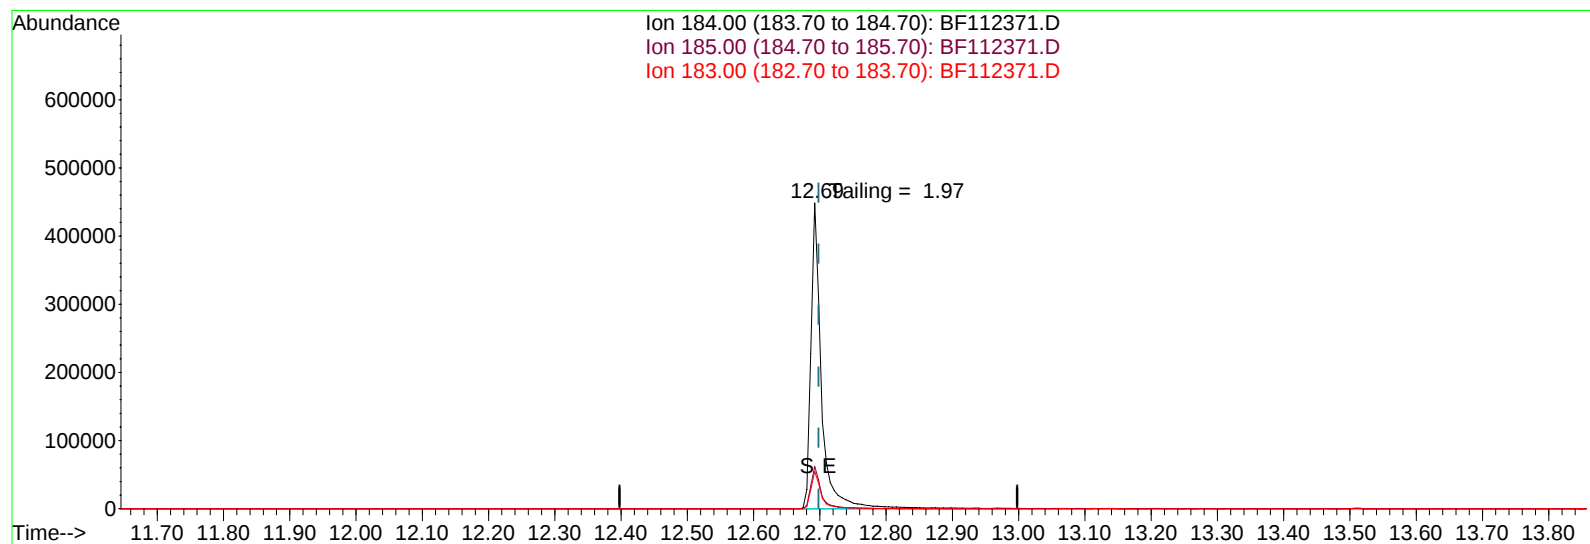

(77) Benzidine




12.692min (-0.006) 150827.31ng

response 494003

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	13.89#
183.00	12.50	12.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020419\
Data File : BF112371.D
Acq On : 4 Feb 2019 9:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 17:30:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

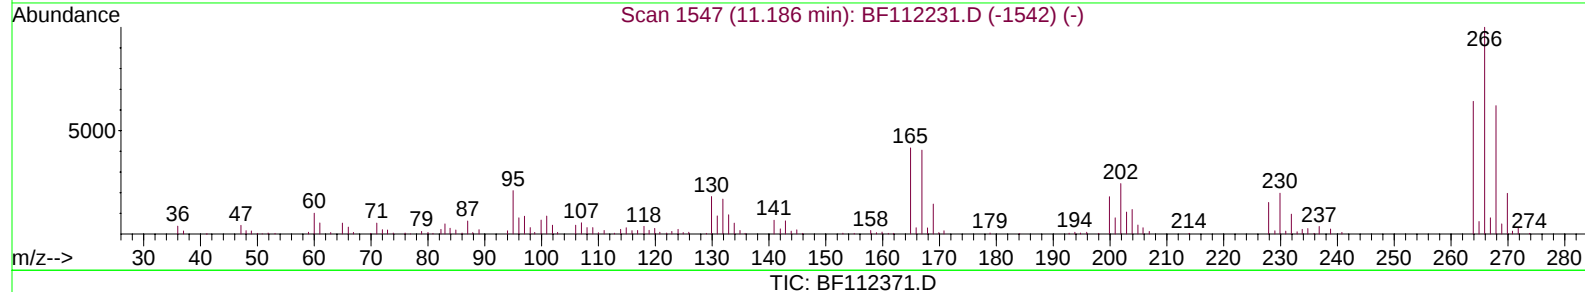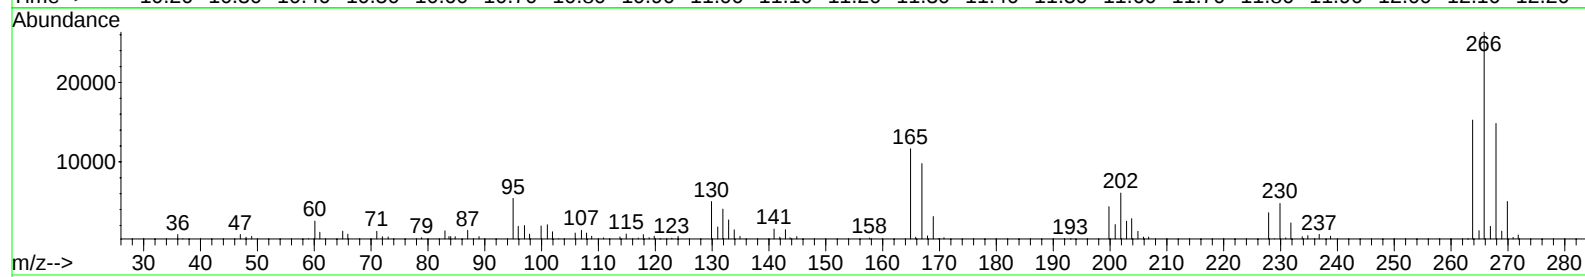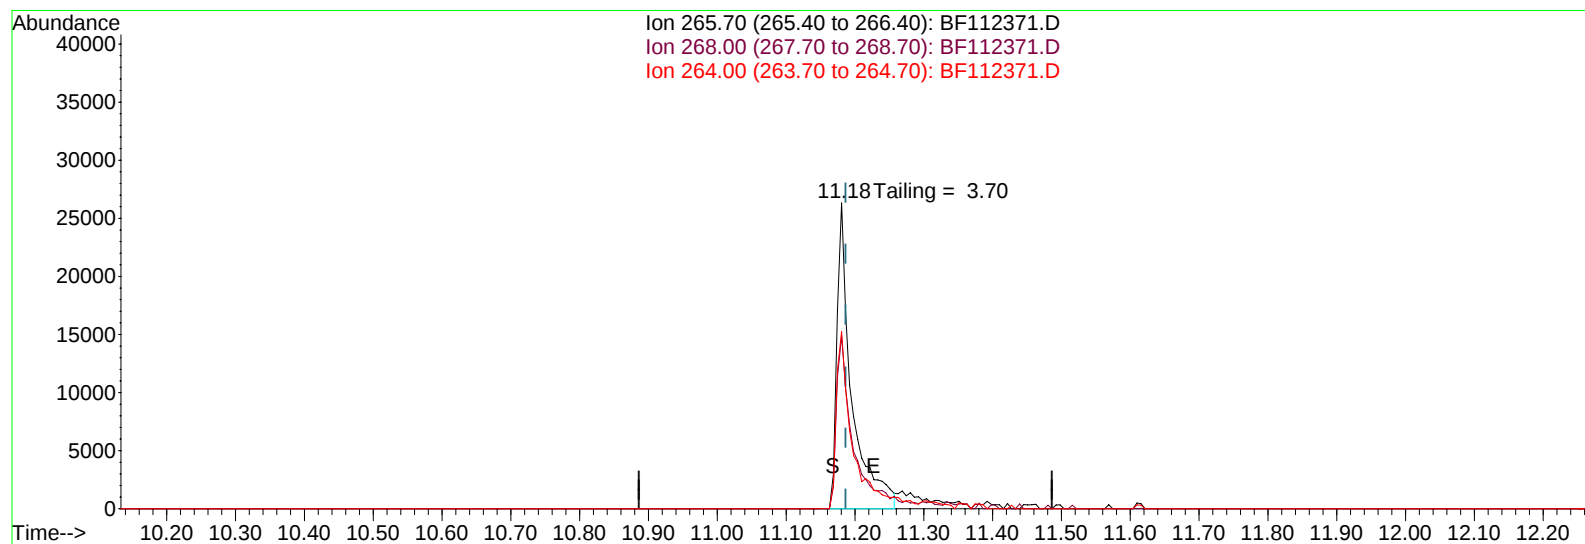

(70) Pentachlorophenol (C)

11.180min (-0.006) 74594.47ng

response 39922

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	56.41
264.00	63.60	58.00
0.00	0.00	0.00