
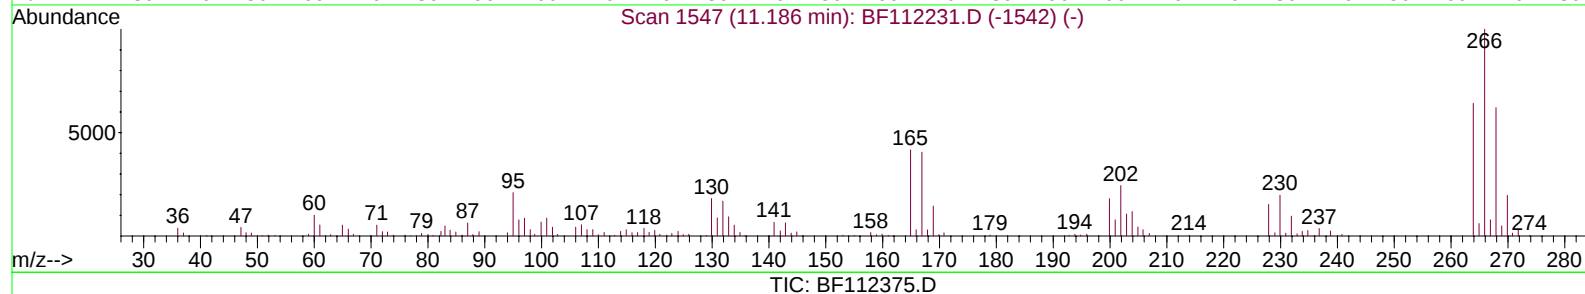
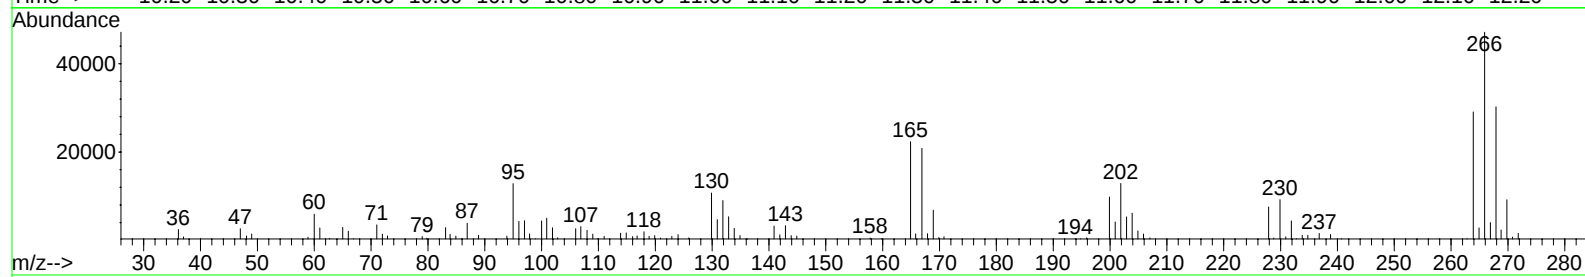


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020419\
Data File : BF112375.D
Acq On : 4 Feb 2019 12:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 17:35:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

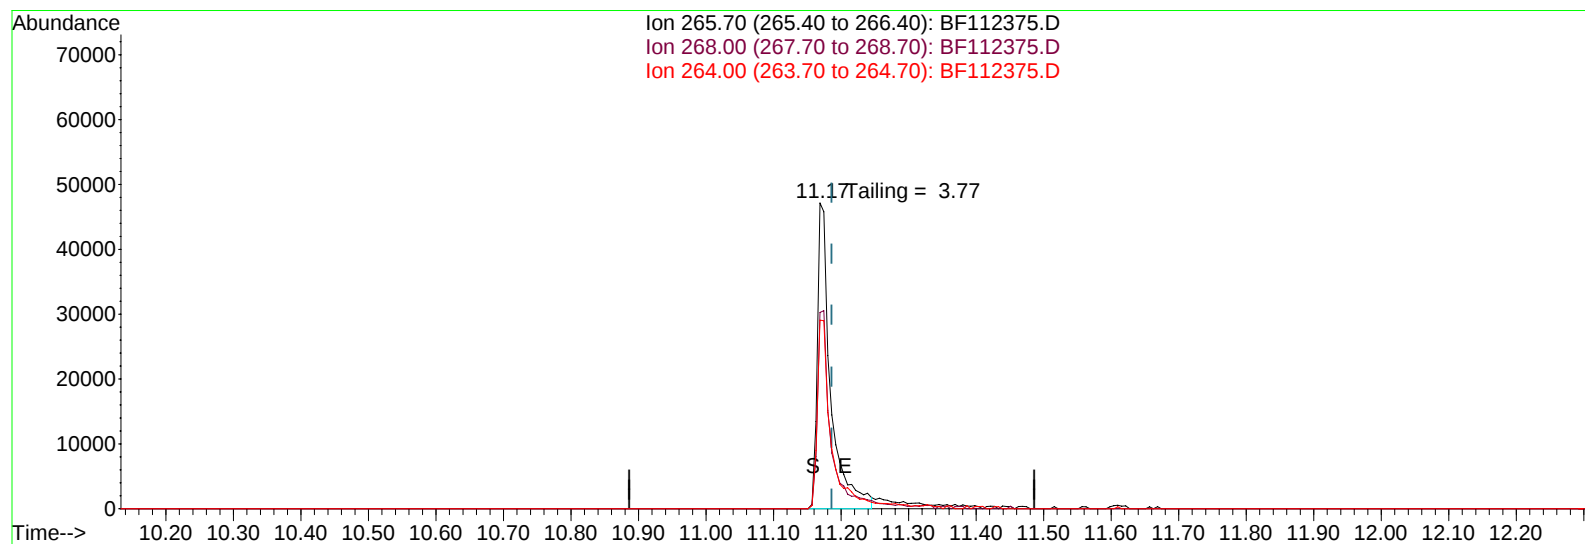

(70) Pentachlorophenol (C)




11.169min (-0.018) 26191.90ng m

response 65844

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	64.19
264.00	63.60	61.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020419\
 Data File : BF112375.D
 Acq On : 4 Feb 2019 12:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 17:35:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

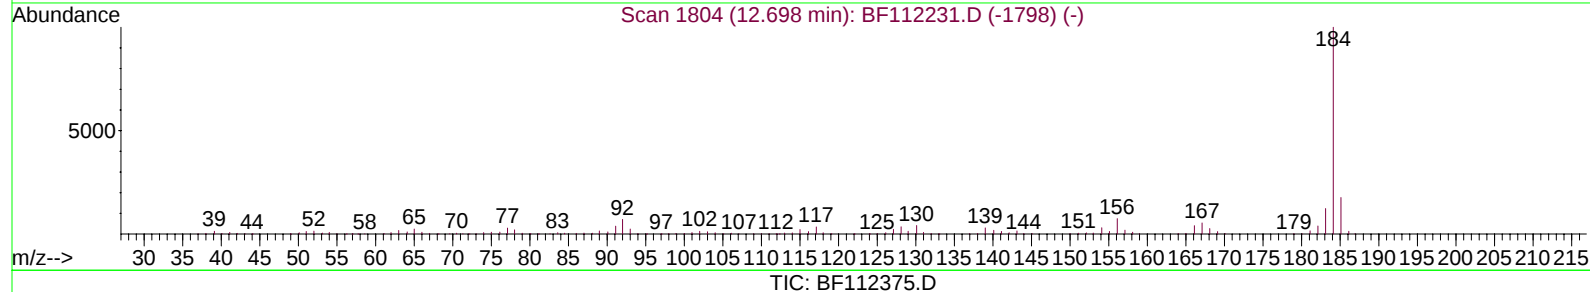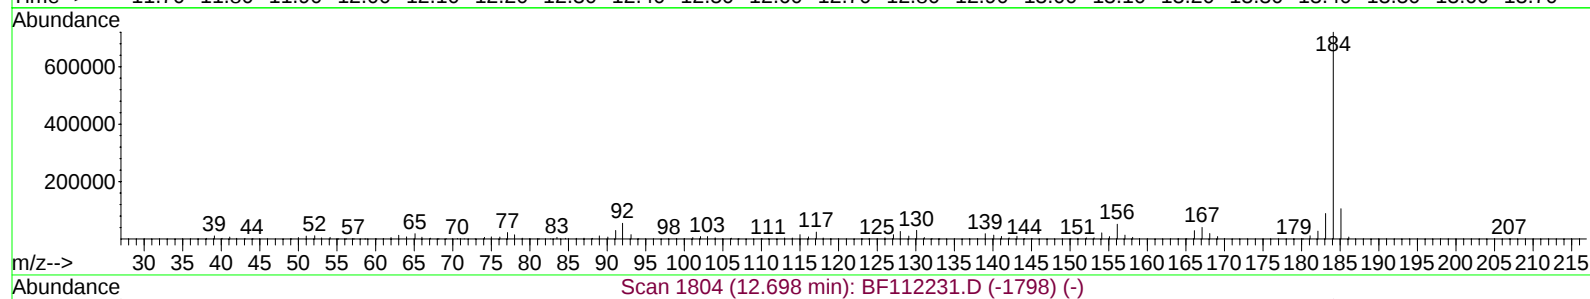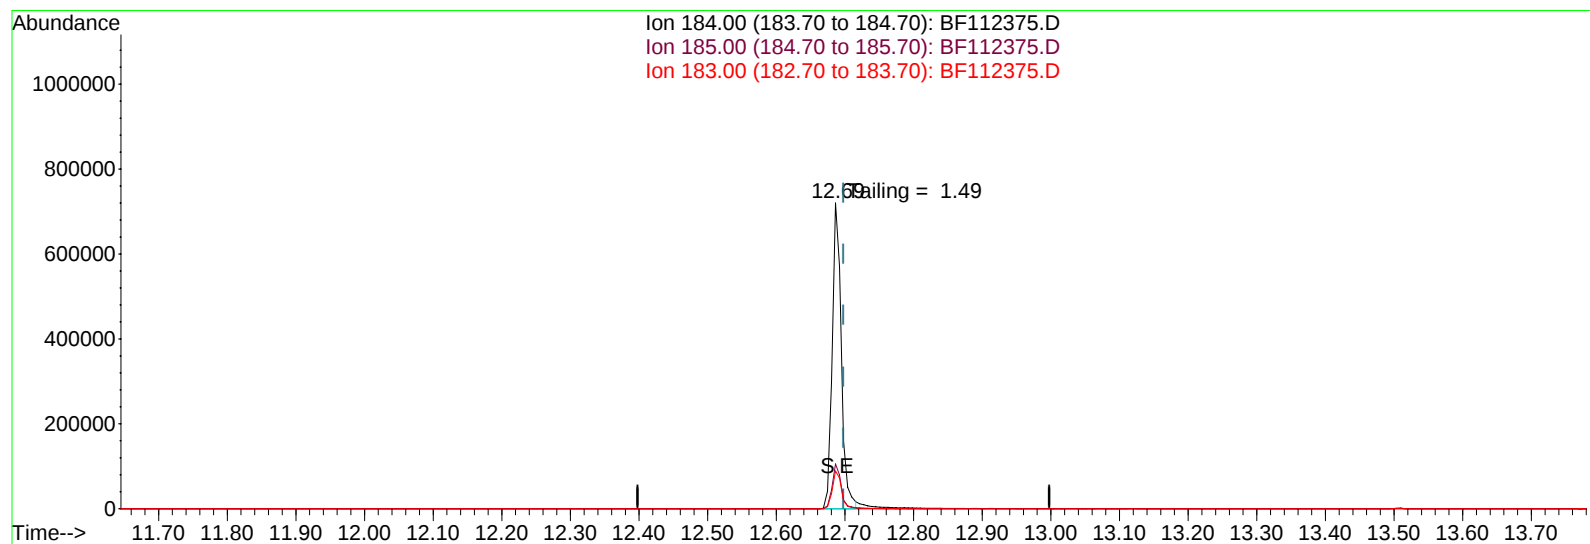

(77) Benzidine

12.686min (-0.012) 0.00ng

response 685298

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.68
183.00	12.50	12.33
0.00	0.00	0.00