


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF020419\  
 Data File : BF112371.D  
 Acq On : 4 Feb 2019 9:12  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF012519.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jan 28 10:38:18 2019

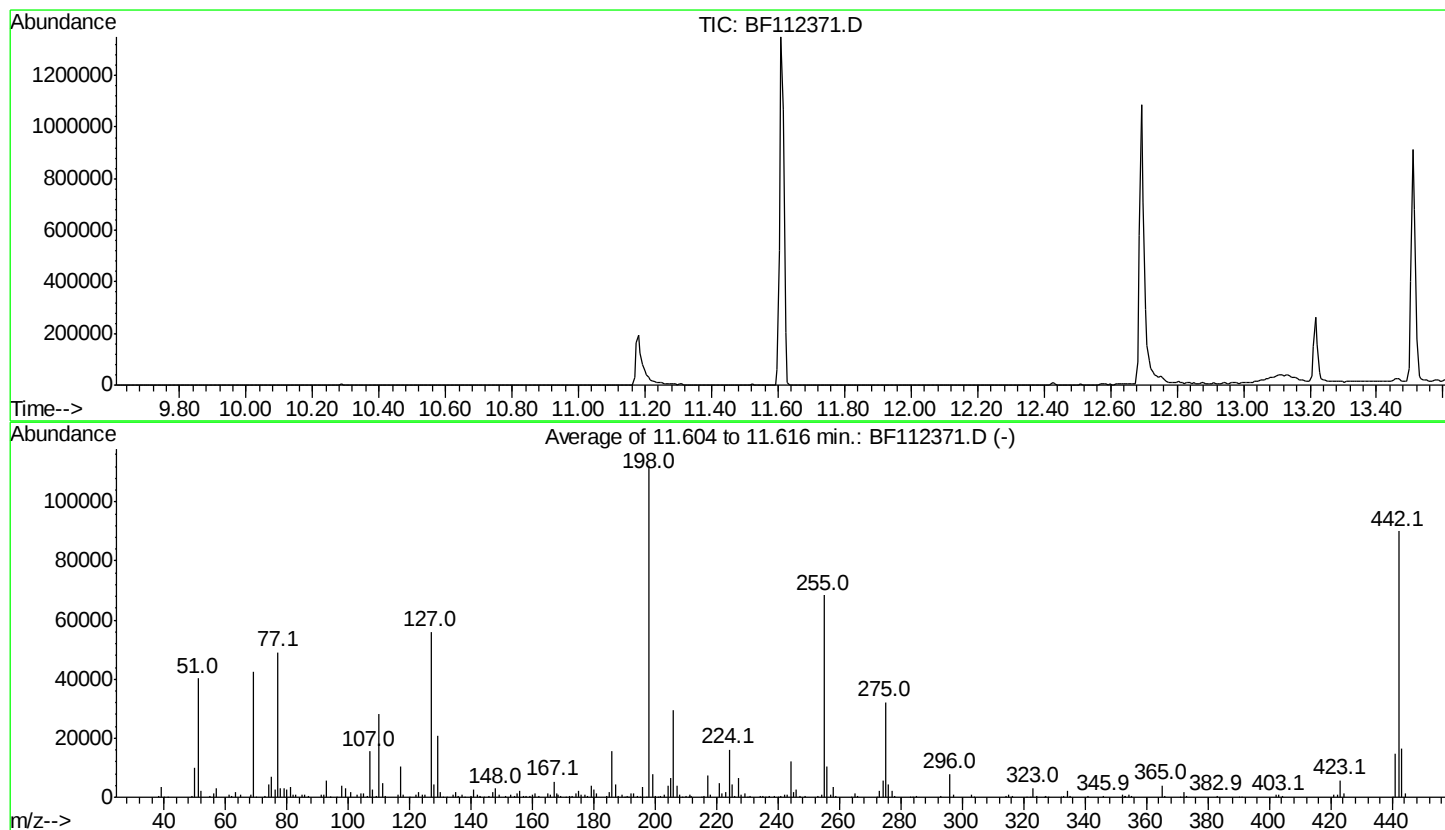

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.8      | 40253   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 687     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.0      | 42677   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 137     | PASS             |
| 127         | 198          | 10           | 80           | 49.9      | 56080   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 231     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 112306  | PASS             |
| 199         | 198          | 5            | 9            | 7.0       | 7843    | PASS             |
| 275         | 198          | 10           | 60           | 28.7      | 32189   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 4102    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.0      | 14555   | PASS             |
| 442         | 198          | 50           | 100          | 80.2      | 90077   | PASS             |
| 443         | 442          | 15           | 24           | 18.4      | 16597   | PASS             |