

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020519\
 Data File : BF112403.D
 Acq On : 5 Feb 2019 18:37
 Operator : JU/SJ
 Sample : K1346-03 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-020419-B

Quant Time: Feb 05 22:29:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	175782	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	658858	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	276048	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	433337	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	337298	20.00	ng	-0.01
87) Perylene-d12	15.47	264	252695	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	175301	21.18	ng	-0.02
7) Phenol-d6	6.48	99	222815	19.38	ng	-0.01
23) Nitrobenzene-d5	7.39	82	130504	11.41	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	48949	15.23	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	276373	14.16	ng	-0.02
79) Terphenyl-d14	12.93	244	213533	11.92	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.39	70	16539	2.086	ng	# 81
25) Isophorone	7.39	82	130502	7.275	ng	# 63
51) 2,6-Dinitrotoluene	9.87	165	35546	7.400	ng	# 34
57) 2,4-Dinitrotoluene	9.87	165	35547	5.813	ng	# 32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020519\
Data File : BF112403.D
Acq On : 5 Feb 2019 18:37
Operator : JU/SJ
Sample : K1346-03 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-020419-B

Quant Time: Feb 05 22:29:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

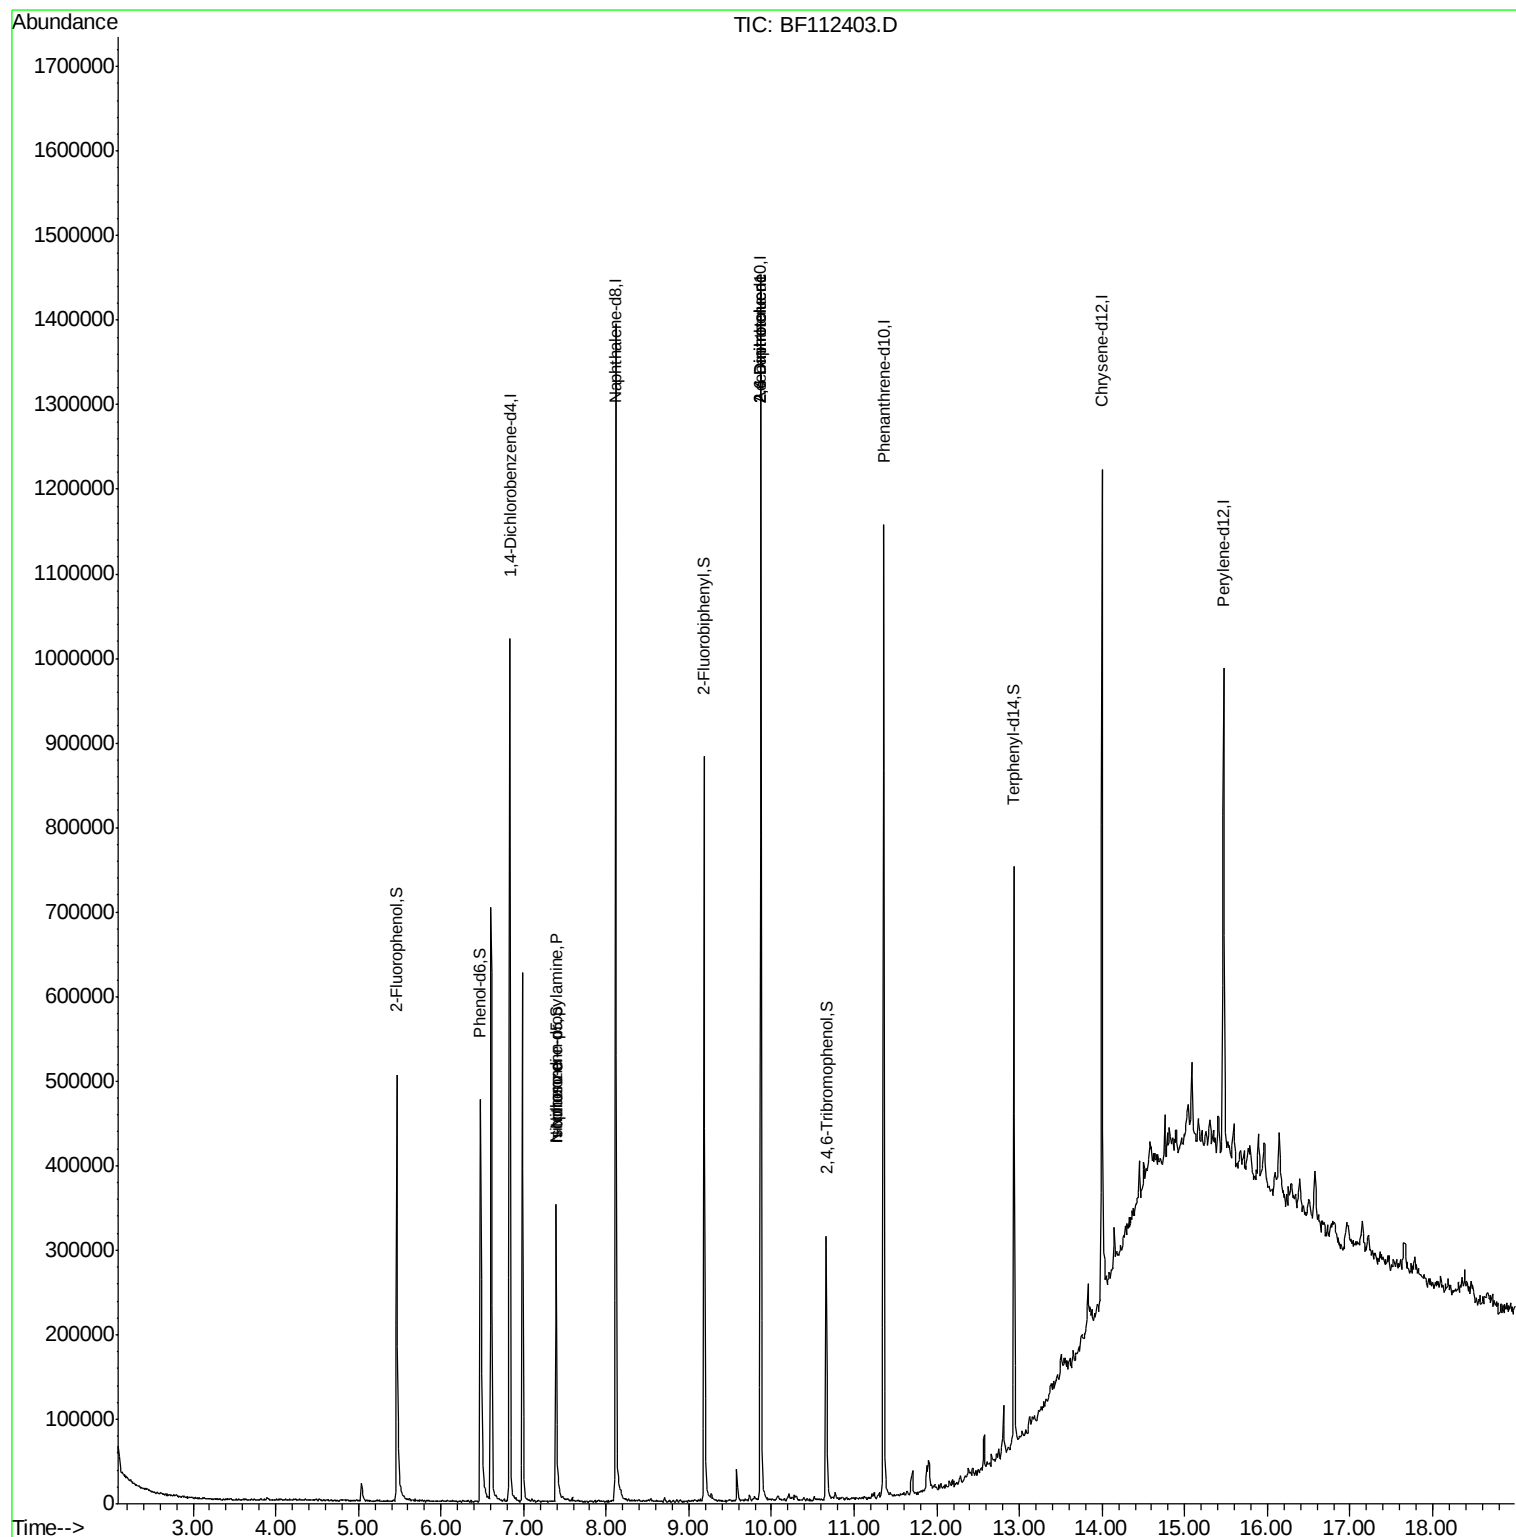


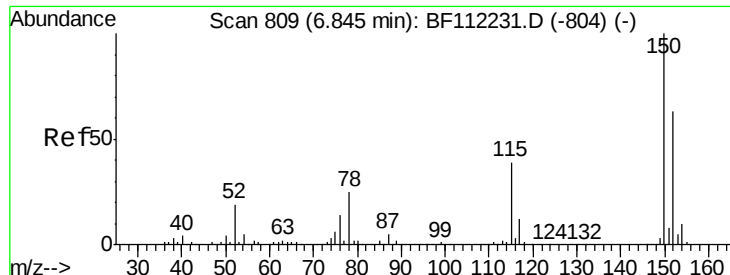




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 807
 Delta R.T. -0.01 min
 Lab File: BF112403.D
 Acq: 5 Feb 2019 18:37

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-020419-B

Tgt Ion:152 Resp: 175782
 Ion Ratio Lower Upper
 152 100
 150 153.7 127.4 191.0
 115 55.4 45.5 68.3

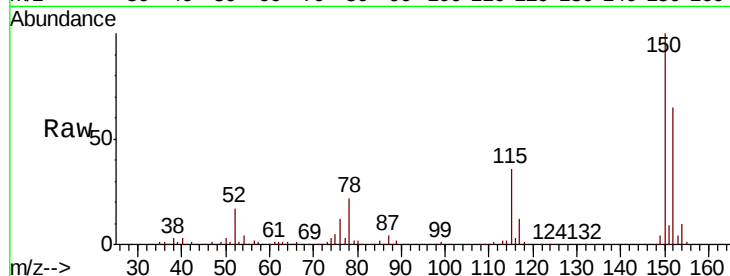


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E


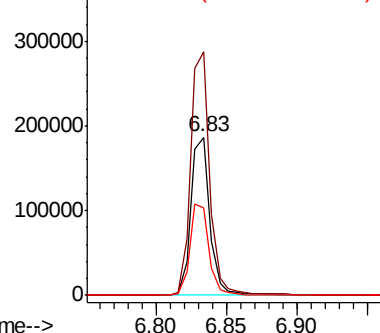


#5
 2-Fluorophenol
 Concen: 21.183 ng
 RT: 5.46 min Scan# 574
 Delta R.T. -0.02 min
 Lab File: BF112403.D
 Acq: 5 Feb 2019 18:37

Tgt Ion:112 Resp: 175301
 Ion Ratio Lower Upper
 112 100
 64 53.0 45.7 68.5
 63 28.0 23.6 35.4



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

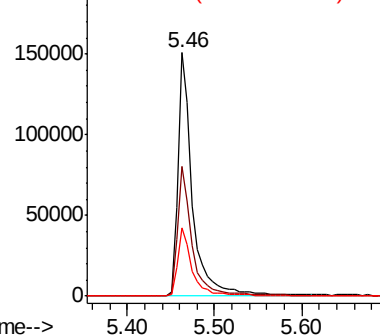



#7

Phenol-d6

Concen: 19.376 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Instrument :

BNA_F

ClientSampleId :

CL-02-020419-B


Tgt Ion: 99 Resp: 222815

Ion Ratio Lower Upper

99 100

42 17.0 15.1 22.7




71 34.4 26.9 40.3

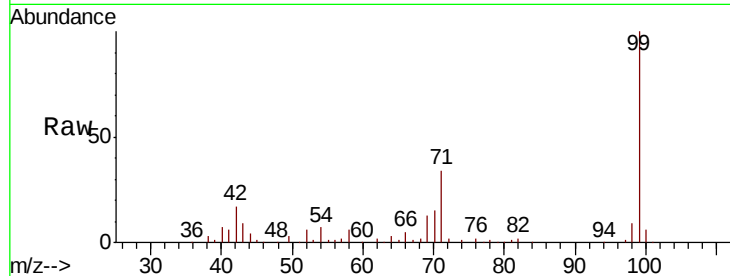

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

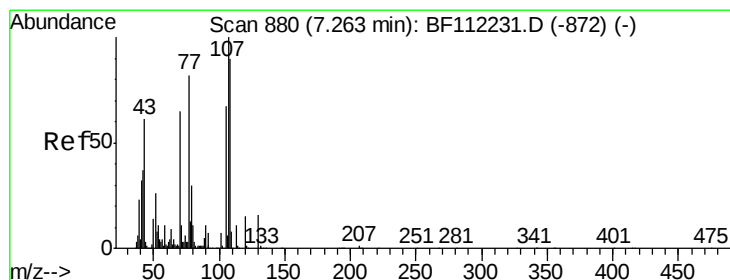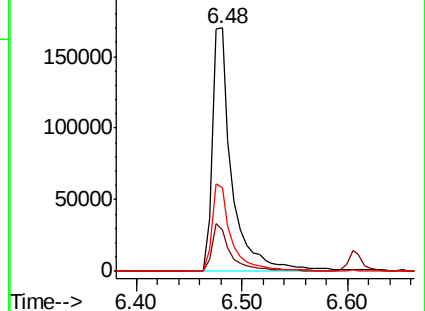

#19

n-Nitroso-di-n-propylamine

Concen: 2.086 ng

RT: 7.39 min Scan# 902

Delta R.T. 0.13 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Tgt Ion: 70 Resp: 16539


Ion Ratio Lower Upper

70 100

42 52.8 47.6 71.4

101 0.0 7.9 11.9#

130 2.0 18.4 27.6#





Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

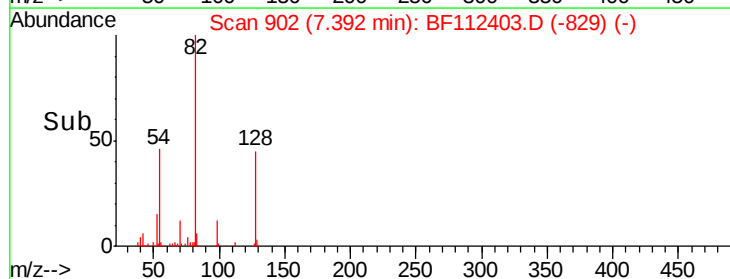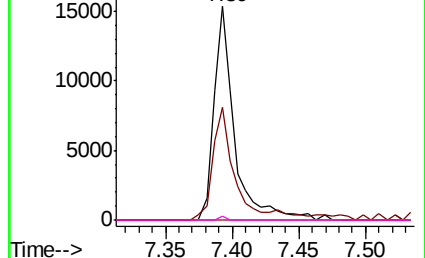



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Instrument :

BNA_F

ClientSampleId :

CL-02-020419-B

Tgt Ion: 136 Resp: 658858


Ion Ratio Lower Upper

136 100

137 10.5 9.1 13.7

54 5.7 5.9 8.9#

68 4.8 5.1 7.7#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

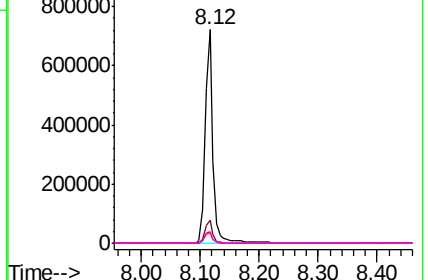

#23

Nitrobenzene-d5

Concen: 11.413 ng

RT: 7.39 min Scan# 902

Delta R.T. -0.02 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37


Tgt Ion: 82 Resp: 130504

Ion Ratio Lower Upper

82 100

128 45.2 37.8 56.8



54 46.3 39.7 59.5



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

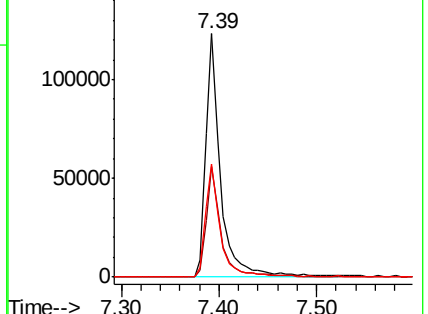



#25

Isophorone

Concen: 7.275 ng

RT: 7.39 min Scan# 902

Delta R.T. -0.28 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Instrument :

BNA_F

ClientSampleId :

CL-02-020419-B


Tgt Ion: 82 Resp: 130502

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#




138 0.0 15.4 23.0#

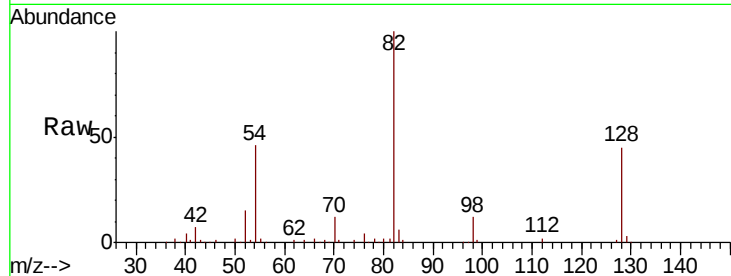

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

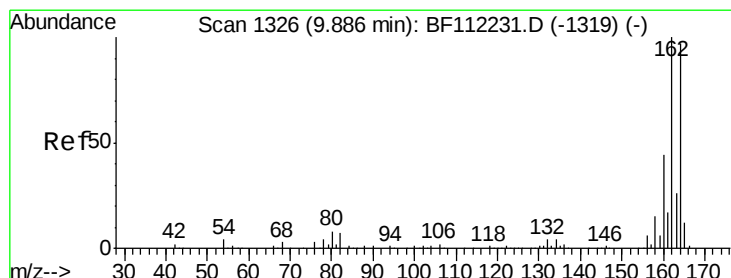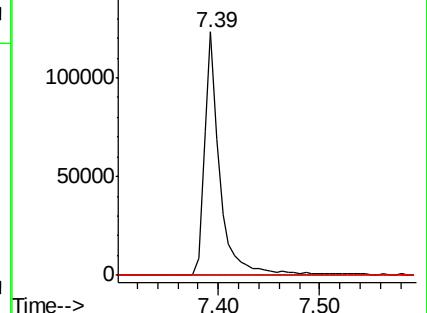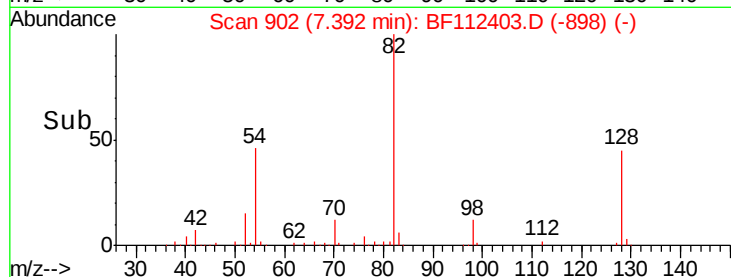

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37


Tgt Ion: 164 Resp: 276048

Ion Ratio Lower Upper

164 100

162 104.8 82.2 123.4



160 46.2 36.2 54.4

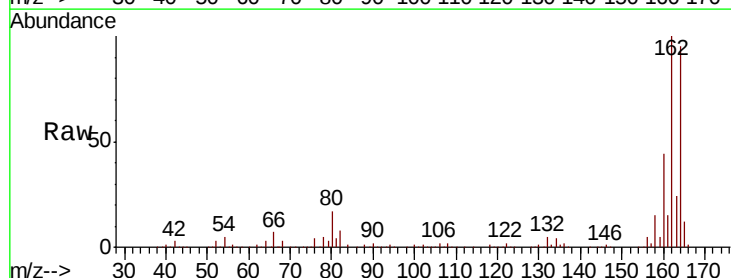

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

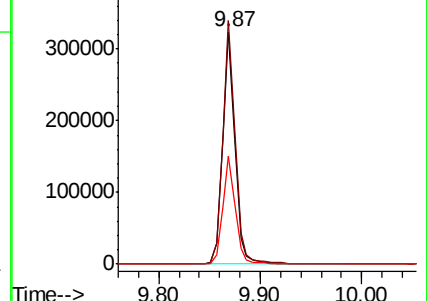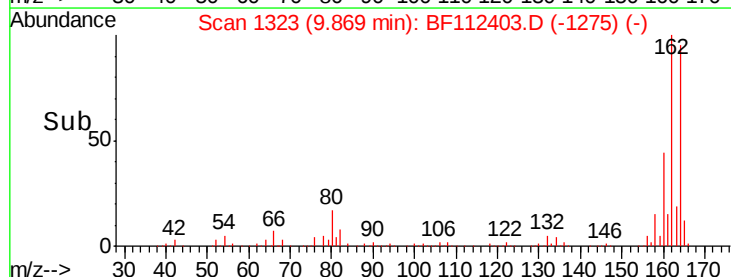







#42
 2,4,6-Tribromophenol
 Concen: 15.234 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.02 min
 Lab File: BF112403.D
 Acq: 5 Feb 2019 18:37

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-020419-B

Tgt Ion:330 Resp: 48949
 Ion Ratio Lower Upper
 330 100
 332 92.8 76.6 114.8
 141 29.6 24.3 36.5

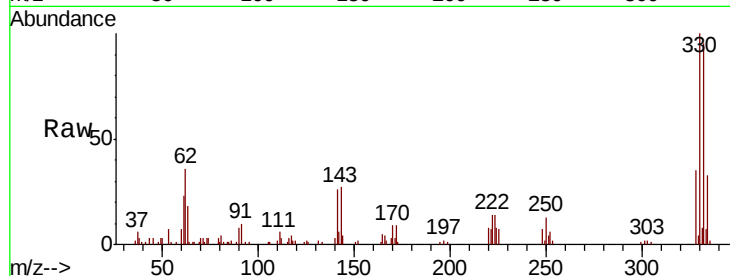


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

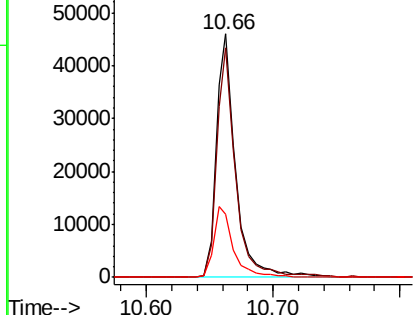




#45
 2-Fluorobiphenyl
 Concen: 14.160 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.02 min
 Lab File: BF112403.D
 Acq: 5 Feb 2019 18:37

Tgt Ion:172 Resp: 276373
 Ion Ratio Lower Upper
 172 100
 171 34.7 30.5 45.7
 170 23.3 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

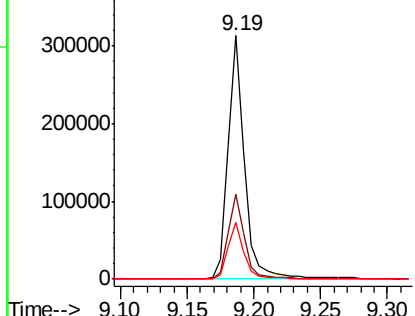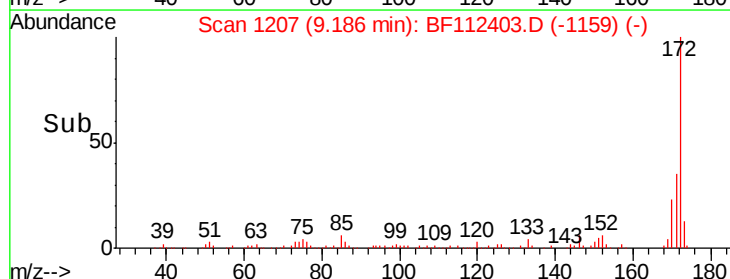



#51

2,6-Dinitrotoluene

Concen: 7.400 ng

RT: 9.87 min Scan# 1323

Delta R.T. 0.20 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Instrument :

BNA_F

ClientSampleId :

CL-02-020419-B


Tgt Ion:165 Resp: 35546

Ion Ratio Lower Upper

165 100

63 1.4 33.8 50.8#




89 1.6 36.9 55.3#



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

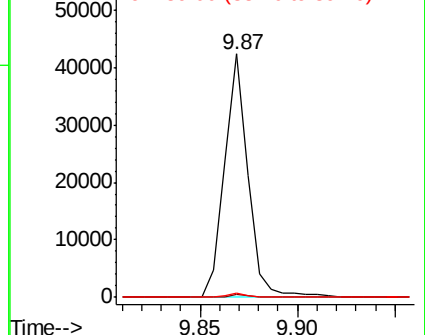

#57

2,4-Dinitrotoluene

Concen: 5.813 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.21 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Tgt Ion:165 Resp: 35547


Ion Ratio Lower Upper

165 100

63 1.4 27.9 41.9#

89 1.6 47.9 71.9#

182 0.0 2.2 3.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E



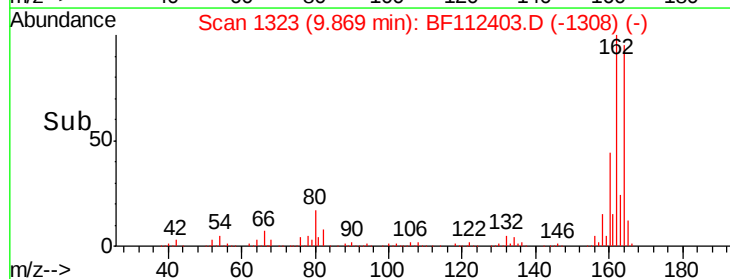
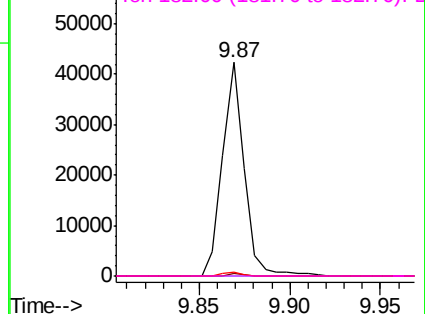


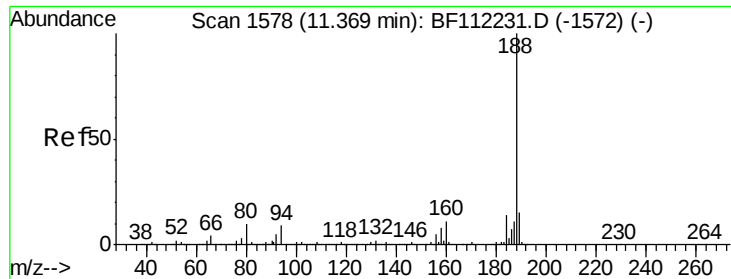

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112403.D
Acq: 5 Feb 2019 18:37




Instrument :
BNA_F
ClientSampleId :
CL-02-020419-B


Tgt Ion:188 Resp: 433337
Ion Ratio Lower Upper
188 100
94 8.0 8.2 12.2#
80 8.7 8.9 13.3#

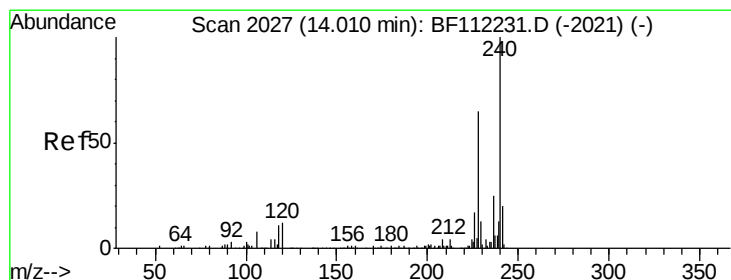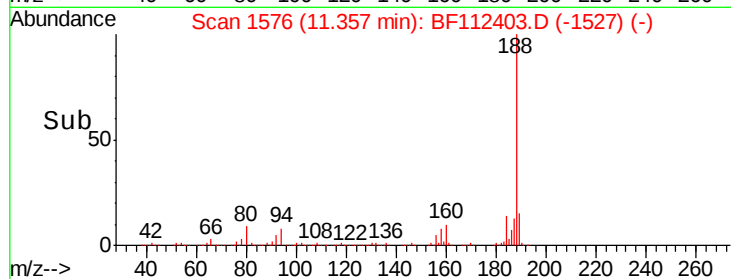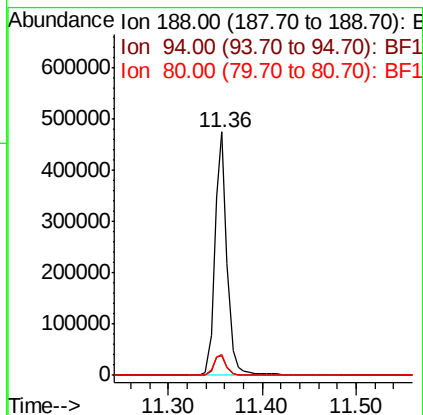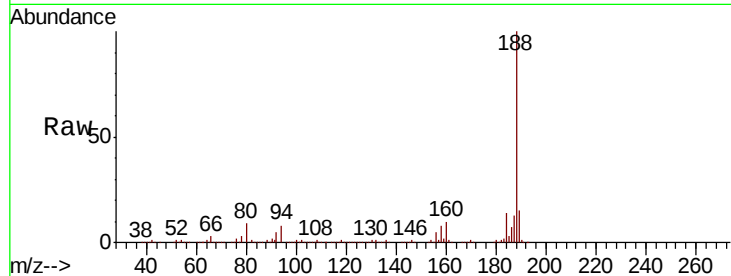

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112403.D
Acq: 5 Feb 2019 18:37

Tgt Ion:240 Resp: 337298
Ion Ratio Lower Upper
240 100
120 11.2 9.0 13.6
236 24.7 20.7 31.1

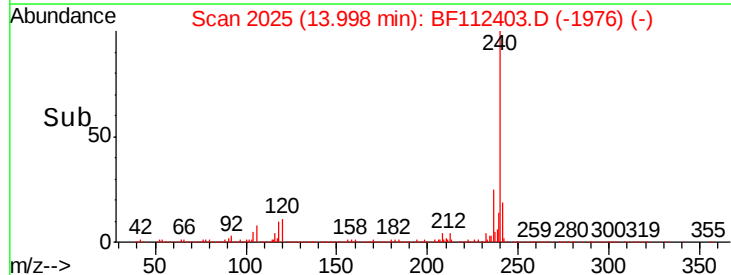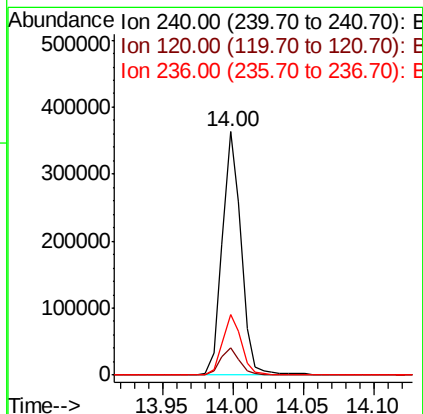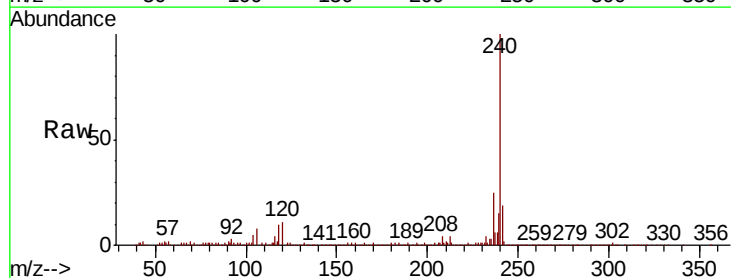



#79

Terphenyl-d14

Concen: 11.924 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.02 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37

Instrument :

BNA_F

ClientSampleId :

CL-02-020419-B


Tgt Ion:244 Resp: 213533

Ion Ratio Lower Upper

244 100

212 6.6 5.9 8.9




122 10.1 9.8 14.6



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

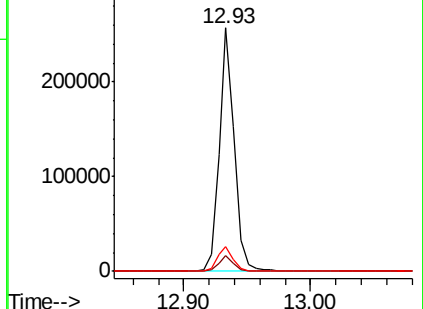

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.47 min Scan# 2275

Delta R.T. -0.01 min

Lab File: BF112403.D

Acq: 5 Feb 2019 18:37


Tgt Ion:264 Resp: 252695

Ion Ratio Lower Upper

264 100

260 23.0 18.2 27.2

265 21.2 17.0 25.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

