
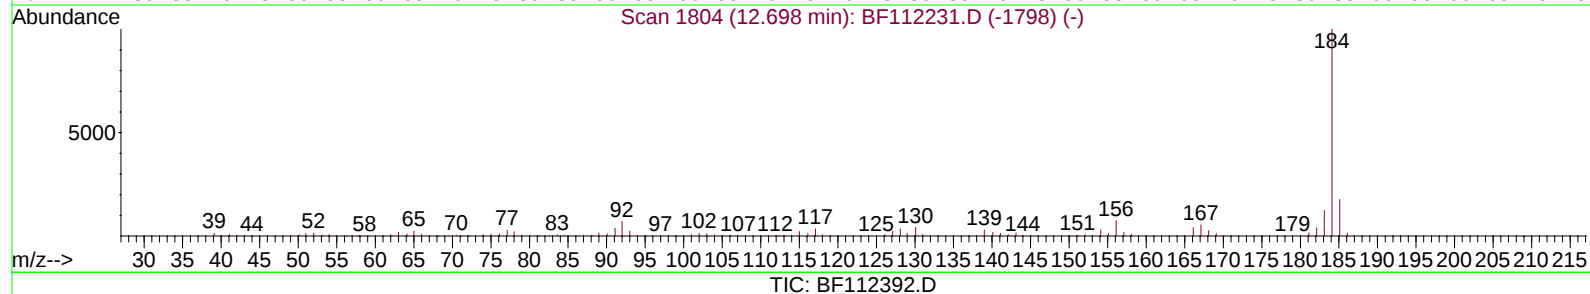
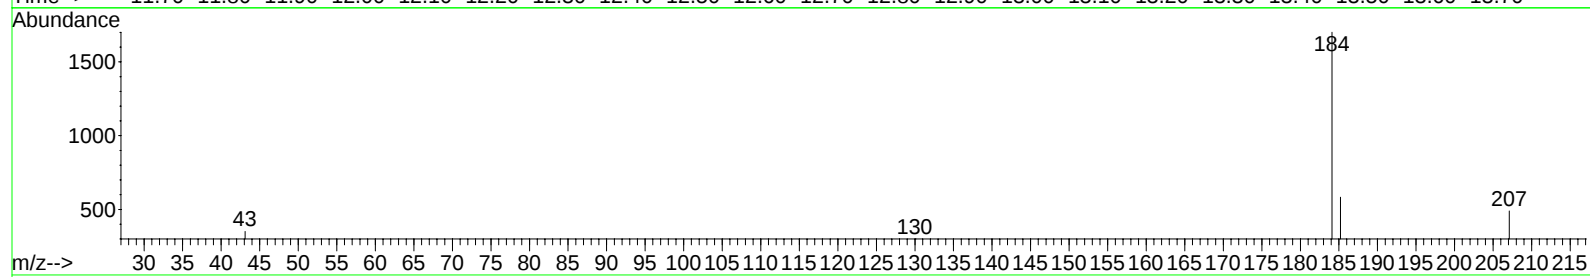


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020519\
 Data File : BF112392.D
 Acq On : 5 Feb 2019 13:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 17:56:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

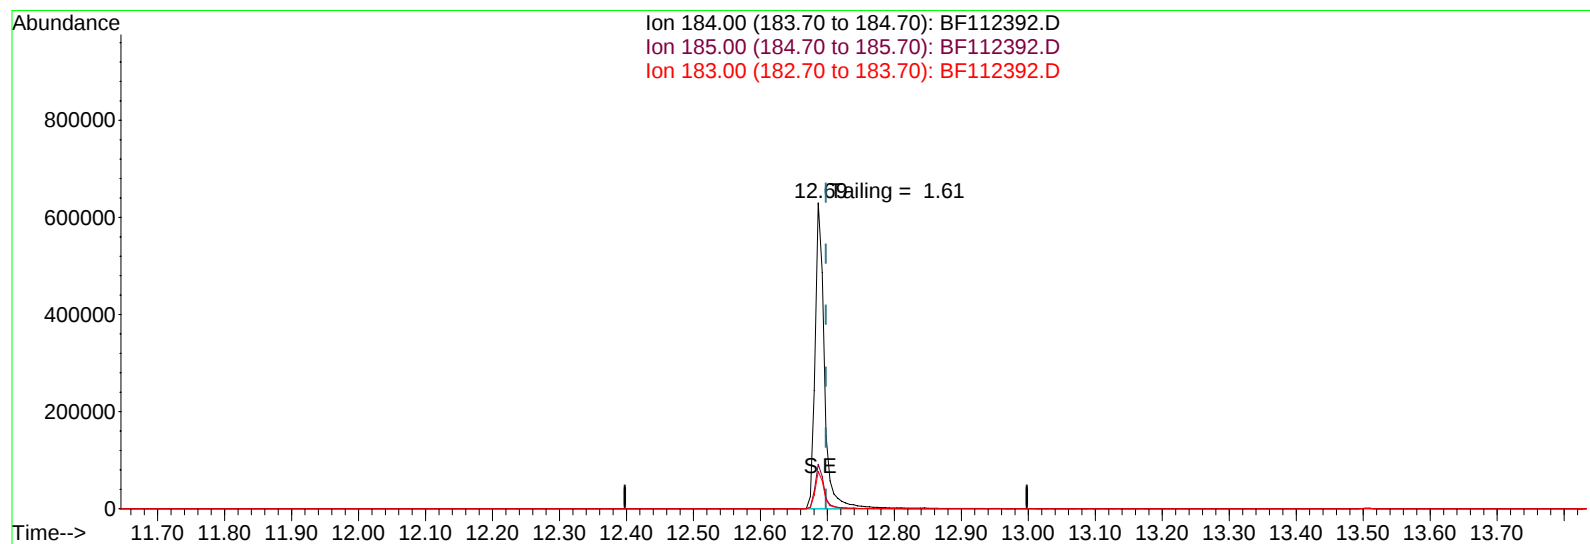

(77) Benzidine




12.686min (-0.012) 0.00ng

response 611078

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.54
183.00	12.50	12.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020519\
Data File : BF112392.D
Acq On : 5 Feb 2019 13:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 17:56:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

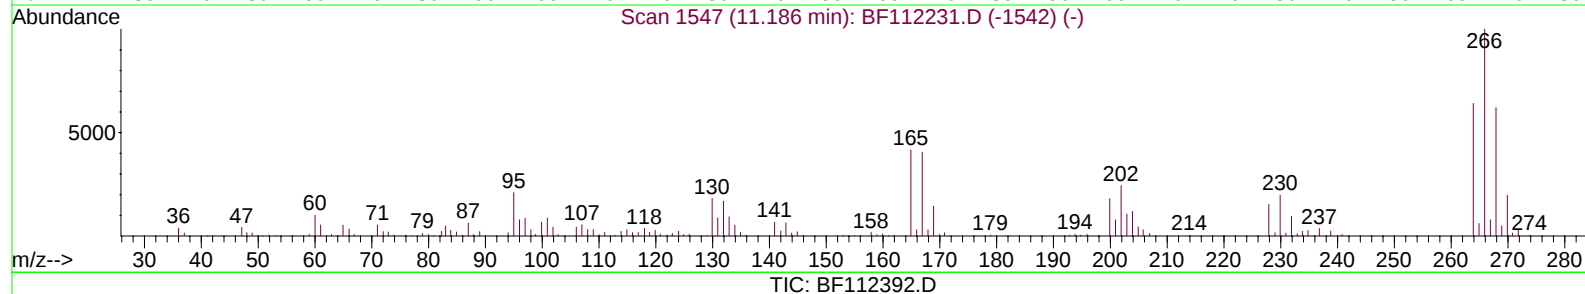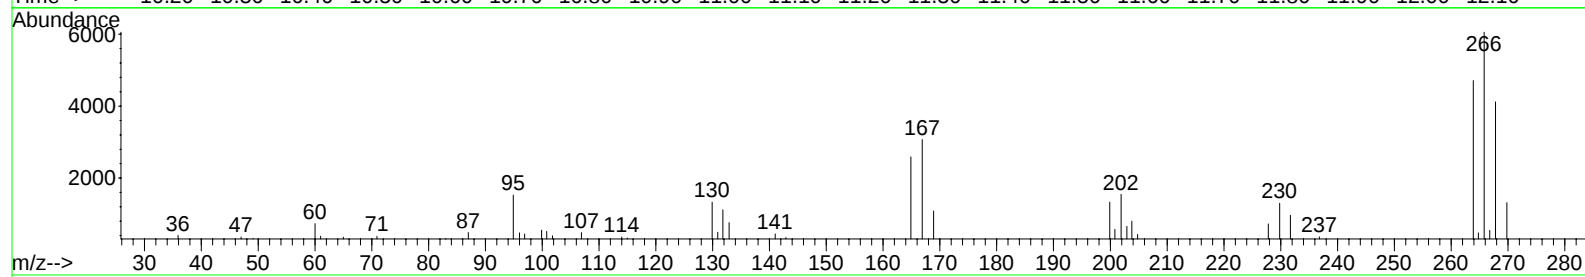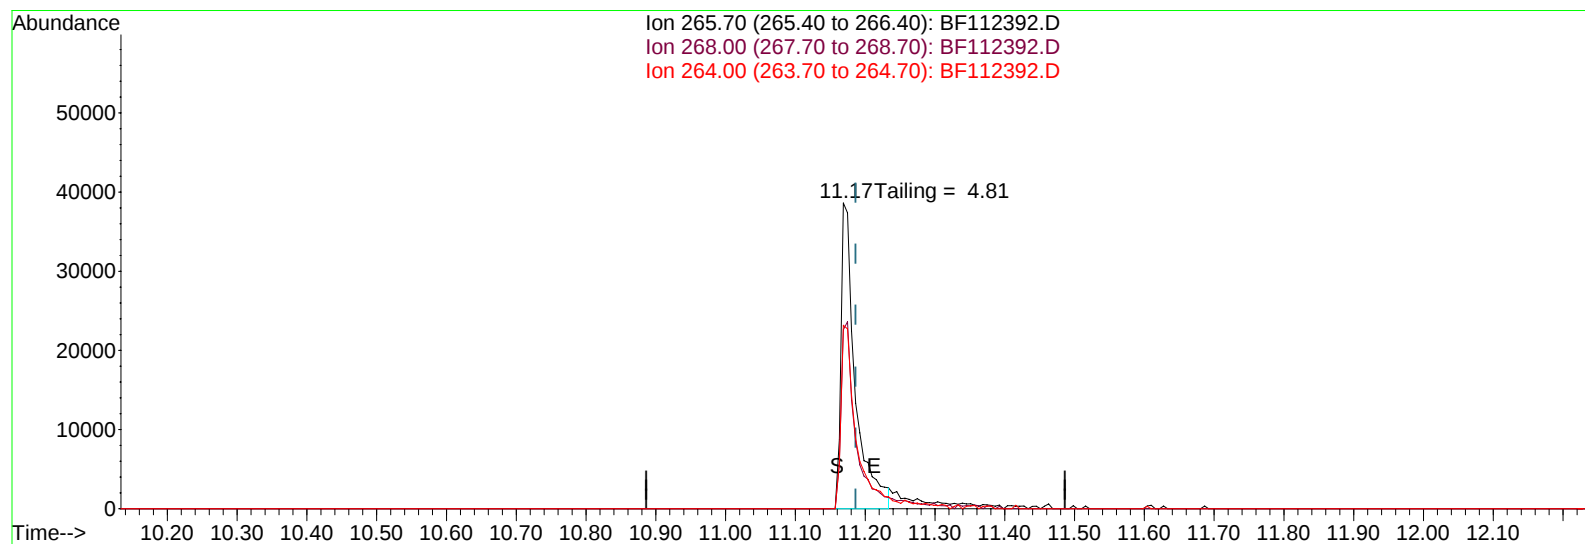

(70) Pentachlorophenol (C)

11.198min (+0.012) 3799.95ng m

response 2071

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	68.07
264.00	63.60	77.82#
0.00	0.00	0.00