

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020519\
 Data File : BF112414.D
 Acq On : 5 Feb 2019 23:46
 Operator : JU/SJ
 Sample : K1341-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-05-020419-C

Quant Time: Feb 06 01:06:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	141751	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	533669	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	252731	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	441502	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	309143	20.00	ng	-0.01
87) Perylene-d12	15.47	264	276177	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	952035	142.66	ng	0.00
7) Phenol-d6	6.49	99	1081144	116.59	ng	0.00
23) Nitrobenzene-d5	7.40	82	807688	87.21	ng	-0.01
42) 2,4,6-Tribromophenol	10.66	330	372253	126.54	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	1606710	89.91	ng	-0.02
79) Terphenyl-d14	12.94	244	1495877	91.14	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020519\
Data File : BF112414.D
Acq On : 5 Feb 2019 23:46
Operator : JU/SJ
Sample : K1341-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-05-020419-C

Quant Time: Feb 06 01:06:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

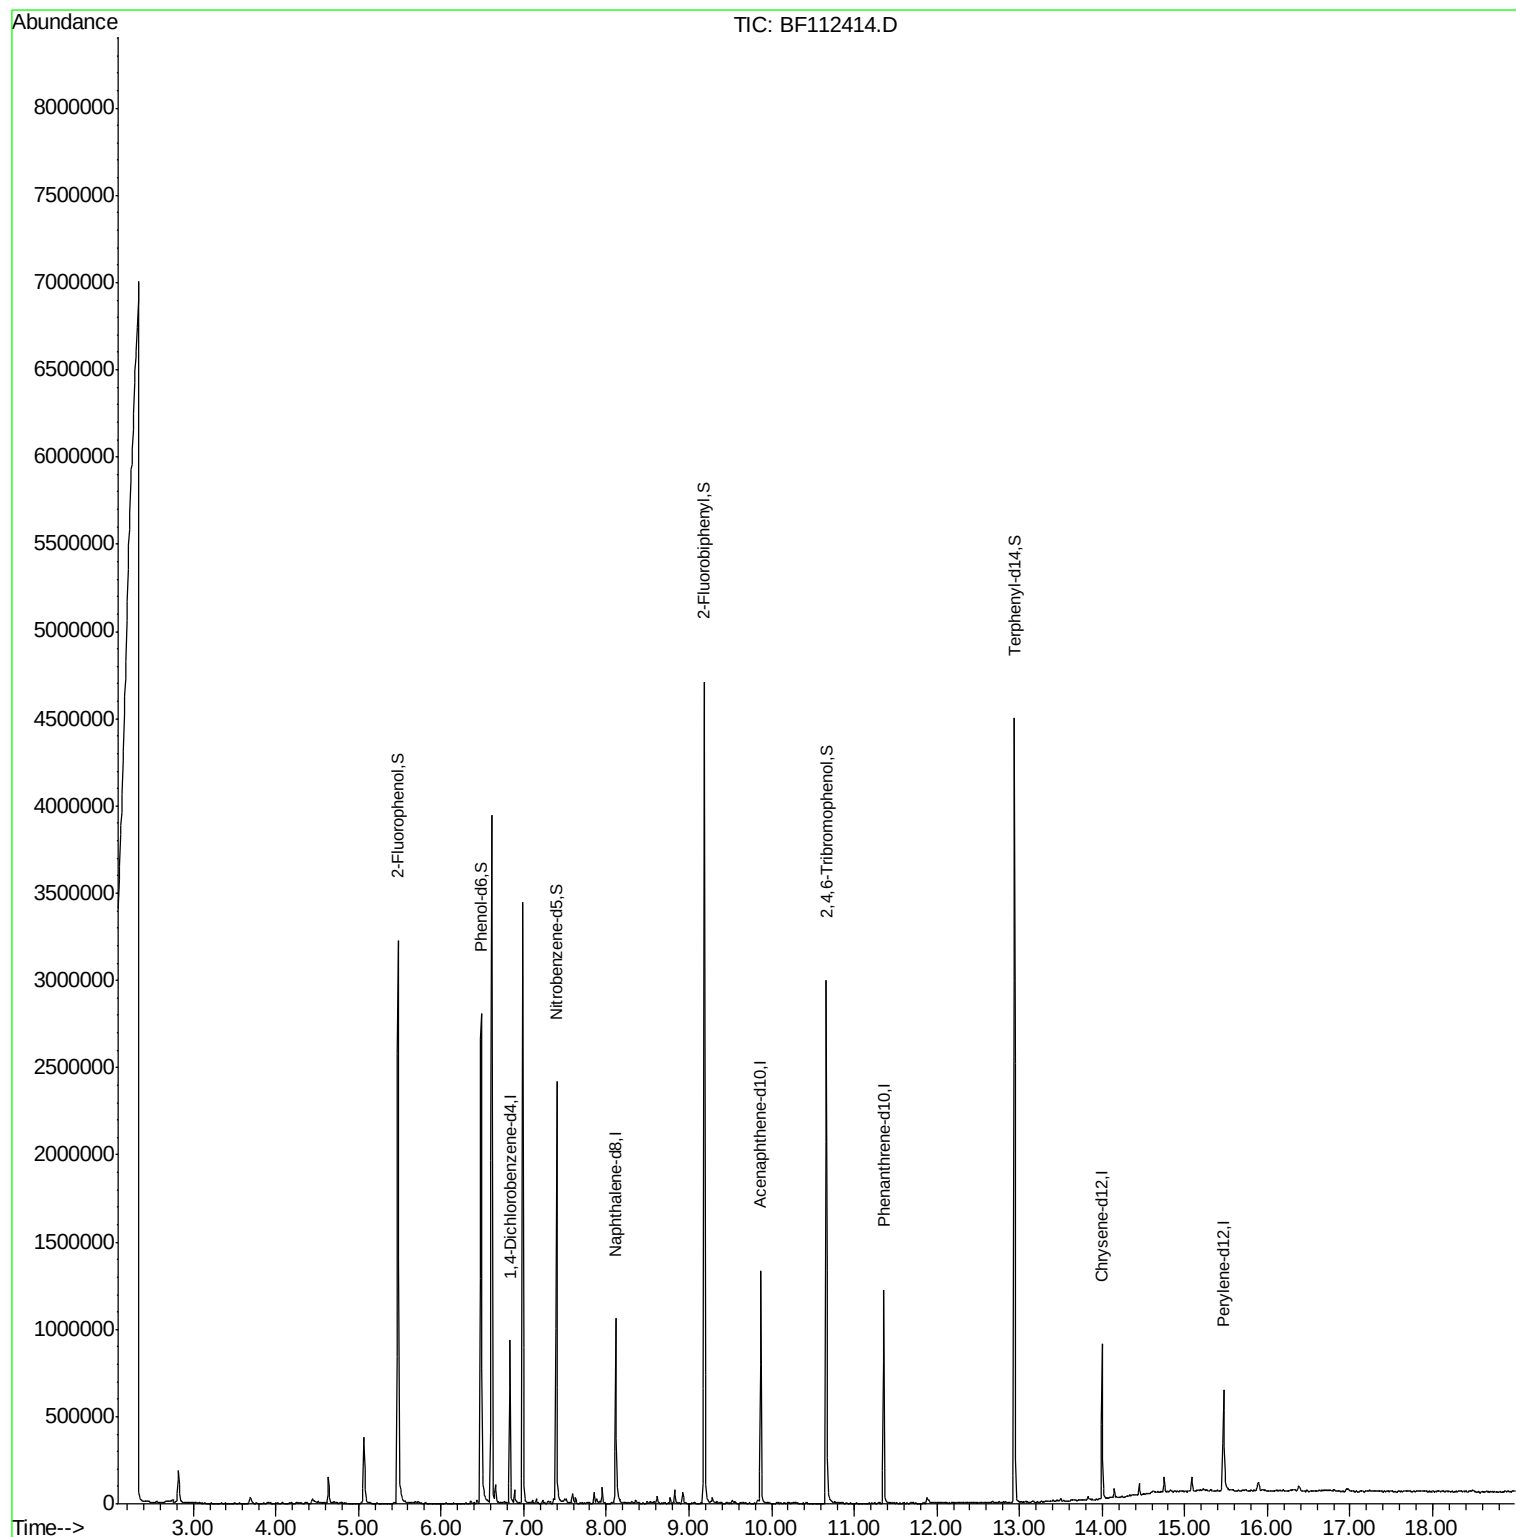

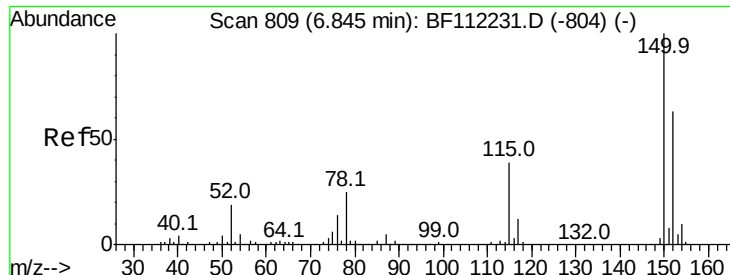


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF112414.D
Acq: 5 Feb 2019 23:46

Instrument :
BNA_F
ClientSampleId :
HR-05-020419-C

Tot Ion:152 Resp: 141751
Ion Ratio Lower Upper
152 100
150 151.0 127.4 191.0
115 57.8 45.5 68.3

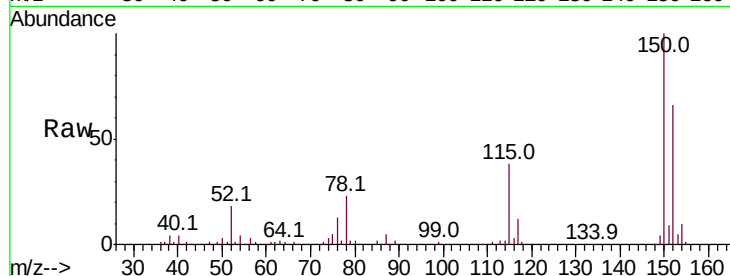


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

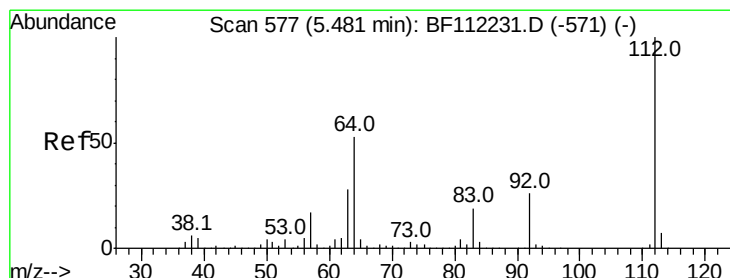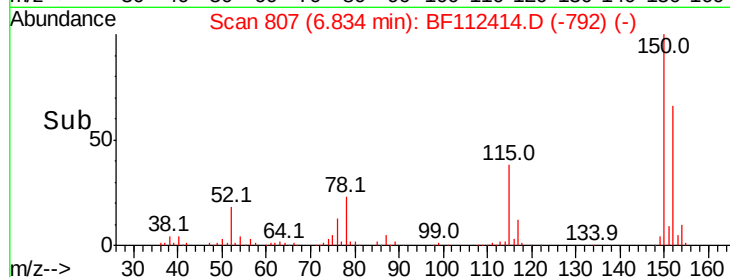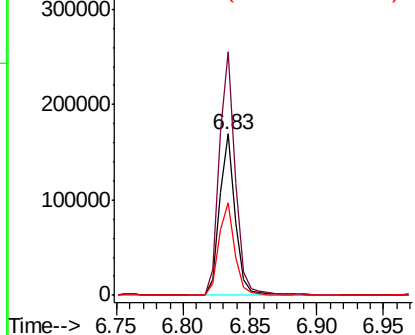



#5


2-Fluorophenol
Concen: 142.658 ng
RT: 5.48 min Scan# 577
Delta R.T. 0.00 min
Lab File: BF112414.D
Acq: 5 Feb 2019 23:46

Tgt Ion:112 Resp: 952035
Ion Ratio Lower Upper
112 100
64 54.8 45.7 68.5
63 29.2 23.6 35.4

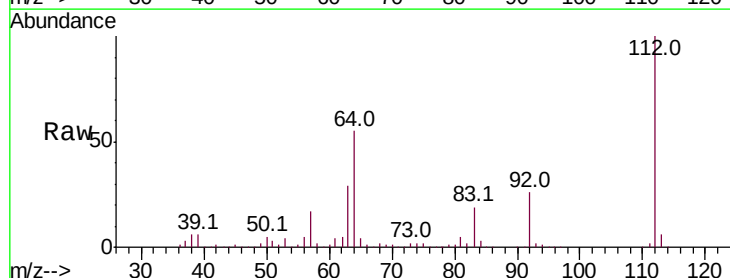

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

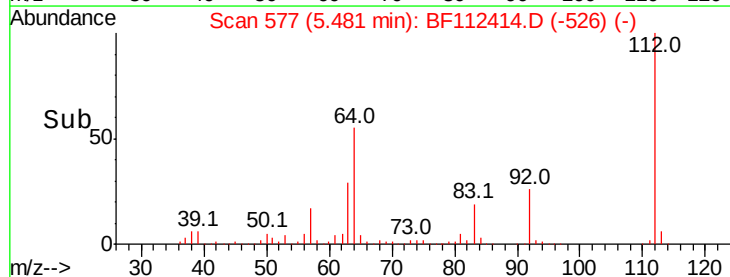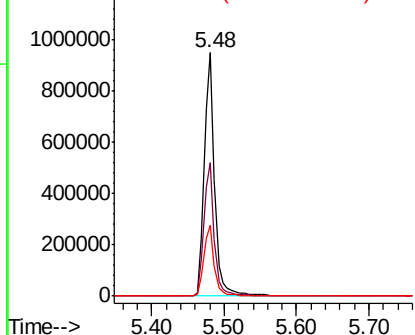

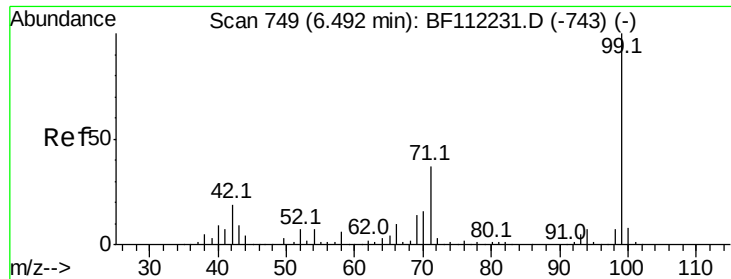

#7

Phenol-d6

Concen: 116.587 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112414.D

Acq: 5 Feb 2019 23:46

Instrument :

BNA_F

ClientSampleId :

HR-05-020419-C


Tot Ion: 99 Resp: 1081144

Ion Ratio Lower Upper




99 100

42 17.9 15.1 22.7

71 35.1 26.9 40.3

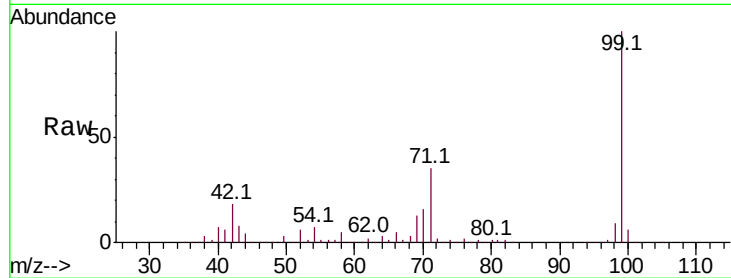

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

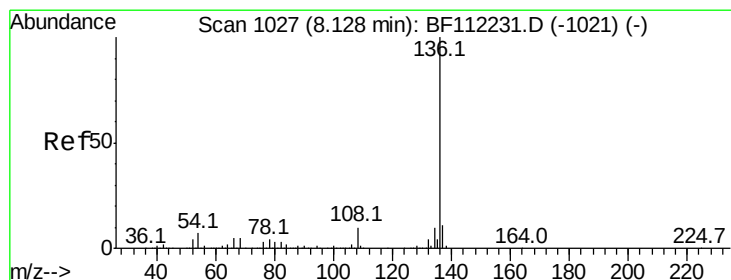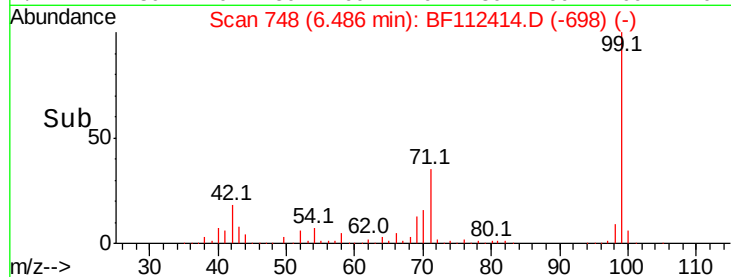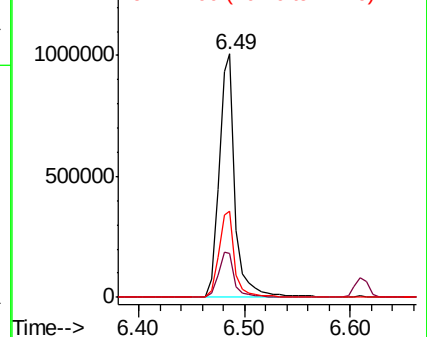

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112414.D

Acq: 5 Feb 2019 23:46

Tgt Ion: 136 Resp: 533669


Ion Ratio Lower Upper

136 100



137 10.6 9.1 13.7


54 5.7 5.9 8.9#

68 4.8 5.1 7.7#

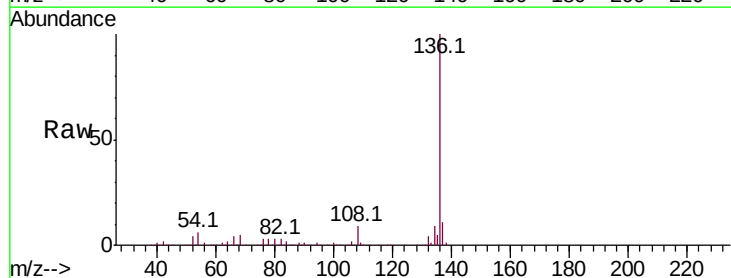

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



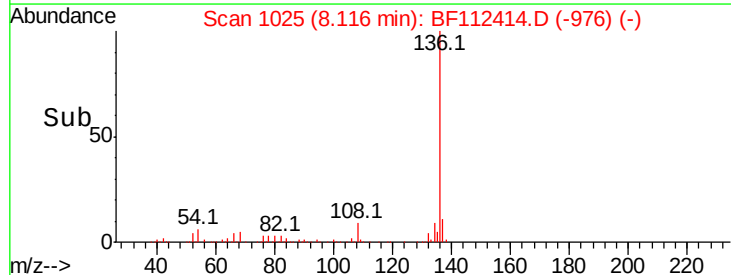
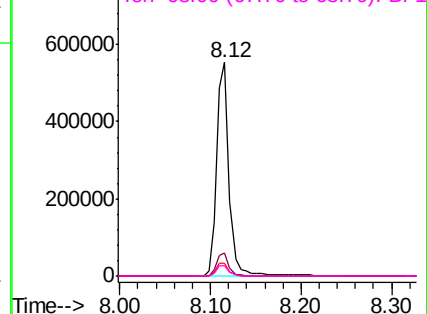


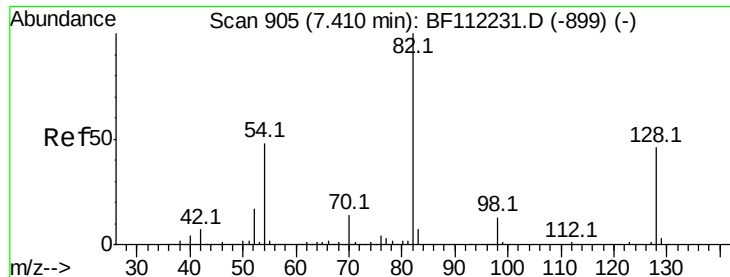

#23
 Nitrobenzene-d5
 Concen: 87.205 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.01 min
 Lab File: BF112414.D
 Acq: 5 Feb 2019 23:46




Instrument :
 BNA_F
 ClientSampleId :
 HR-05-020419-C


Tot Ion	82	Resp	807688
Ion Ratio	Lower	Upper	
82	100		
128	48.2	37.8	56.8
54	47.2	39.7	59.5

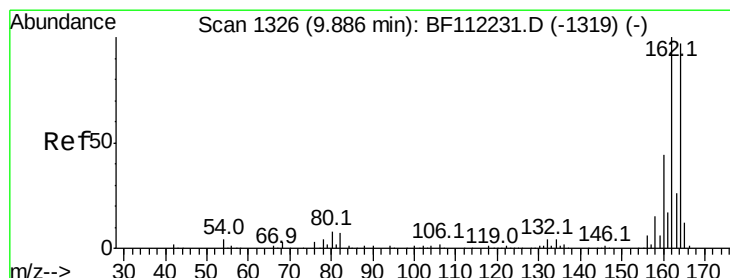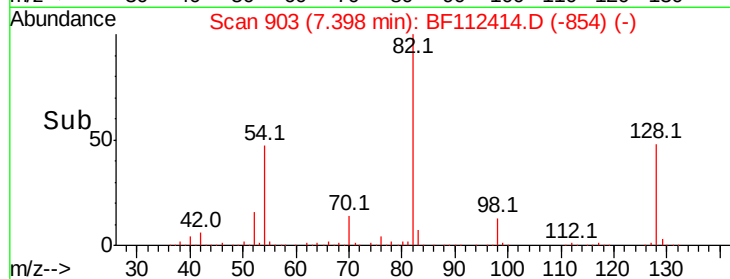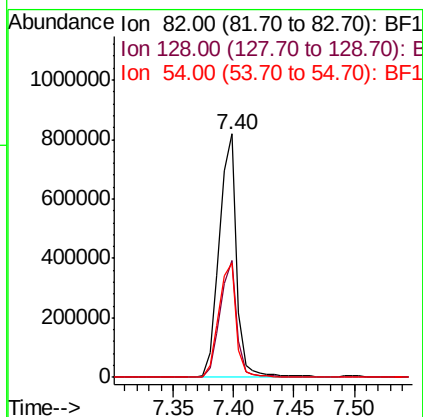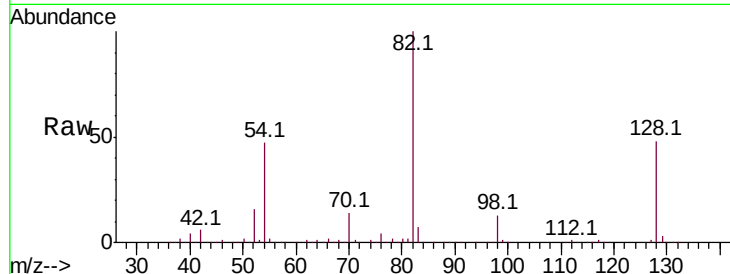

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.02 min
 Lab File: BF112414.D
 Acq: 5 Feb 2019 23:46

Tgt Ion	164	Resp	252731
Ion Ratio	Lower	Upper	
164	100		
162	101.6	82.2	123.4
160	45.6	36.2	54.4

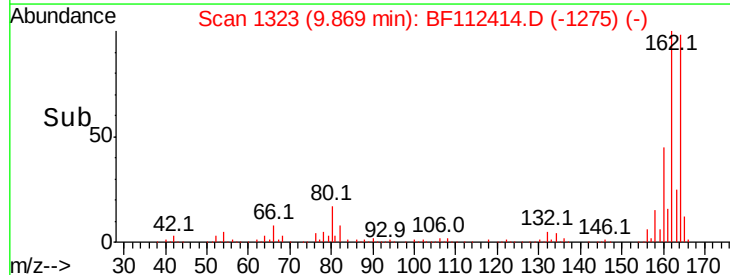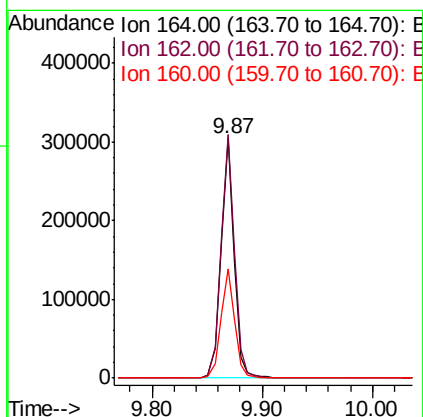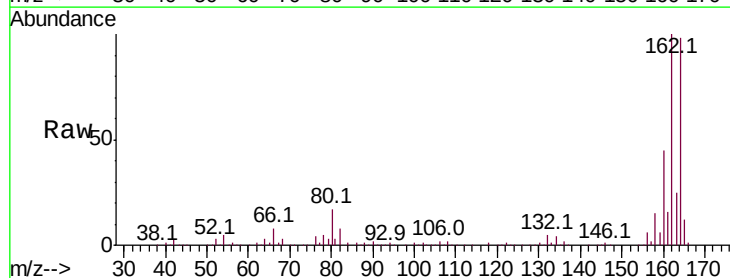

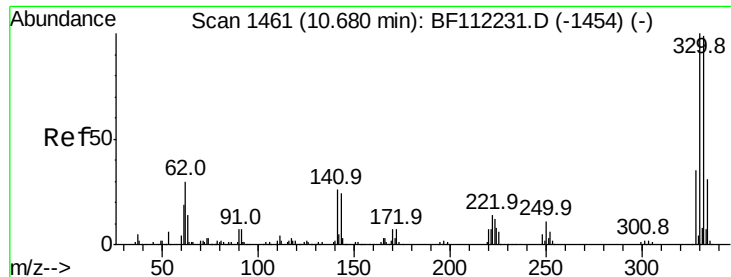

#42

2,4,6-Tribromophenol

Concen: 126.543 ng

RT: 10.66 min Scan# 1458

Delta R.T. -0.02 min

Lab File: BF112414.D

Acq: 5 Feb 2019 23:46

Instrument :

BNA_F

ClientSampleId :

HR-05-020419-C


Tot Ion:330 Resp: 372253

Ion Ratio Lower Upper




330 100

332 96.2 76.6 114.8

141 32.5 24.3 36.5

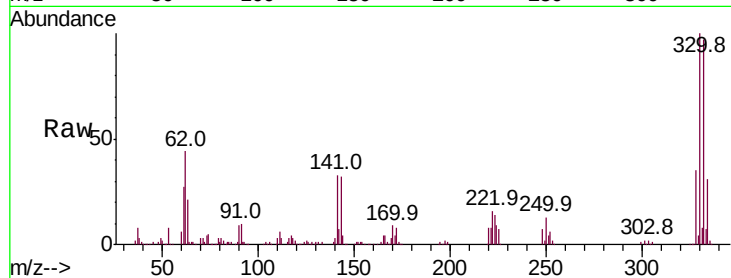

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

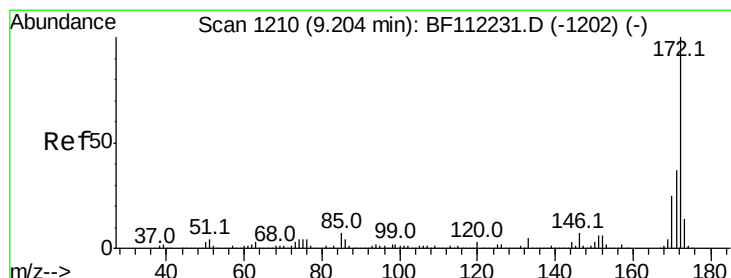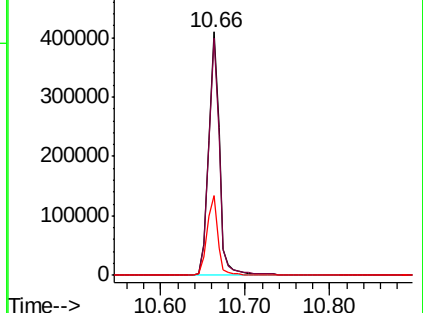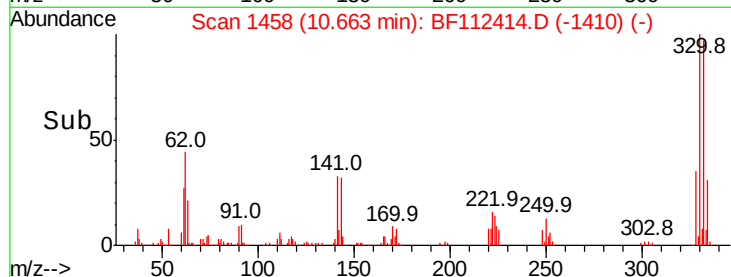

#45

2-Fluorobiphenyl

Concen: 89.915 ng

RT: 9.19 min Scan# 1207

Delta R.T. -0.02 min

Lab File: BF112414.D

Acq: 5 Feb 2019 23:46


Tgt Ion:172 Resp: 1606710

Ion Ratio Lower Upper



172 100


171 36.8 30.5 45.7

170 24.4 20.2 30.4

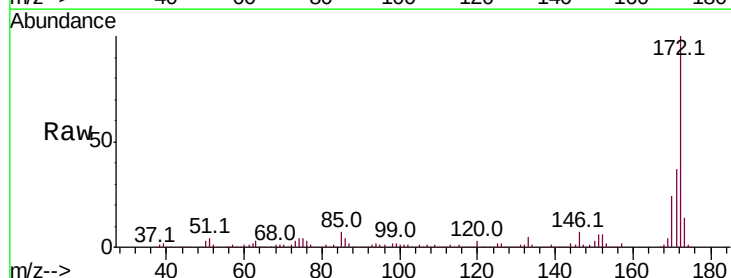

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



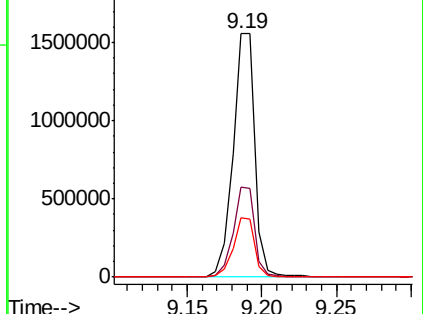
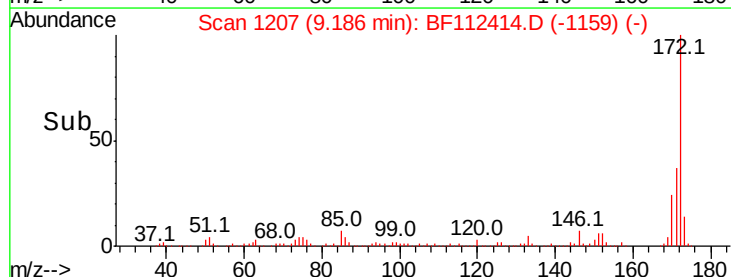


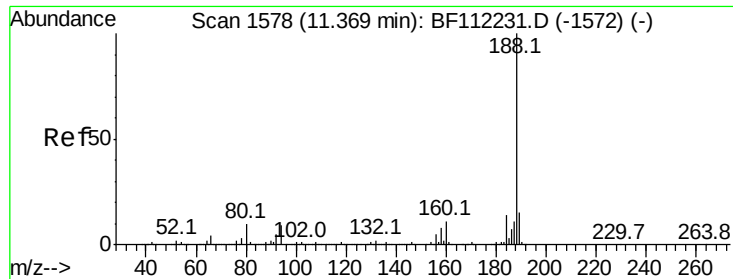

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112414.D
Acq: 5 Feb 2019 23:46




Instrument :
BNA_F
ClientSampleId :
HR-05-020419-C


Tot Ion:188 Resp: 441502
Ion Ratio Lower Upper
188 100
94 8.4 8.2 12.2
80 8.7 8.9 13.3#

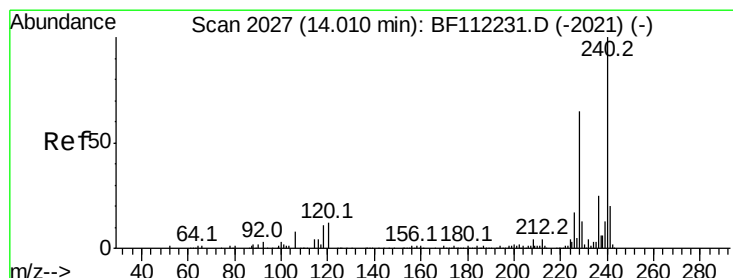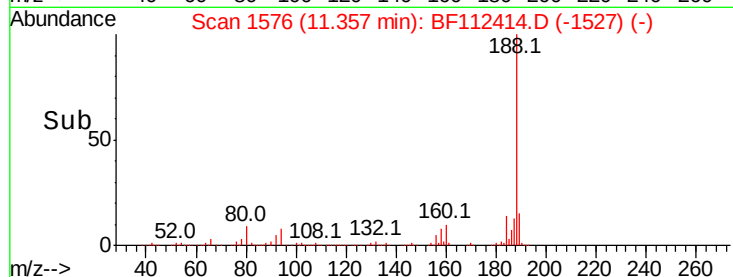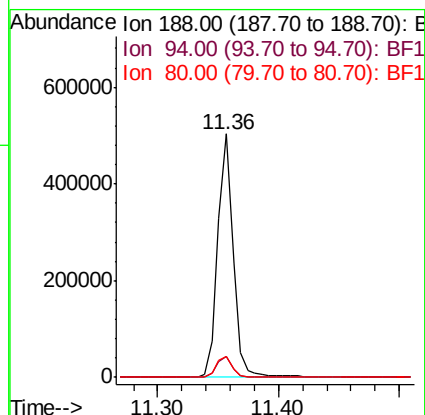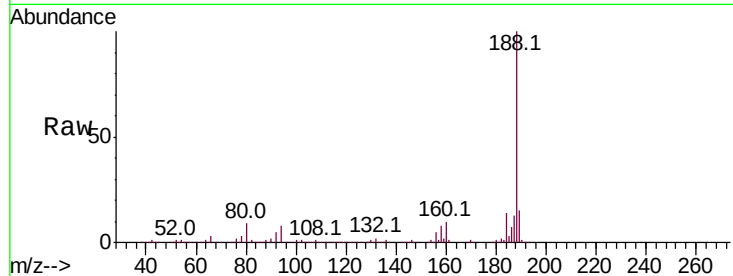

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112414.D
Acq: 5 Feb 2019 23:46

Tgt Ion:240 Resp: 309143
Ion Ratio Lower Upper
240 100
120 11.5 9.0 13.6
236 25.5 20.7 31.1

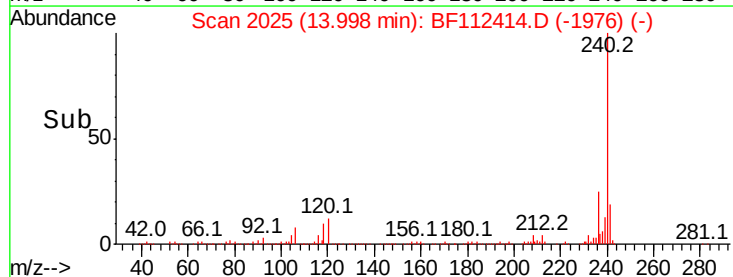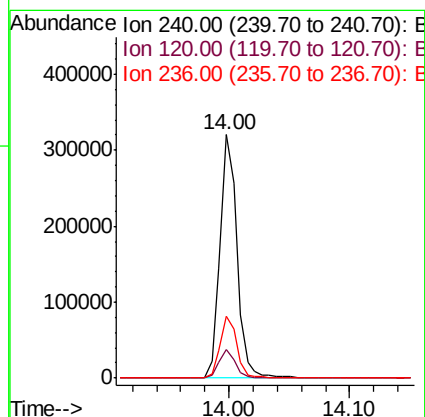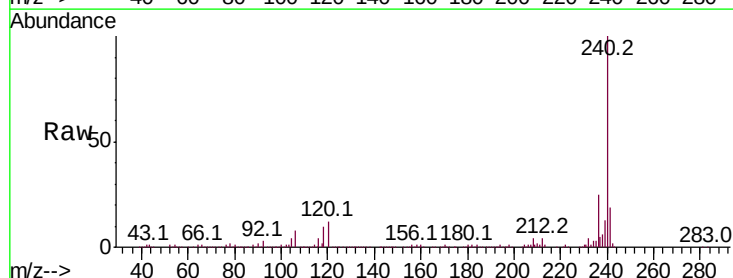

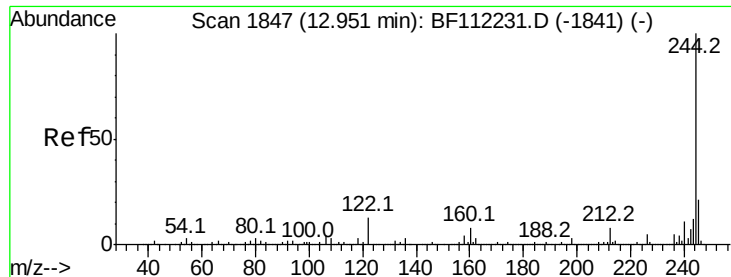

#79

Terphenyl-d14

Concen: 91.136 ng

RT: 12.94 min Scan# 1845

Delta R.T. -0.01 min

Lab File: BF112414.D

Acq: 5 Feb 2019 23:46

Instrument :

BNA_F

ClientSampleId :

HR-05-020419-C


Tot Ion:244 Resp: 1495877

Ion Ratio Lower Upper

244 100

212 7.0 5.9 8.9




122 11.9 9.8 14.6

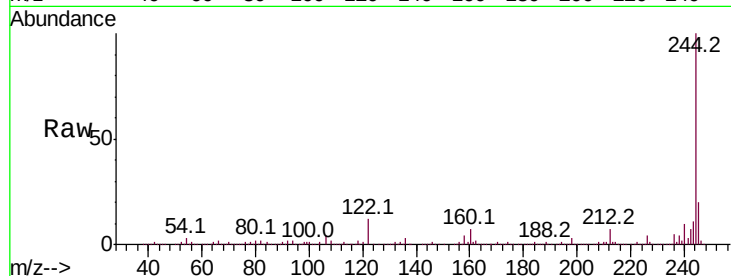

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

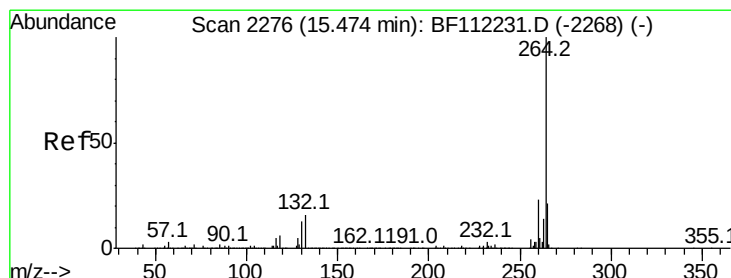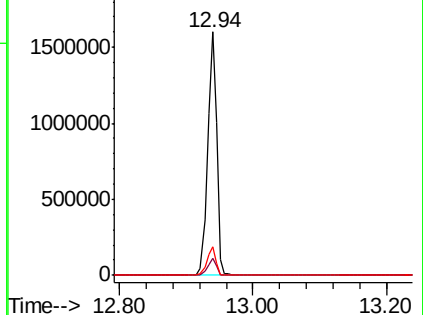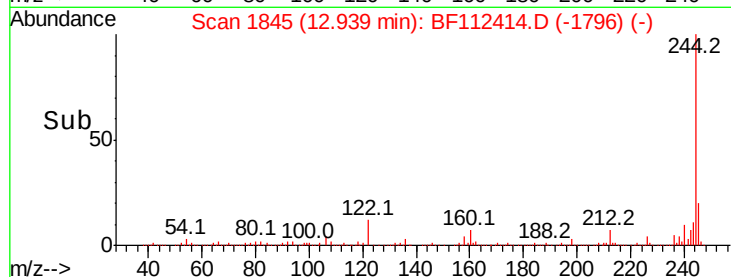

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.47 min Scan# 2275

Delta R.T. -0.01 min

Lab File: BF112414.D

Acq: 5 Feb 2019 23:46


Tgt Ion:264 Resp: 276177

Ion Ratio Lower Upper

264 100

260 22.1 18.2 27.2

265 21.2 17.0 25.4

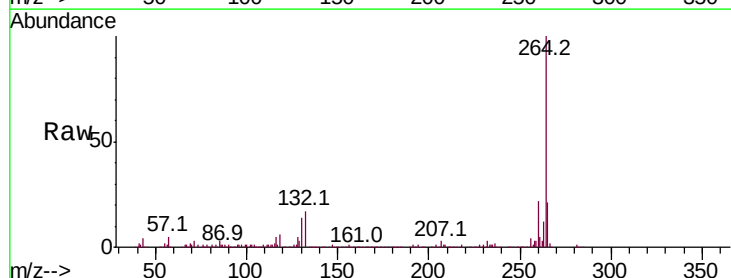

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

