
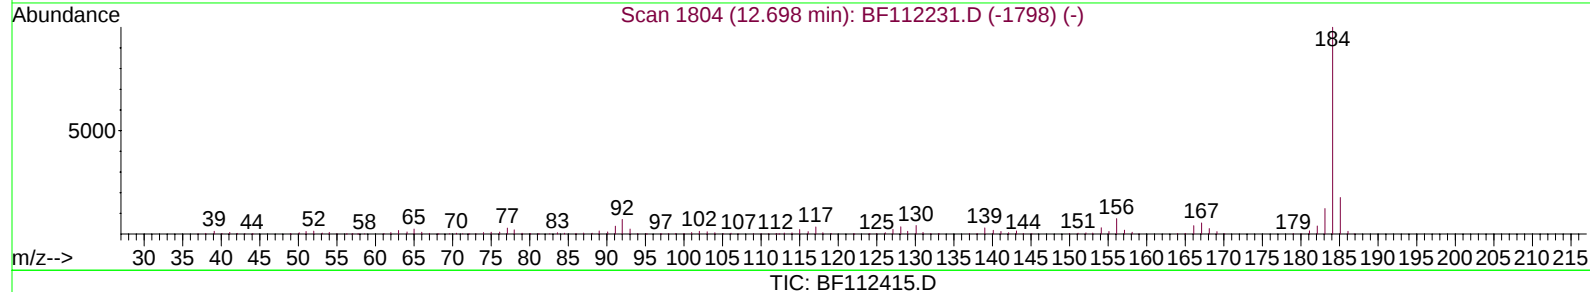
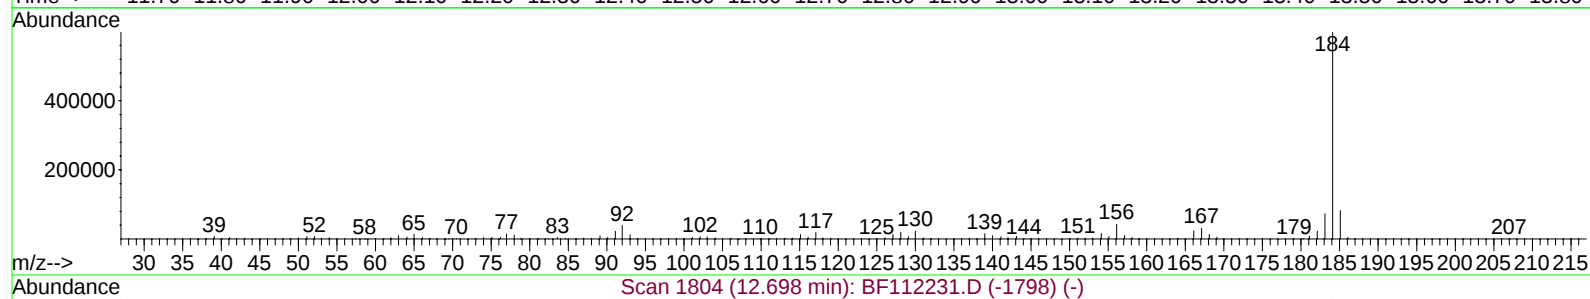


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020619\
 Data File : BF112415.D
 Acq On : 6 Feb 2019 12:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 16:00:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

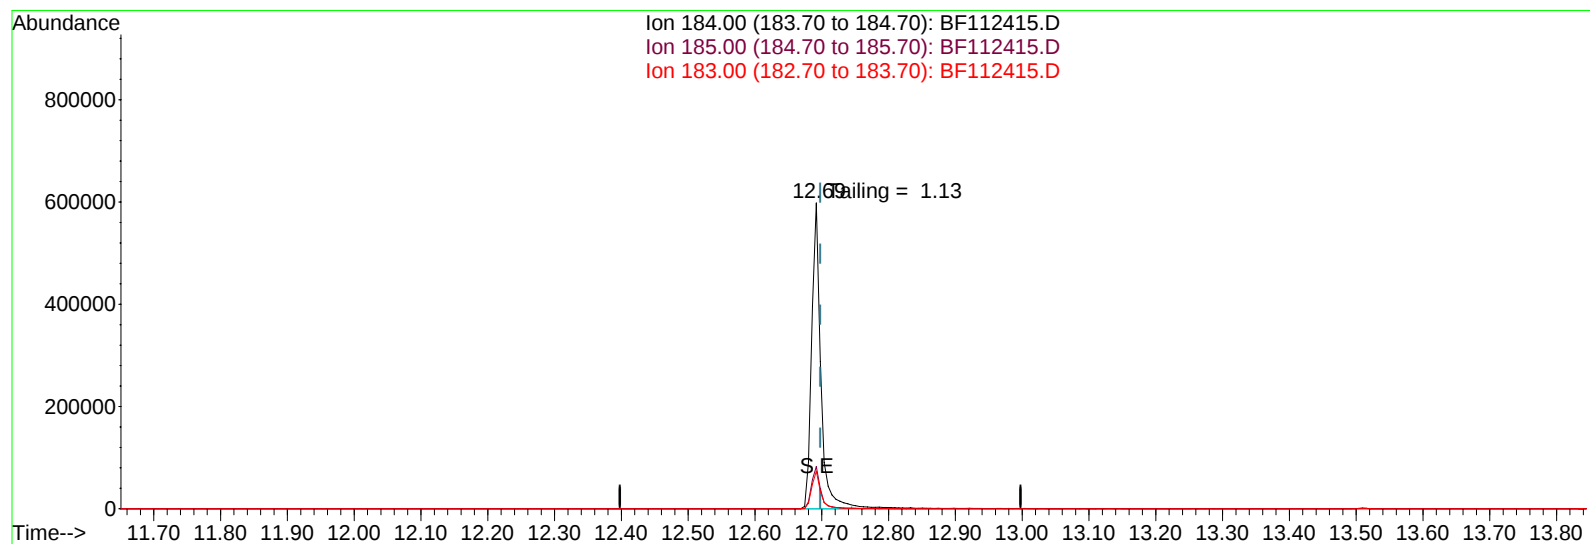

(77) Benzidine




12.692min (-0.006) 83119.29ng

response 581083

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	13.81#
183.00	12.50	12.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020619\
Data File : BF112415.D
Acq On : 6 Feb 2019 12:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 16:00:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

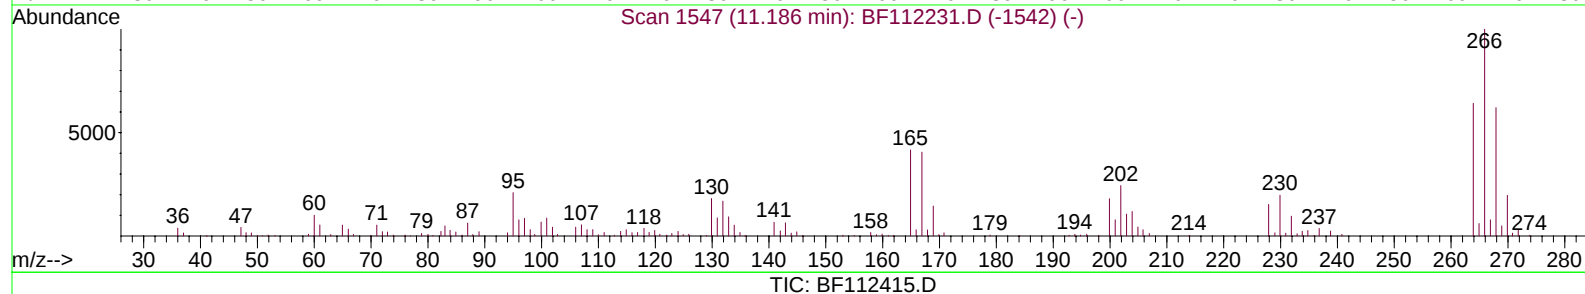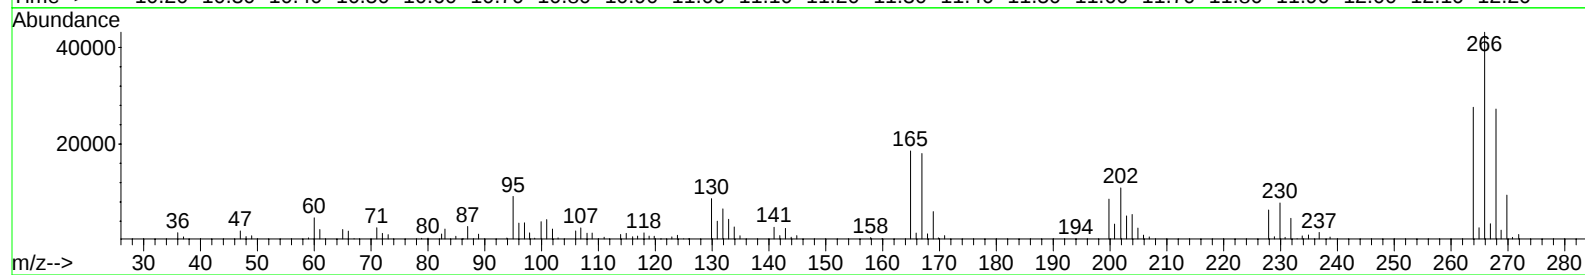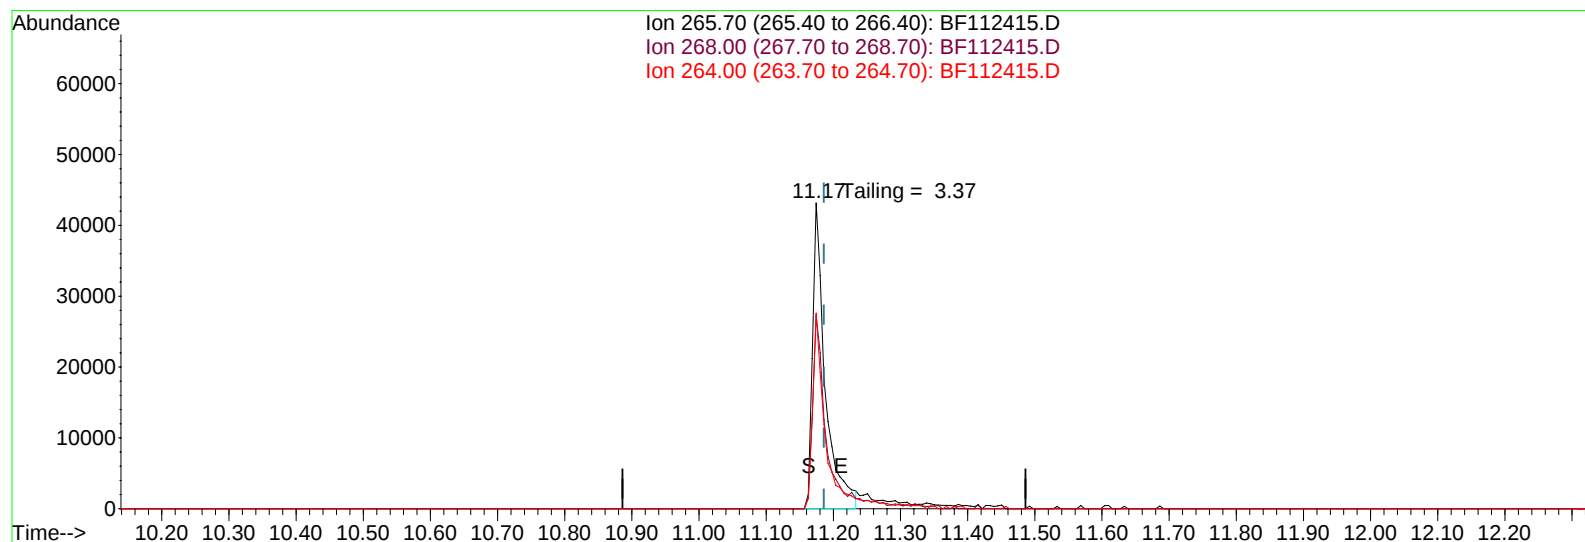

(70) Pentachlorophenol (C)

11.174min (-0.012) 120056.98ng

response 63074

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.15
264.00	63.60	64.00
0.00	0.00	0.00