

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020619\
 Data File : BF112420.D
 Acq On : 6 Feb 2019 15:19
 Operator : JU/SJ
 Sample : K1338-05 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-C

Quant Time: Feb 06 16:19:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	150719	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	613031	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	288928	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	512488	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	324626	20.00	ng	-0.01
87) Perylene-d12	15.47	264	331131	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	177753	25.05	ng	-0.02
7) Phenol-d6	6.48	99	232809	23.61	ng	-0.01
23) Nitrobenzene-d5	7.39	82	143074	13.45	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	66455	19.76	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	273090	13.37	ng	-0.02
79) Terphenyl-d14	12.94	244	219018	12.71	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020619\
Data File : BF112420.D
Acq On : 6 Feb 2019 15:19
Operator : JU/SJ
Sample : K1338-05 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AU-06-020519-C

Quant Time: Feb 06 16:19:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

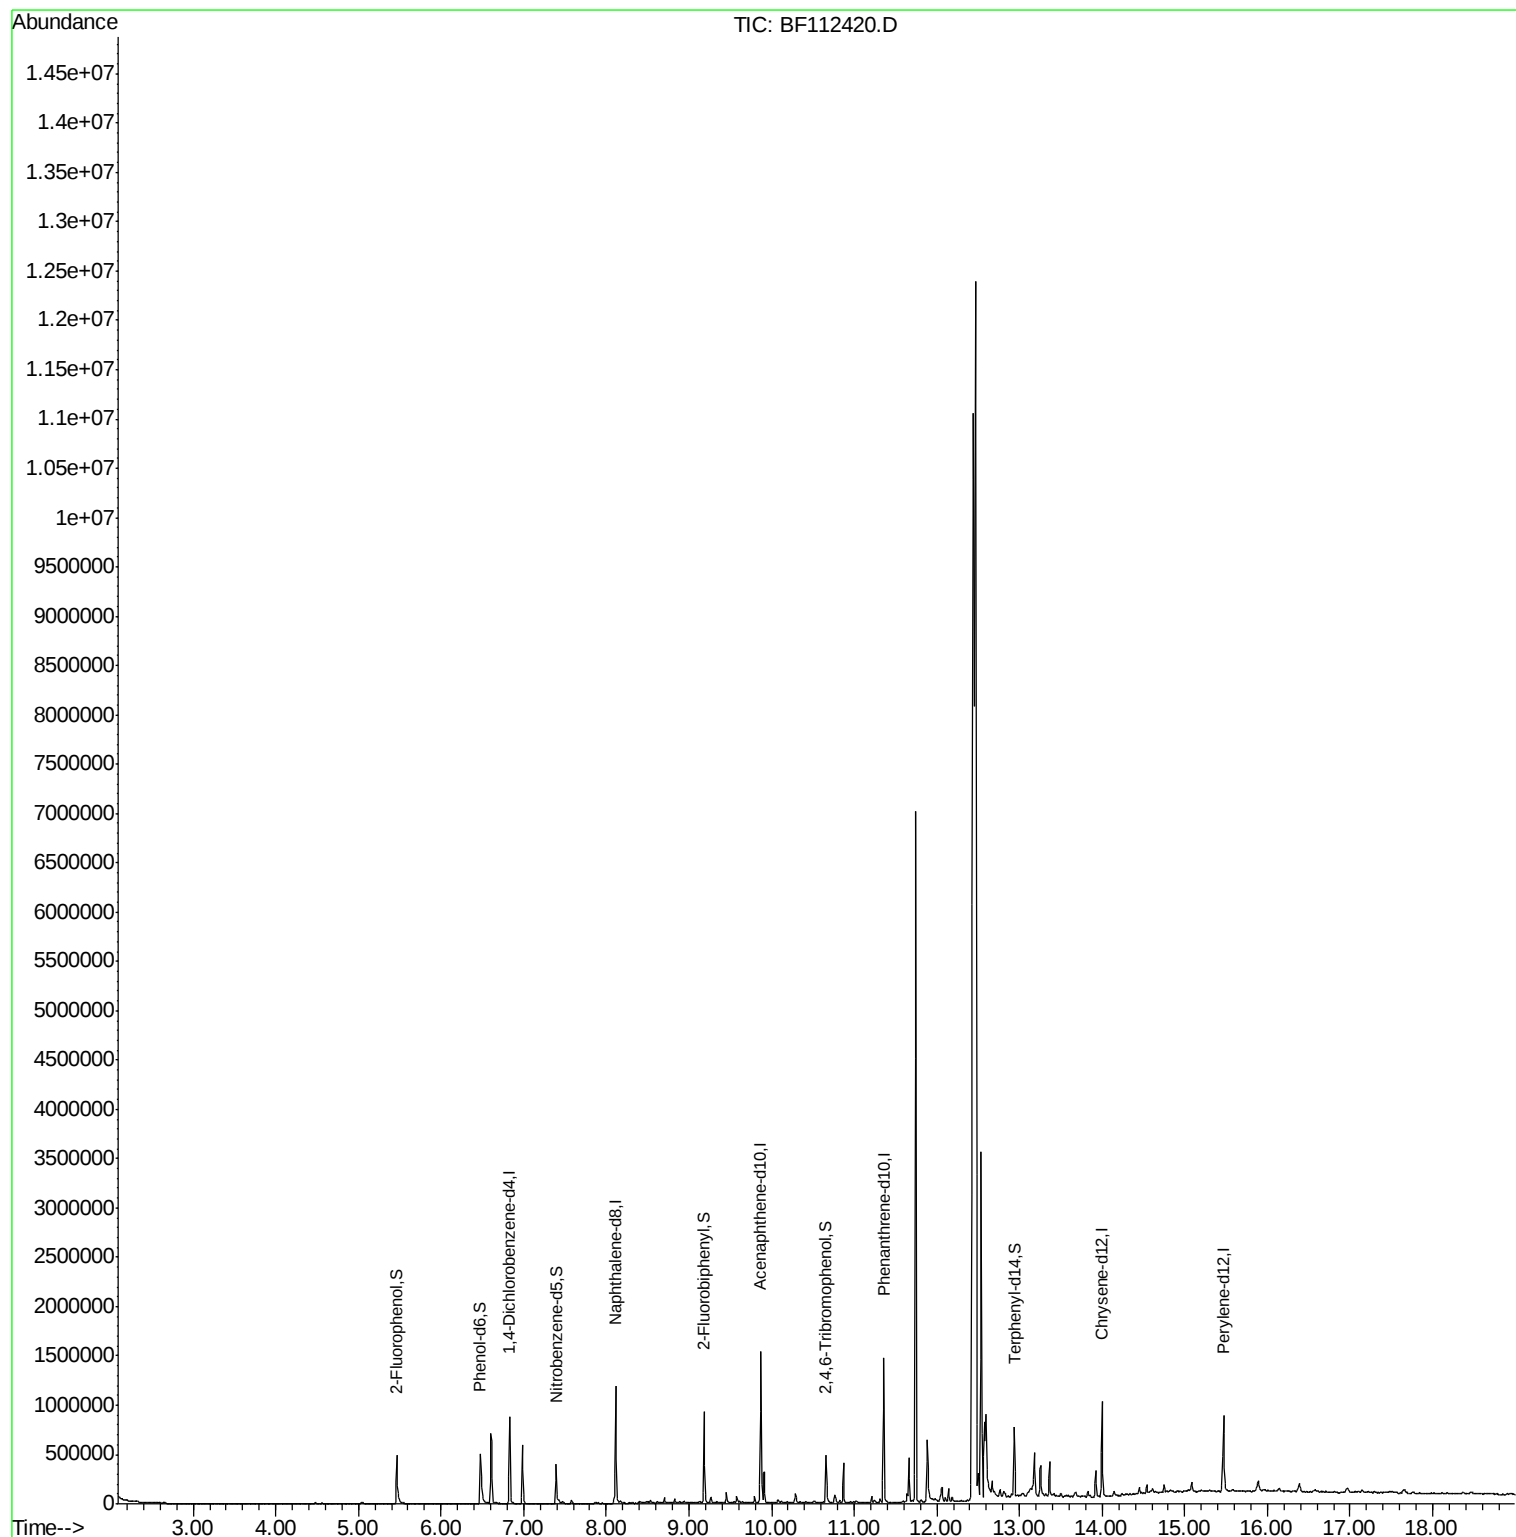

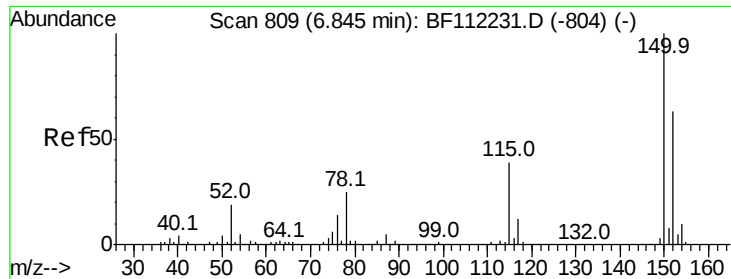


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF112420.D
Acq: 6 Feb 2019 15:19

Instrument :
BNA_F
ClientSampleId :
AU-06-020519-C

Tot Ion:152 Resp: 150719
Ion Ratio Lower Upper
152 100
150 154.2 127.4 191.0
115 57.5 45.5 68.3

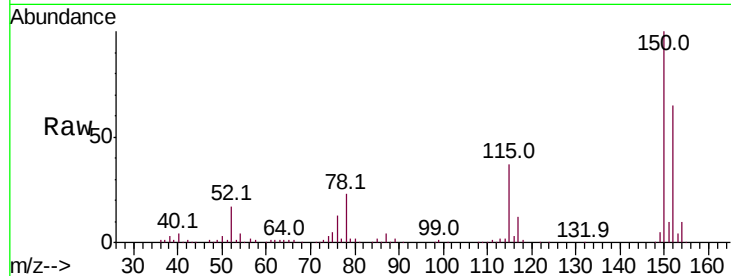


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

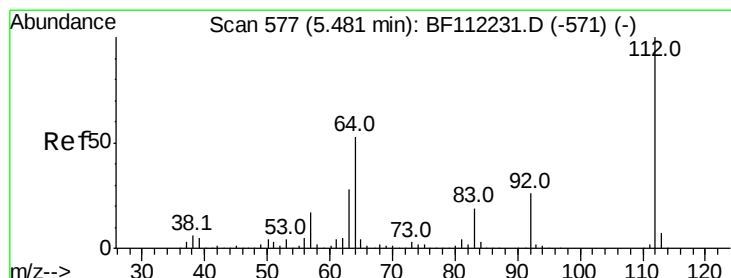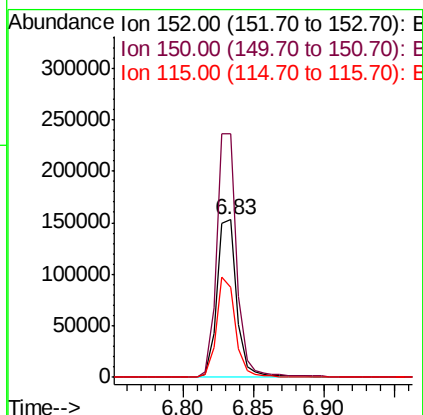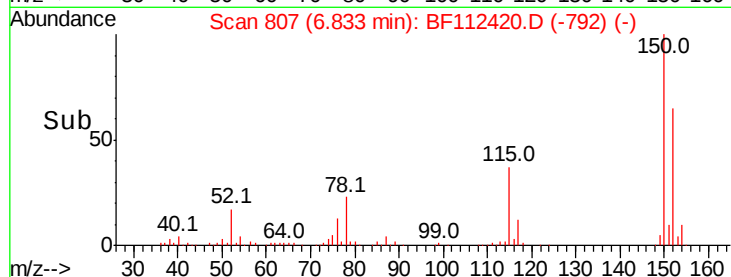



#5

2-Fluorophenol
Concen: 25.051 ng
RT: 5.46 min Scan# 574
Delta R.T. -0.02 min
Lab File: BF112420.D
Acq: 6 Feb 2019 15:19

Tgt Ion:112 Resp: 177753
Ion Ratio Lower Upper
112 100
64 53.7 45.7 68.5
63 29.4 23.6 35.4

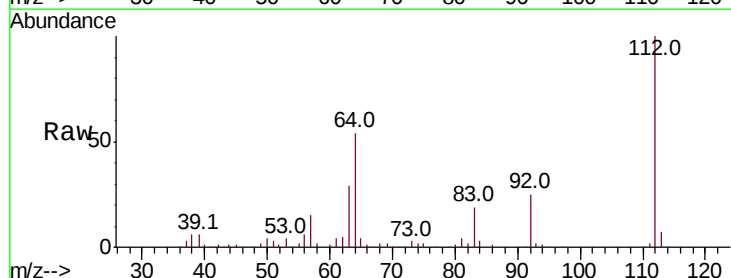

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

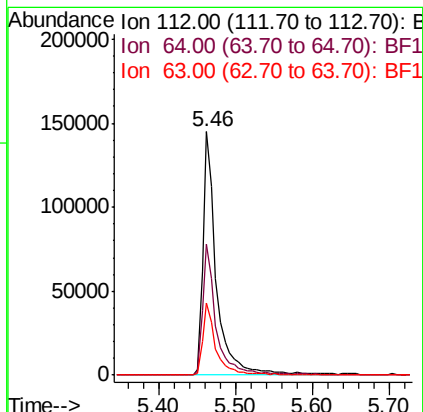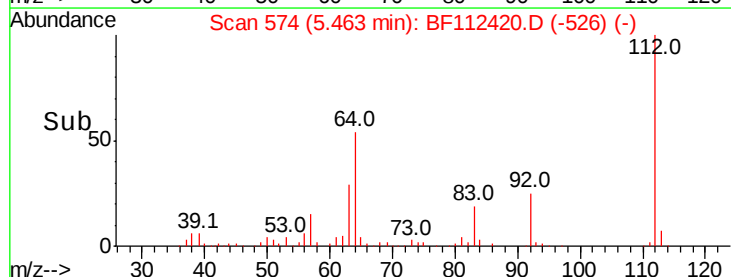



#7

Phenol-d6

Concen: 23.612 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF112420.D

Acq: 6 Feb 2019 15:19

Instrument :

BNA_F

ClientSampleId :

AU-06-020519-C


Tot Ion: 99 Resp: 232809

Ion Ratio Lower Upper




99 100

42 17.2 15.1 22.7

71 33.7 26.9 40.3

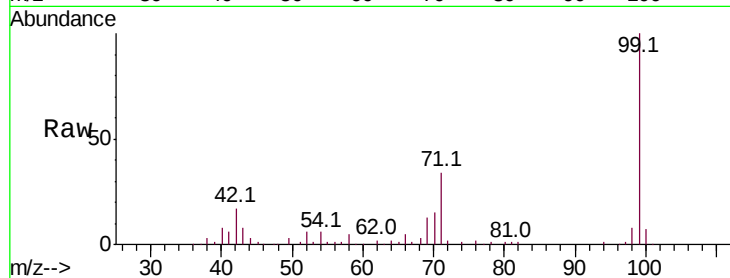

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

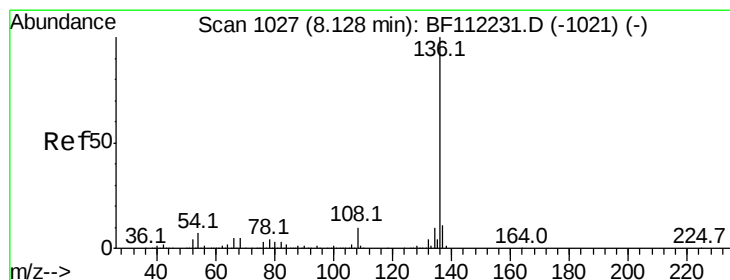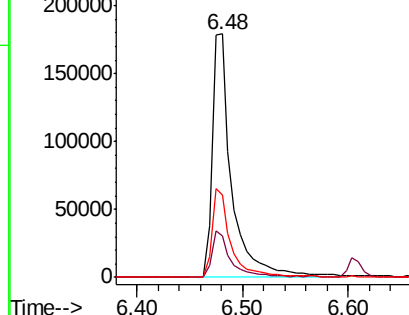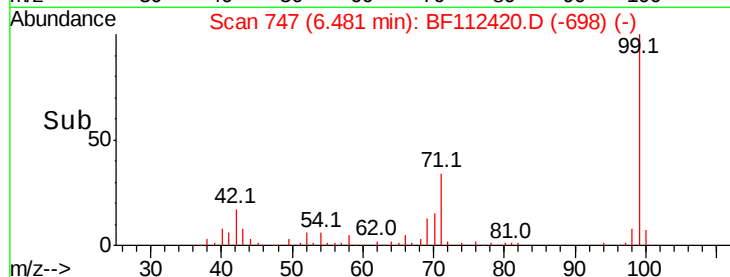

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112420.D

Acq: 6 Feb 2019 15:19

Tgt Ion: 136 Resp: 613031


Ion Ratio Lower Upper

136 100



137 10.4 9.1 13.7


54 5.9 5.9 8.9#

68 4.7 5.1 7.7#

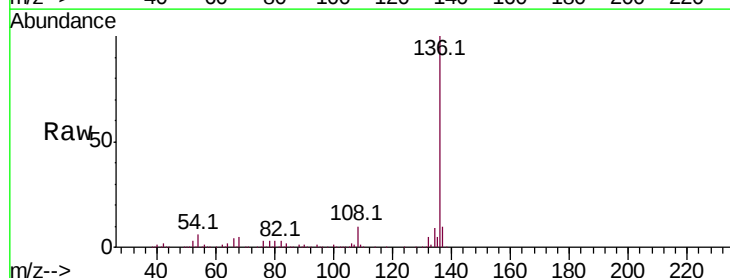

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

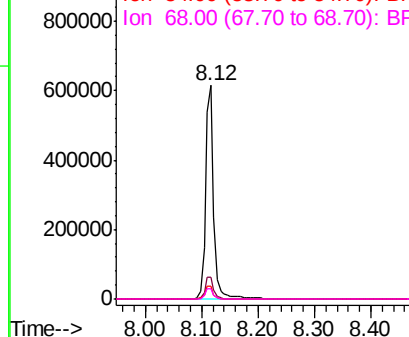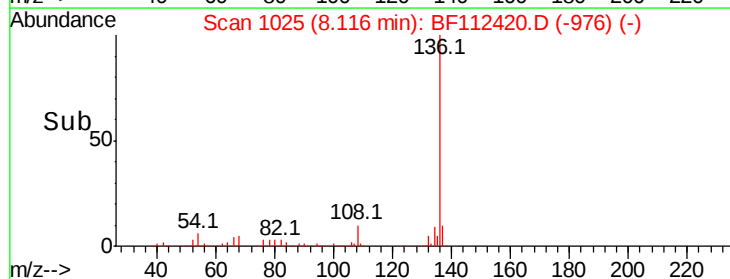


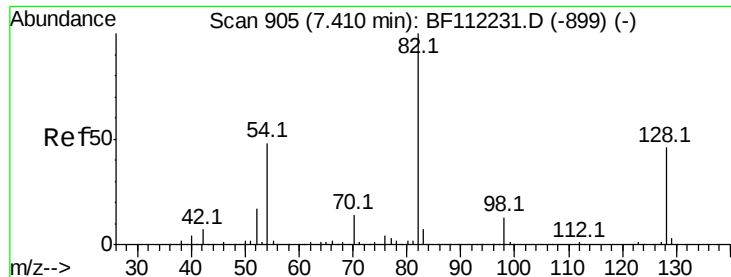




#23
 Nitrobenzene-d5
 Concen: 13.448 ng
 RT: 7.39 min Scan# 902
 Delta R.T. -0.02 min
 Lab File: BF112420.D
 Acq: 6 Feb 2019 15:19

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-C

Tot Ion: 82 Resp: 143074
 Ion Ratio Lower Upper
 82 100
 128 45.1 37.8 56.8
 54 46.1 39.7 59.5

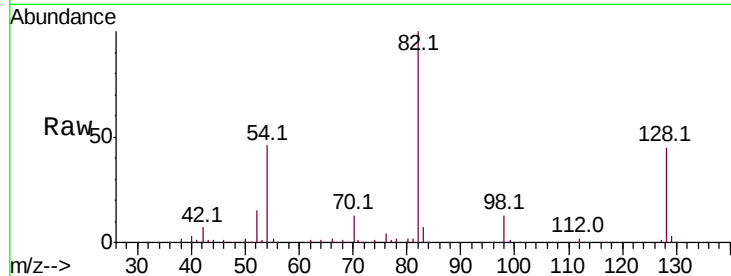


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

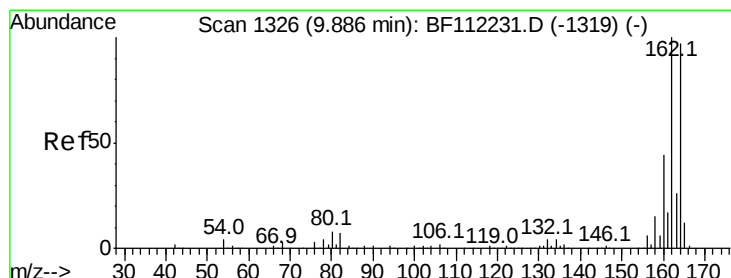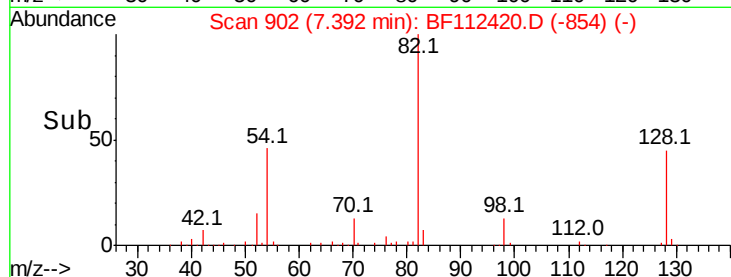
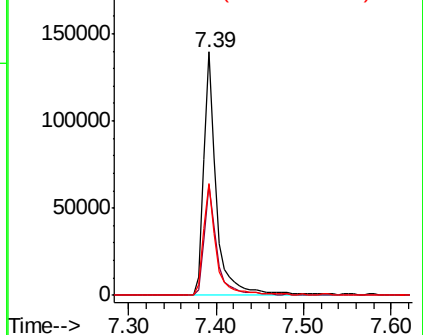


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.02 min
 Lab File: BF112420.D
 Acq: 6 Feb 2019 15:19

Tgt Ion: 164 Resp: 288928
 Ion Ratio Lower Upper
 164 100
 162 106.1 82.2 123.4
 160 47.3 36.2 54.4

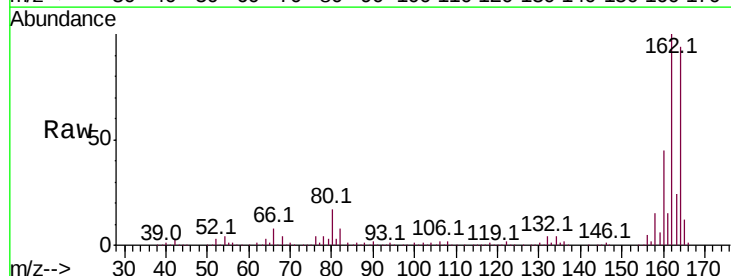

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

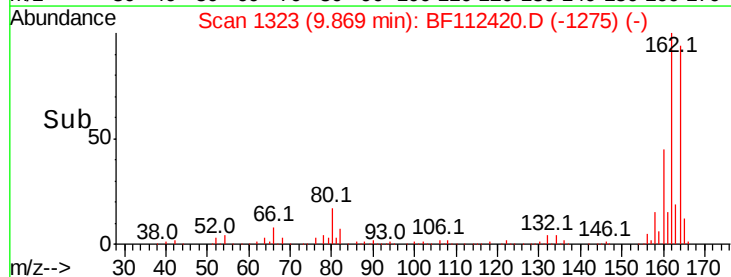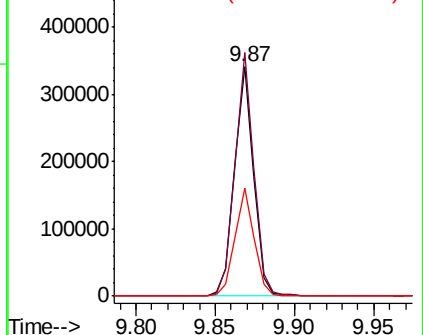







#42
 2,4,6-Tribromophenol
 Concen: 19.760 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.02 min
 Lab File: BF112420.D
 Acq: 6 Feb 2019 15:19

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-C

Tot Ion	Ratio	Lower	Upper
330	100		
332	99.1	76.6	114.8
141	33.3	24.3	36.5

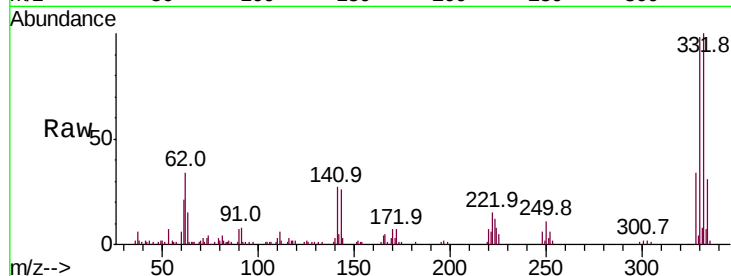


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

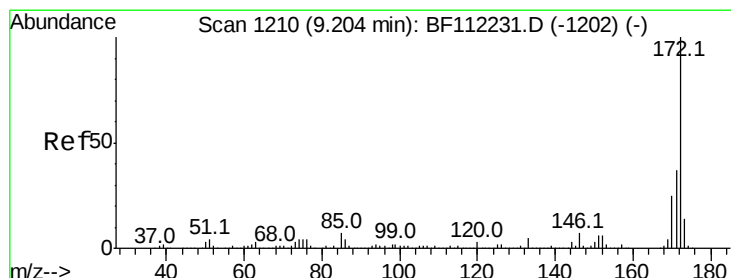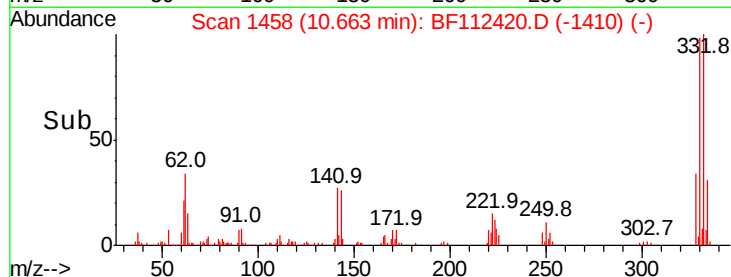
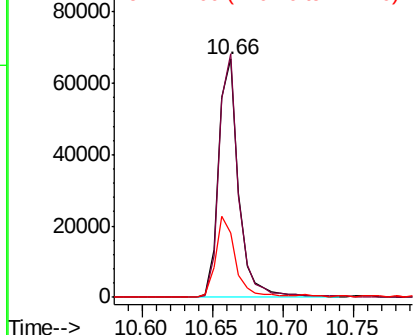


#45
 2-Fluorobiphenyl
 Concen: 13.368 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.02 min
 Lab File: BF112420.D
 Acq: 6 Feb 2019 15:19

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	30.5	45.7
170	23.4	20.2	30.4

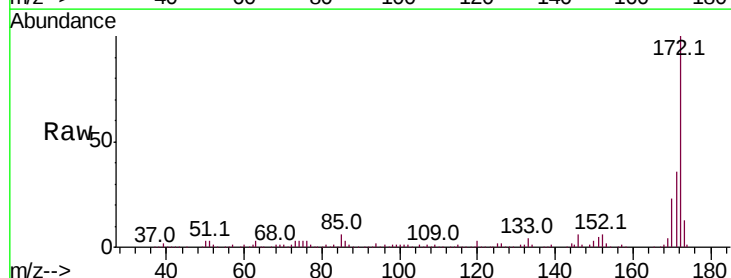

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

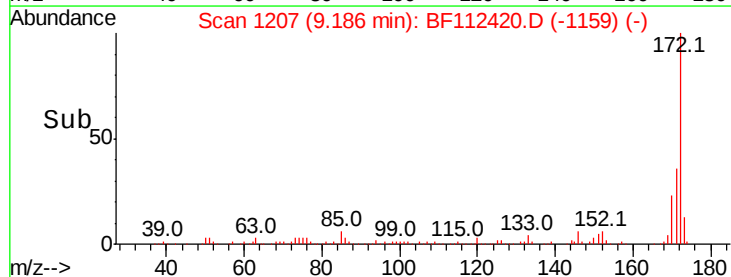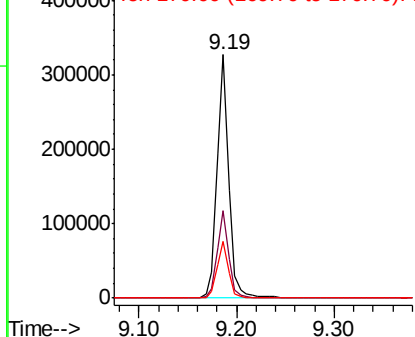



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.36 min Scan# 1576

Delta R.T. -0.01 min

Lab File: BF112420.D

Acq: 6 Feb 2019 15:19

Instrument :

BNA_F

ClientSampleId :

AU-06-020519-C





Tot Ion:188 Resp: 512488

Ion Ratio Lower Upper

188 100

94 8.0 8.2 12.2#

80 8.8 8.9 13.3#

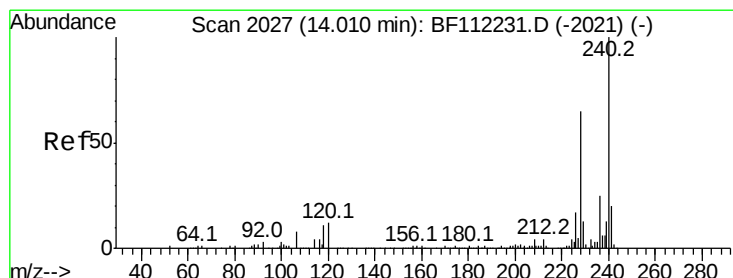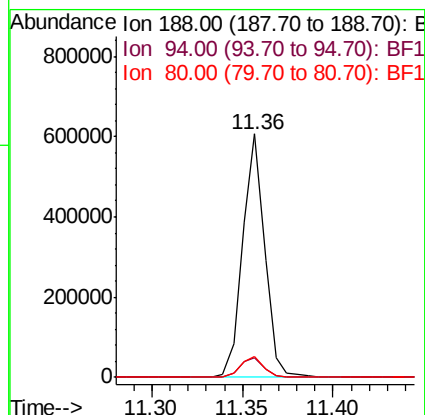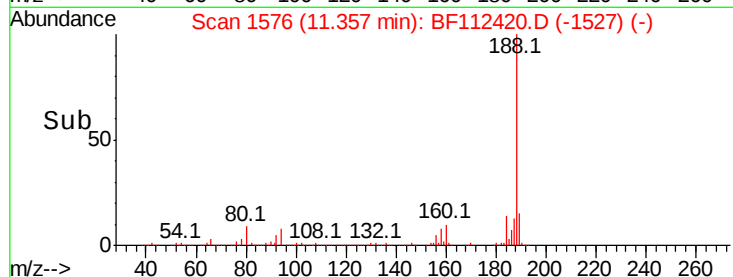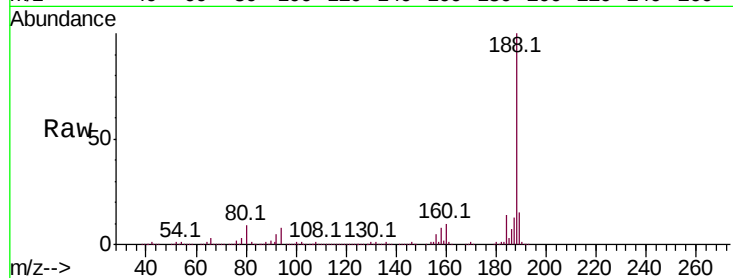

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.00 min Scan# 2025

Delta R.T. -0.01 min

Lab File: BF112420.D

Acq: 6 Feb 2019 15:19




Tgt Ion:240 Resp: 324626


Ion Ratio Lower Upper

240 100

120 11.9 9.0 13.6

236 24.9 20.7 31.1


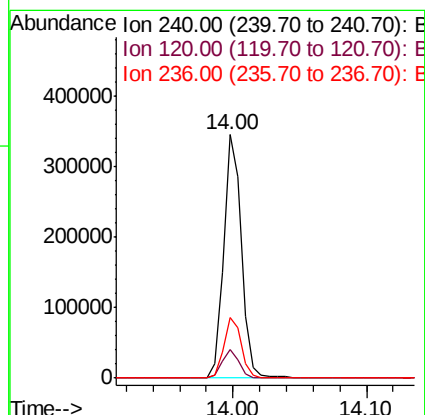
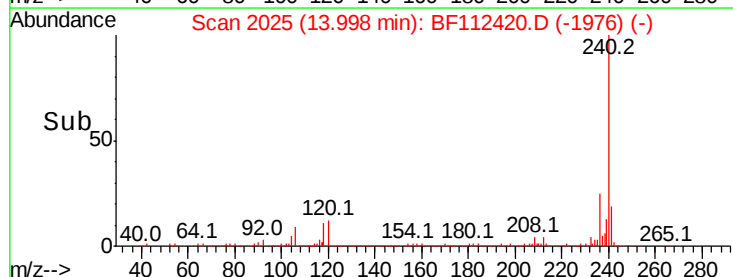
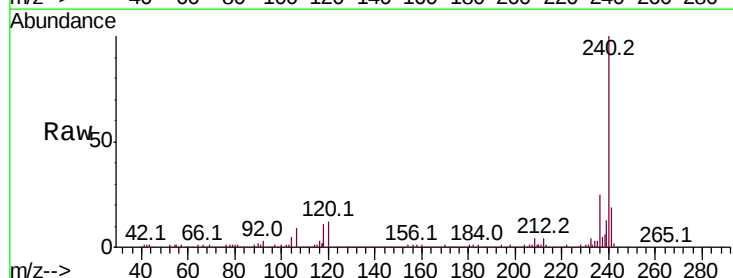


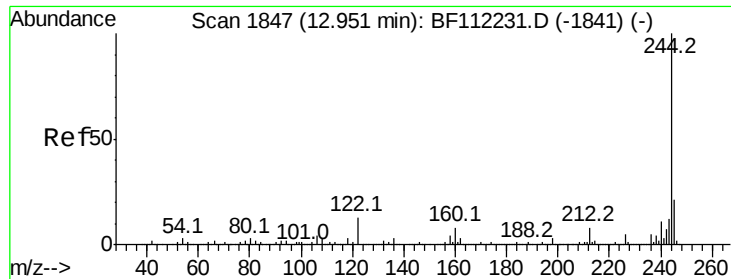

#79
 Terphenyl-d14
 Concen: 12.707 ng
 RT: 12.94 min Scan# 1845
 Delta R.T. -0.01 min
 Lab File: BF112420.D
 Acq: 6 Feb 2019 15:19

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-C

Tot Ion:244 Resp: 219018
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.9 8.9
 122 9.7 9.8 14.6#

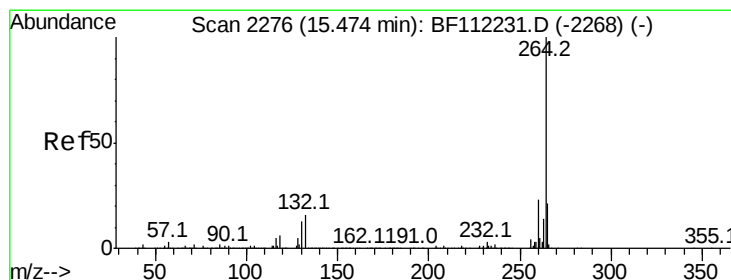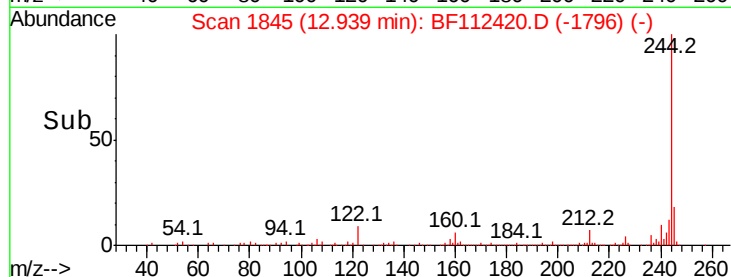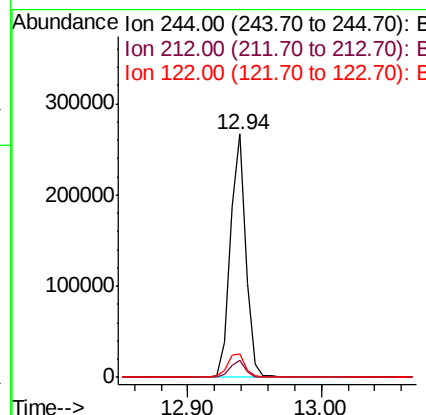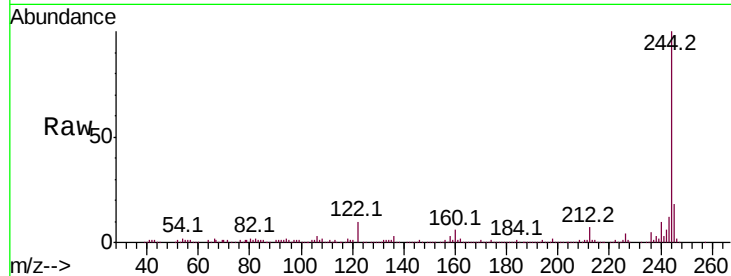

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2275
 Delta R.T. -0.01 min
 Lab File: BF112420.D
 Acq: 6 Feb 2019 15:19

Tgt Ion:264 Resp: 331131
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.2 27.2
 265 21.6 17.0 25.4

