

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020619\
 Data File : BF112425.D
 Acq On : 6 Feb 2019 17:37
 Operator : JU/SJ
 Sample : K1338-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-B

Quant Time: Feb 07 00:39:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	146364	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	547407	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	245907	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	388027	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	305109	20.00	ng	-0.01
87) Perylene-d12	15.47	264	292415	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	896289	130.07	ng	0.00
7) Phenol-d6	6.49	99	965425	100.83	ng	0.00
23) Nitrobenzene-d5	7.40	82	820885	86.41	ng	-0.01
42) 2,4,6-Tribromophenol	10.66	330	332324	116.10	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	1605862	92.36	ng	-0.01
79) Terphenyl-d14	12.94	244	1210877	74.75	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020619\
Data File : BF112425.D
Acq On : 6 Feb 2019 17:37
Operator : JU/SJ
Sample : K1338-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AU-06-020519-B

Quant Time: Feb 07 00:39:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

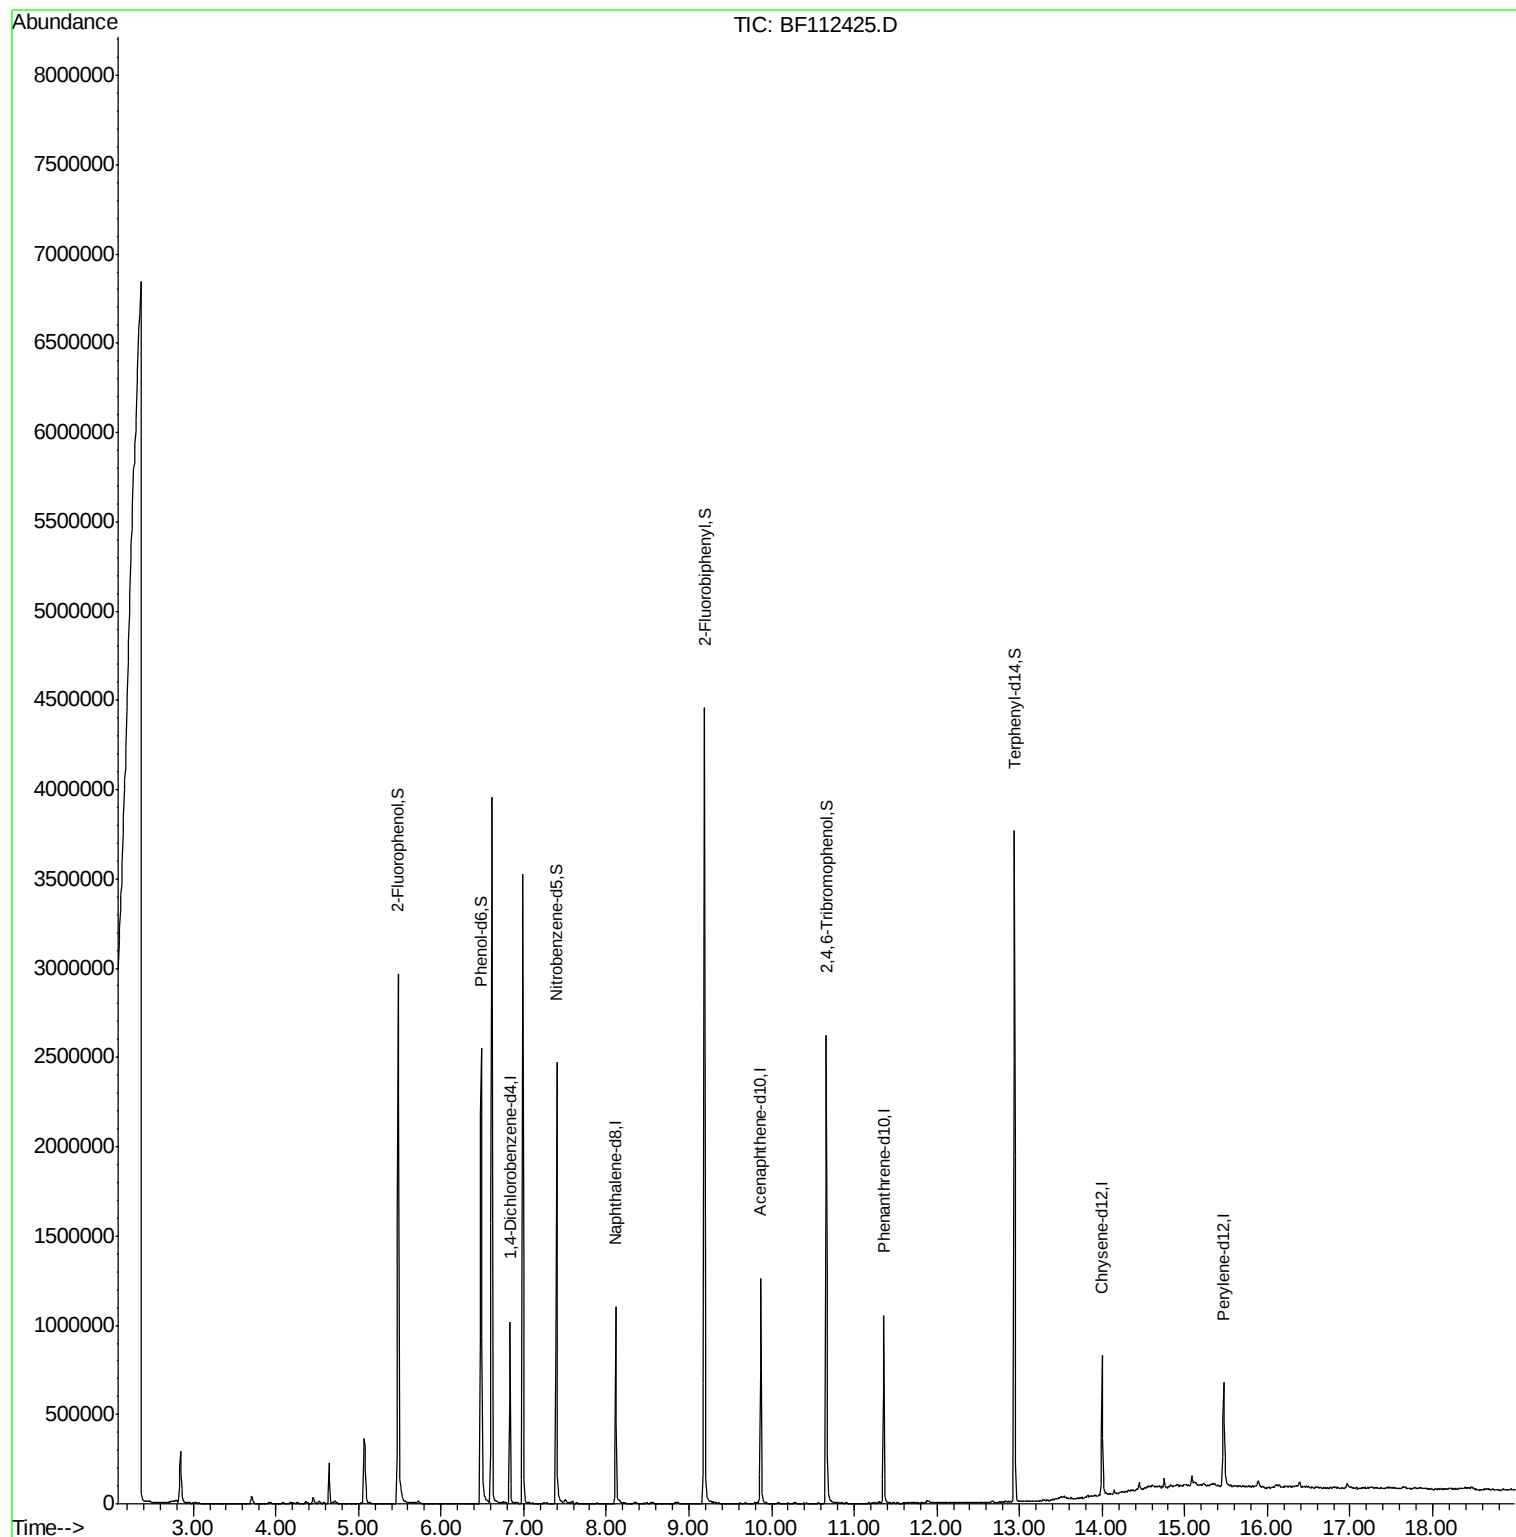




#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 807
 Delta R.T. -0.01 min
 Lab File: BF112425.D
 Acq: 6 Feb 2019 17:37

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-B

Tot Ion:152 Resp: 146364
 Ion Ratio Lower Upper
 152 100
 150 154.9 127.4 191.0
 115 59.6 45.5 68.3

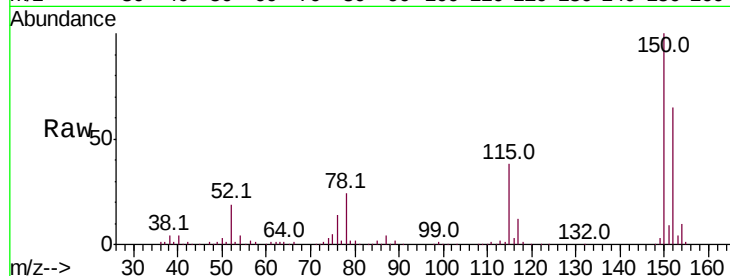


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

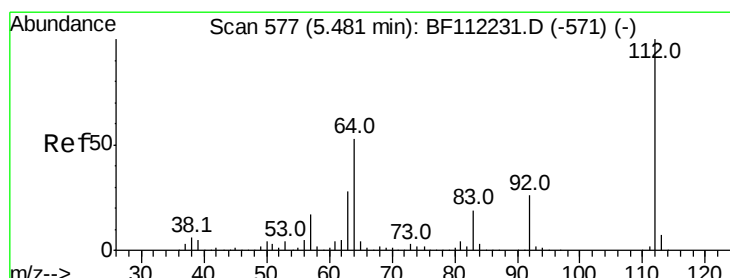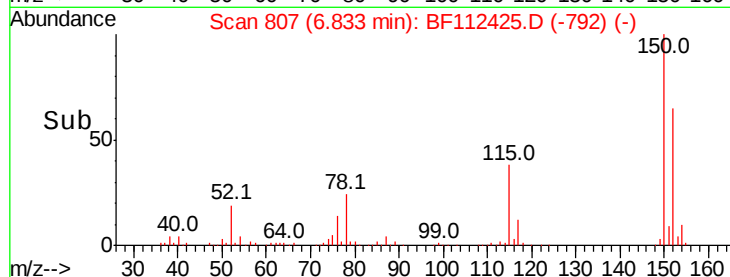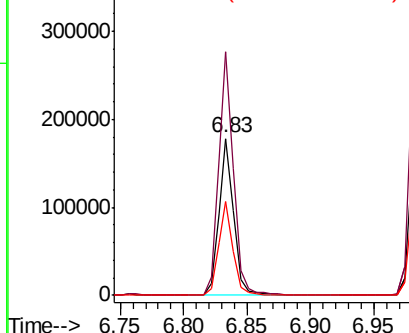



#5

2-Fluorophenol
 Concen: 130.071 ng
 RT: 5.48 min Scan# 577
 Delta R.T. -0.00 min
 Lab File: BF112425.D
 Acq: 6 Feb 2019 17:37

Tgt Ion:112 Resp: 896289
 Ion Ratio Lower Upper
 112 100
 64 56.2 45.7 68.5
 63 31.0 23.6 35.4

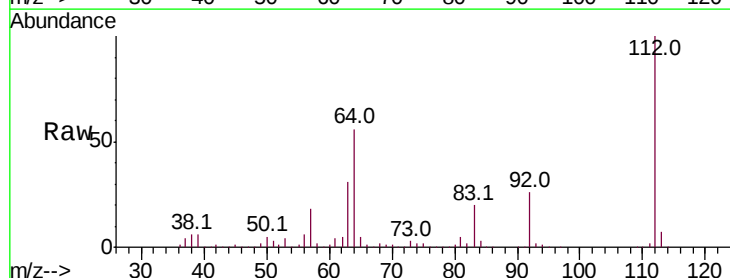

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

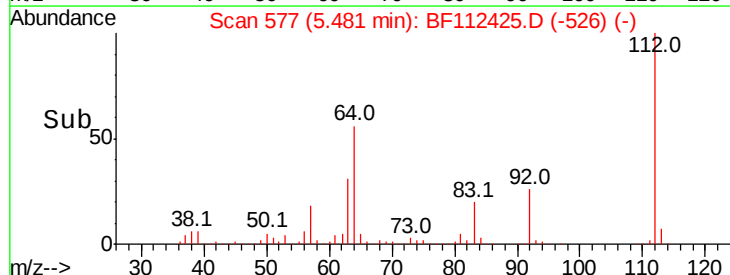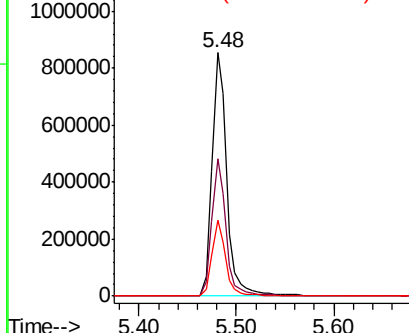



#7

Phenol-d6

Concen: 100.827 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112425.D

Acq: 6 Feb 2019 17:37

Instrument :

BNA_F

ClientSampleId :

AU-06-020519-B


Tot Ion: 99 Resp: 965425

Ion Ratio Lower Upper




99 100

42 18.0 15.1 22.7

71 35.6 26.9 40.3

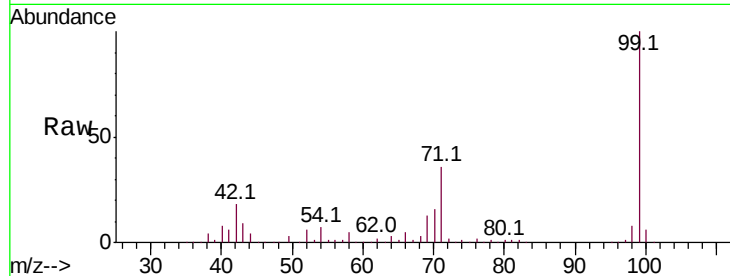

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

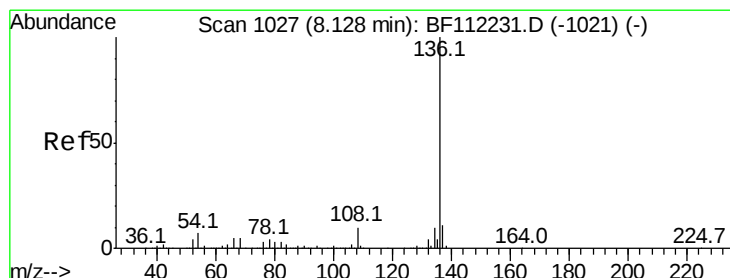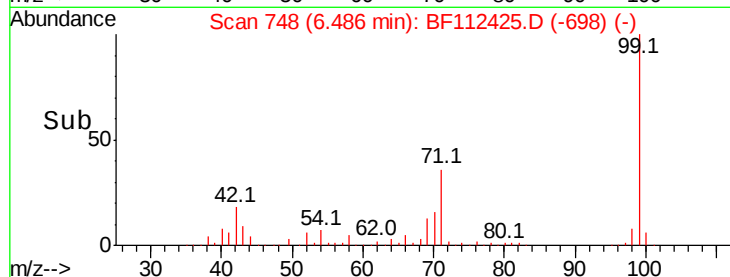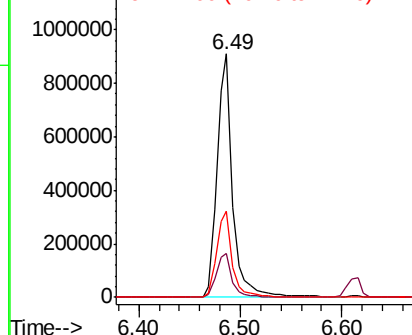

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112425.D

Acq: 6 Feb 2019 17:37

Tgt Ion: 136 Resp: 547407


Ion Ratio Lower Upper

136 100



137 10.5 9.1 13.7


54 6.4 5.9 8.9

68 4.8 5.1 7.7#

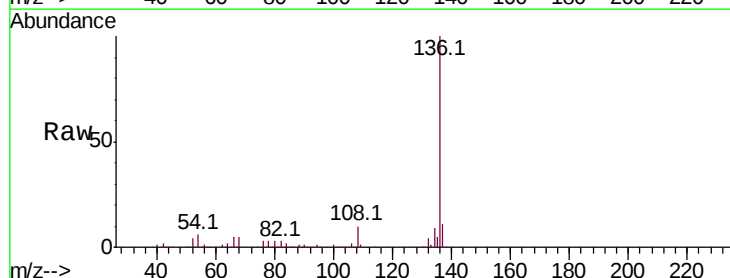

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

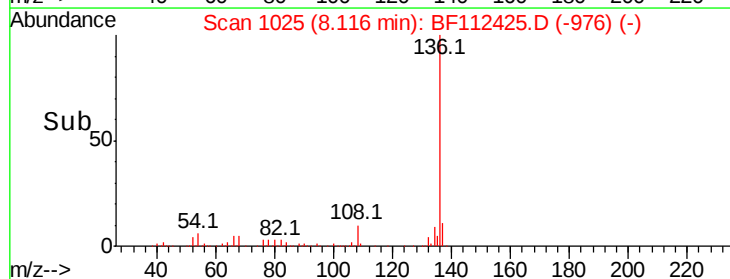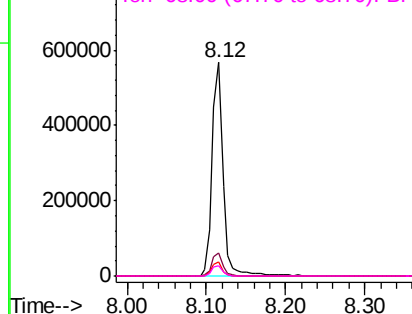


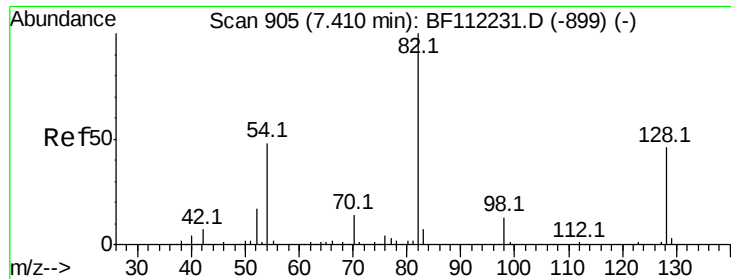




#23
Nitrobenzene-d5
Concen: 86.406 ng
RT: 7.40 min Scan# 903
Delta R.T. -0.01 min
Lab File: BF112425.D
Acq: 6 Feb 2019 17:37

Instrument :
BNA_F
ClientSampleId :
AU-06-020519-B

Tot Ion: 82 Resp: 820885
Ion Ratio Lower Upper
82 100
128 45.6 37.8 56.8
54 47.2 39.7 59.5

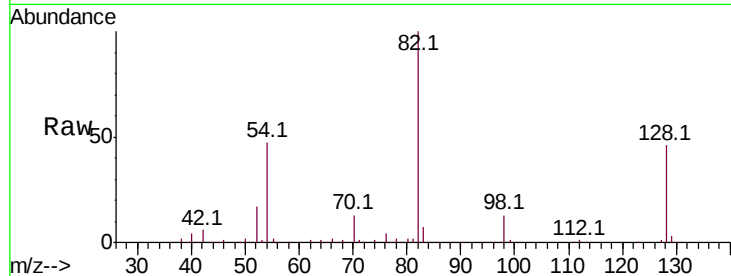


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

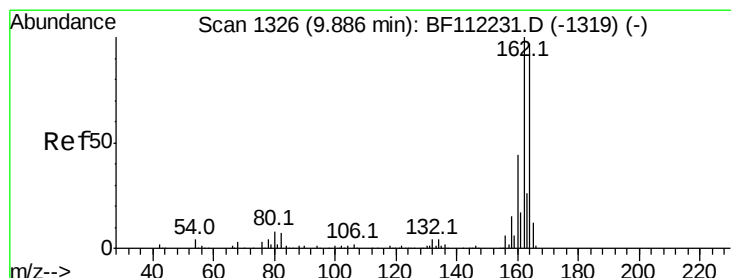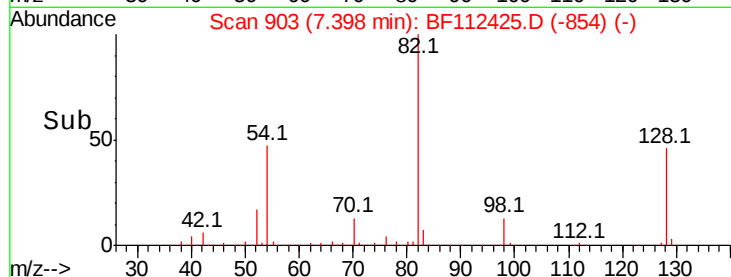
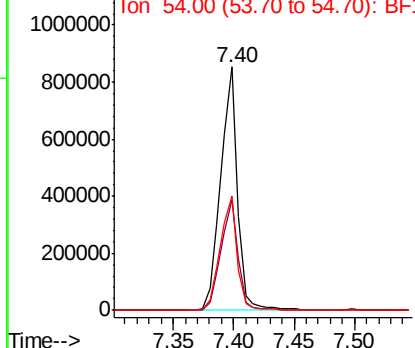


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.87 min Scan# 1323
Delta R.T. -0.02 min
Lab File: BF112425.D
Acq: 6 Feb 2019 17:37

Tgt Ion:164 Resp: 245907
Ion Ratio Lower Upper
164 100
162 106.5 82.2 123.4
160 46.7 36.2 54.4

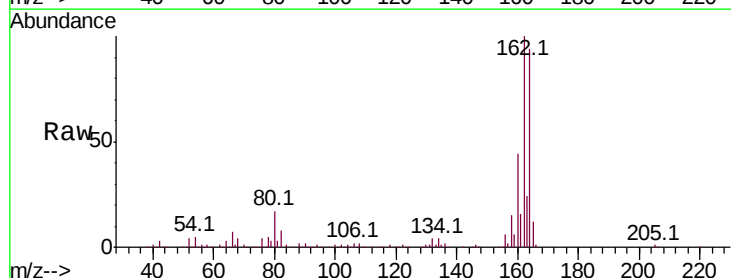

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

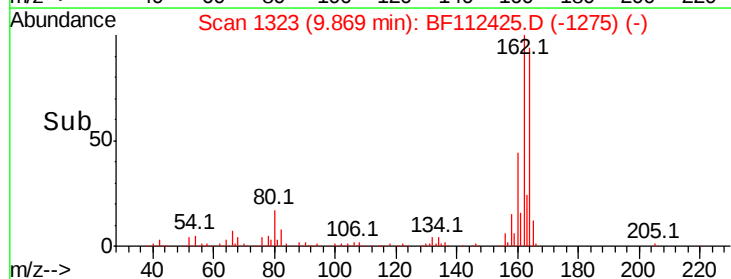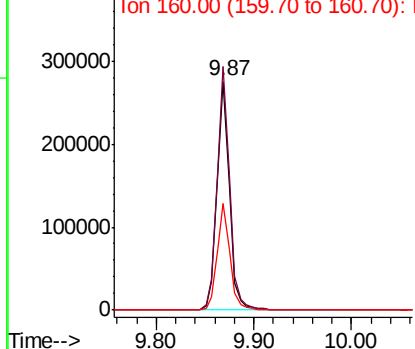




#42
 2,4,6-Tribromophenol
 Concen: 116.104 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.02 min
 Lab File: BF112425.D
 Acq: 6 Feb 2019 17:37

Instrument :
 BNA_F
 ClientSampleId :
 AU-06-020519-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	76.6	114.8
141	32.9	24.3	36.5



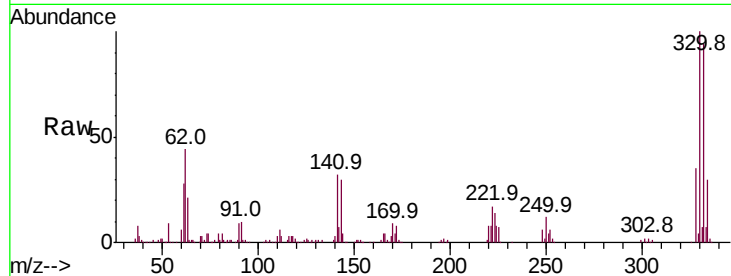


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

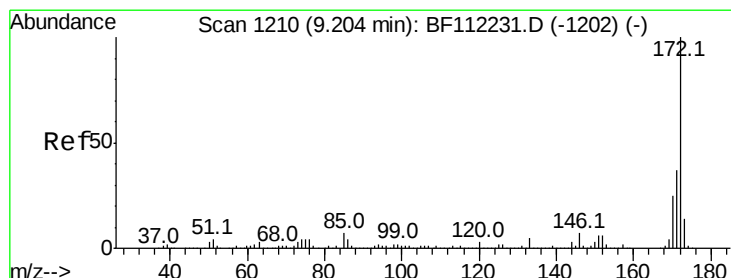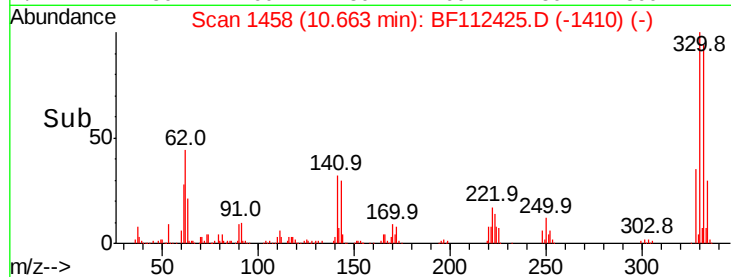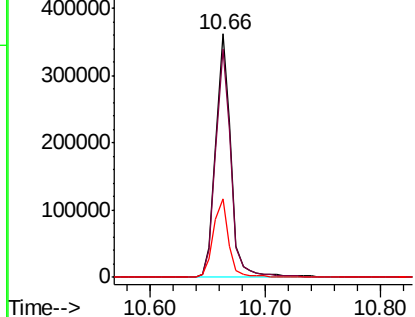

#45
 2-Fluorobiphenyl
 Concen: 92.361 ng
 RT: 9.19 min Scan# 1208
 Delta R.T. -0.01 min
 Lab File: BF112425.D
 Acq: 6 Feb 2019 17:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	30.5	45.7
170	24.3	20.2	30.4


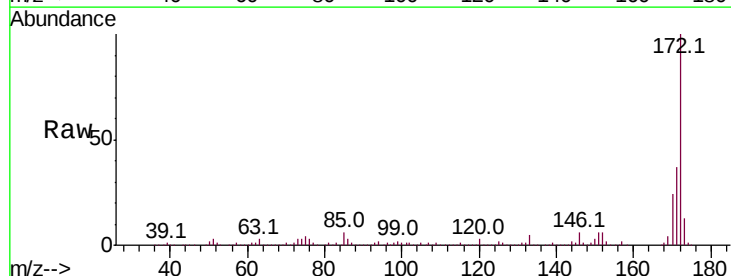



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



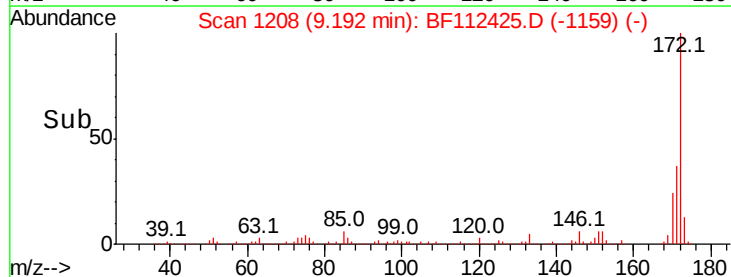
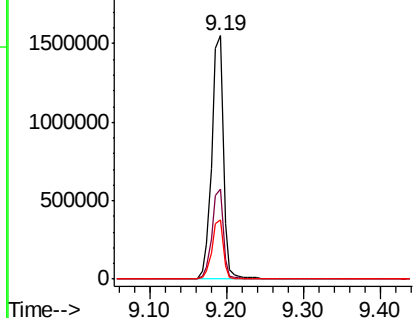


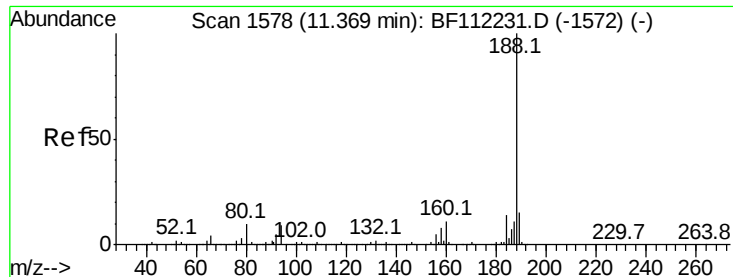

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112425.D
Acq: 6 Feb 2019 17:37




Instrument :
BNA_F
ClientSampleId :
AU-06-020519-B


Tot Ion	Ratio	Lower	Upper
188	100		
94	8.3	8.2	12.2
80	9.2	8.9	13.3

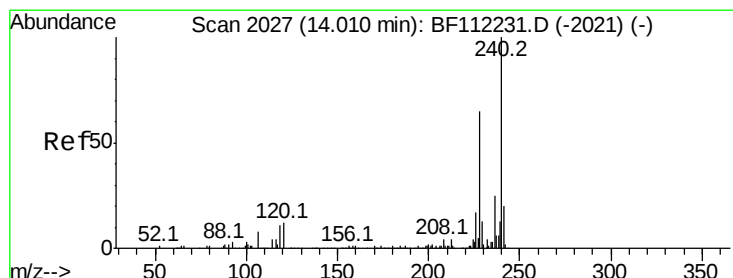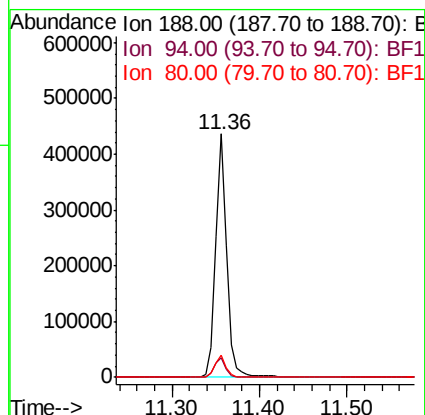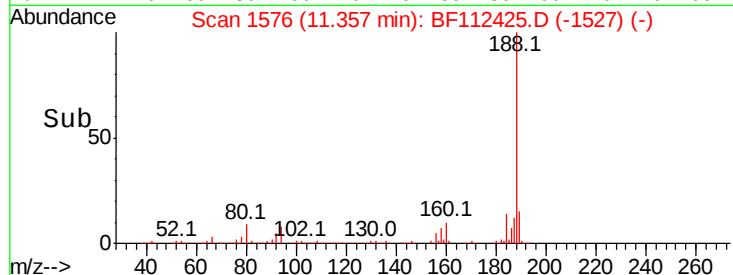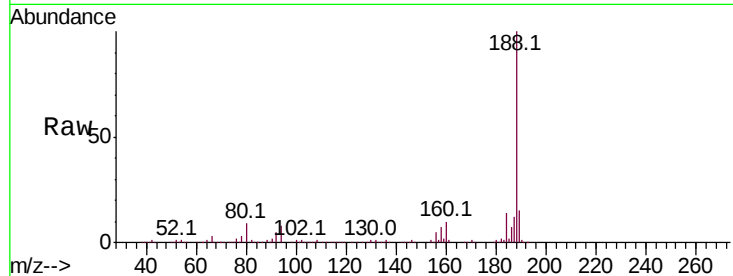

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112425.D
Acq: 6 Feb 2019 17:37

Tgt Ion	Ratio	Lower	Upper
240	100		
120	12.0	9.0	13.6
236	24.3	20.7	31.1

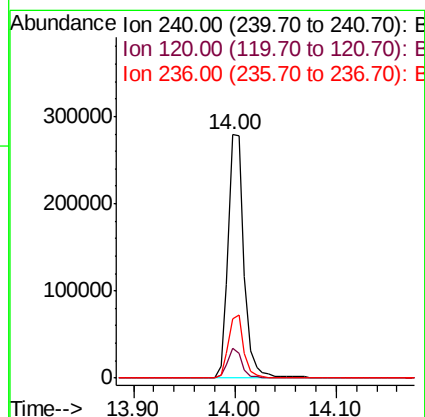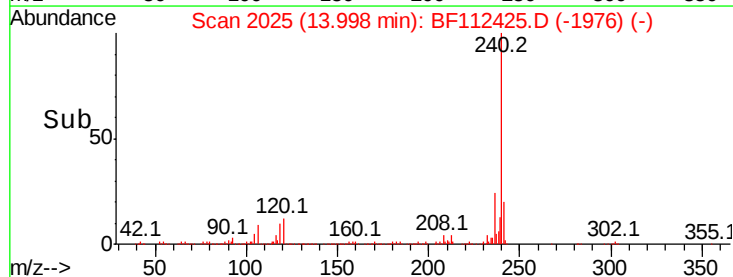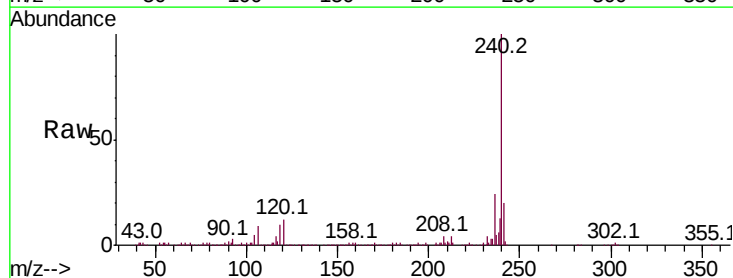

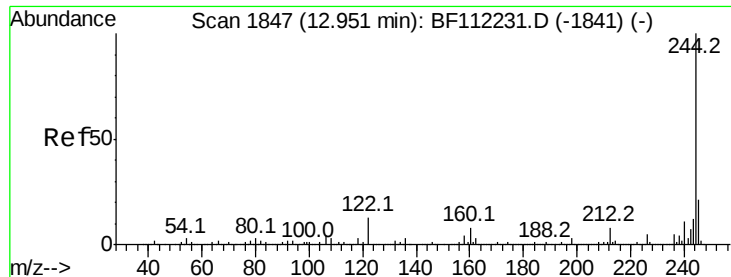

#79

Terphenyl-d14

Concen: 74.748 ng

RT: 12.94 min Scan# 1845

Delta R.T. -0.01 min

Lab File: BF112425.D

Acq: 6 Feb 2019 17:37

Instrument :

BNA_F

ClientSampleId :

AU-06-020519-B


Tot Ion:244 Resp: 1210877

Ion Ratio Lower Upper

244 100

212 7.1 5.9 8.9




122 11.6 9.8 14.6

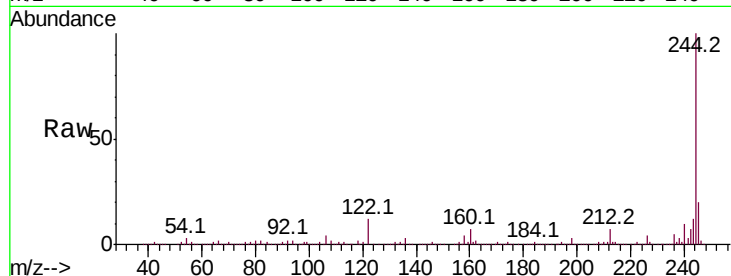

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

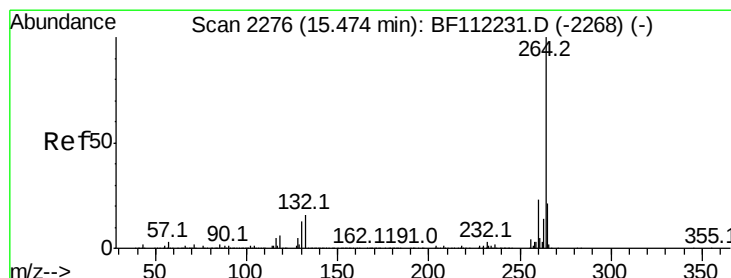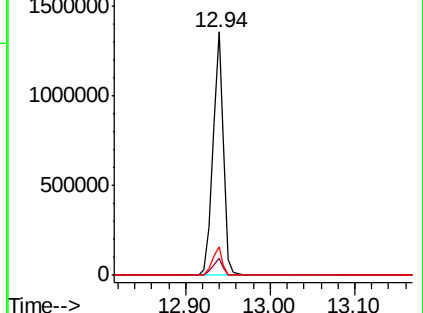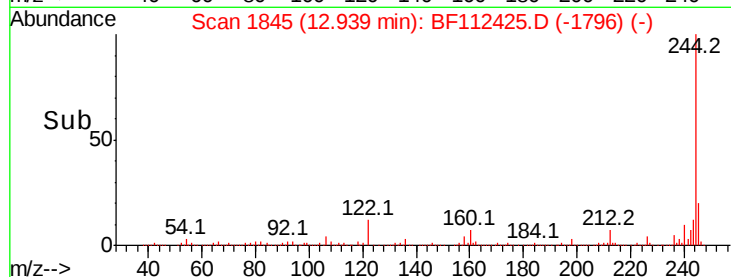

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.47 min Scan# 2276

Delta R.T. -0.00 min

Lab File: BF112425.D

Acq: 6 Feb 2019 17:37


Tgt Ion:264 Resp: 292415

Ion Ratio Lower Upper

264 100

260 24.2 18.2 27.2

265 21.3 17.0 25.4

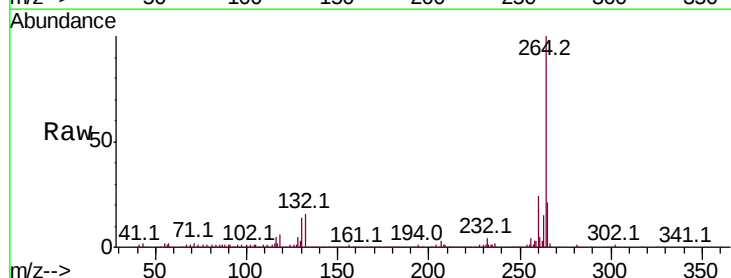

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

