

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020619\
 Data File : BF112427.D
 Acq On : 6 Feb 2019 18:31
 Operator : JU/SJ
 Sample : K1356-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-020519-A

Quant Time: Feb 07 00:40:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	151716	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	579524	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	270732	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	448089	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	319461	20.00	ng	-0.01
87) Perylene-d12	15.47	264	305556	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	946537	132.52	ng	0.00
7) Phenol-d6	6.49	99	1046489	105.44	ng	0.00
23) Nitrobenzene-d5	7.40	82	836946	83.21	ng	-0.01
42) 2,4,6-Tribromophenol	10.66	330	376092	119.35	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	1643926	85.88	ng	-0.02
79) Terphenyl-d14	12.94	244	1354115	79.83	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF020619\
Data File : BF112427.D
Acq On : 6 Feb 2019 18:31
Operator : JU/SJ
Sample : K1356-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SU-01-020519-A

Quant Time: Feb 07 00:40:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

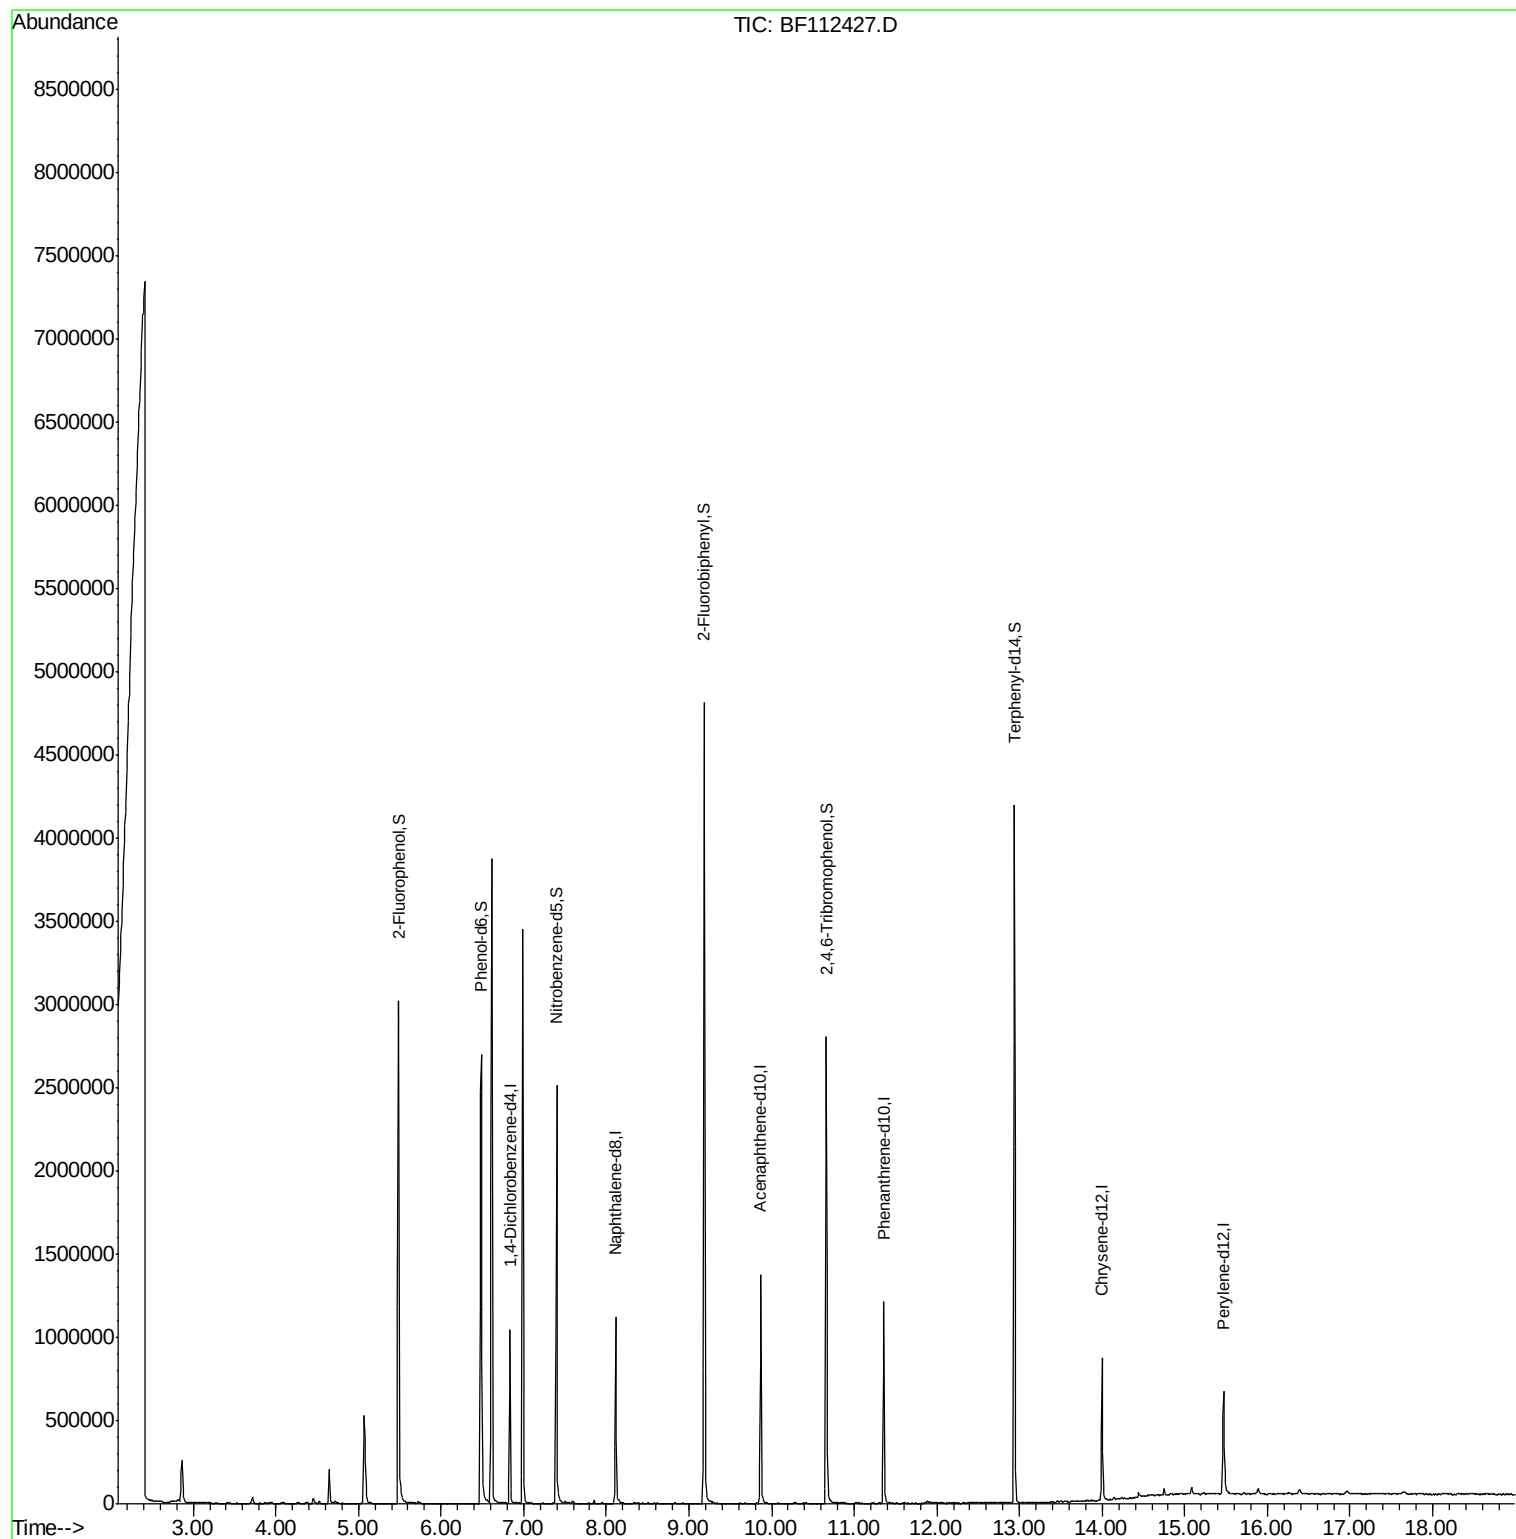

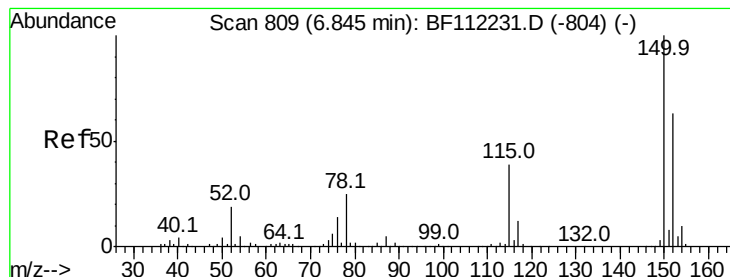


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF112427.D
Acq: 6 Feb 2019 18:31

Instrument :
BNA_F
ClientSampleId :
SU-01-020519-A

Tot Ion:152 Resp: 151716
Ion Ratio Lower Upper
152 100
150 154.9 127.4 191.0
115 59.5 45.5 68.3

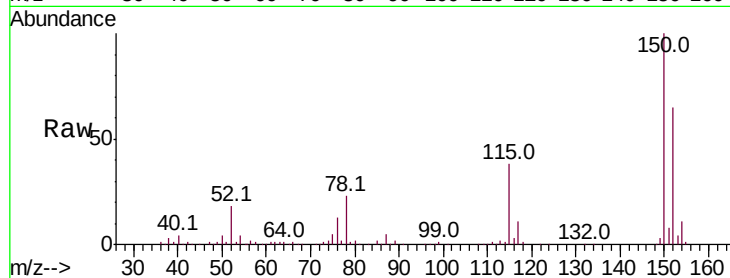


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

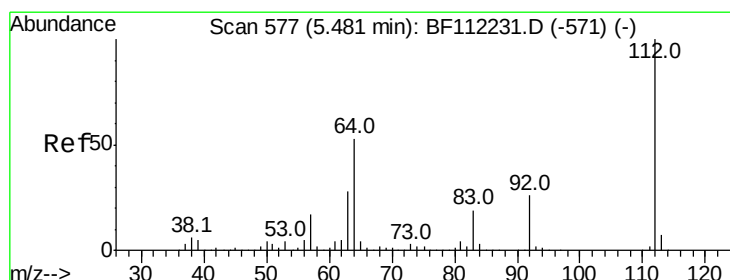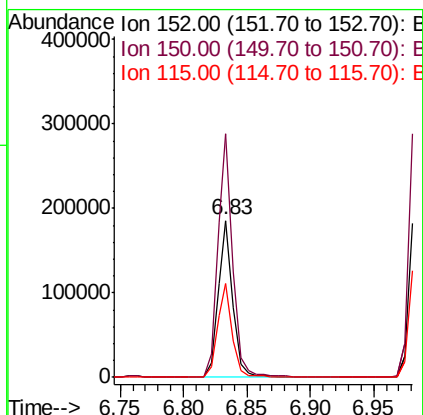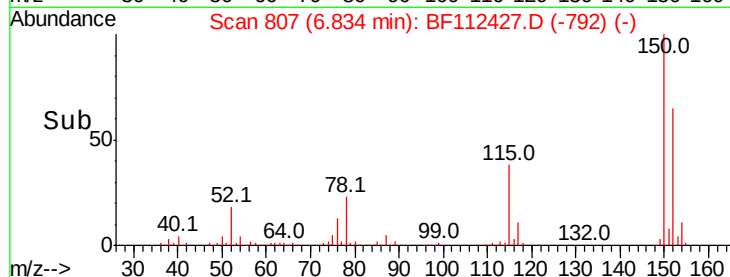



#5


2-Fluorophenol
Concen: 132.518 ng
RT: 5.49 min Scan# 578
Delta R.T. 0.01 min
Lab File: BF112427.D
Acq: 6 Feb 2019 18:31

Tgt Ion:112 Resp: 946537
Ion Ratio Lower Upper
112 100
64 52.6 45.7 68.5
63 28.3 23.6 35.4

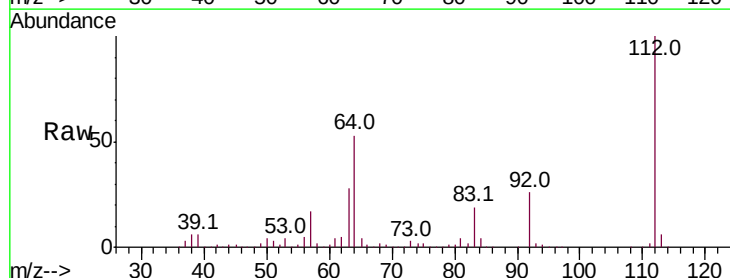

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

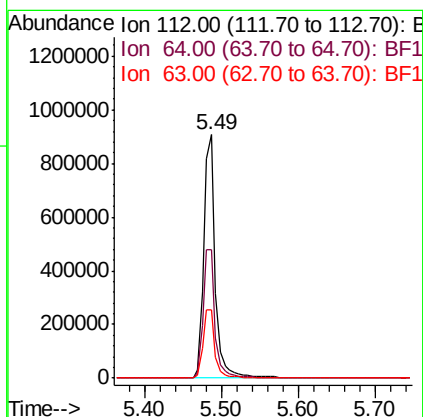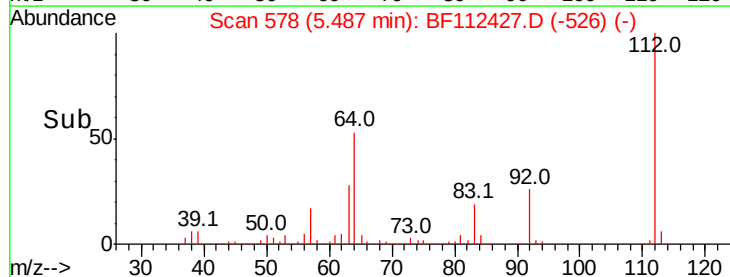

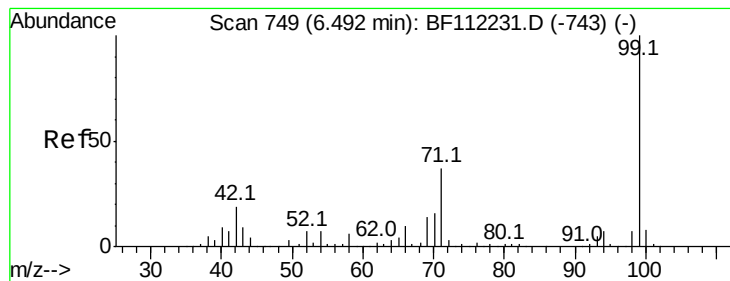

#7

Phenol-d6

Concen: 105.438 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112427.D

Acq: 6 Feb 2019 18:31

Instrument :

BNA_F

ClientSampleId :

SU-01-020519-A


Tot Ion: 99 Resp: 1046489

Ion Ratio Lower Upper




99 100

42 17.7 15.1 22.7

71 35.7 26.9 40.3

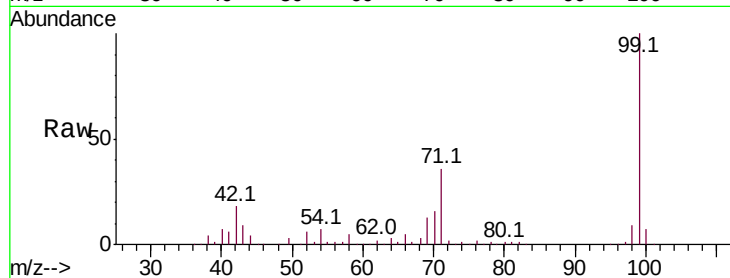

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

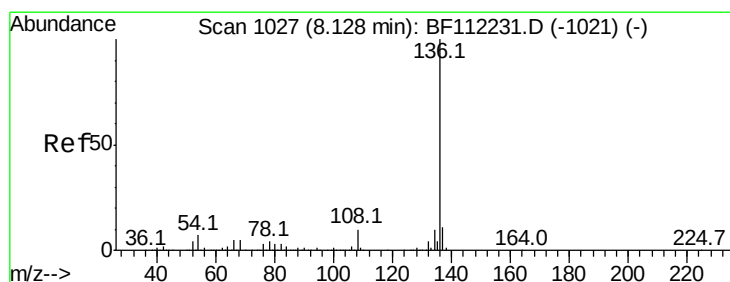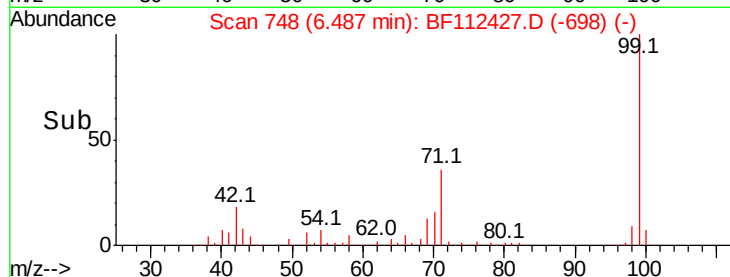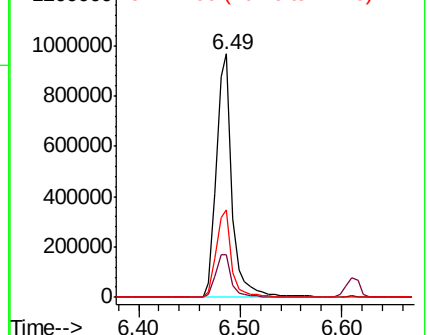

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112427.D

Acq: 6 Feb 2019 18:31

Tgt Ion: 136 Resp: 579524


Ion Ratio Lower Upper

136 100



137 10.6 9.1 13.7


54 5.5 5.9 8.9#

68 4.4 5.1 7.7#

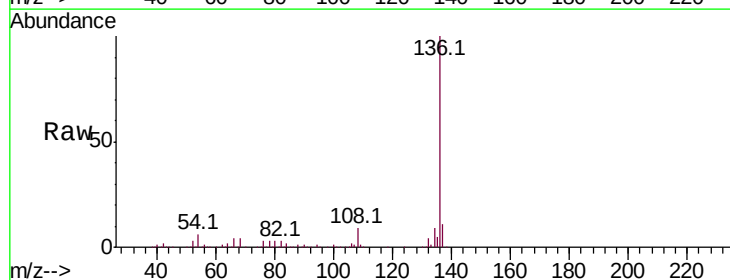

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

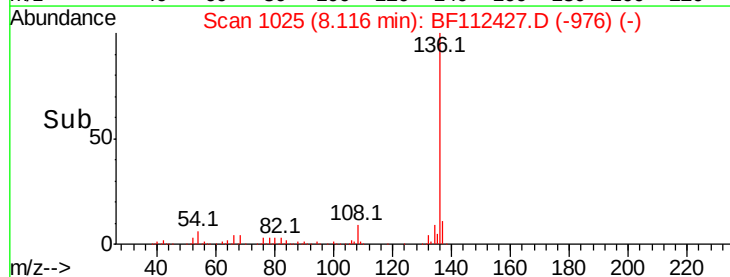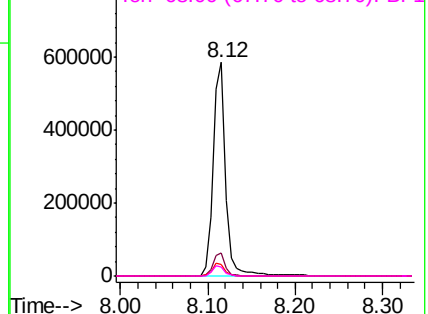


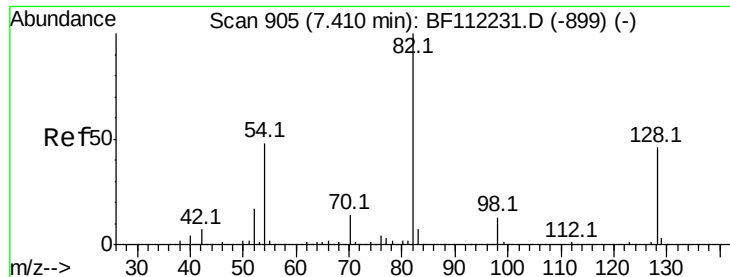




#23
 Nitrobenzene-d5
 Concen: 83.214 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.01 min
 Lab File: BF112427.D
 Acq: 6 Feb 2019 18:31

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-020519-A

Tot Ion	82	Resp	836946
Ion Ratio	100	Lower	Upper
128	46.7	37.8	56.8
54	46.8	39.7	59.5

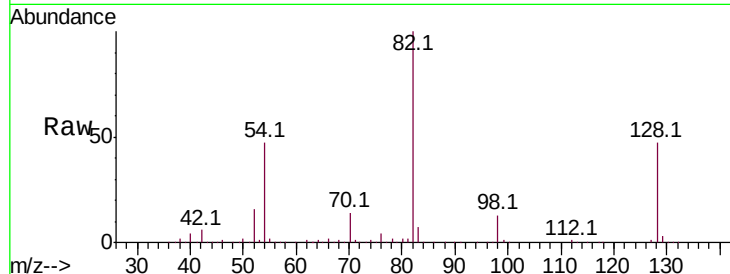


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

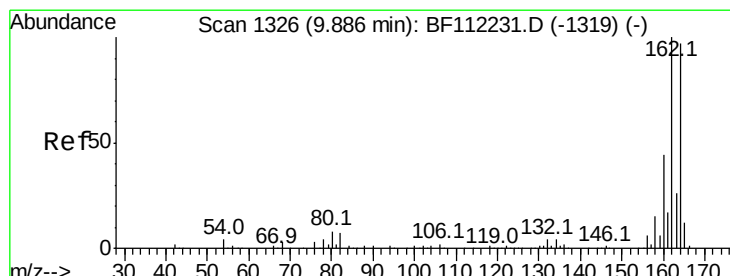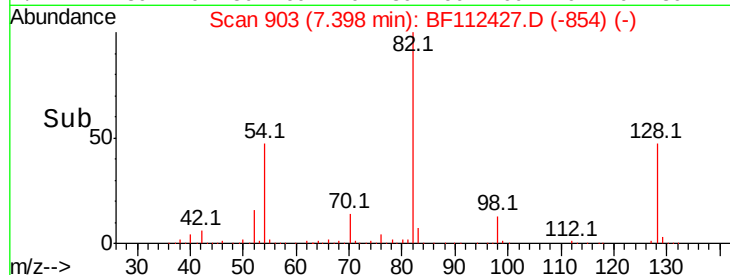
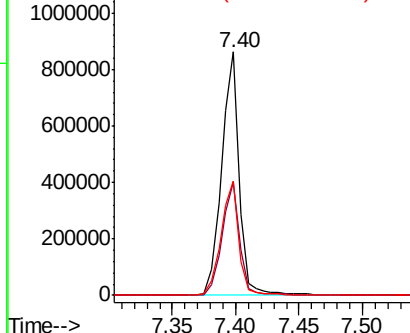



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.02 min
 Lab File: BF112427.D
 Acq: 6 Feb 2019 18:31

Tgt Ion	164	Resp	270732
Ion Ratio	100	Lower	Upper
162	102.6	82.2	123.4
160	45.8	36.2	54.4

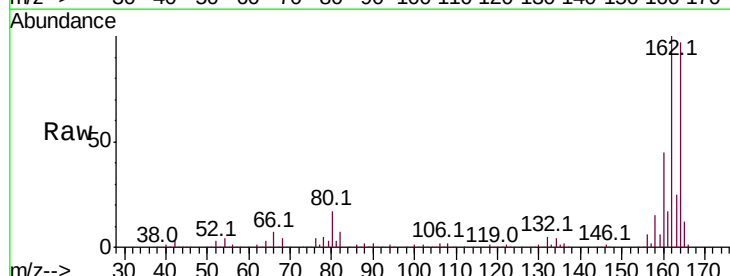

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

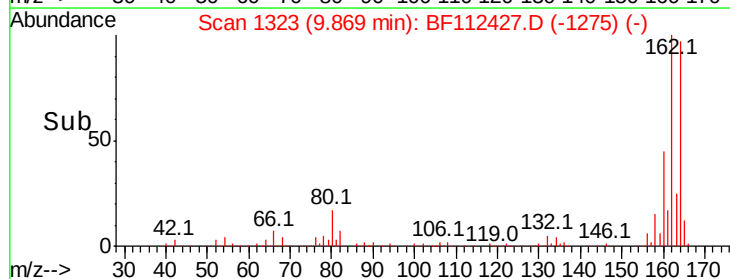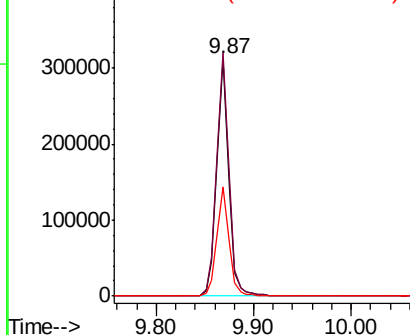


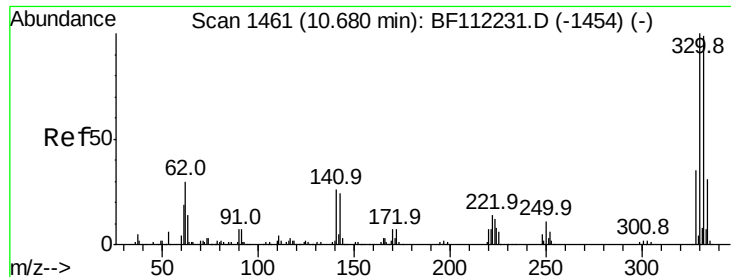

#42
 2,4,6-Tribromophenol
 Concen: 119.347 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.02 min
 Lab File: BF112427.D
 Acq: 6 Feb 2019 18:31

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-020519-A

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	76.6	114.8
141	31.5	24.3	36.5



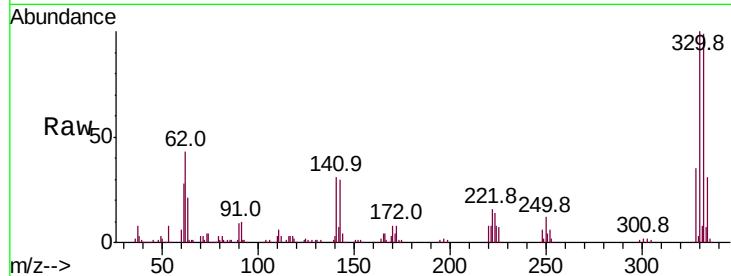


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

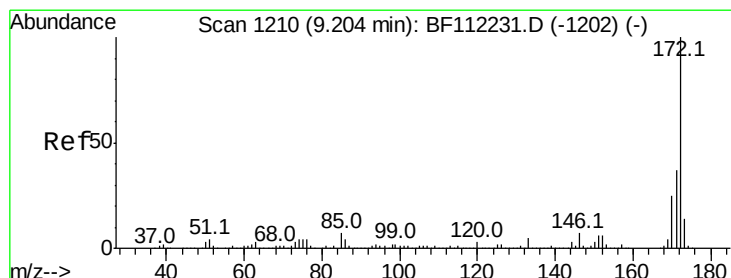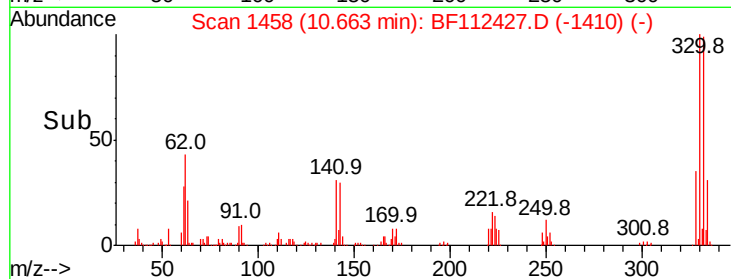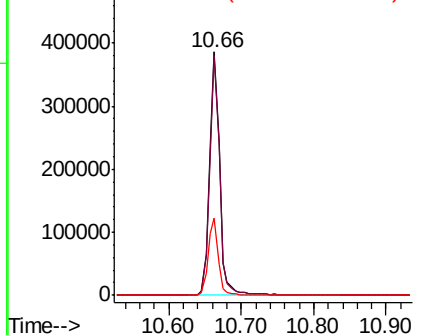

#45
 2-Fluorobiphenyl
 Concen: 85.881 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.02 min
 Lab File: BF112427.D
 Acq: 6 Feb 2019 18:31

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	30.5	45.7
170	24.2	20.2	30.4


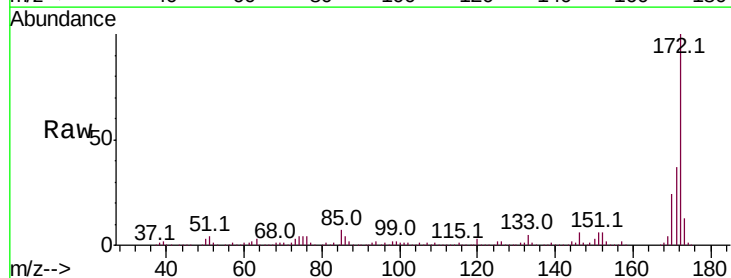



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



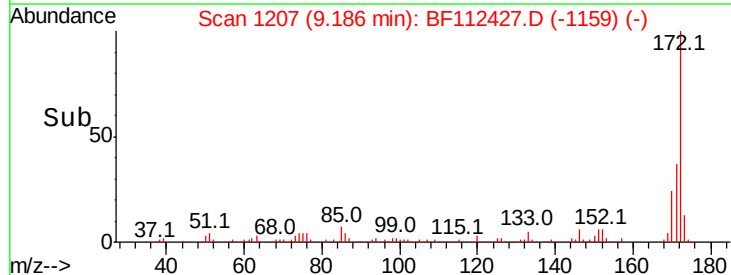
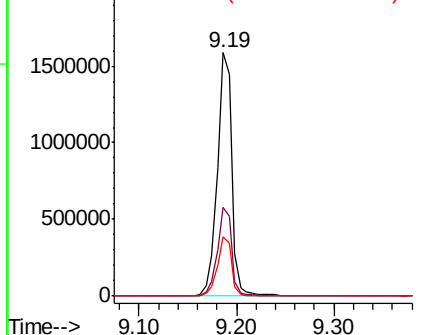


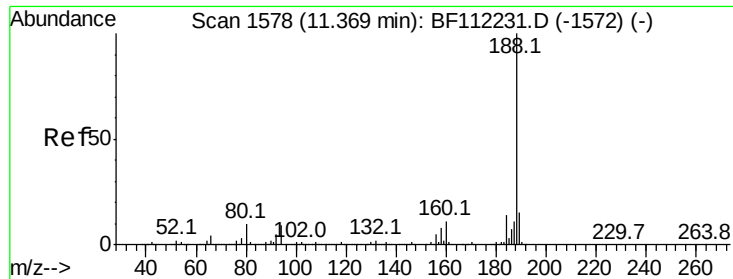

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112427.D
Acq: 6 Feb 2019 18:31




Instrument :
BNA_F
ClientSampleId :
SU-01-020519-A


Tot Ion:188 Resp: 448089
Ion Ratio Lower Upper
188 100
94 8.4 8.2 12.2
80 9.0 8.9 13.3

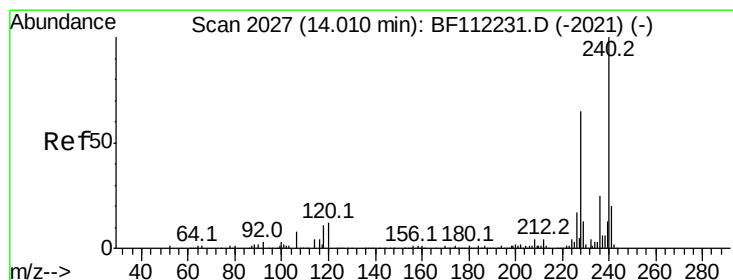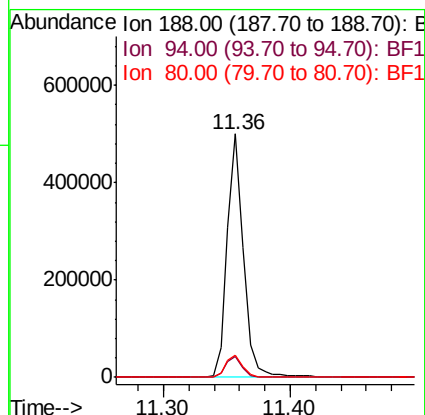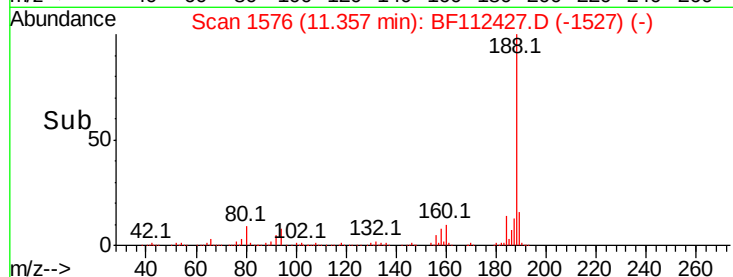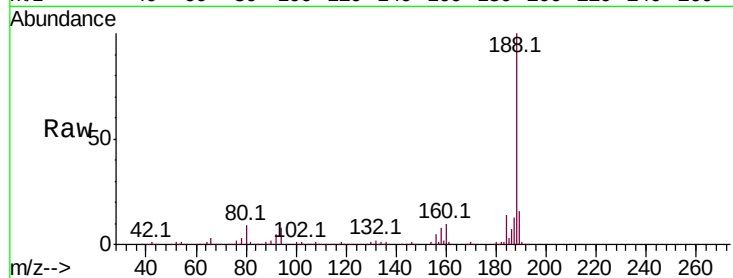

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112427.D
Acq: 6 Feb 2019 18:31

Tgt Ion:240 Resp: 319461
Ion Ratio Lower Upper
240 100
120 11.8 9.0 13.6
236 26.2 20.7 31.1

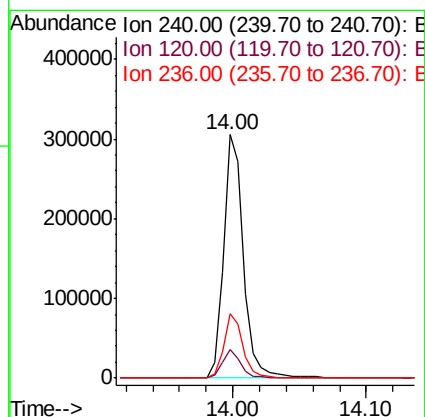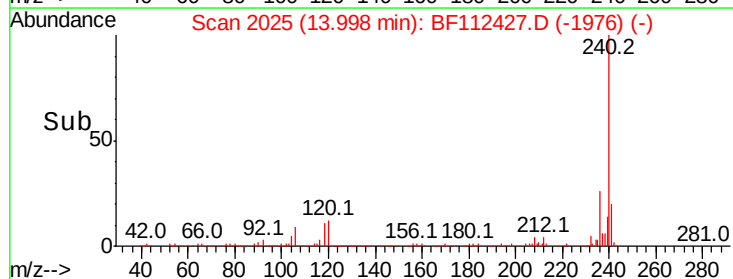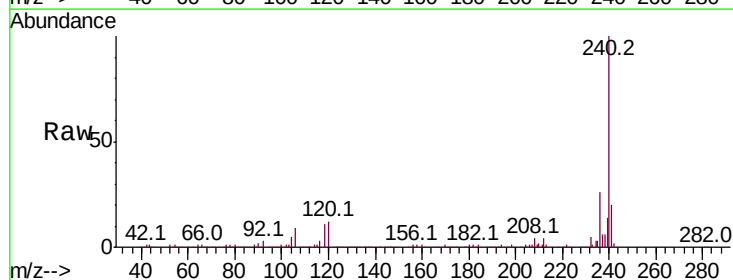


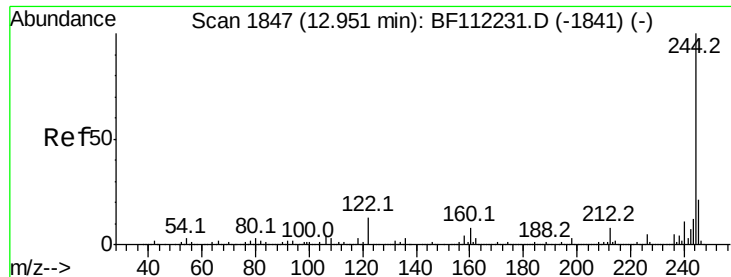




#79
 Terphenyl-d14
 Concen: 79.835 ng
 RT: 12.94 min Scan# 1845
 Delta R.T. -0.01 min
 Lab File: BF112427.D
 Acq: 6 Feb 2019 18:31

Instrument :
 BNA_F
 ClientSampleId :
 SU-01-020519-A

Tot Ion:244 Resp: 1354115
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.9 8.9
 122 11.8 9.8 14.6

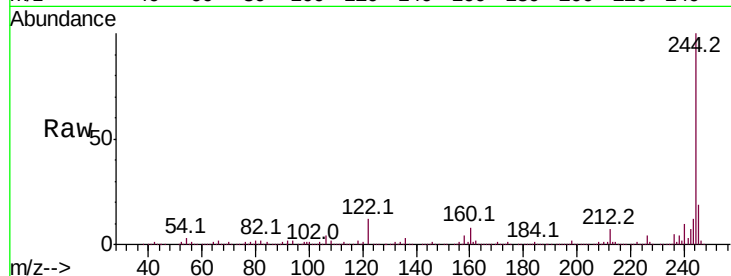


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

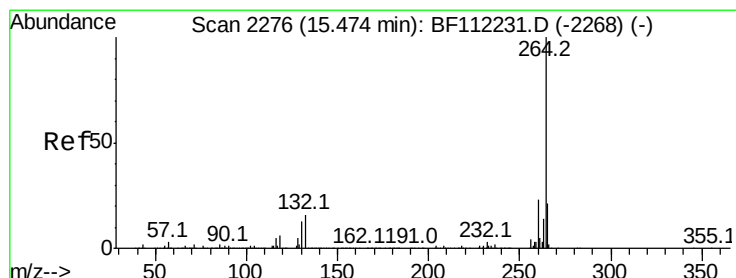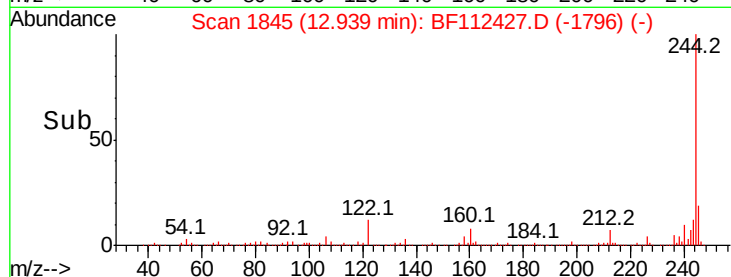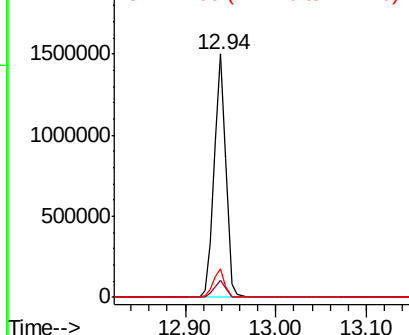

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2275
 Delta R.T. -0.01 min
 Lab File: BF112427.D
 Acq: 6 Feb 2019 18:31

Tgt Ion:264 Resp: 305556
 Ion Ratio Lower Upper
 264 100
 260 22.8 18.2 27.2
 265 20.9 17.0 25.4

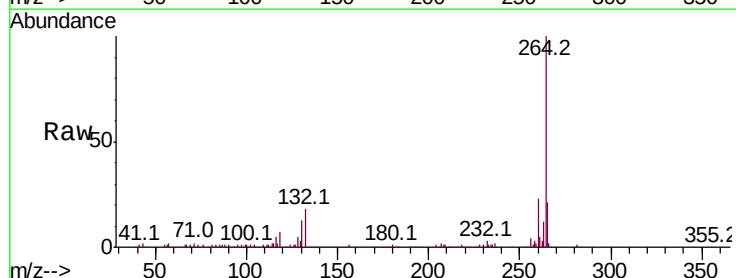

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

