


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020619\
 Data File : BF112415.D
 Acq On : 6 Feb 2019 12:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

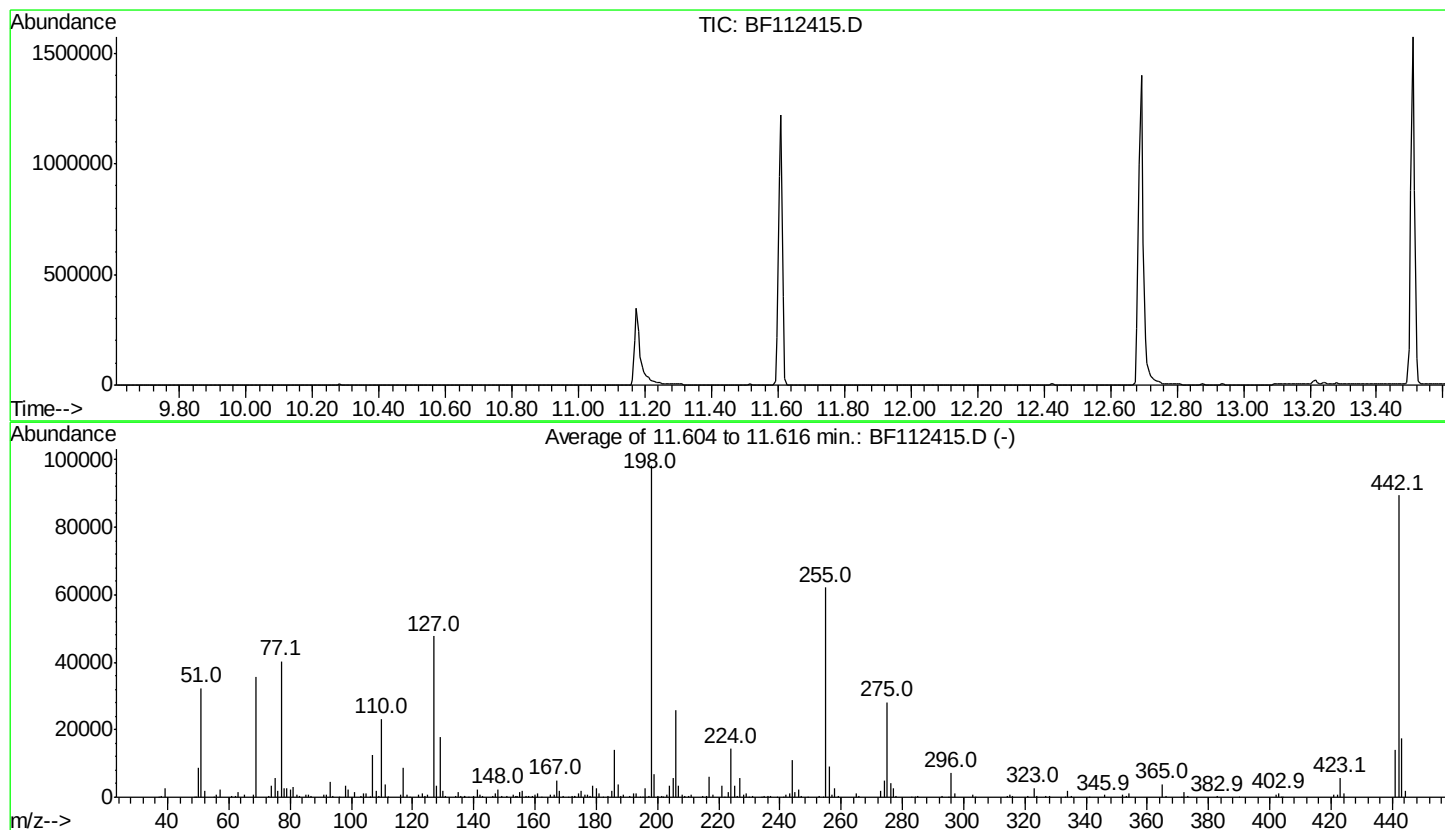

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	32387	PASS
68	69	0.00	2	2.0	694	PASS
69	198	0.00	100	36.1	35500	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	47682	PASS
197	198	0.00	2	0.5	468	PASS
198	198	100	100	100.0	98218	PASS
199	198	5	9	6.9	6755	PASS
275	198	10	60	28.7	28218	PASS
365	198	1	100	4.0	3891	PASS
441	198	0.01	100	14.4	14151	PASS
442	198	50	100	91.0	89400	PASS
443	442	15	24	19.6	17492	PASS