
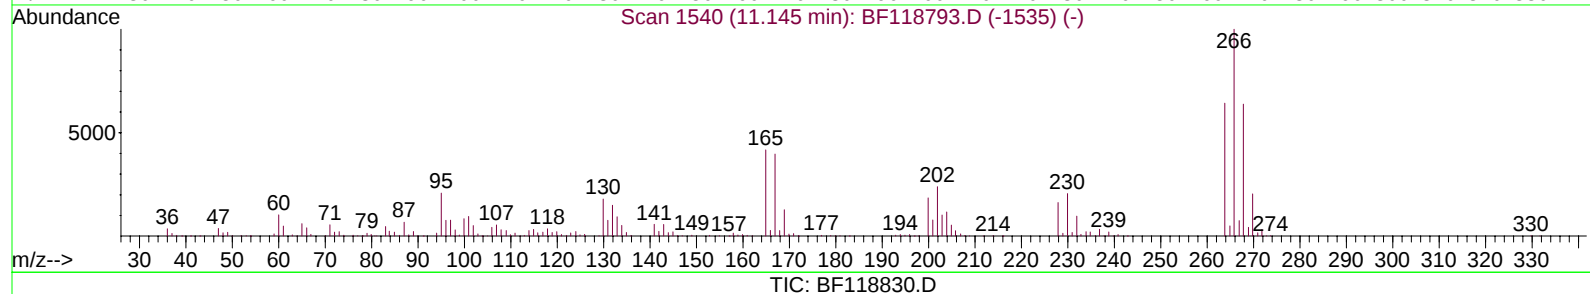
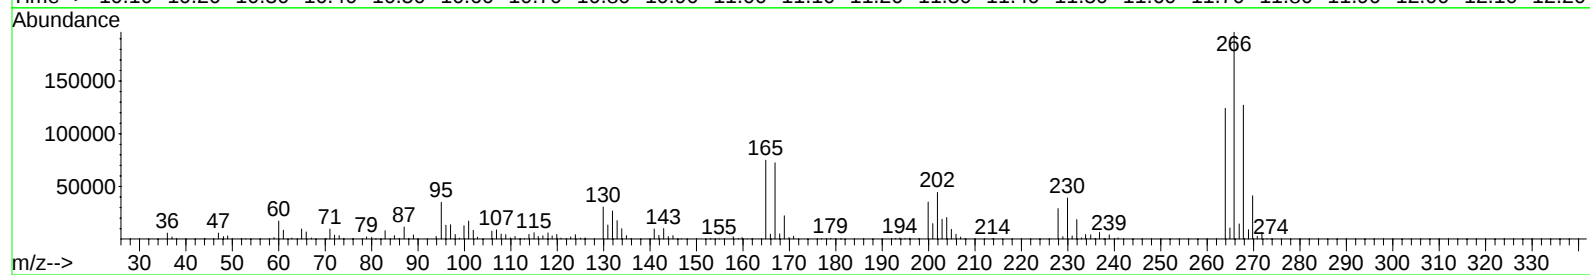


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020620\
Data File : BF118830.D
Acq On : 6 Feb 2020 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 18:08:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 16:26:03 2020
Response via : Initial Calibration

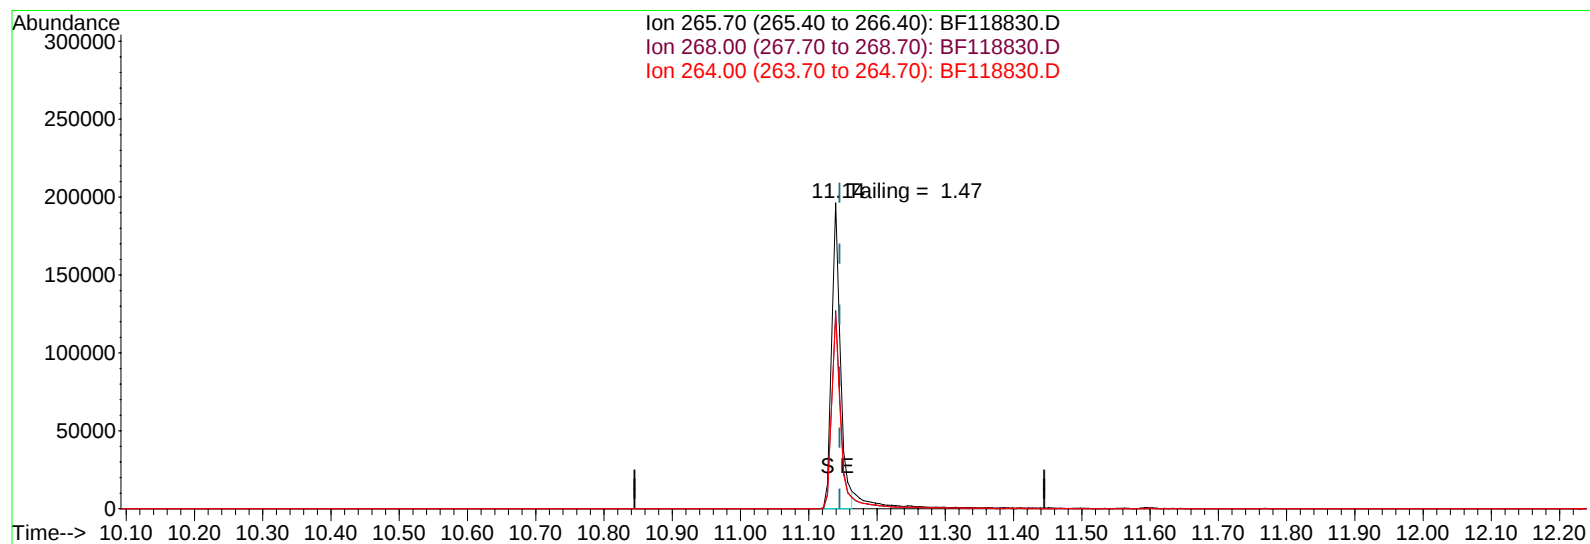

(70) Pentachlorophenol (C)




11.139min (-0.006) 30866.70ng

response 191508

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	64.73
264.00	64.30	63.27
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020620\  
Data File   : BF118830.D  
Acq On      : 6 Feb 2020    9:32  
Operator    : CG/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Feb 06 18:08:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 16:26:03 2020
Response via : Initial Calibration

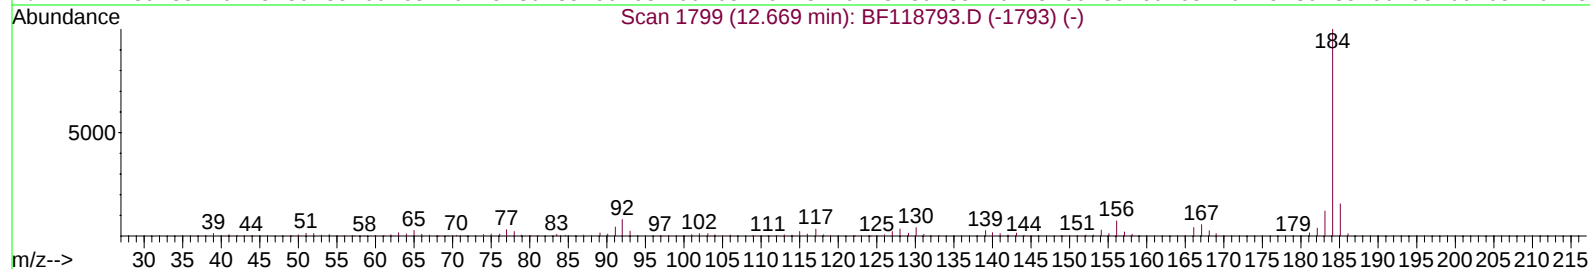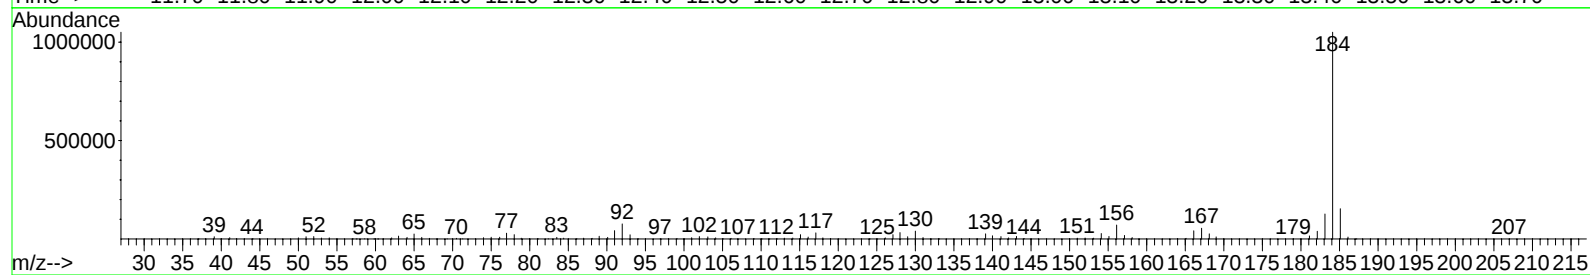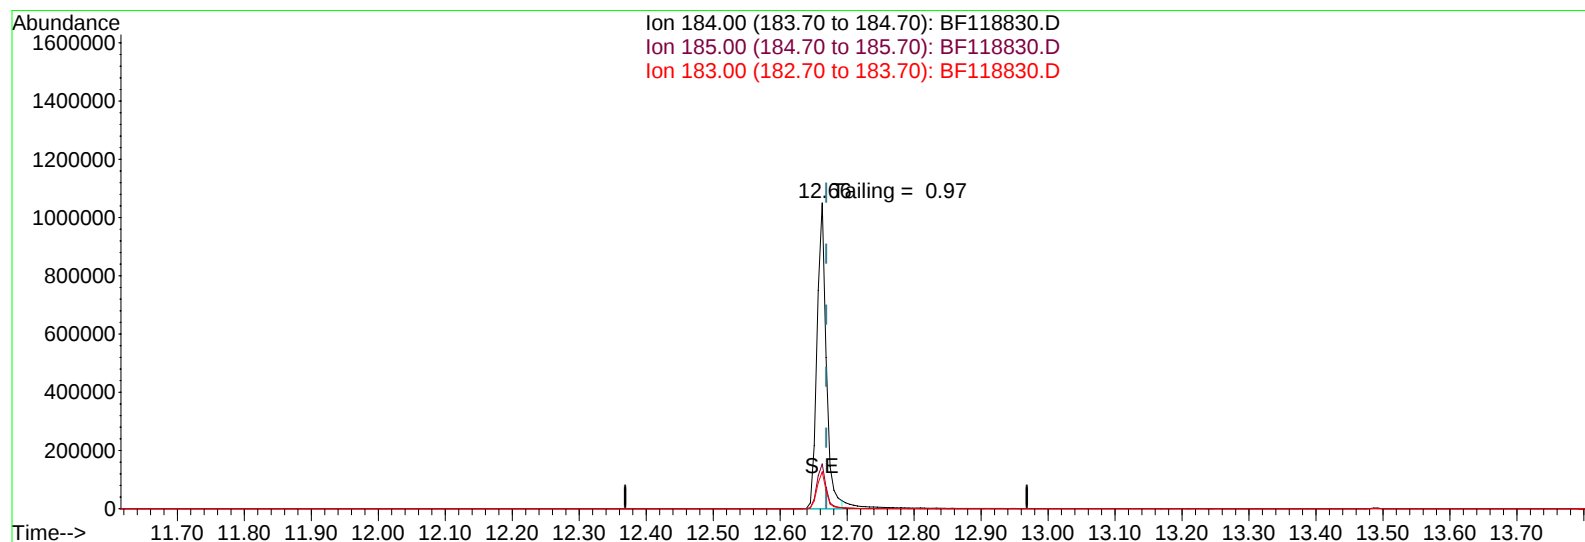

TIC: BF118830.D

(77) Benzidine

12.663min (-0.006) 0.00ng

response 1042929

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.67
183.00	12.10	12.08
0.00	0.00	0.00