


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020620\
 Data File : BF118830.D
 Acq On : 6 Feb 2020 9:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 03 16:26:03 2020

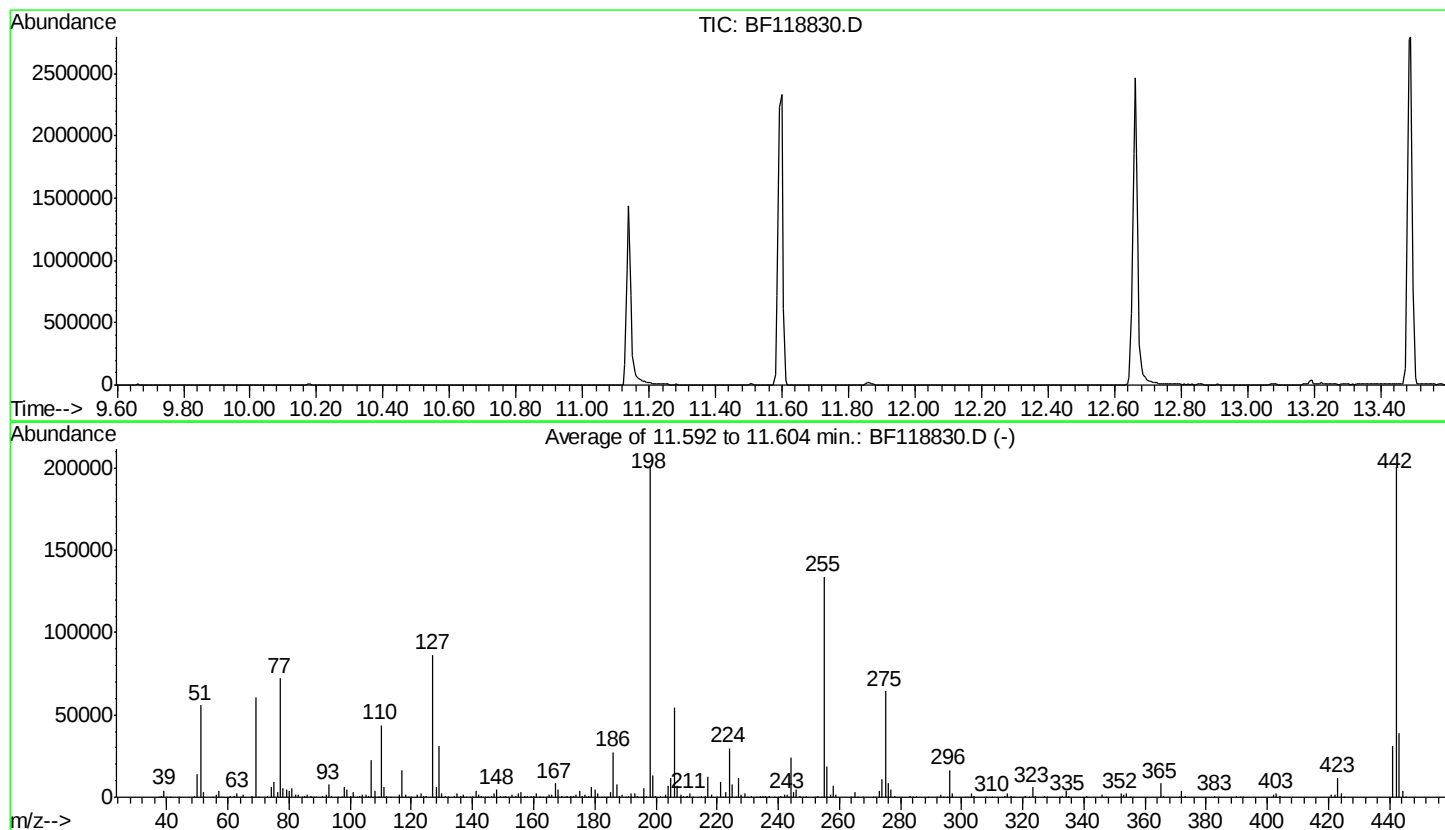

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	55707	PASS
68	69	0.00	2	1.7	1010	PASS
69	198	0.00	100	30.2	60857	PASS
70	69	0.00	2	0.5	319	PASS
127	198	10	80	42.9	86456	PASS
197	198	0.00	2	0.3	612	PASS
198	198	100	100	100.0	201517	PASS
199	198	5	9	6.5	13147	PASS
275	198	10	60	31.9	64290	PASS
365	198	1	100	4.2	8391	PASS
441	198	0.01	100	15.5	31290	PASS
442	198	50	100	99.5	200448	PASS
443	442	15	24	19.4	38928	PASS