


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020719\
 Data File : BF112431.D
 Acq On : 7 Feb 2019 11:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

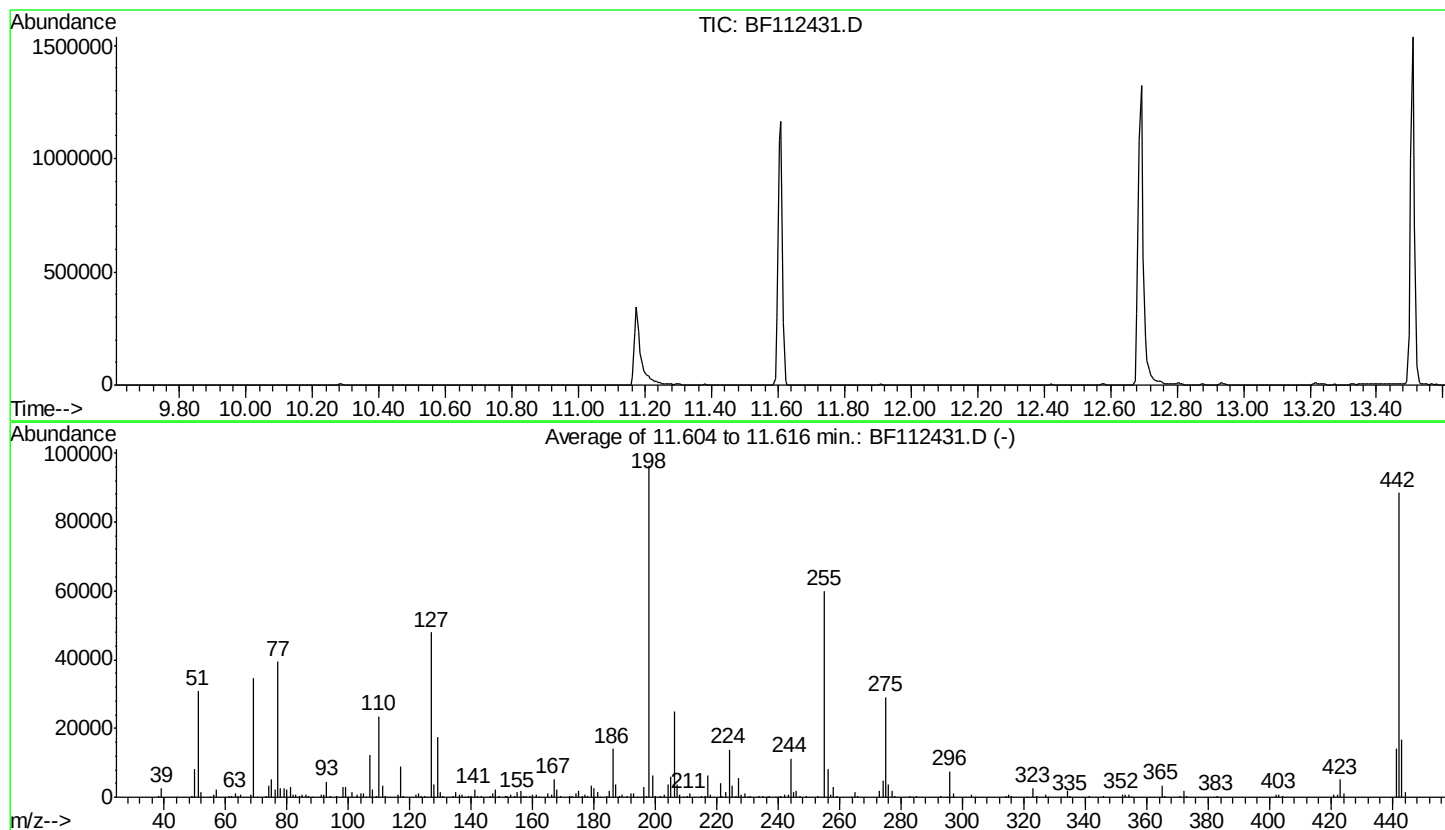

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	31049	PASS
68	69	0.00	2	2.0	686	PASS
69	198	0.00	100	35.8	34526	PASS
70	69	0.00	2	0.3	105	PASS
127	198	10	80	49.6	47834	PASS
197	198	0.00	2	0.3	308	PASS
198	198	100	100	100.0	96370	PASS
199	198	5	9	6.6	6371	PASS
275	198	10	60	30.1	29036	PASS
365	198	1	100	3.6	3489	PASS
441	198	0.01	100	14.7	14155	PASS
442	198	50	100	91.8	88496	PASS
443	442	15	24	18.8	16598	PASS