
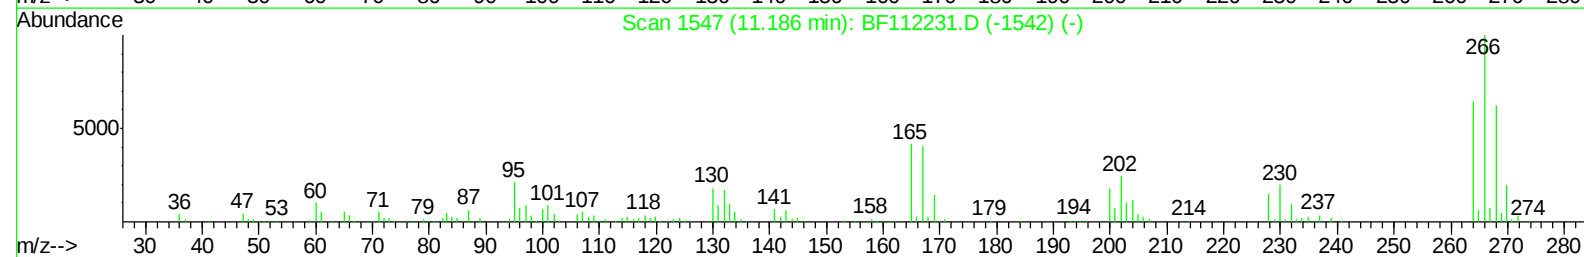
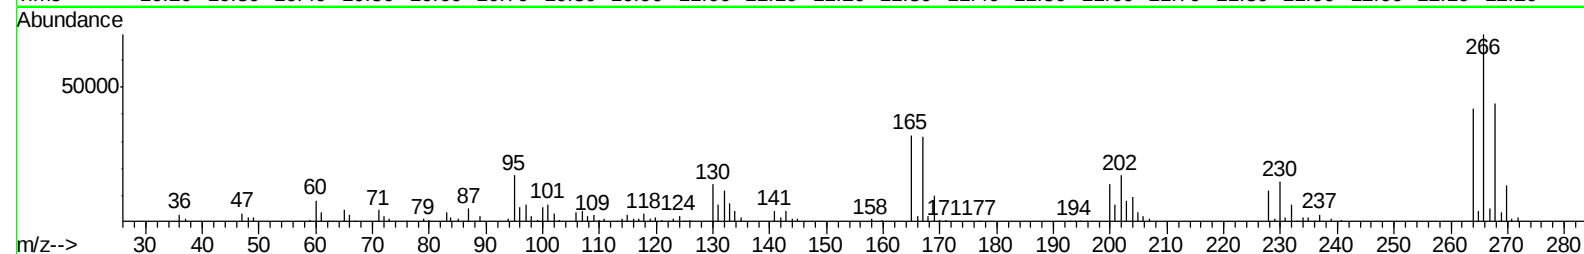


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020819\
 Data File : BF112455.D
 Acq On : 8 Feb 2019 13:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:48:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

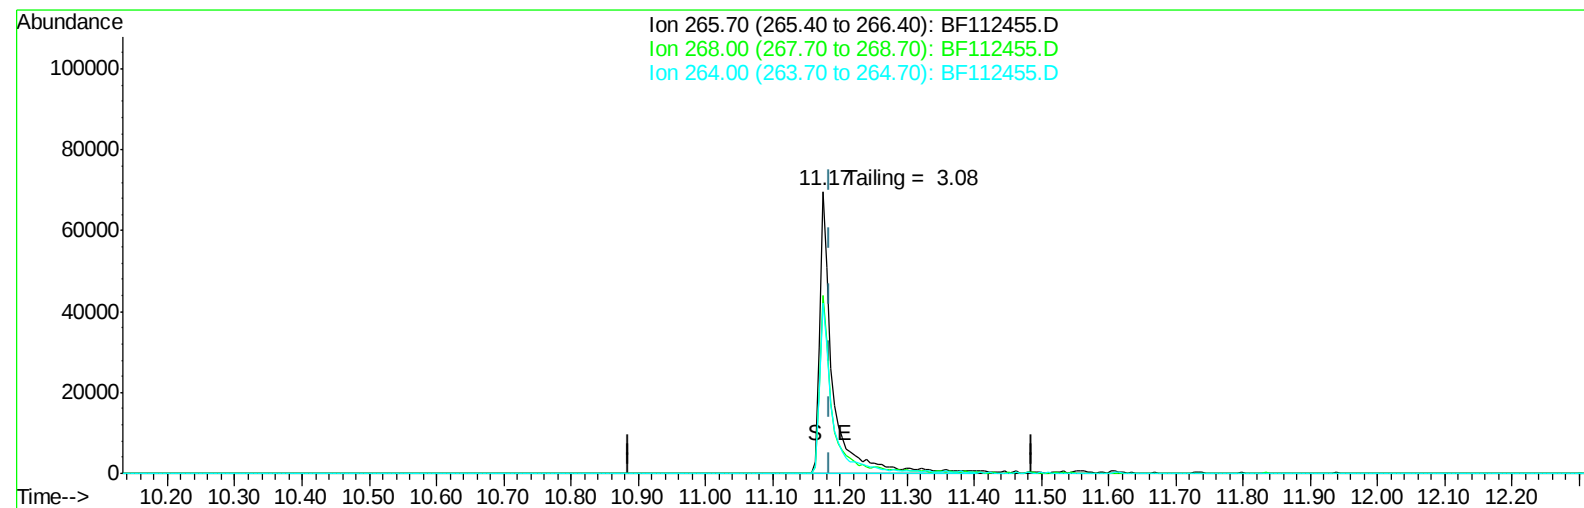

TIC: BF112455.D

(70) Pentachlorophenol (C)




11.175min (-0.012) 19313.04ng

response 92930

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.09
264.00	63.60	60.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF020819\
Data File : BF112455.D
Acq On : 8 Feb 2019 13:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:48:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

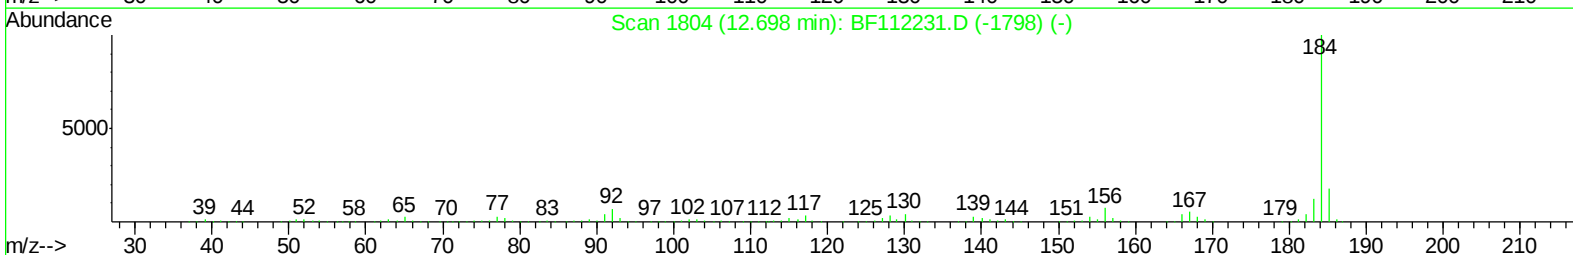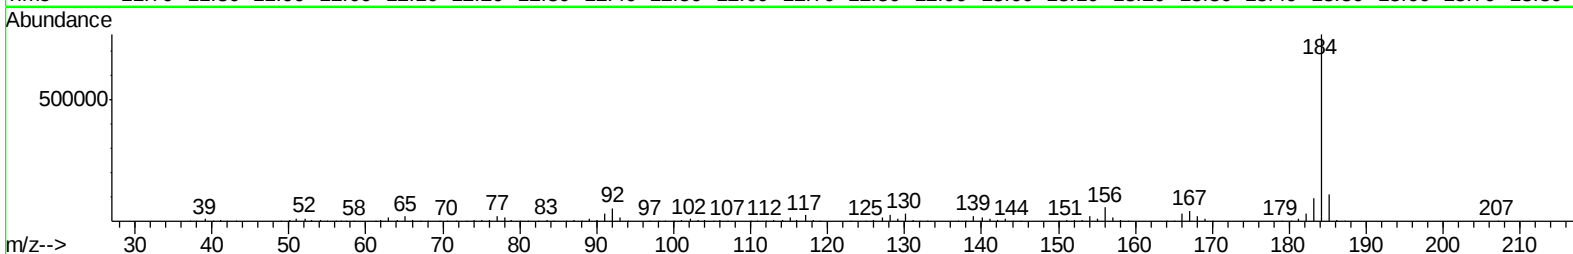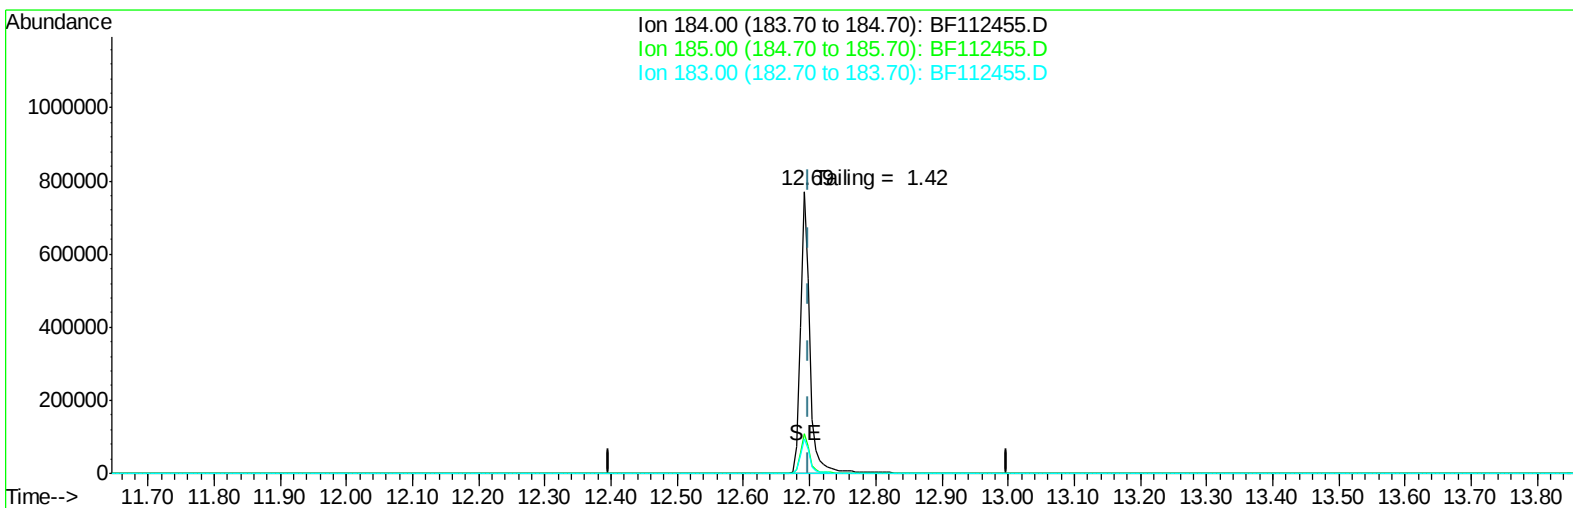

TIC: BF112455.D

(77) Benzidine

12.692min (-0.006) 29527.18ng

response 761490

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.23
183.00	12.50	12.27
0.00	0.00	0.00