


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF020819\
 Data File : BF112455.D
 Acq On : 8 Feb 2019 13:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

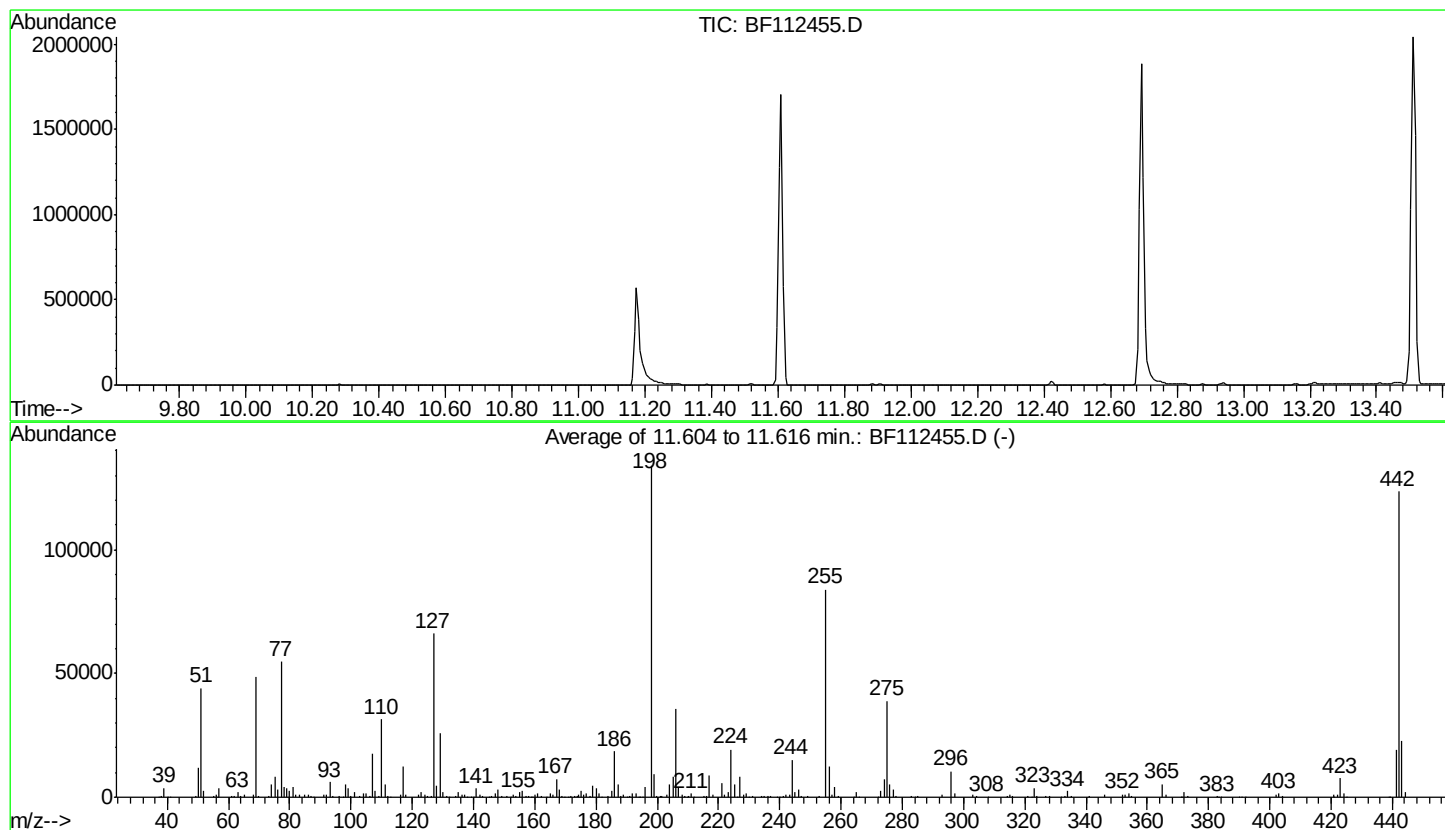

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	44182	PASS
68	69	0.00	2	2.0	984	PASS
69	198	0.00	100	36.4	48797	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	49.4	66093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133906	PASS
199	198	5	9	6.8	9074	PASS
275	198	10	60	29.1	38954	PASS
365	198	1	100	3.9	5248	PASS
441	198	0.01	100	14.2	19041	PASS
442	198	50	100	92.2	123496	PASS
443	442	15	24	18.6	22979	PASS