
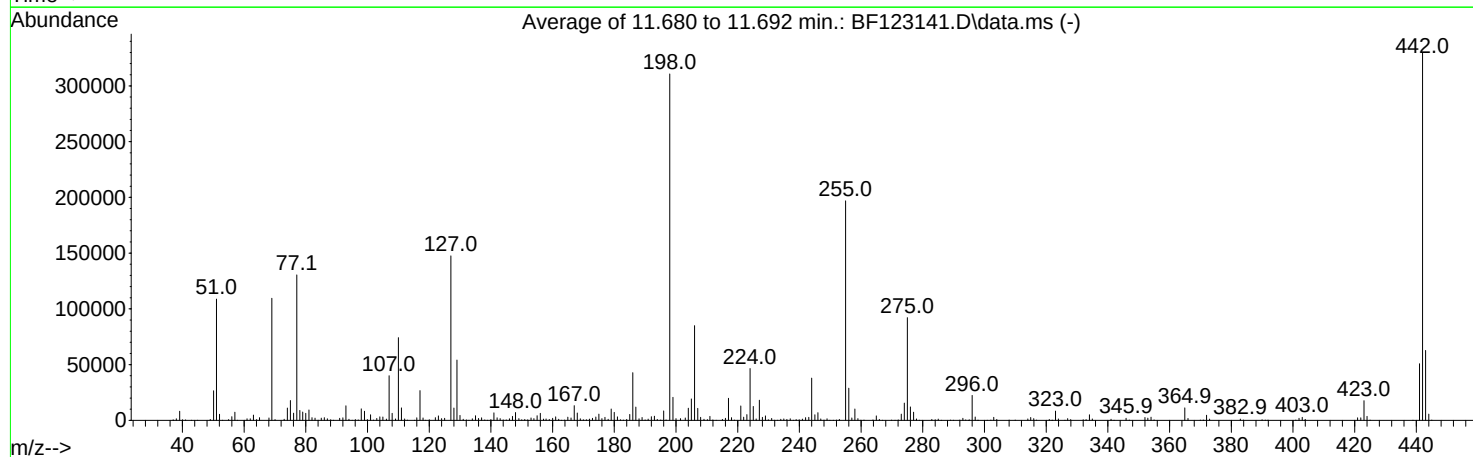


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020821\
 Data File : BF123141.D
 Acq On : 8 Feb 2021 9:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 29 12:29:00 2021

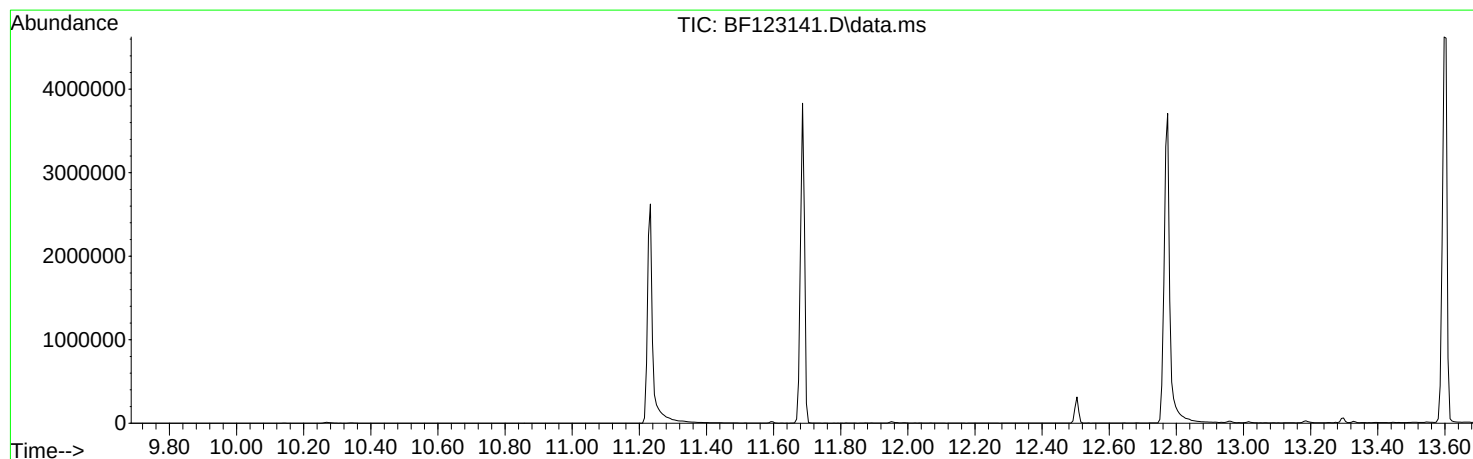




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	108779	PASS
68	69	0.00	2	2.0	2149	PASS
69	198	0.00	100	35.2	109539	PASS
70	69	0.00	2	0.7	717	PASS
127	198	10	80	47.5	147541	PASS
197	198	0.00	2	0.2	502	PASS
198	198	100	100	100.0	310763	PASS
199	198	5	9	6.7	20672	PASS
275	198	10	60	29.7	92171	PASS
365	198	1	100	3.6	11207	PASS
441	198	0.01	100	16.4	50835	PASS
442	442	50	100	100.0	329941	PASS
443	442	15	24	19.0	62720	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020821\
Data File : BF123141.D
Acq On : 8 Feb 2021 9:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 08 17:11:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

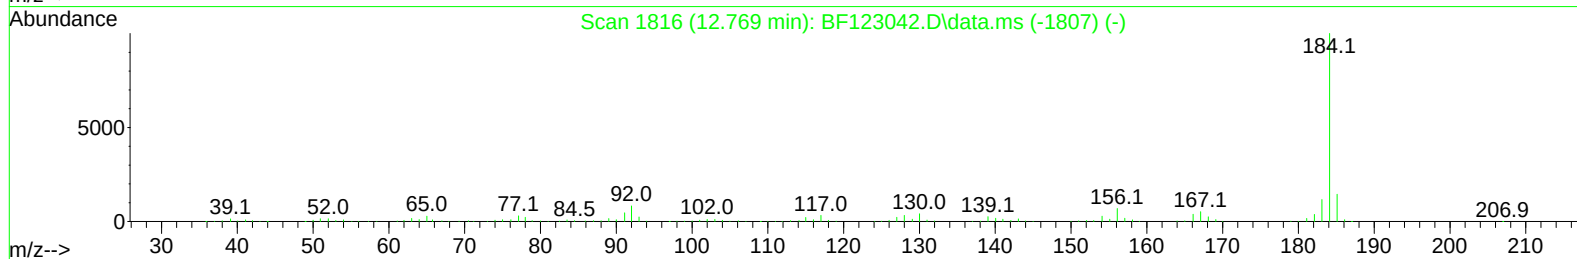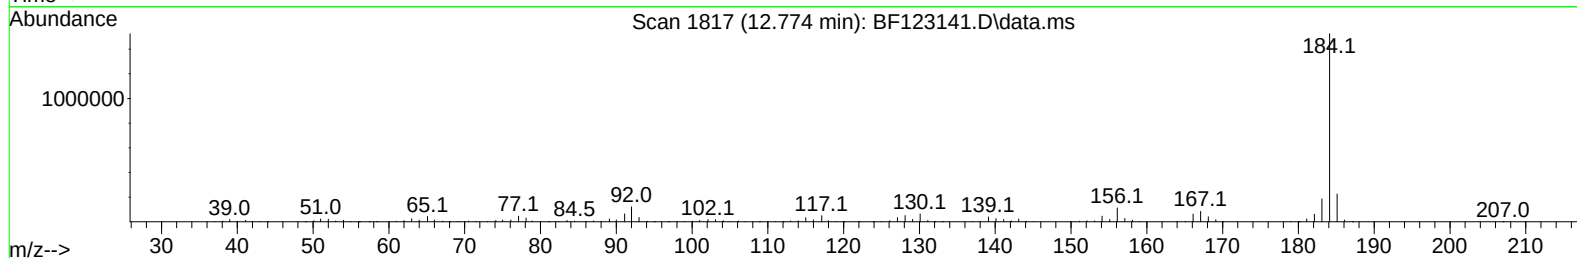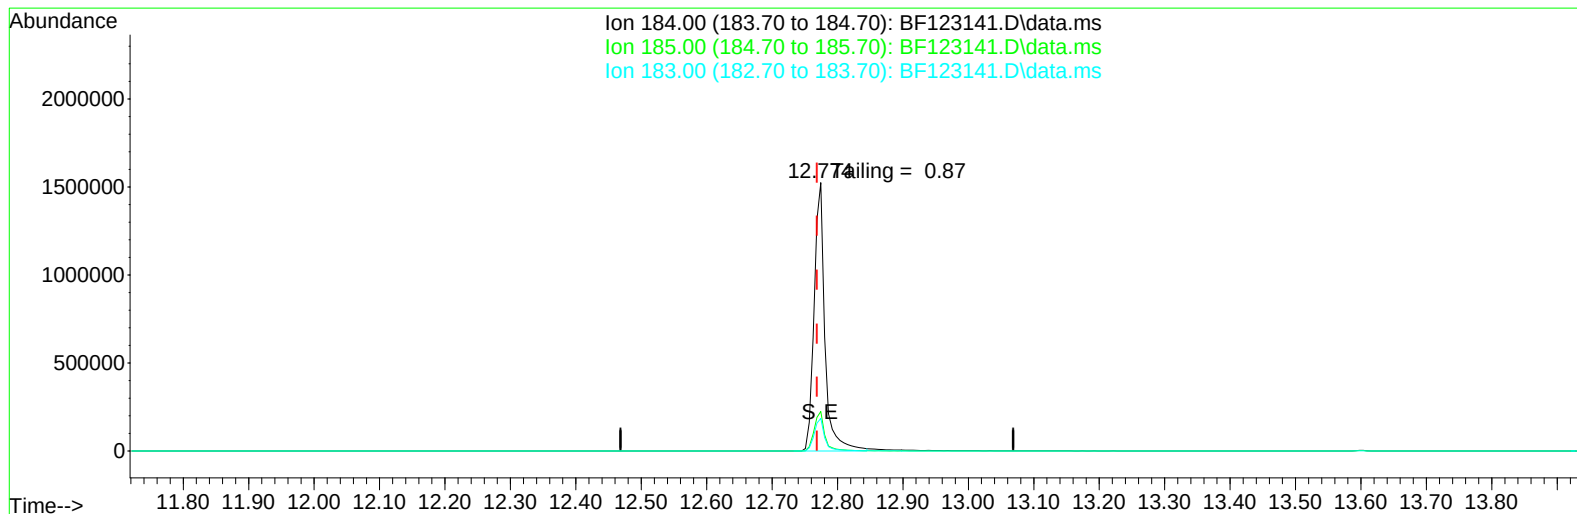

TIC: BF123141.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng




response 1789131

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.72
183.00	12.10	12.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020821\
Data File : BF123141.D
Acq On : 8 Feb 2021 9:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 08 17:11:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

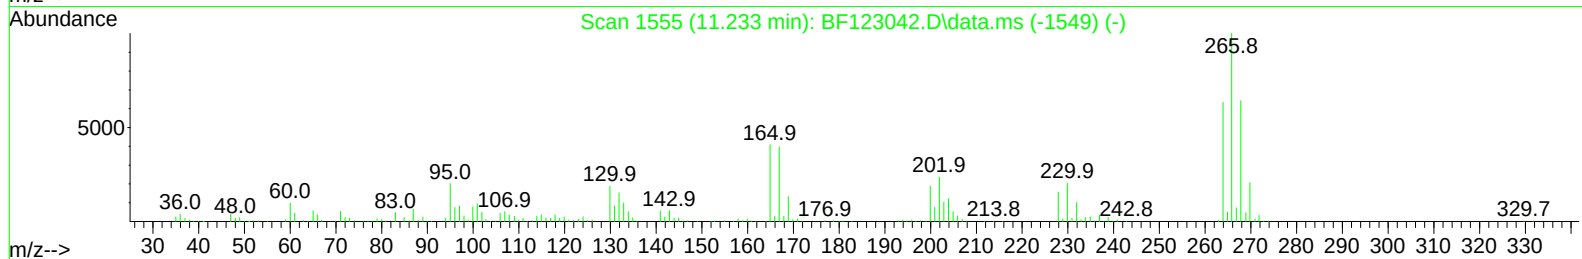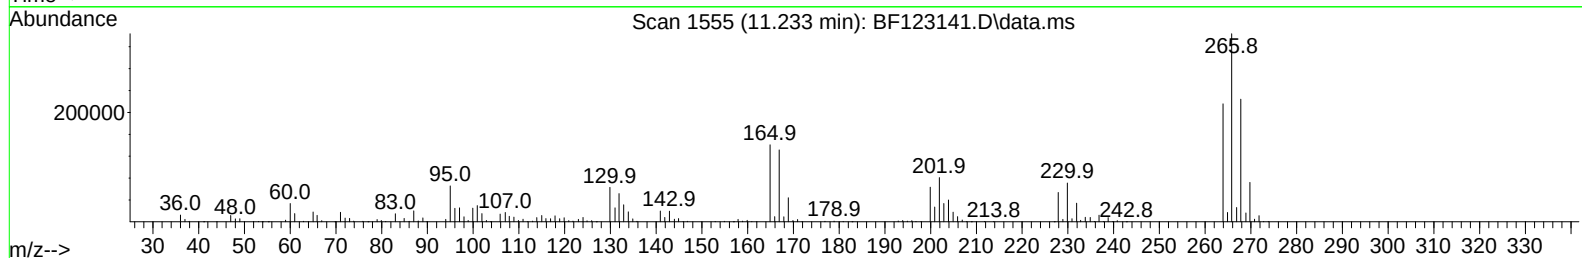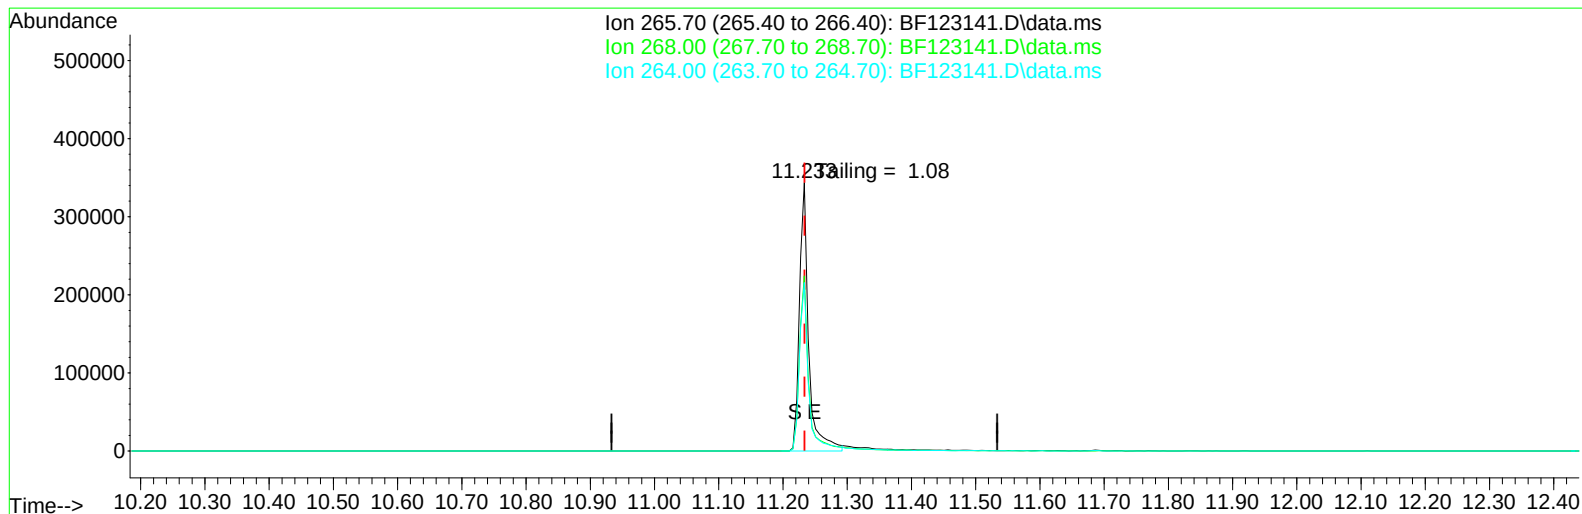

TIC: BF123141.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 32661.55 ng

response 367050

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.23
264.00	62.30	62.72
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2021	BNA_F	<u>BF123141.D</u>
Compound Name	Response	Retention Time
DDT	903853	13.6
DDD	11109	13.29
DDE	3269	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14378	918231	1.57