
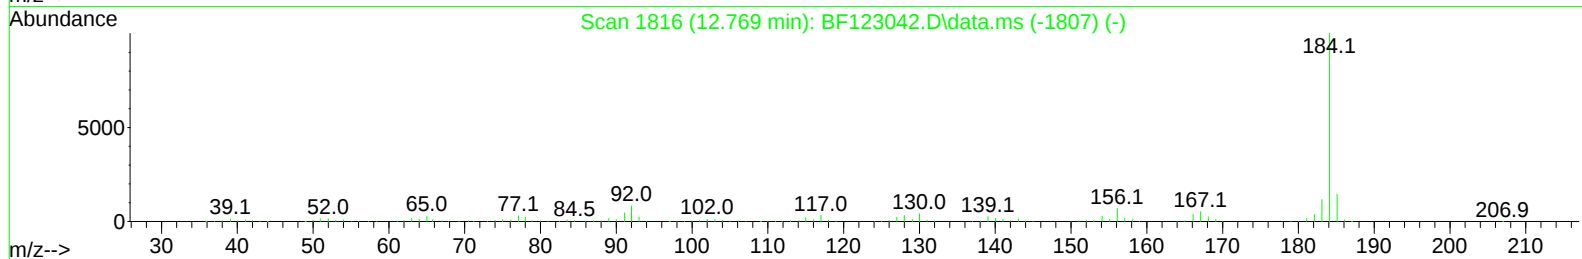
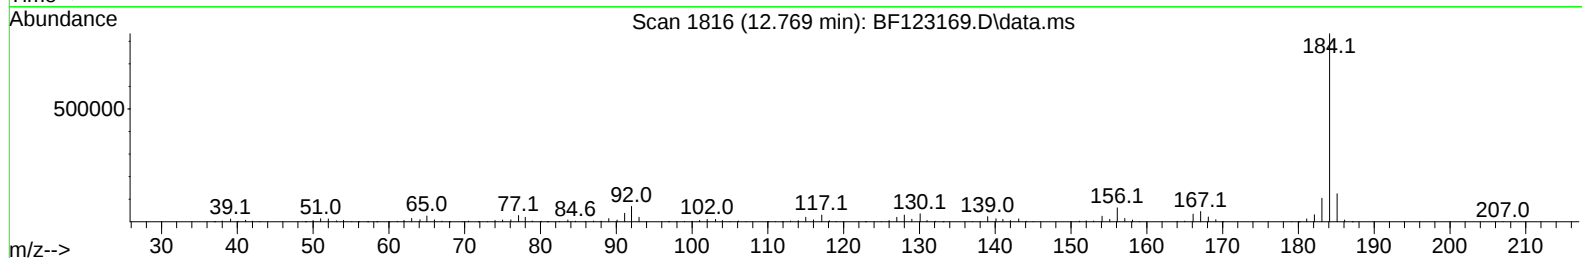


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021021\
Data File : BF123169.D
Acq On : 10 Feb 2021 12:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 15:16:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

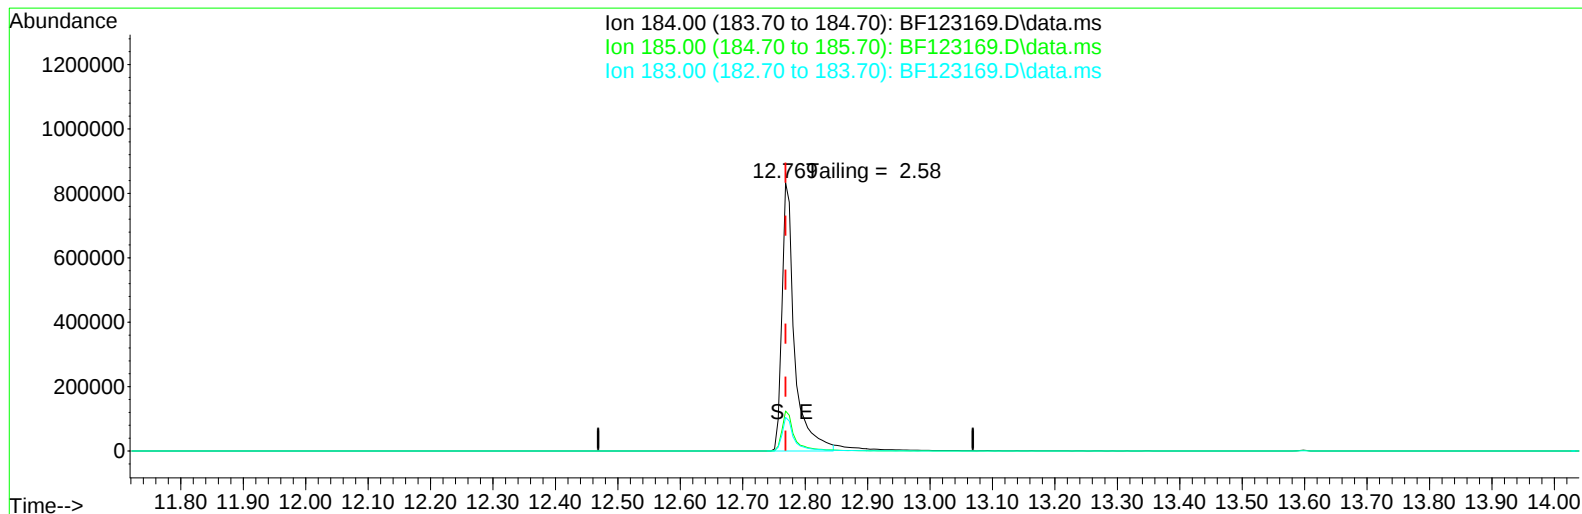

TIC: BF123169.D\data.ms

(77) Benzidine




12.769min (-0.000) 0.00 ng

response 1225370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.91
183.00	12.10	12.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021021\
 Data File : BF123169.D
 Acq On : 10 Feb 2021 12:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 15:16:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

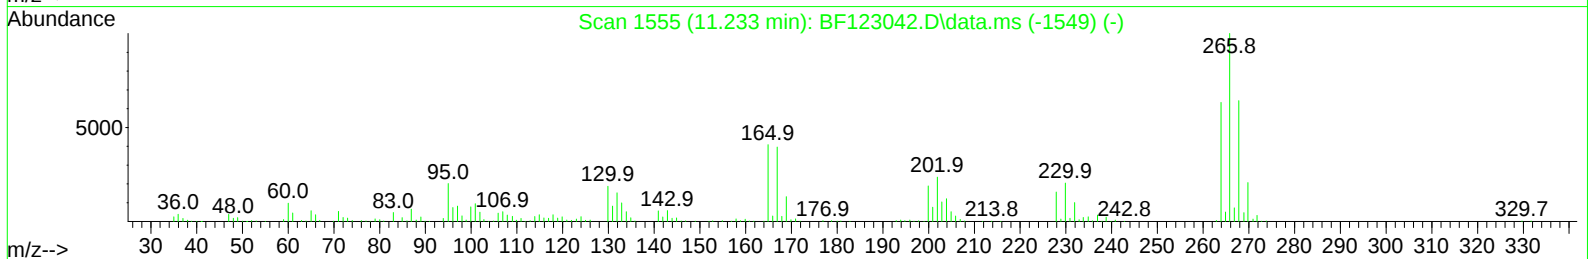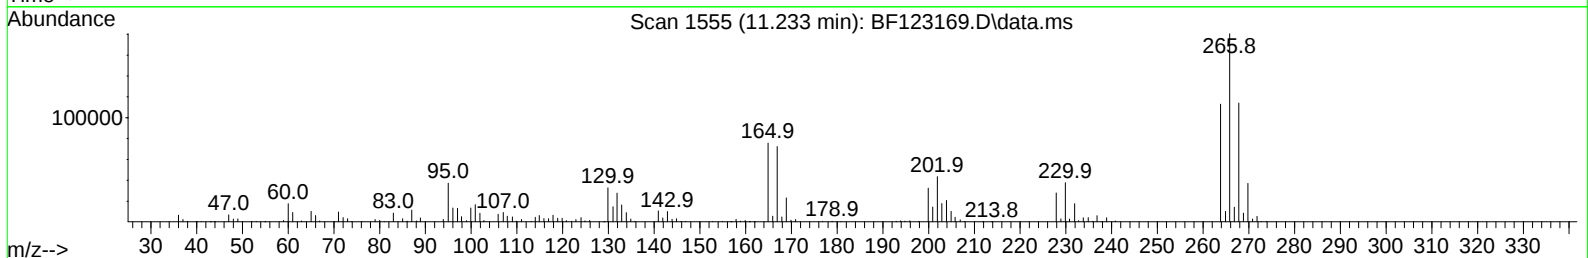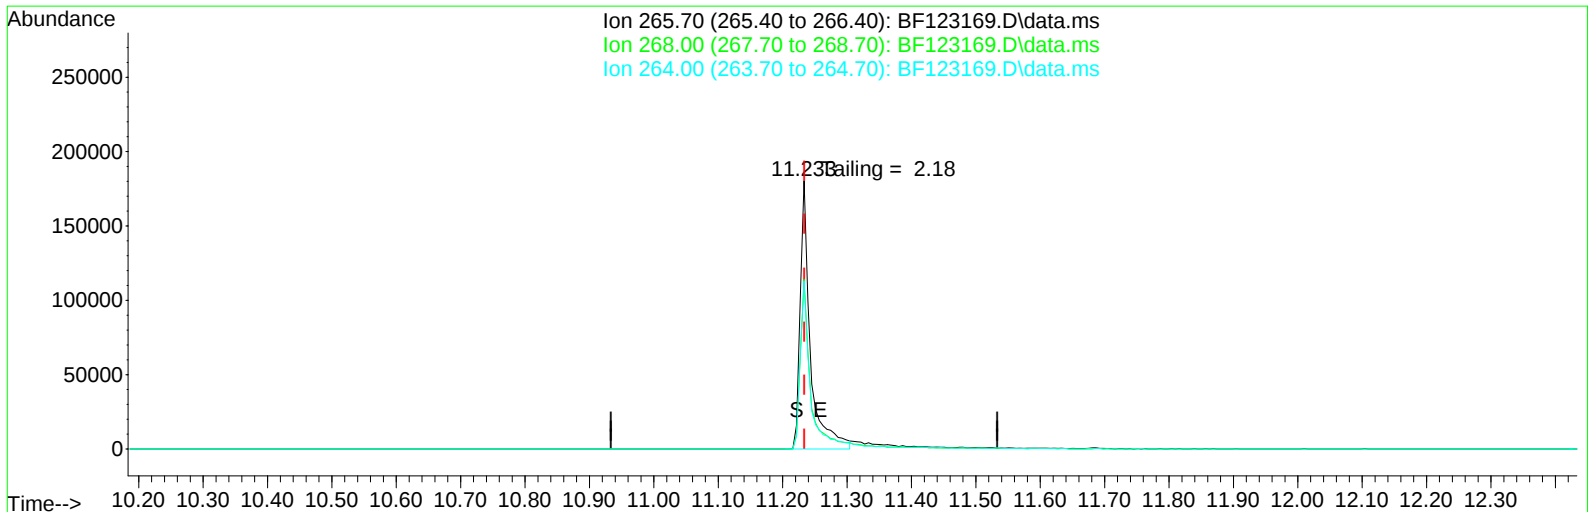

TIC: BF123169.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 28463.68 ng

response 221257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.21
264.00	62.30	62.62
0.00	0.00	0.00