
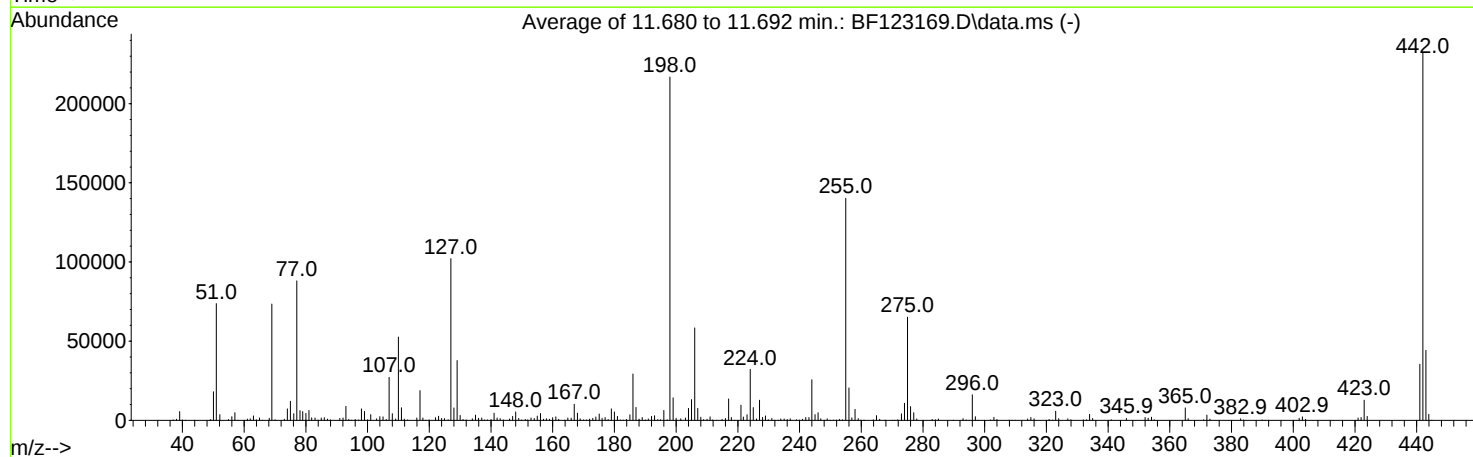


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021021\
 Data File : BF123169.D
 Acq On : 10 Feb 2021 12:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 11 01:29:27 2021

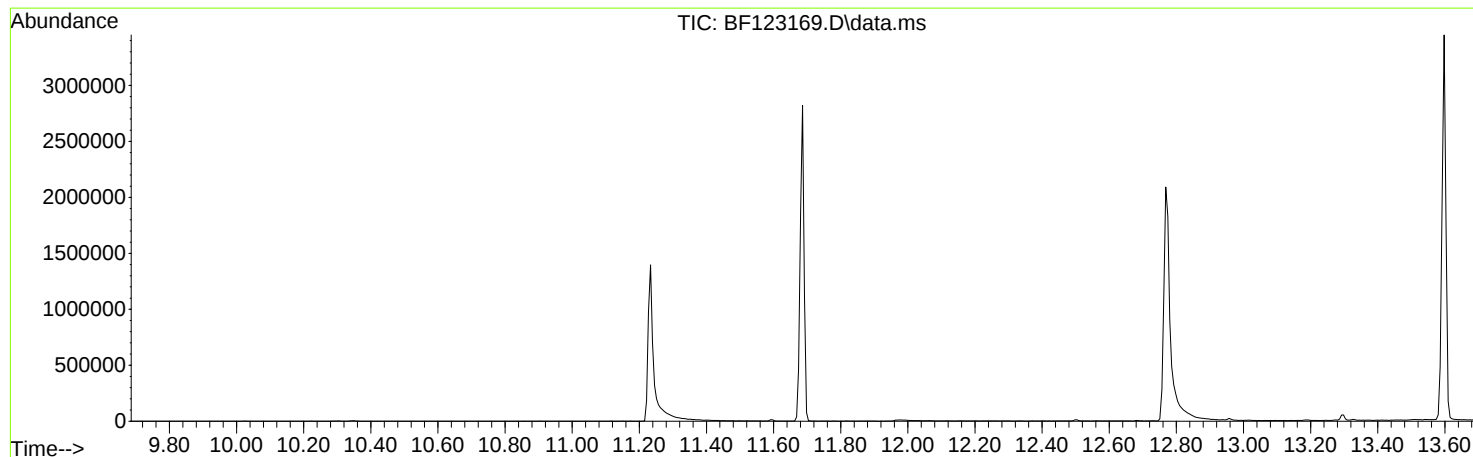

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	73720	PASS
68	69	0.00	2	1.9	1363	PASS
69	198	0.00	100	33.9	73467	PASS
70	69	0.00	2	0.5	373	PASS
127	198	10	80	47.1	102165	PASS
197	198	0.00	2	0.2	364	PASS
198	198	100	100	100.0	216840	PASS
199	198	5	9	6.6	14255	PASS
275	198	10	60	30.1	65163	PASS
365	198	1	100	3.6	7844	PASS
441	198	0.01	100	16.4	35488	PASS
442	442	50	100	100.0	232299	PASS
443	442	15	24	19.1	44267	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/10/2021	BNA_F	<u>BF123169.D</u>
Compound Name	Response	Retention Time
DDT	571648	13.59
DDD	10797	13.29
DDE	2103	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12900	584548	2.21

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021021\
 Data File : BF123169.D
 Acq On : 10 Feb 2021 12:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 10 15:16:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 29 12:29:00 2021
 Response via : Initial Calibration

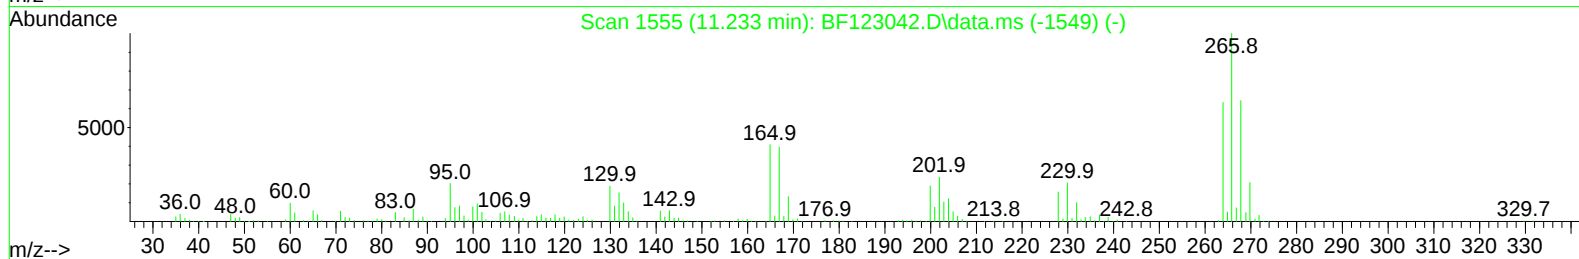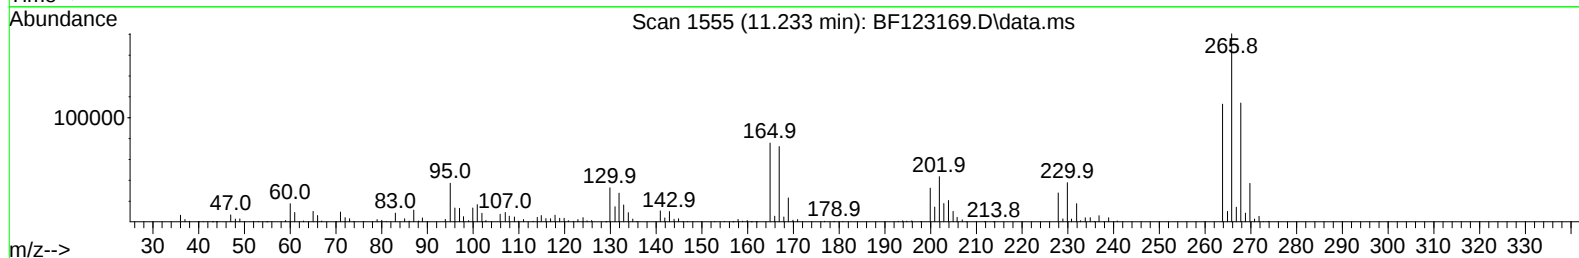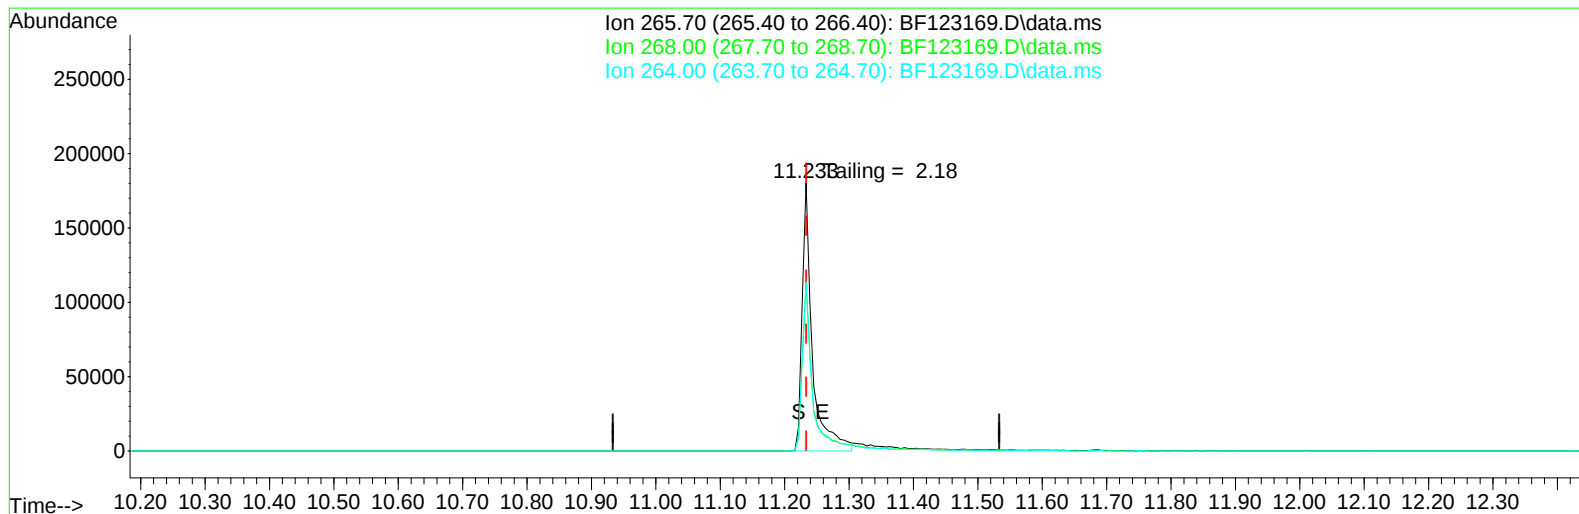

TIC: BF123169.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 28463.68 ng




response 221257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.21
264.00	62.30	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021021\
Data File : BF123169.D
Acq On : 10 Feb 2021 12:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 10 15:16:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 29 12:29:00 2021
Response via : Initial Calibration

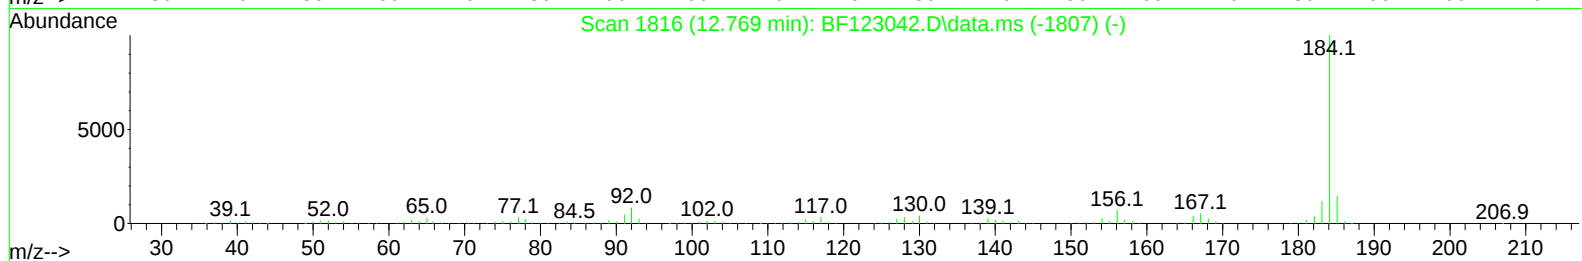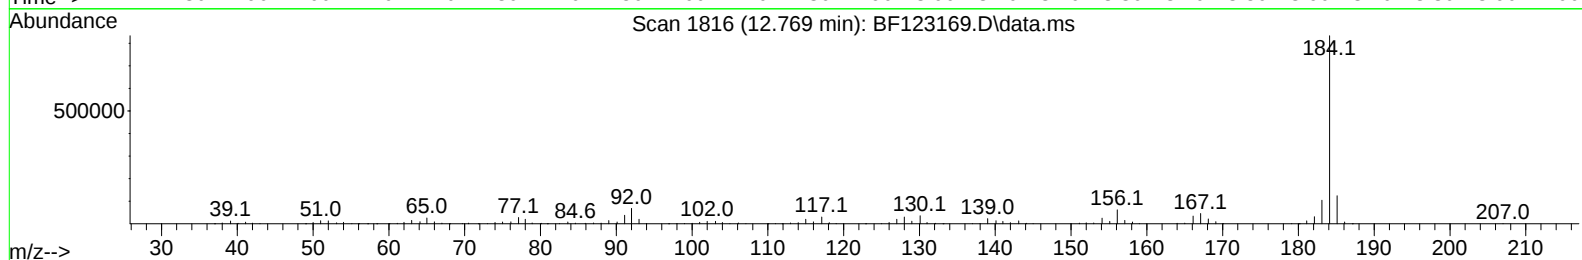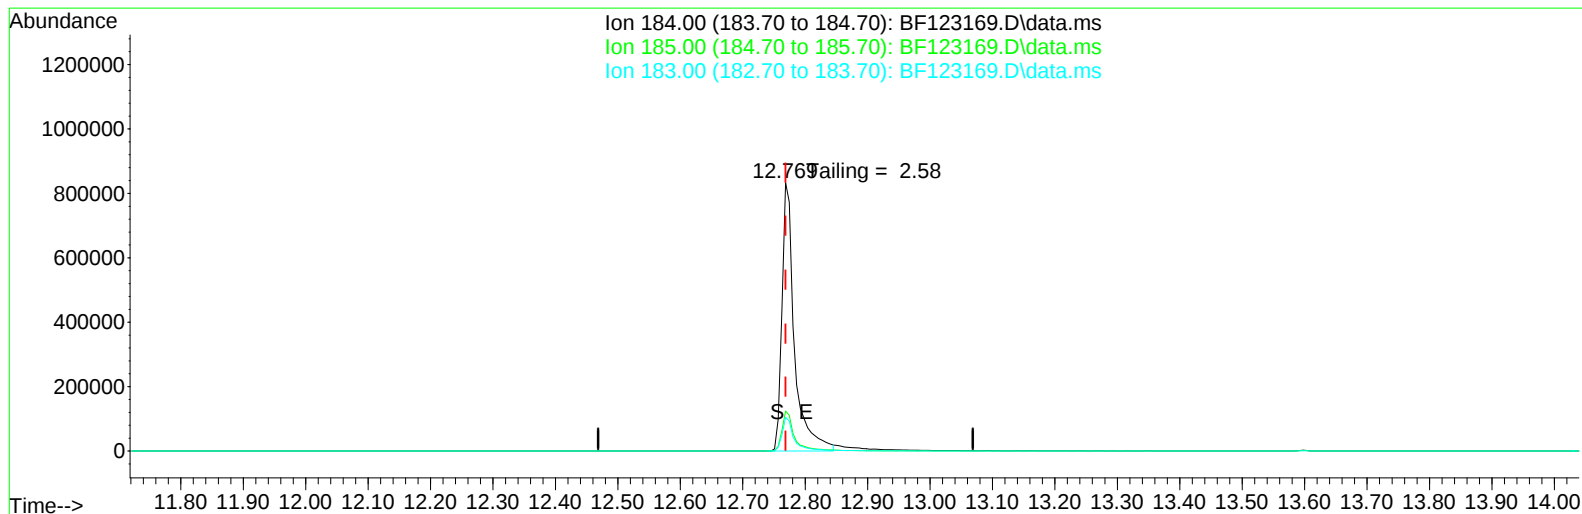

TIC: BF123169.D\data.ms

(77) Benzidine

12.769min (-0.000) 0.00 ng

response 1225370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.91
183.00	12.10	12.54
0.00	0.00	0.00