

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021119\
 Data File : BF112495.D
 Acq On : 11 Feb 2019 21:47
 Operator : JU/SJ
 Sample : K1450-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SHORE-RD-BOX-CULVERT-TP

Quant Time: Feb 12 00:01:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	116910	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	436441	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	184077	20.00	ng	-0.02
64) Phenanthrene-d10	11.36	188	293152	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	260339	20.00	ng	0.00
87) Perylene-d12	15.47	264	273559	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	796673	144.74	ng	0.00
7) Phenol-d6	6.49	99	889031	116.24	ng	0.00
23) Nitrobenzene-d5	7.40	82	688689	90.92	ng	-0.01
42) 2,4,6-Tribromophenol	10.66	330	262667	122.59	ng	-0.02
45) 2-Fluorobiphenyl	9.19	172	1335221	102.59	ng	-0.02
79) Terphenyl-d14	12.94	244	1109979	80.30	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.40	70	93505	17.730	ng	# 74
25) Isophorone	7.40	82	688680	57.956	ng	# 63
51) 2,6-Dinitrotoluene	9.87	165	23890	7.458	ng	# 33
57) 2,4-Dinitrotoluene	9.87	165	23890	5.859	ng	# 31
67) 4-Bromophenyl-phenylether	10.66	248	15916	4.616	ng	# 1
77) Benzidine	12.93	184	14878	2.076	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021119\
Data File : BF112495.D
Acq On : 11 Feb 2019 21:47
Operator : JU/SJ
Sample : K1450-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

Quant Time: Feb 12 00:01:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

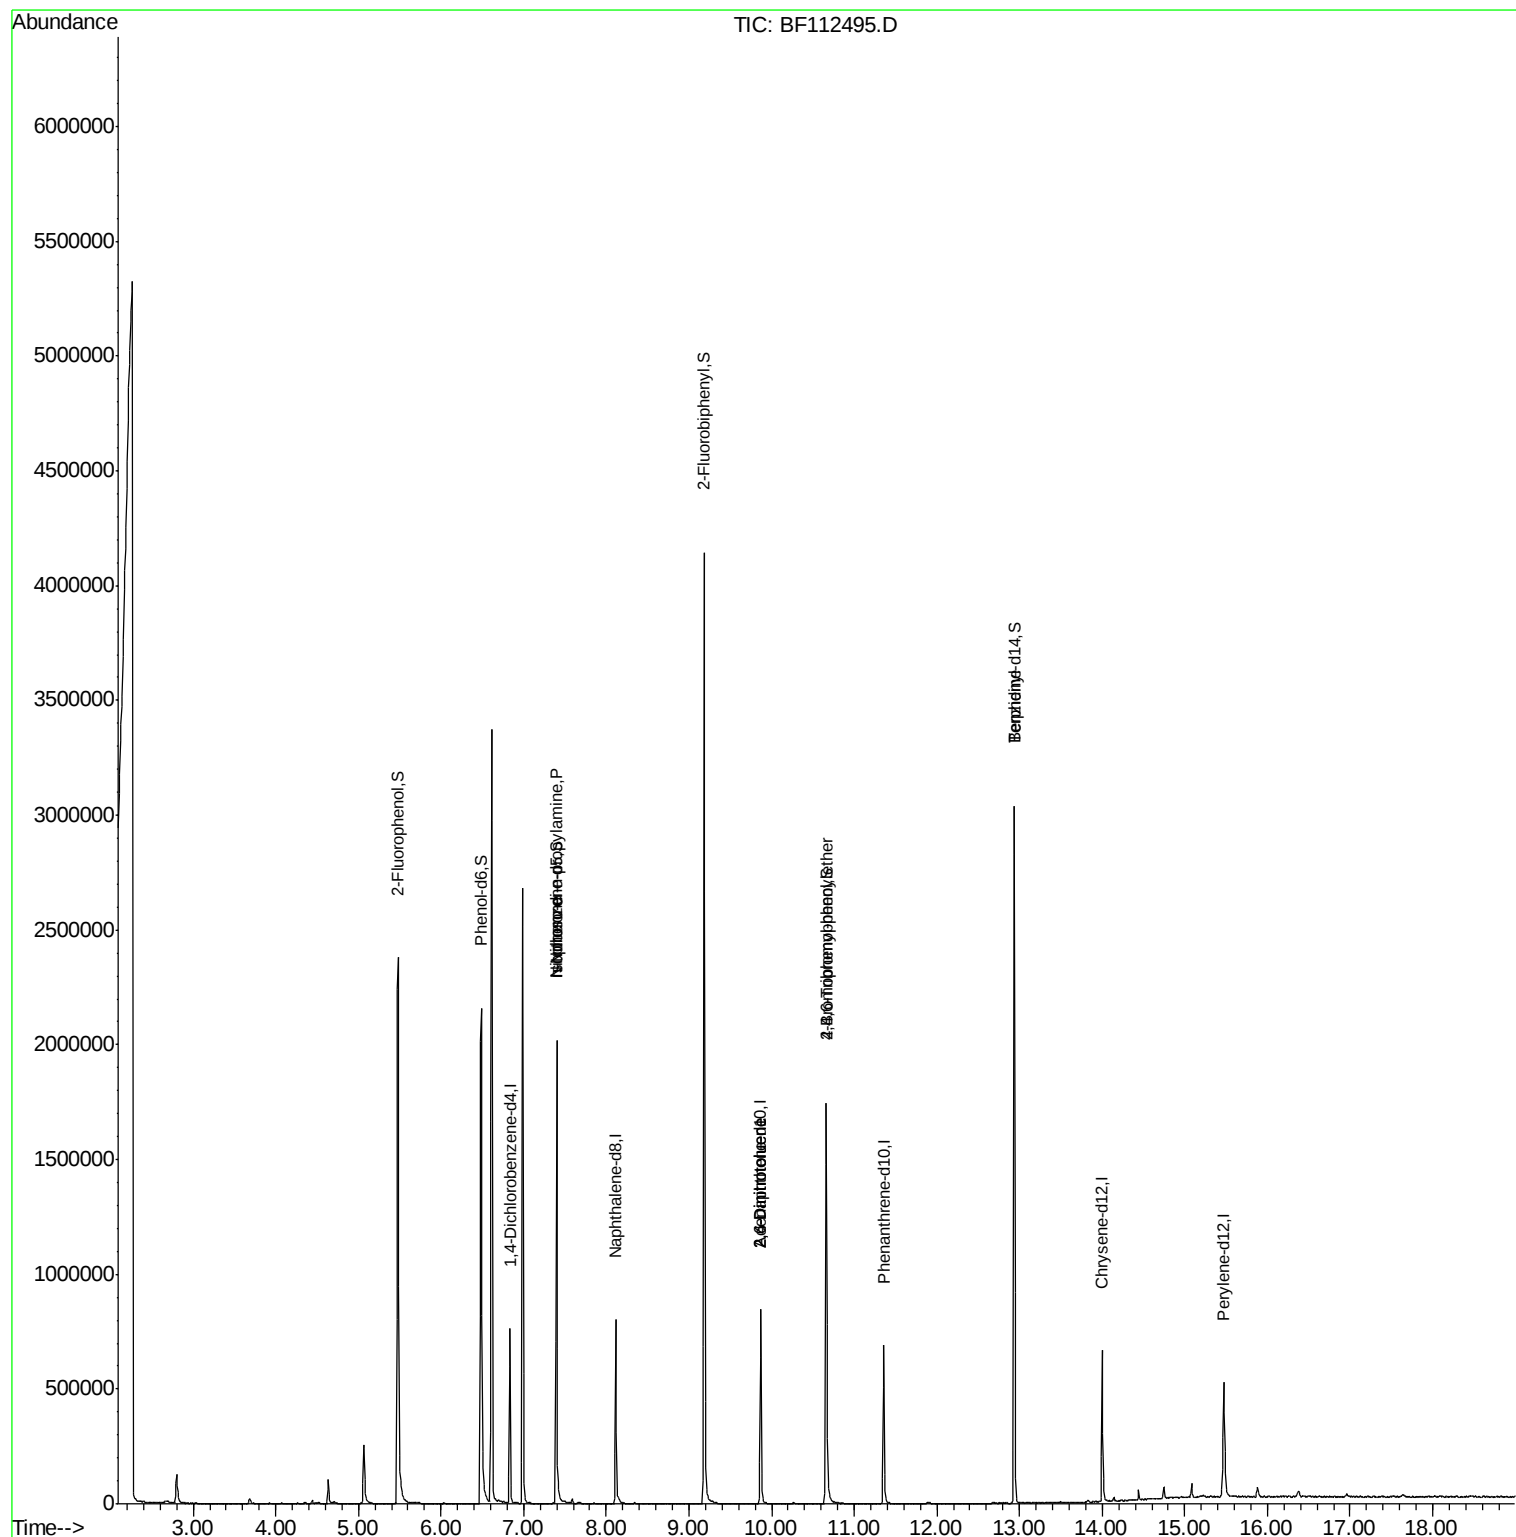




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF112495.D
Acq: 11 Feb 2019 21:47

Instrument :
BNA_F
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

Tgt Ion:152 Resp: 116910
Ion Ratio Lower Upper
152 100
150 152.9 127.4 191.0
115 57.4 45.5 68.3

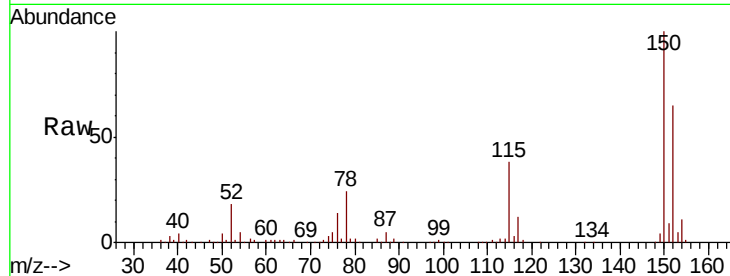


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

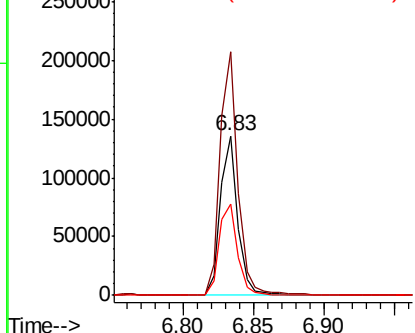



#5


2-Fluorophenol
Concen: 144.743 ng
RT: 5.48 min Scan# 577
Delta R.T. 0.00 min
Lab File: BF112495.D
Acq: 11 Feb 2019 21:47

Tgt Ion:112 Resp: 796673
Ion Ratio Lower Upper
112 100
64 53.4 45.7 68.5
63 29.2 23.6 35.4



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

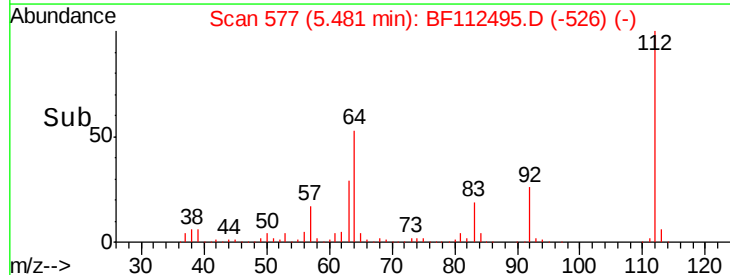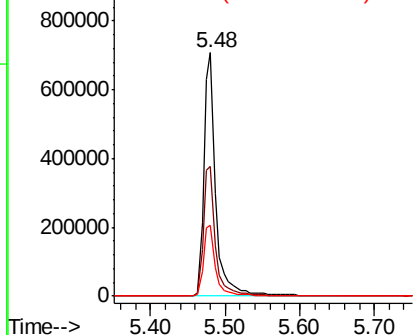

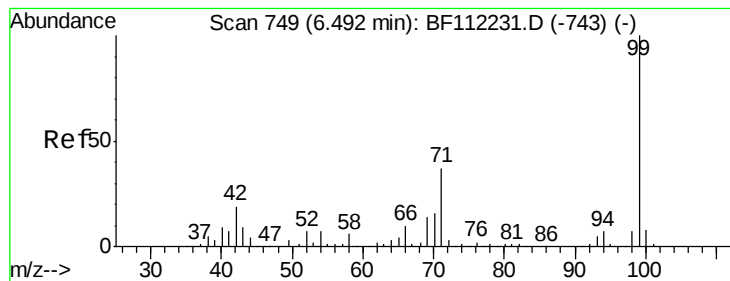

#7

Phenol-d6

Concen: 116.241 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112495.D

Acq: 11 Feb 2019 21:47

Instrument :

BNA_F

ClientSampleId :

SHORE-RD-BOX-CULVERT-TP





Tgt Ion: 99 Resp: 889031

Ion Ratio Lower Upper

99 100

42 17.6 15.1 22.7

71 36.3 26.9 40.3

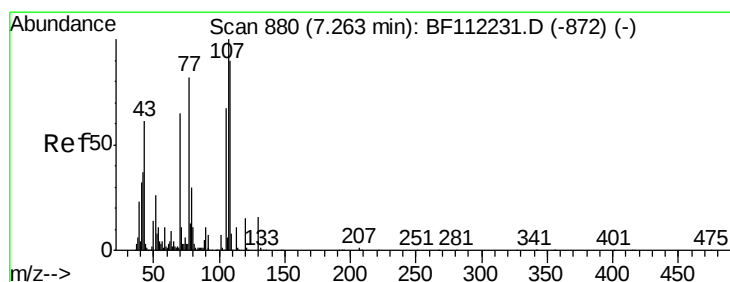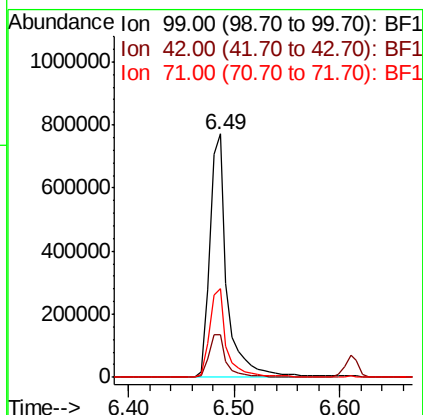

#19

n-Nitroso-di-n-propylamine

Concen: 17.730 ng

RT: 7.40 min Scan# 903

Delta R.T. 0.14 min

Lab File: BF112495.D

Acq: 11 Feb 2019 21:47

Tgt Ion: 70 Resp: 93505




Ion Ratio Lower Upper

70 100

42 45.0 47.6 71.4#

101 0.0 7.9 11.9#

130 1.8 18.4 27.6#

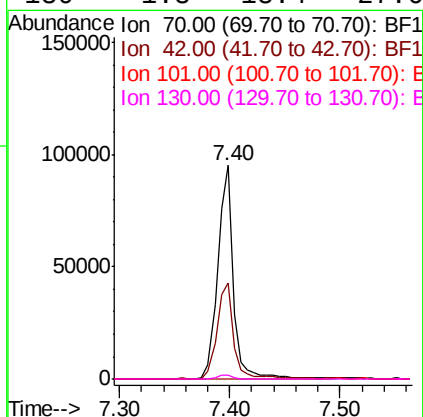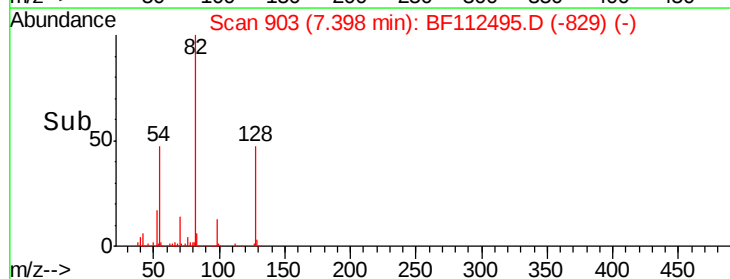



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112495.D

Acq: 11 Feb 2019 21:47

Instrument :

BNA_F

ClientSampleId :

SHORE-RD-BOX-CULVERT-TP

Tgt Ion: 136 Resp: 436441


Ion Ratio Lower Upper

136 100

137 10.4 9.1 13.7

54 5.3 5.9 8.9#

68 4.0 5.1 7.7#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

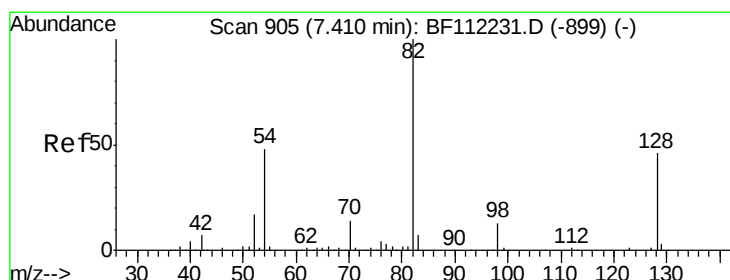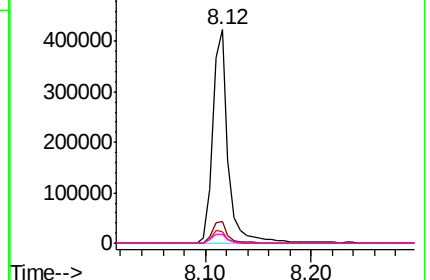

#23

Nitrobenzene-d5

Concen: 90.922 ng

RT: 7.40 min Scan# 903

Delta R.T. -0.01 min

Lab File: BF112495.D

Acq: 11 Feb 2019 21:47


Tgt Ion: 82 Resp: 688689

Ion Ratio Lower Upper

82 100

128 47.0 37.8 56.8



54 47.4 39.7 59.5




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

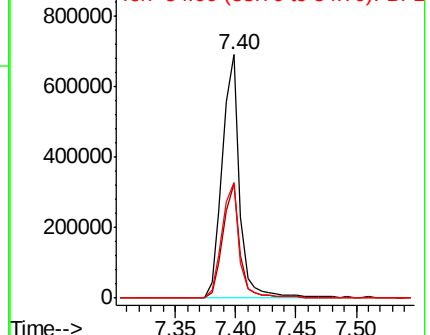

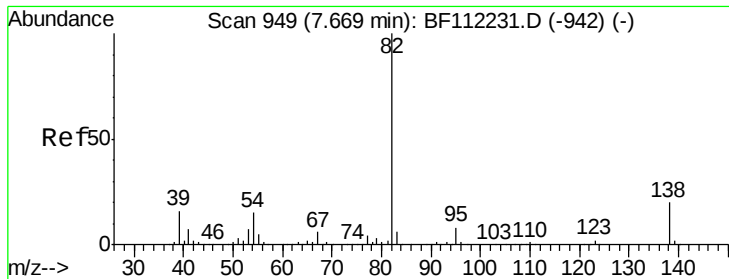

#25

Isophorone

Concen: 57.956 ng

RT: 7.40 min Scan# 903

Delta R.T. -0.27 min

Lab File: BF112495.D

Acq: 11 Feb 2019 21:47

Instrument :

BNA_F

ClientSampleId :

SHORE-RD-BOX-CULVERT-TP


Tgt Ion: 82 Resp: 688680

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#




138 0.0 15.4 23.0#

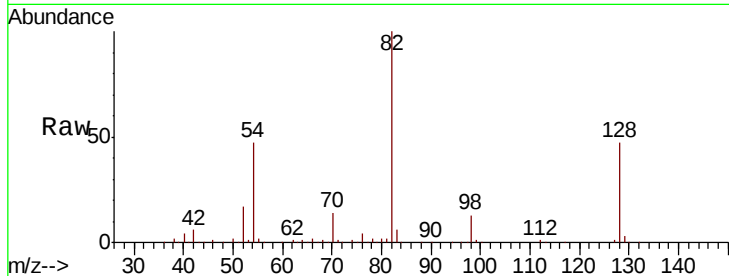

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

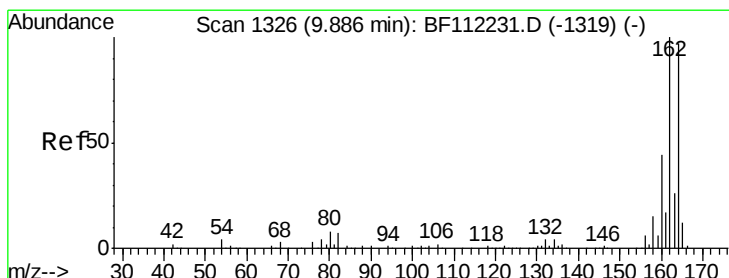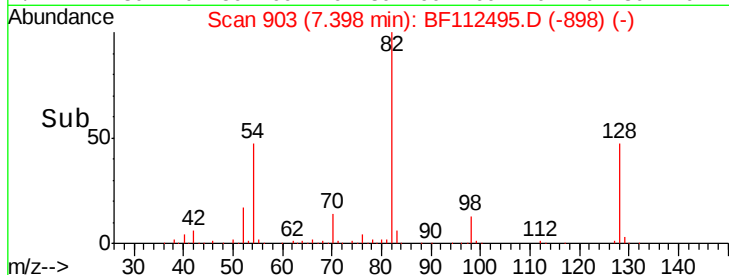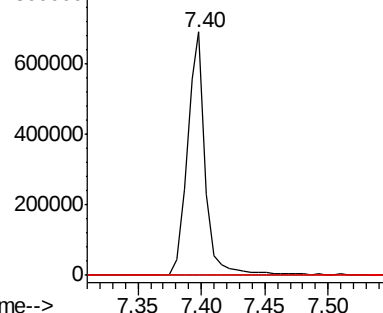

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.87 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BF112495.D

Acq: 11 Feb 2019 21:47


Tgt Ion: 164 Resp: 184077

Ion Ratio Lower Upper

164 100

162 106.6 82.2 123.4



160 47.3 36.2 54.4

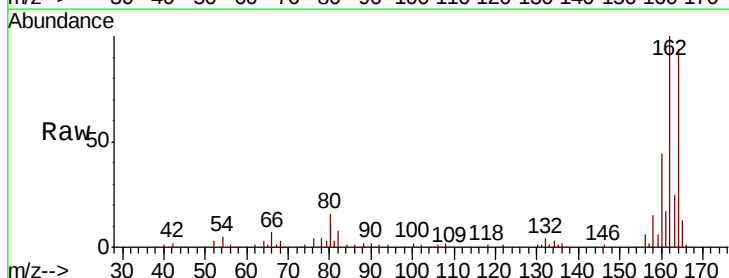

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

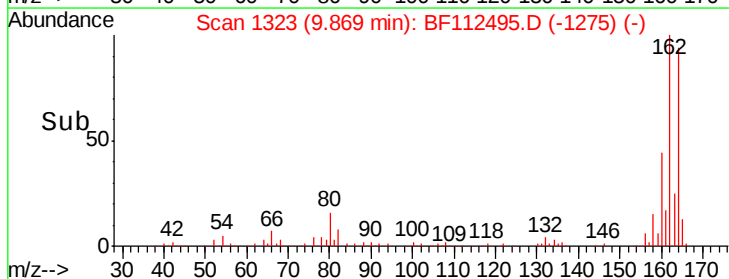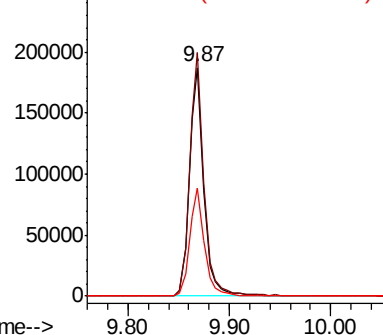







#42
 2,4,6-Tribromophenol
 Concen: 122.592 ng
 RT: 10.66 min Scan# 1458
 Delta R.T. -0.02 min
 Lab File: BF112495.D
 Acq: 11 Feb 2019 21:47

Instrument :
 BNA_F
 ClientSampleId :
 SHORE-RD-BOX-CULVERT-TP

Tgt Ion:330 Resp: 262667
 Ion Ratio Lower Upper
 330 100
 332 94.6 76.6 114.8
 141 32.3 24.3 36.5

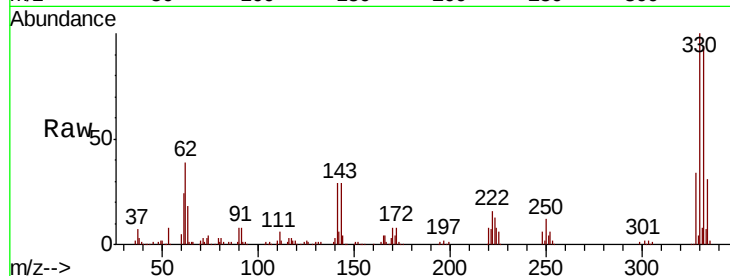


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


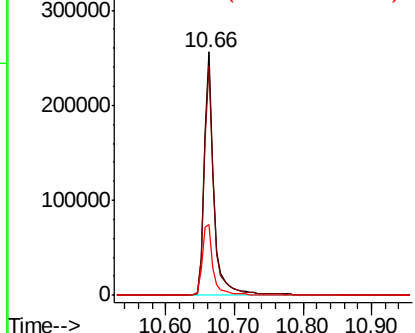



#45
 2-Fluorobiphenyl
 Concen: 102.590 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.02 min
 Lab File: BF112495.D
 Acq: 11 Feb 2019 21:47

Tgt Ion:172 Resp: 1335221
 Ion Ratio Lower Upper
 172 100
 171 37.1 30.5 45.7
 170 24.2 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

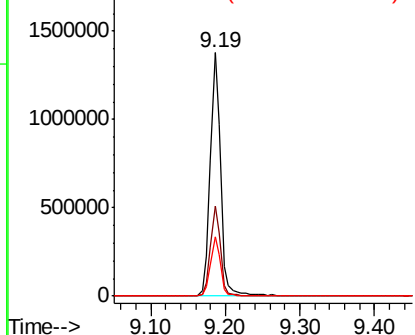


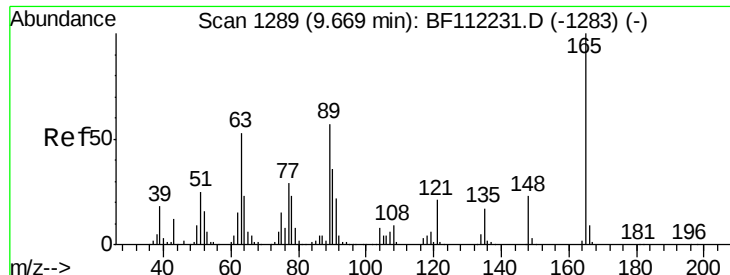




#51
 2,6-Dinitrotoluene
 Concen: 7.458 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. 0.20 min
 Lab File: BF112495.D
 Acq: 11 Feb 2019 21:47

Instrument :
 BNA_F
 ClientSampleId :
 SHORE-RD-BOX-CULVERT-TP

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.8	50.8#
89	1.4	36.9	55.3#

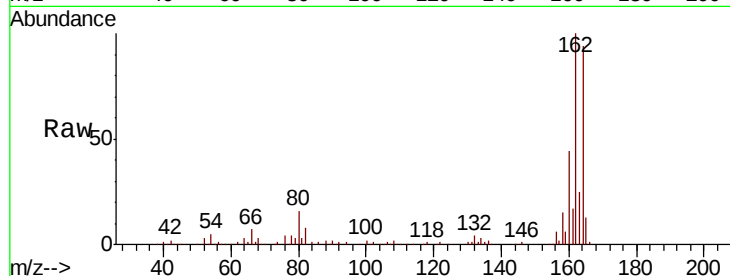




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

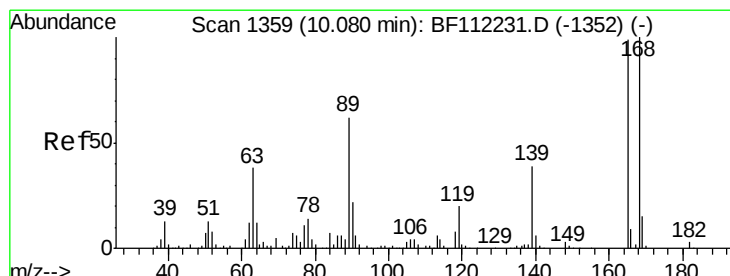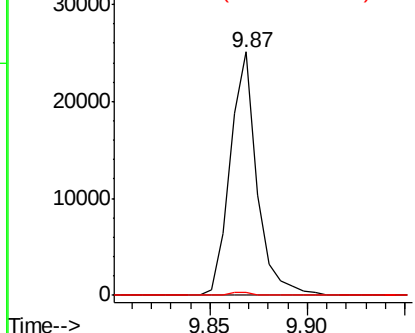


#57
 2,4-Dinitrotoluene
 Concen: 5.859 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.21 min
 Lab File: BF112495.D
 Acq: 11 Feb 2019 21:47

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	27.9	41.9#
89	1.4	47.9	71.9#
182	0.0	2.2	3.4#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E


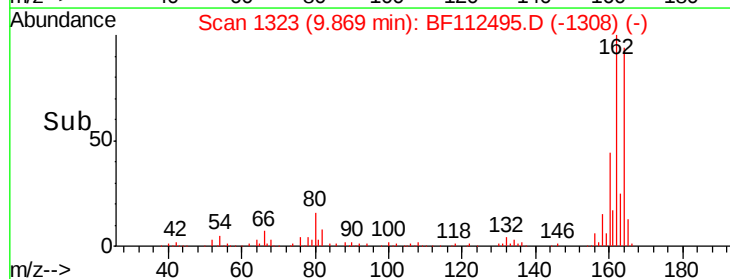
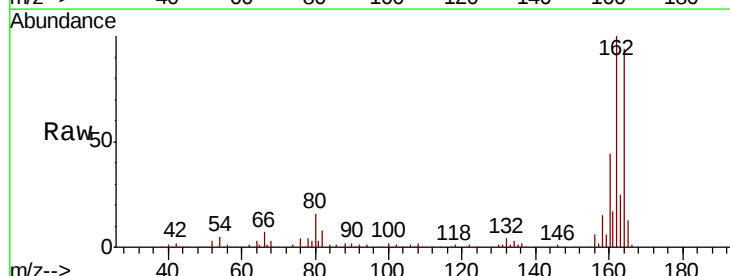
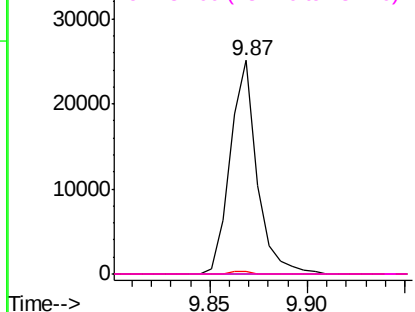


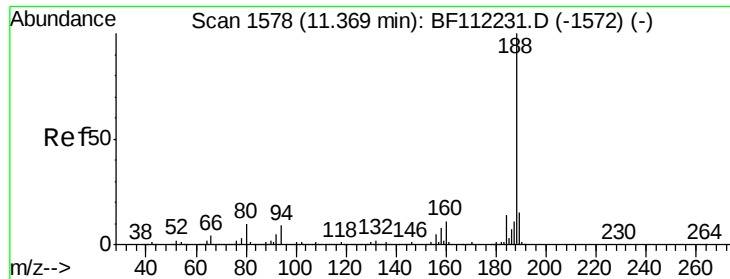

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1576
Delta R.T. -0.01 min
Lab File: BF112495.D
Acq: 11 Feb 2019 21:47




Instrument :
BNA_F
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP


Tgt Ion:188 Resp: 293152
Ion Ratio Lower Upper
188 100
94 7.7 8.2 12.2#
80 8.0 8.9 13.3#

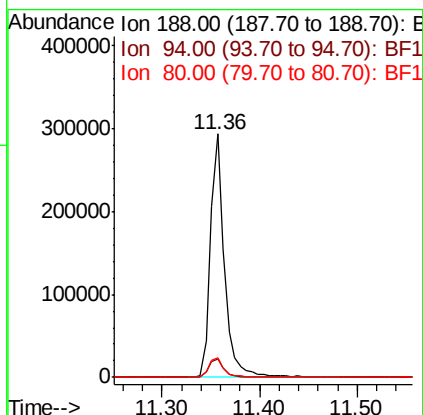

#67
4-Bromophenyl-phenylether
Concen: 4.616 ng
RT: 10.66 min Scan# 1458
Delta R.T. -0.25 min
Lab File: BF112495.D
Acq: 11 Feb 2019 21:47

Tgt Ion:248 Resp: 15916
Ion Ratio Lower Upper
248 100
250 192.0 79.7 119.5#
141 479.1 60.3 90.5#



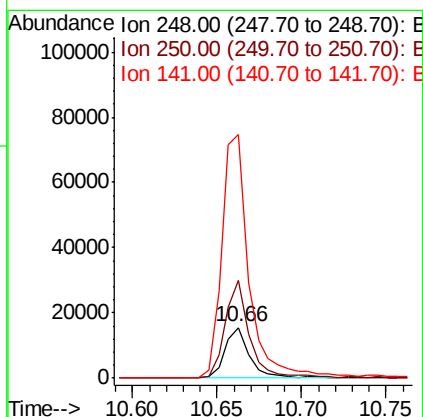





#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.01 min
Lab File: BF112495.D
Acq: 11 Feb 2019 21:47




Instrument :
BNA_F
ClientSampleId :
SHORE-RD-BOX-CULVERT-TP

Tgt Ion:240 Resp: 260339
Ion Ratio Lower Upper
240 100
120 10.1 9.0 13.6
236 25.4 20.7 31.1

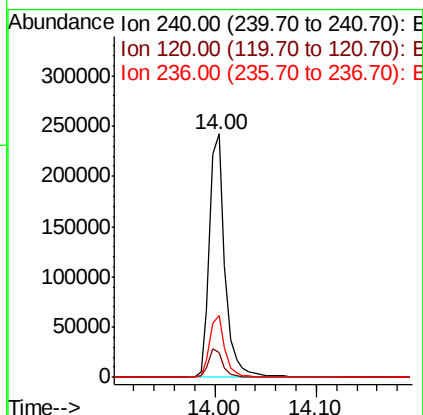

#77
Benzidine
Concen: 2.076 ng
RT: 12.93 min Scan# 1844
Delta R.T. 0.24 min
Lab File: BF112495.D
Acq: 11 Feb 2019 21:47

Tgt Ion:184 Resp: 14878
Ion Ratio Lower Upper
184 100
185 18.2 13.9 20.9
183 7.2 10.0 15.0#

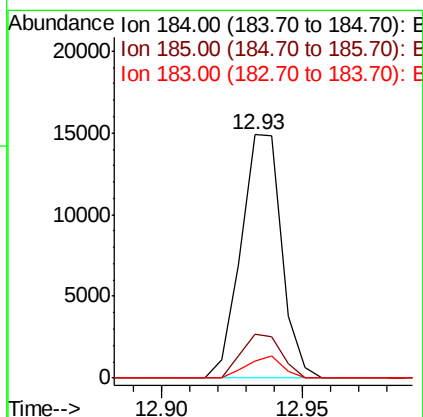







#79
 Terphenyl-d14
 Concen: 80.302 ng
 RT: 12.94 min Scan# 1845
 Delta R.T. -0.01 min
 Lab File: BF112495.D
 Acq: 11 Feb 2019 21:47

Instrument :
 BNA_F
 ClientSampleId :
 SHORE-RD-BOX-CULVERT-TP

Tgt Ion:244 Resp: 1109979
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.9 8.9
 122 10.0 9.8 14.6

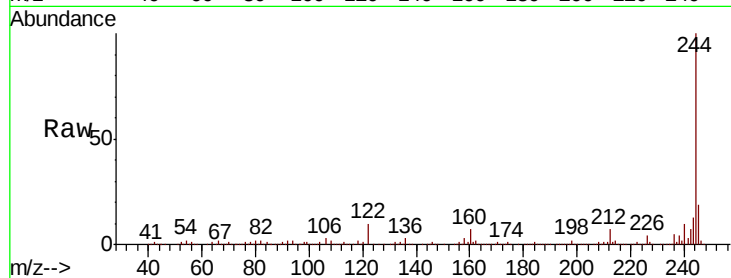


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

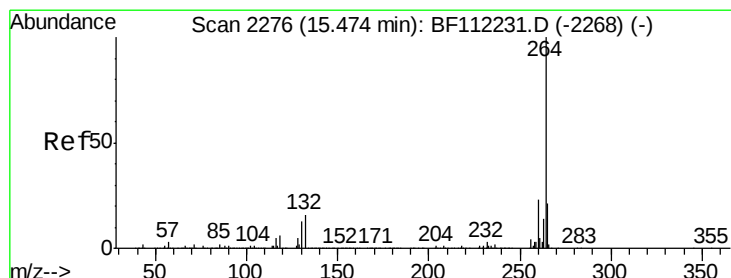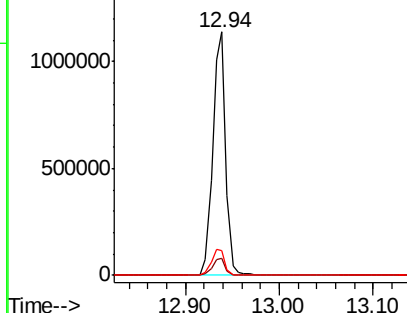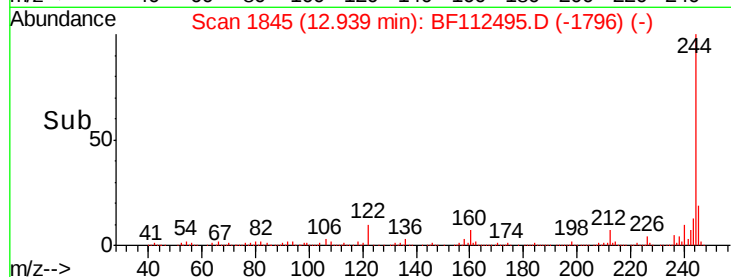

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2276
 Delta R.T. 0.00 min
 Lab File: BF112495.D
 Acq: 11 Feb 2019 21:47

Tgt Ion:264 Resp: 273559
 Ion Ratio Lower Upper
 264 100
 260 23.1 18.2 27.2
 265 21.8 17.0 25.4

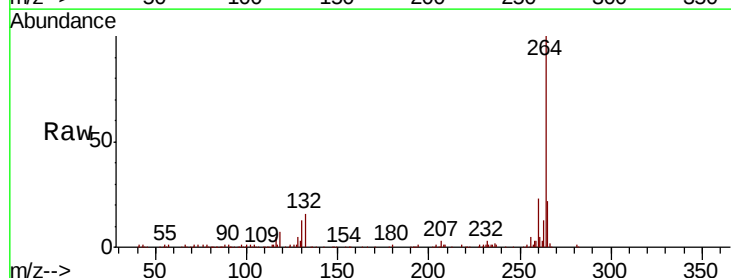

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

