

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021119\
 Data File : BF112498.D
 Acq On : 11 Feb 2019 23:08
 Operator : JU/SJ
 Sample : K1442-05 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-11

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	573	576	592	rBV	105515	185288	18.79%	2.544%
2	6.492	746	749	766	rBV	108290	233825	23.71%	3.210%
3	6.610	766	769	780	rVB	208426	249770	25.33%	3.429%
4	6.828	803	806	817	rBV	739961	721443	73.17%	9.904%
5	6.986	829	833	843	rBV	211286	217109	22.02%	2.980%
6	7.398	900	903	919	rBV	82296	138012	14.00%	1.895%
7	8.116	1021	1025	1042	rBV	828965	932114	94.53%	12.796%
8	9.186	1203	1207	1219	rBV	227265	273003	27.69%	3.748%
9	9.592	1272	1276	1283	rBB	8715	11115	1.13%	0.153%
10	9.869	1319	1323	1339	rBV	953212	986034	100.00%	13.536%
11	10.669	1456	1459	1473	rBV	74073	91786	9.31%	1.260%
12	11.357	1572	1576	1589	rBV	883030	910148	92.30%	12.495%
13	11.974	1677	1681	1684	rBV4	6448	10429	1.06%	0.143%
14	12.574	1780	1783	1788	rBV	48834	46322	4.70%	0.636%
15	12.804	1816	1822	1827	rBV	54891	67521	6.85%	0.927%
16	12.933	1841	1844	1854	rBV	242495	226357	22.96%	3.107%
17	13.333	1908	1912	1914	rBV4	8030	11552	1.17%	0.159%
18	13.498	1937	1940	1945	rBV7	10106	12319	1.25%	0.169%
19	13.962	2016	2019	2021	rBV3	10664	13271	1.35%	0.182%
20	13.998	2021	2025	2036	rVV	751061	882203	89.47%	12.111%
21	14.139	2046	2049	2052	rBV4	19422	21396	2.17%	0.294%
22	14.445	2099	2101	2104	rBV2	21768	13810	1.40%	0.190%
23	14.568	2119	2122	2127	rVB	41399	36127	3.66%	0.496%
24	14.751	2150	2153	2155	rBV2	22139	21220	2.15%	0.291%
25	15.080	2206	2209	2214	rVB3	57427	73222	7.43%	1.005%
26	15.474	2269	2276	2285	rBV	516278	751985	76.26%	10.323%
27	15.880	2342	2345	2352	rVB2	45762	63972	6.49%	0.878%
28	16.374	2426	2429	2436	rBV4	31048	46771	4.74%	0.642%
29	17.639	2642	2644	2651	rVB7	19291	36253	3.68%	0.498%


Sum of corrected areas: 7284377

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021119\
Data File : BF112498.D
Acq On : 11 Feb 2019 23:08
Operator : JU/SJ
Sample : K1442-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-11

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

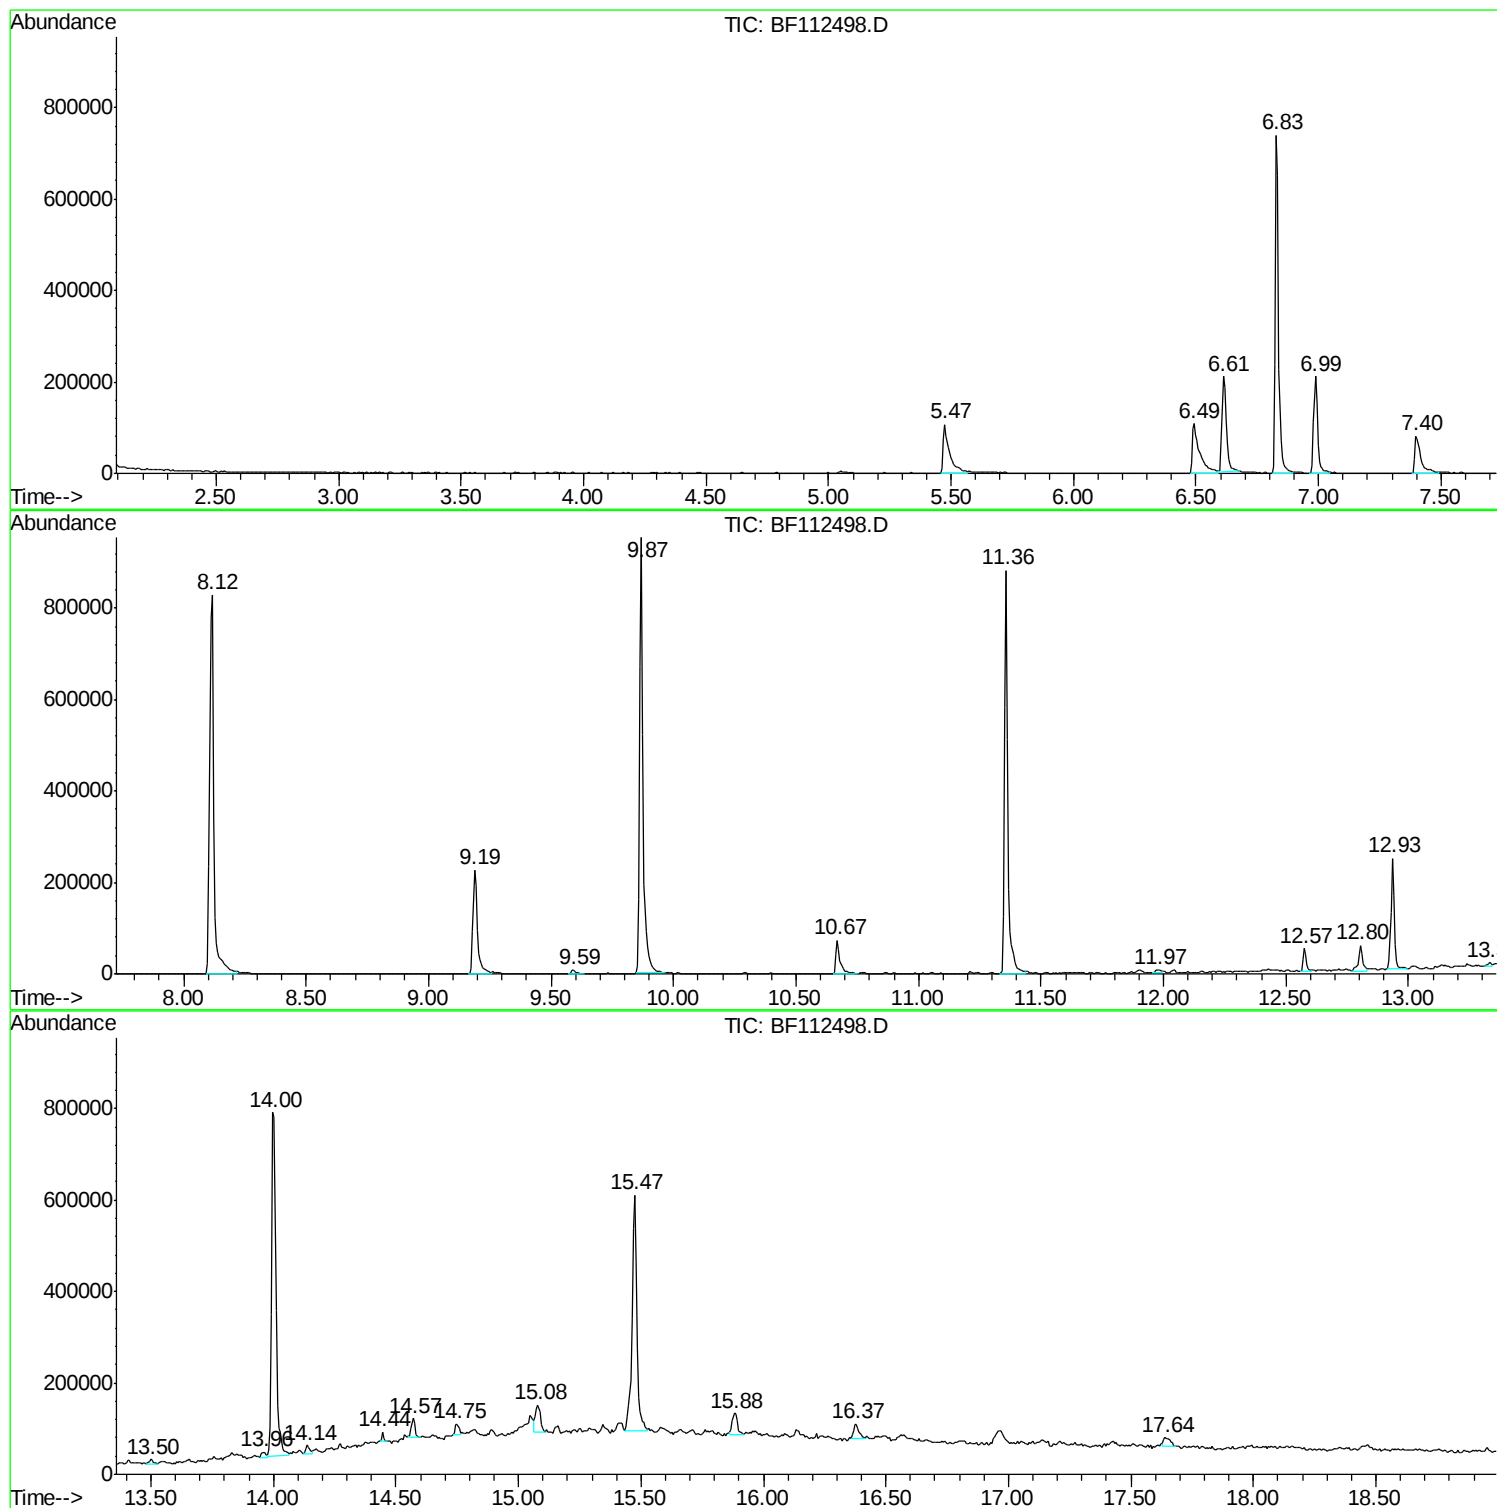

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021119\
Data File : BF112498.D
Acq On : 11 Feb 2019 23:08
Operator : JU/SJ
Sample : K1442-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-11










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	6.92 ng	249770	1,4-Dichlorobenzene-d4	6.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3			5-Aminoindole	132	C8H8N2	005192-03-0	12
4			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

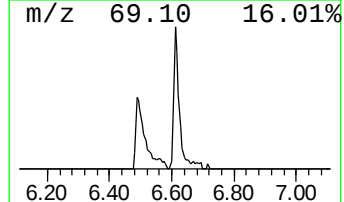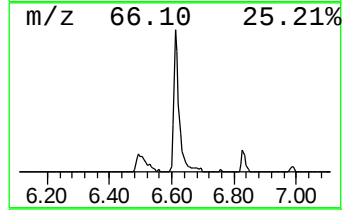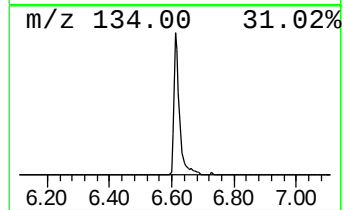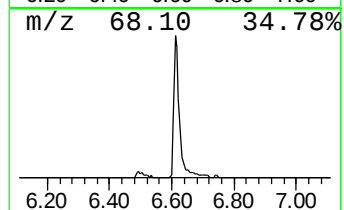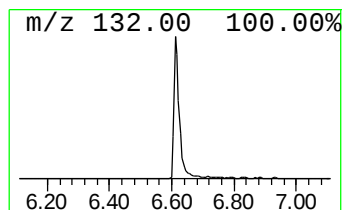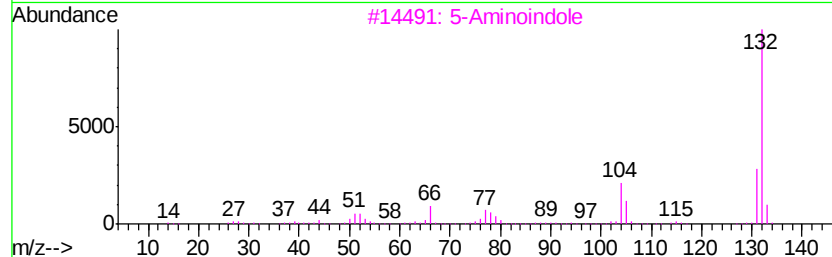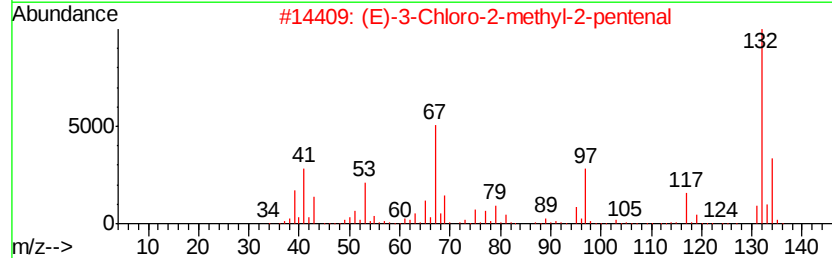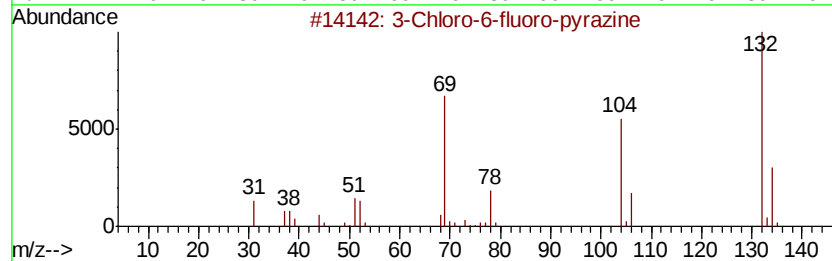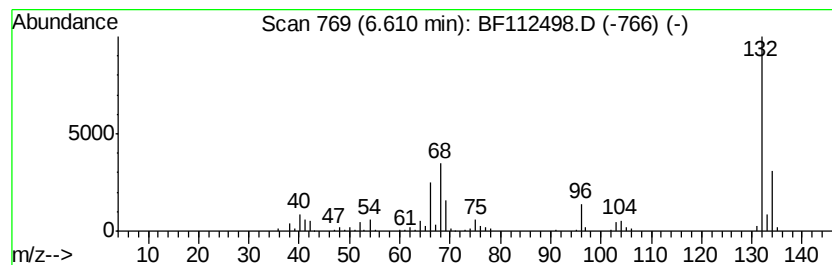

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021119\
Data File : BF112498.D
Acq On : 11 Feb 2019 23:08
Operator : JU/SJ
Sample : K1442-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-11

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.61	6.61	6.9	ng	249770	1	6.83	721443	20.0