


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021119\
 Data File : BF112476.D
 Acq On : 11 Feb 2019 12:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

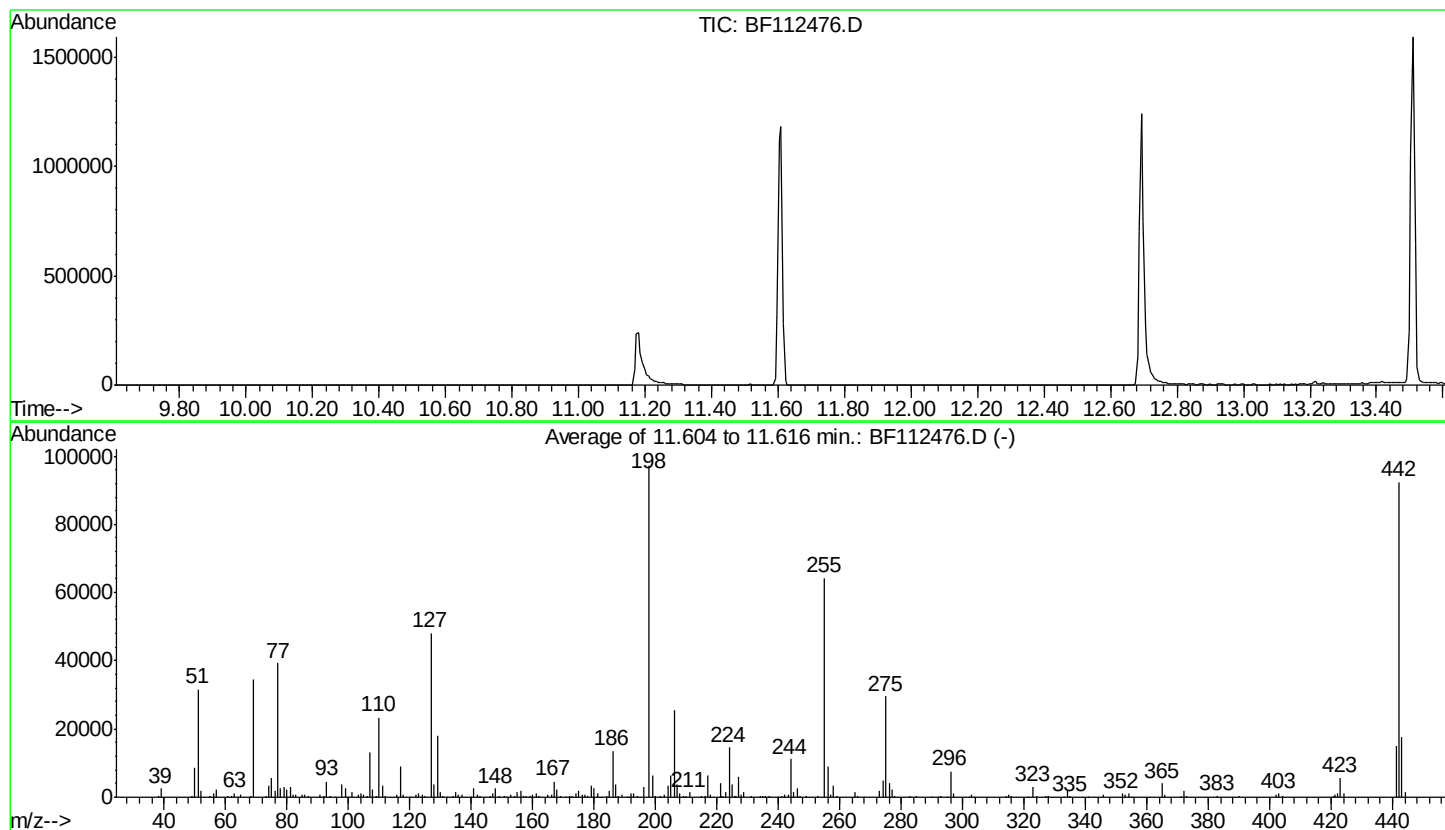

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	31526	PASS
68	69	0.00	2	1.3	436	PASS
69	198	0.00	100	35.5	34498	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	48208	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97208	PASS
199	198	5	9	6.7	6472	PASS
275	198	10	60	30.5	29604	PASS
365	198	1	100	4.1	4009	PASS
441	198	0.01	100	15.4	14991	PASS
442	198	50	100	95.0	92362	PASS
443	442	15	24	19.1	17624	PASS