
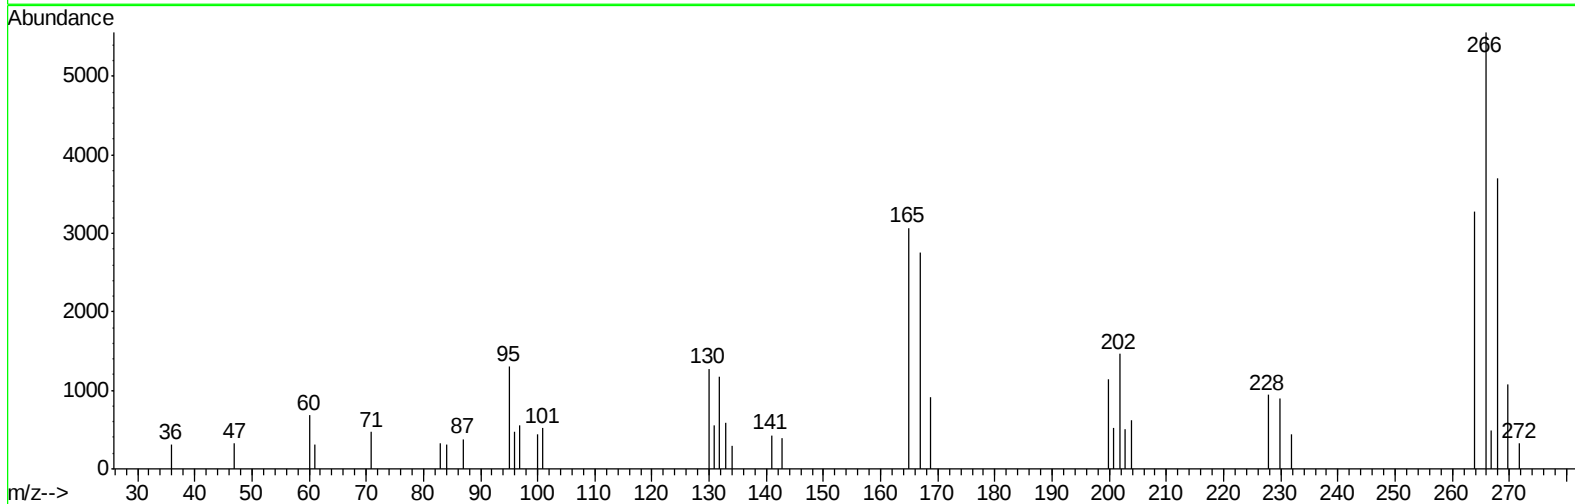


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021319\
Data File : BF112554.D
Acq On : 14 Feb 2019 00:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 08:06:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

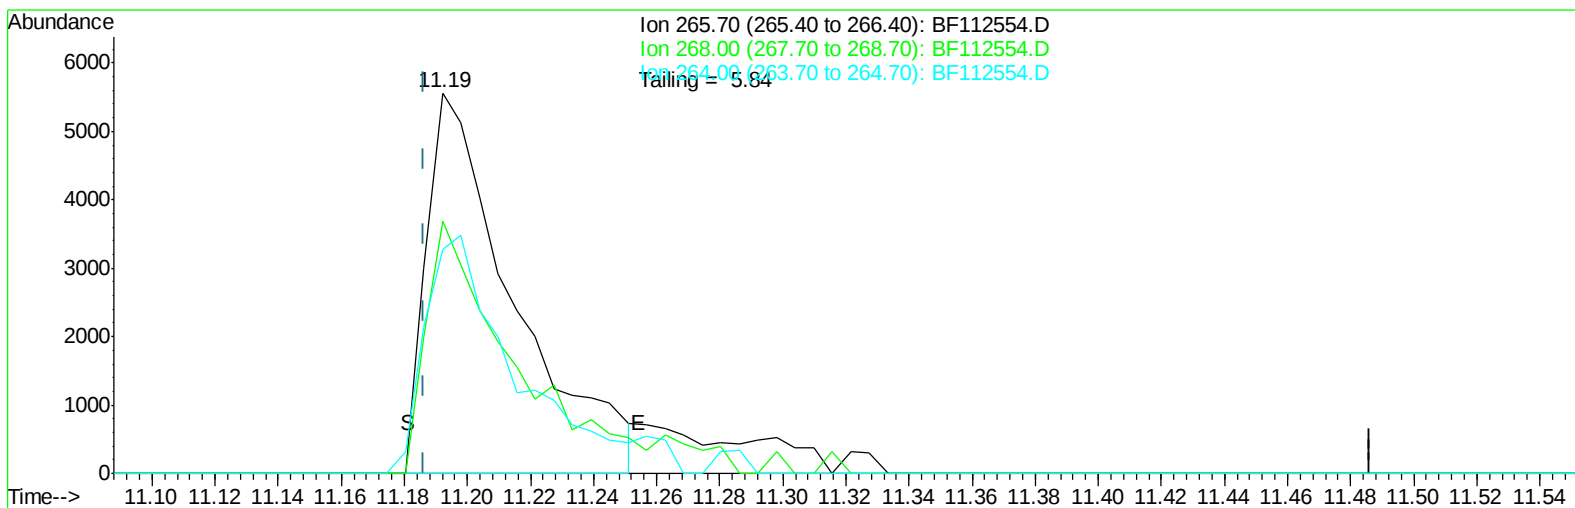

TIC: BF112554.D

(70) Pentachlorophenol (C)



11.192min (+0.006) 0.00ng

response 11821

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	66.49
264.00	63.60	59.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021319\
Data File : BF112554.D
Acq On : 14 Feb 2019 00:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 14 08:06:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

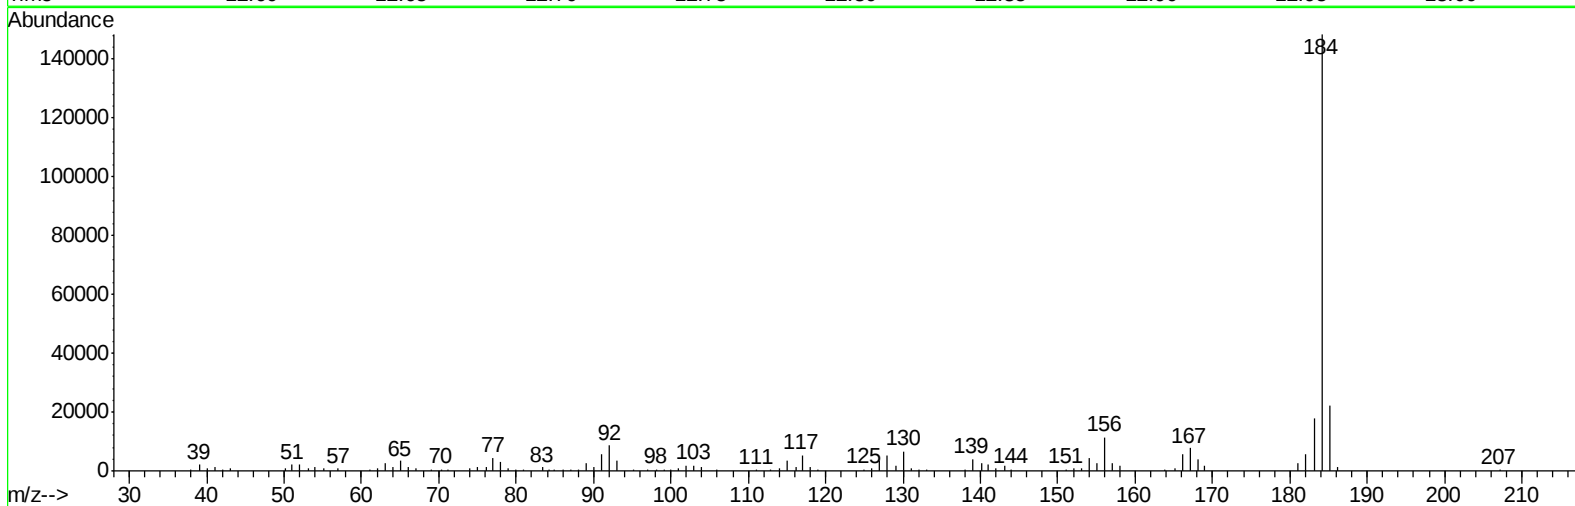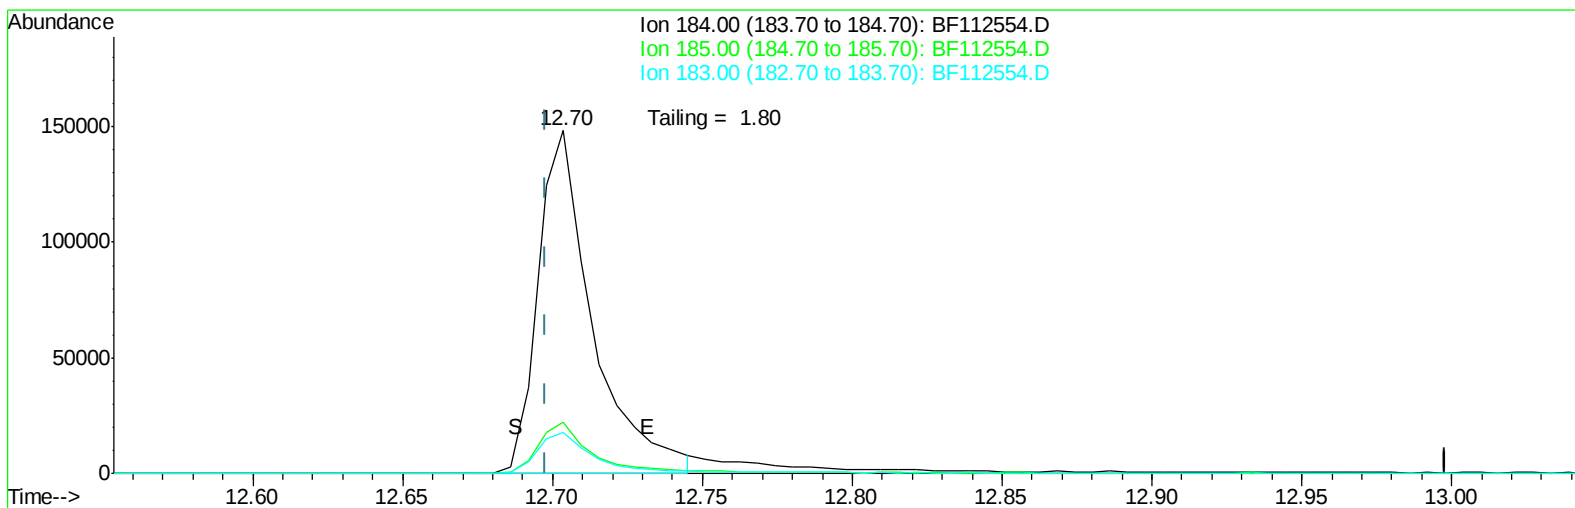

TIC: BF112554.D

(77) Benzidine

12.704min (+0.006) 26821.38ng

response 204486

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.84
183.00	12.50	11.99
0.00	0.00	0.00