

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021319\
 Data File : BF112530.D
 Acq On : 13 Feb 2019 11:06
 Operator : JU/SJ
 Sample : PB117061BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB117061BL

Quant Time: Feb 14 04:33:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	113863	20.00	ng	-0.01
21) Naphthalene-d8	8.12	136	438580	20.00	ng	-0.01
39) Acenaphthene-d10	9.87	164	221753	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	452180	20.00	ng	0.00
76) Chrysene-d12	14.02	240	370919	20.00	ng	0.00
87) Perylene-d12	15.50	264	307463	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	792579	147.85	ng	0.00
7) Phenol-d6	6.49	99	981055	131.71	ng	0.00
23) Nitrobenzene-d5	7.40	82	628619	82.59	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	332198	128.70	ng	0.00
45) 2-Fluorobiphenyl	9.19	172	1335611	85.19	ng	-0.01
79) Terphenyl-d14	12.95	244	1545405	78.47	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021319\
Data File : BF112530.D
Acq On : 13 Feb 2019 11:06
Operator : JU/SJ
Sample : PB117061BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB117061BL

Quant Time: Feb 14 04:33:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

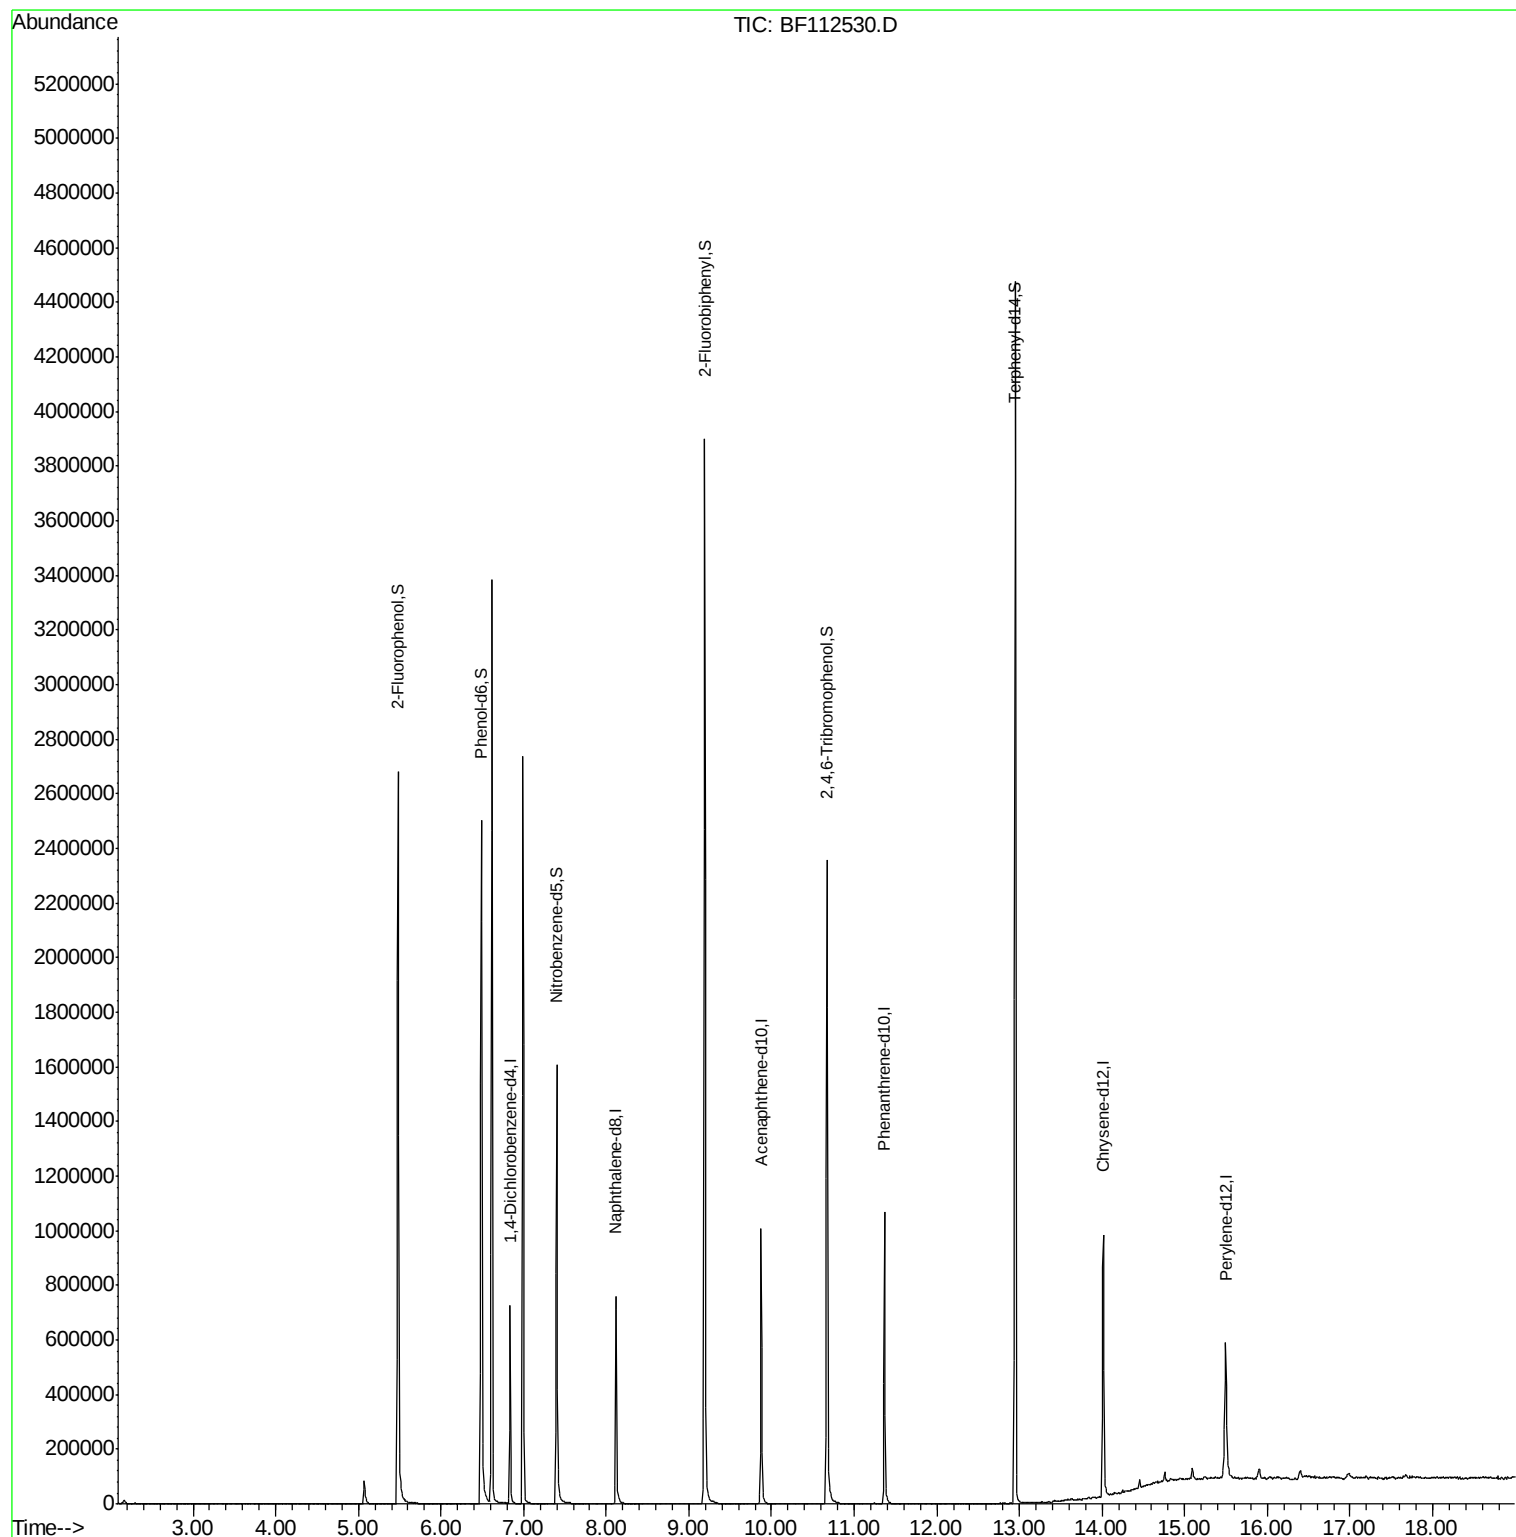

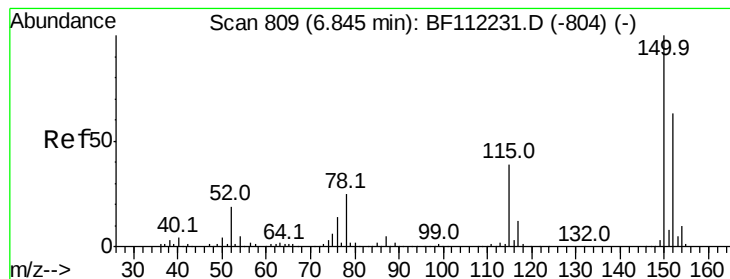


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 807
 Delta R.T. -0.01 min
 Lab File: BF112530.D
 Acq: 13 Feb 2019 11:06

Instrument :
 BNA_F
 ClientSampleId :
 PB117061BL

Tot Ion:152 Resp: 113863
 Ion Ratio Lower Upper
 152 100
 150 157.0 127.4 191.0
 115 62.5 45.5 68.3

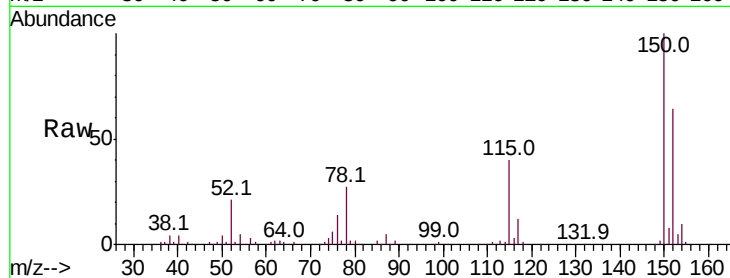


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

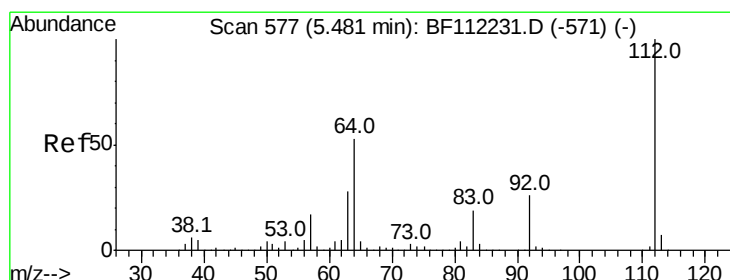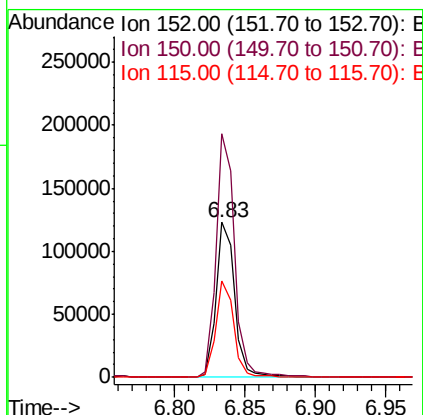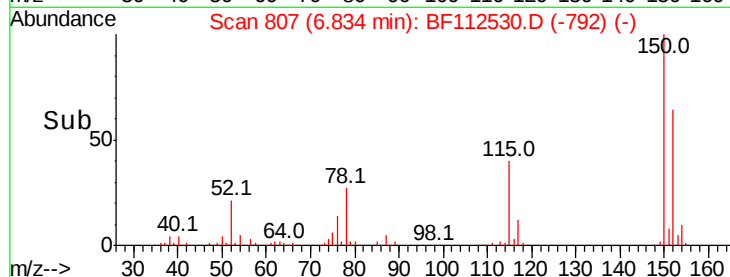



#5


2-Fluorophenol
 Concen: 147.852 ng
 RT: 5.48 min Scan# 577
 Delta R.T. 0.00 min
 Lab File: BF112530.D
 Acq: 13 Feb 2019 11:06

Tgt Ion:112 Resp: 792579
 Ion Ratio Lower Upper
 112 100
 64 55.4 45.7 68.5
 63 29.7 23.6 35.4

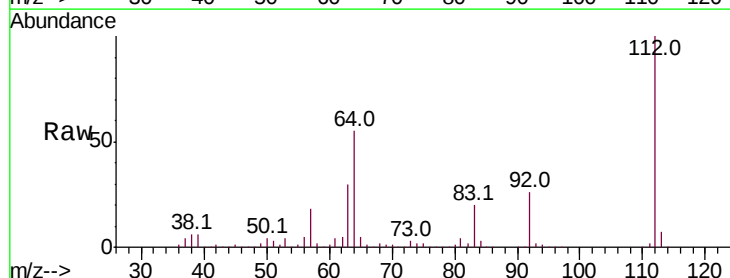

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

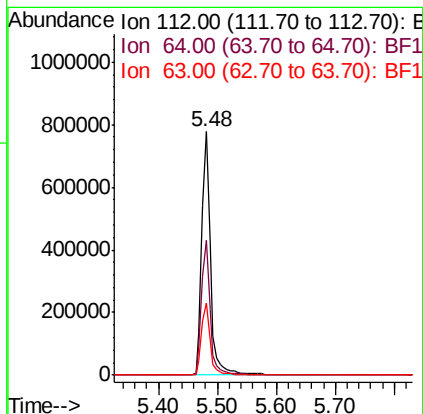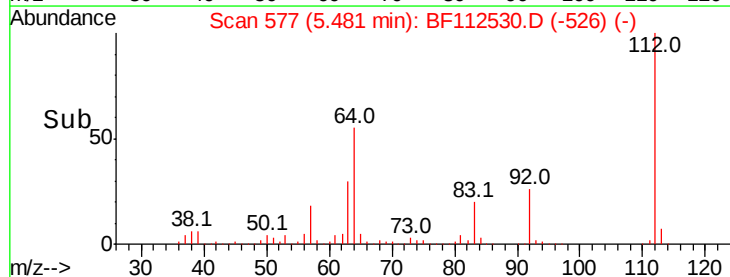

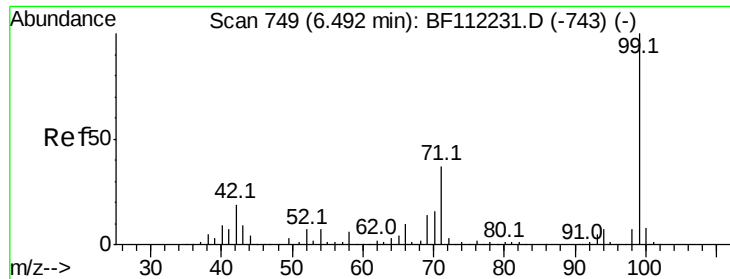

#7

Phenol-d6

Concen: 131.706 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.01 min

Lab File: BF112530.D

Acq: 13 Feb 2019 11:06

Instrument :

BNA_F

ClientSampleId :

PB117061BL


Tot Ion: 99 Resp: 981055

Ion Ratio Lower Upper




99 100

42 20.1 15.1 22.7

71 38.3 26.9 40.3

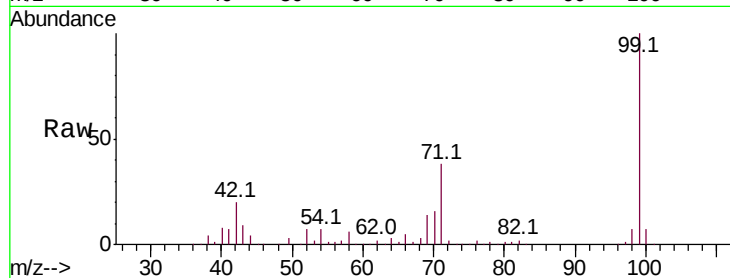

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

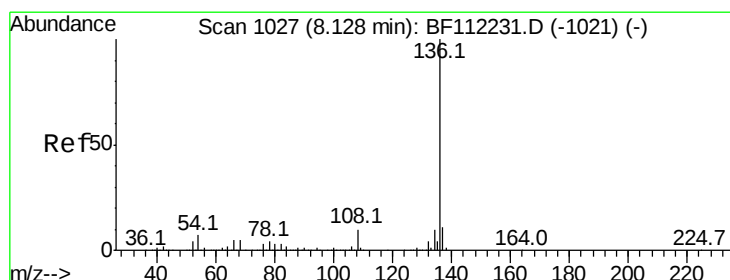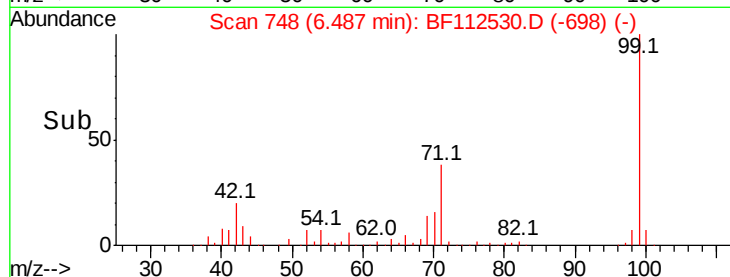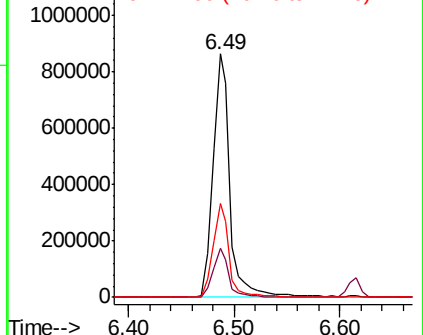

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF112530.D

Acq: 13 Feb 2019 11:06

Tgt Ion: 136 Resp: 438580


Ion Ratio Lower Upper

136 100



137 11.0 9.1 13.7


54 6.7 5.9 8.9

68 4.9 5.1 7.7#

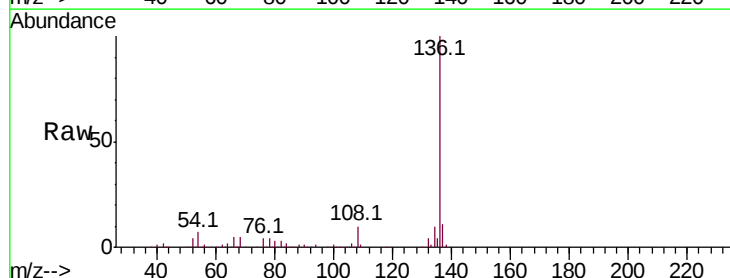

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

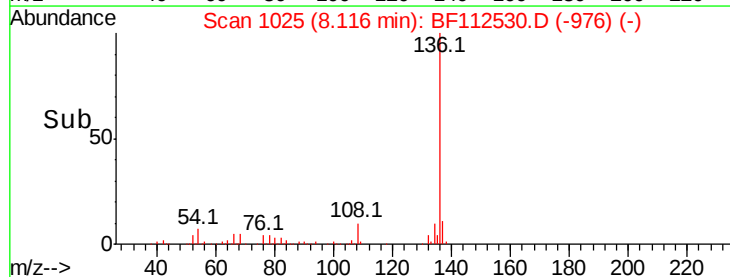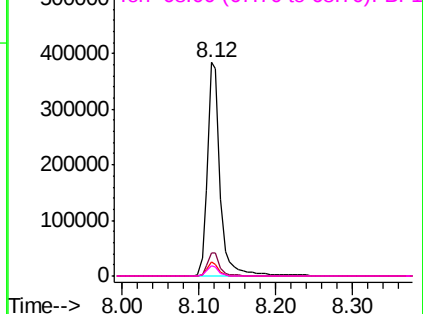


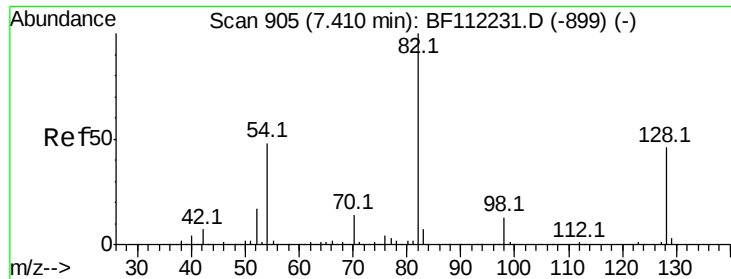




#23
 Nitrobenzene-d5
 Concen: 82.587 ng
 RT: 7.40 min Scan# 904
 Delta R.T. -0.01 min
 Lab File: BF112530.D
 Acq: 13 Feb 2019 11:06

Instrument :
 BNA_F
 ClientSampleId :
 PB117061BL

Tot Ion	Ratio	Lower	Upper
82	100		
128	48.1	37.8	56.8
54	45.4	39.7	59.5

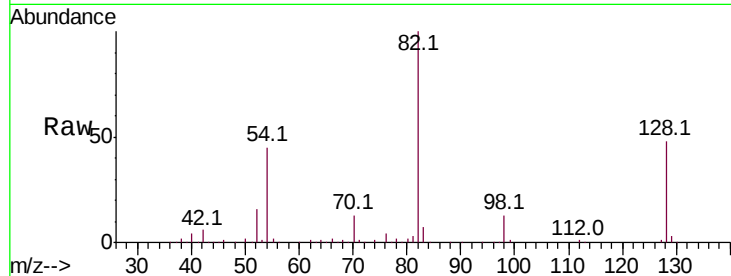


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

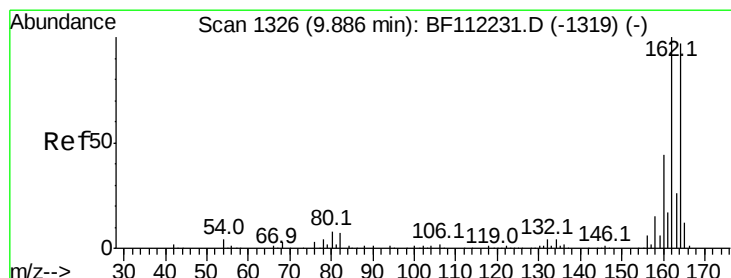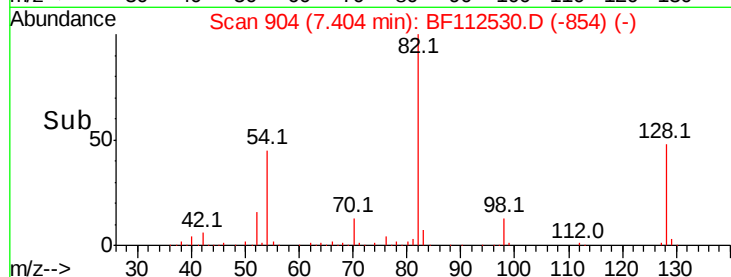
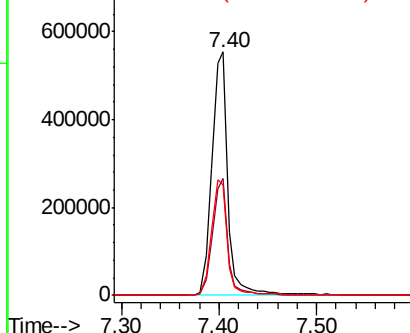



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1324
 Delta R.T. -0.01 min
 Lab File: BF112530.D
 Acq: 13 Feb 2019 11:06

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.8	82.2	123.4
160	46.9	36.2	54.4

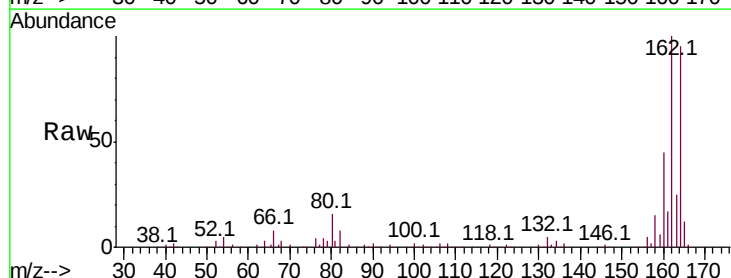

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

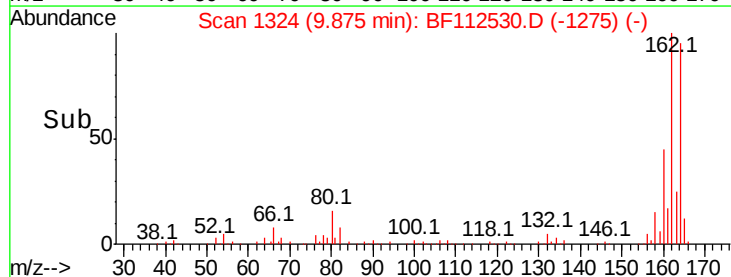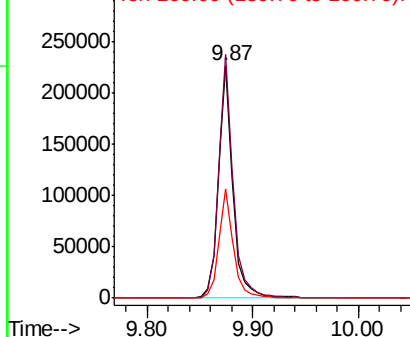


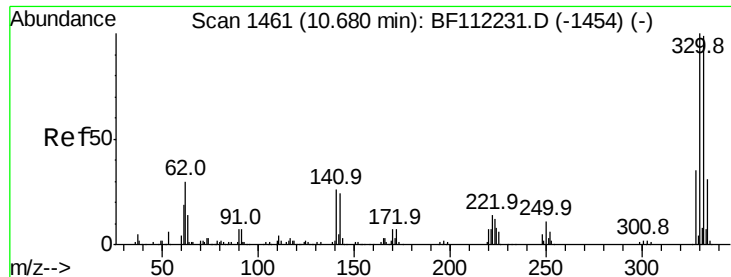




#42
 2,4,6-Tribromophenol
 Concen: 128.702 ng
 RT: 10.67 min Scan# 1460
 Delta R.T. -0.01 min
 Lab File: BF112530.D
 Acq: 13 Feb 2019 11:06

Instrument :
 BNA_F
 ClientSampleId :
 PB117061BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	76.6	114.8
141	32.8	24.3	36.5

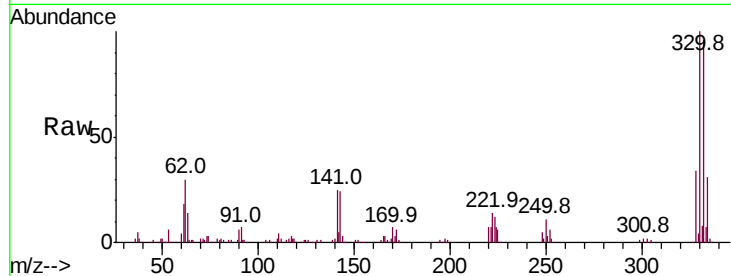


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

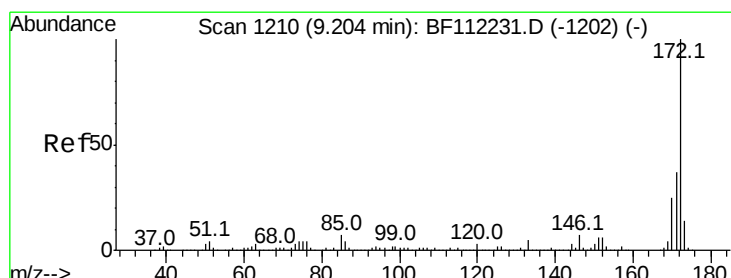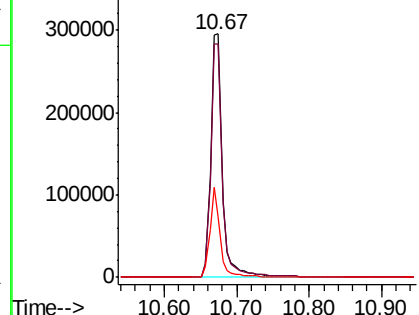
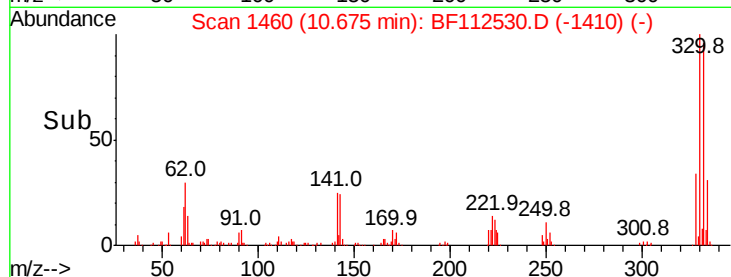



#45
 2-Fluorobiphenyl
 Concen: 85.185 ng
 RT: 9.19 min Scan# 1208
 Delta R.T. -0.01 min
 Lab File: BF112530.D
 Acq: 13 Feb 2019 11:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	30.5	45.7
170	24.0	20.2	30.4

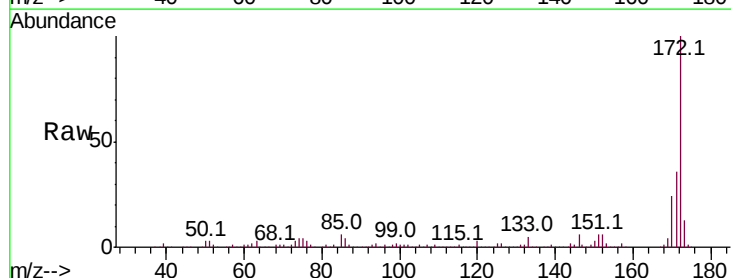

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



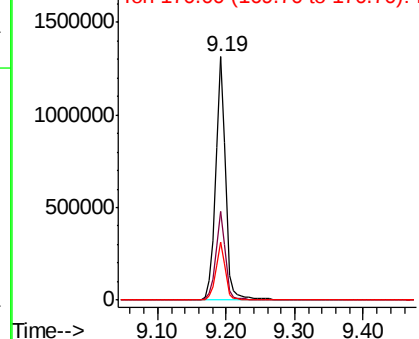
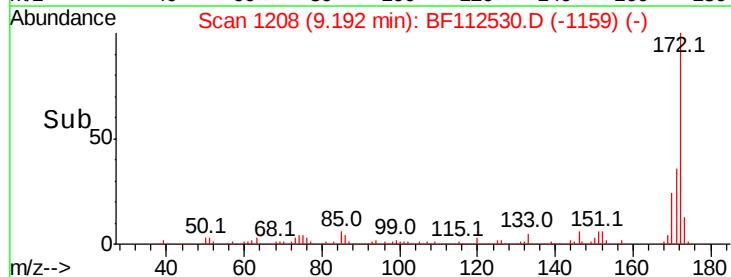


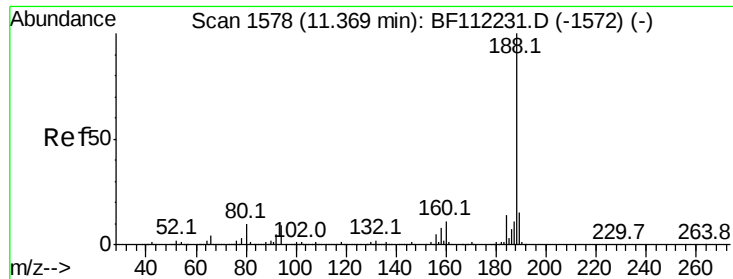

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1577
Delta R.T. -0.01 min
Lab File: BF112530.D
Acq: 13 Feb 2019 11:06




Instrument :
BNA_F
ClientSampleId :
PB117061BL


Tot Ion:188 Resp: 452180
Ion Ratio Lower Upper
188 100
94 8.3 8.2 12.2
80 9.5 8.9 13.3

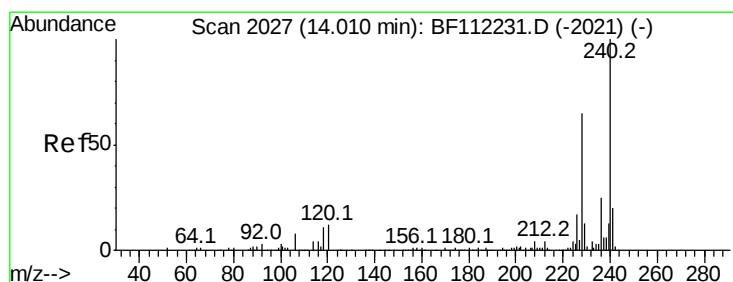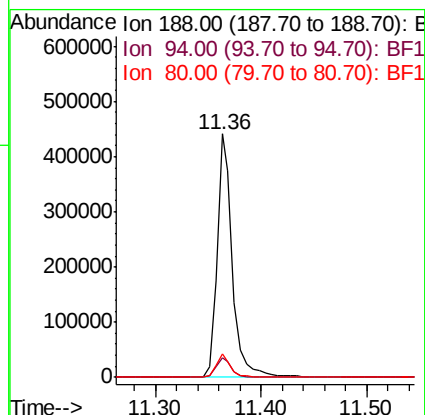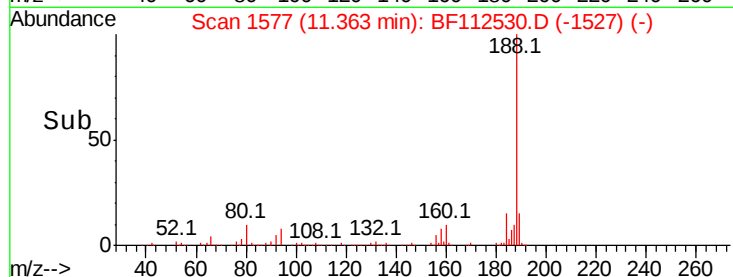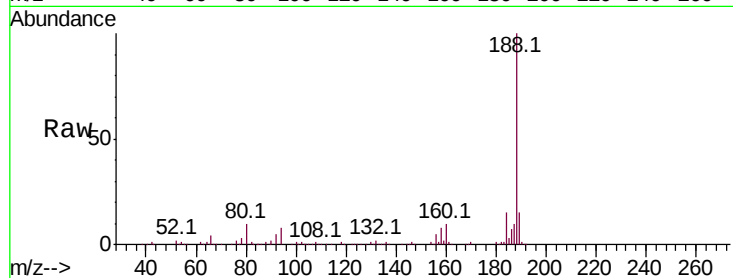

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2028
Delta R.T. 0.01 min
Lab File: BF112530.D
Acq: 13 Feb 2019 11:06

Tgt Ion:240 Resp: 370919
Ion Ratio Lower Upper
240 100
120 9.7 9.0 13.6
236 25.5 20.7 31.1

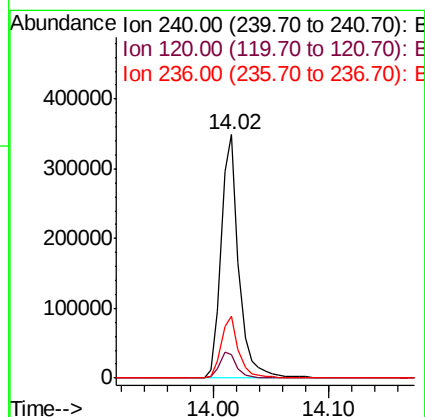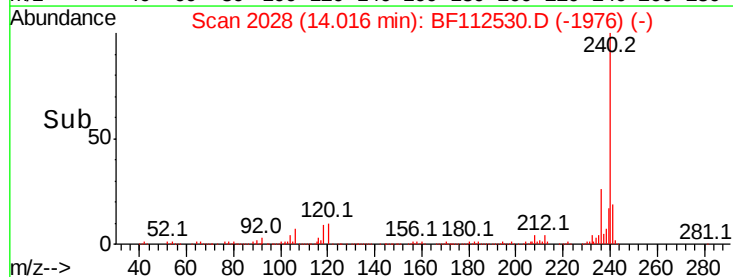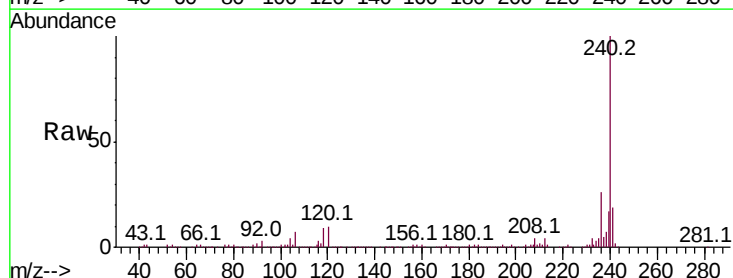

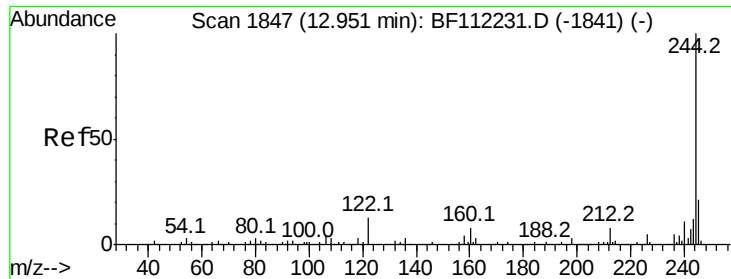

#79

Terphenyl-d14

Concen: 78.472 ng

RT: 12.95 min Scan# 1847

Delta R.T. 0.00 min

Lab File: BF112530.D

Acq: 13 Feb 2019 11:06

Instrument :

BNA_F

ClientSampleId :

PB117061BL


Tot Ion:244 Resp: 1545405

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9




122 10.9 9.8 14.6

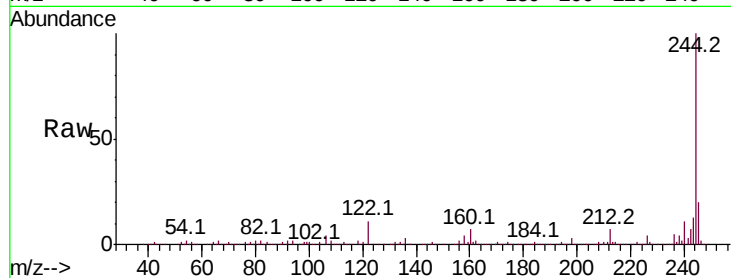

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

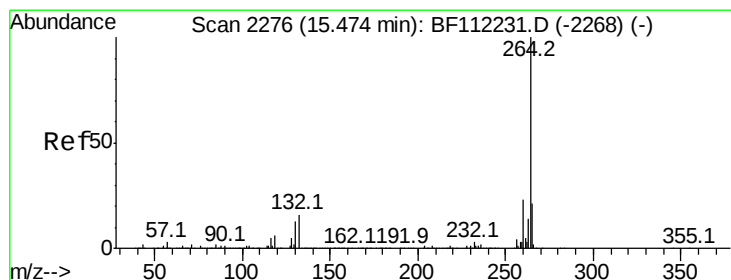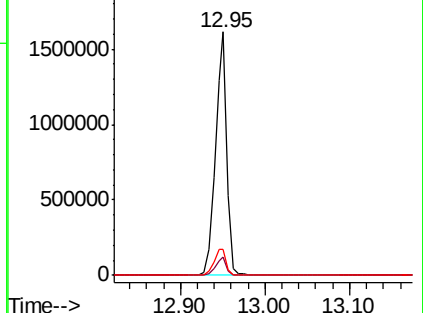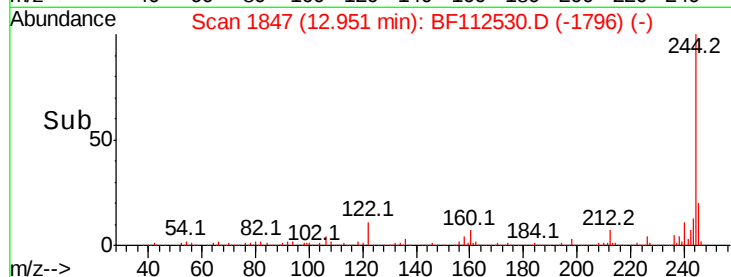

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.50 min Scan# 2280

Delta R.T. 0.02 min

Lab File: BF112530.D

Acq: 13 Feb 2019 11:06


Tgt Ion:264 Resp: 307463

Ion Ratio Lower Upper

264 100

260 21.9 18.2 27.2

265 20.6 17.0 25.4

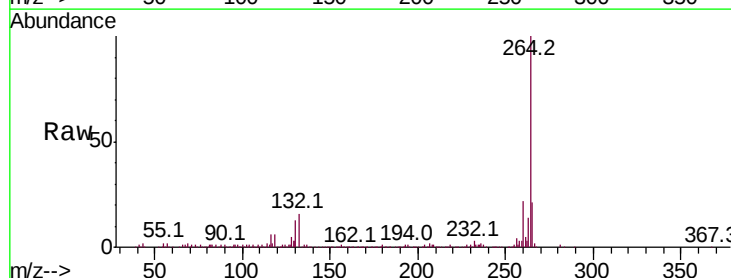

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

