


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021319\
 Data File : BF112554.D
 Acq On : 14 Feb 2019 00:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

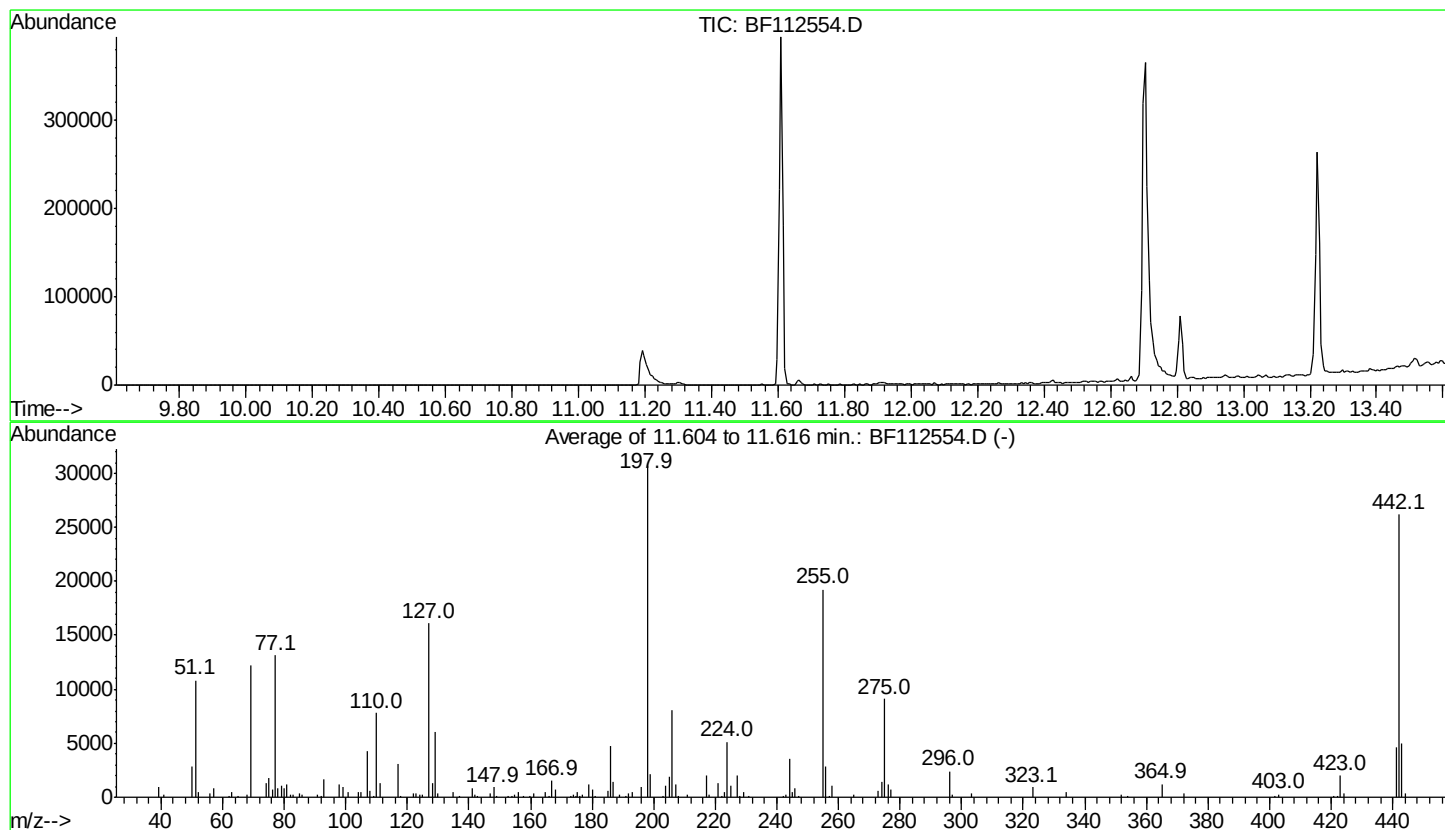

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	10840	PASS
68	69	0.00	2	1.7	211	PASS
69	198	0.00	100	39.7	12203	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	16077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30709	PASS
199	198	5	9	6.9	2112	PASS
275	198	10	60	29.6	9084	PASS
365	198	1	100	4.0	1242	PASS
441	198	0.01	100	15.0	4596	PASS
442	198	50	100	85.2	26176	PASS
443	442	15	24	19.3	5039	PASS