
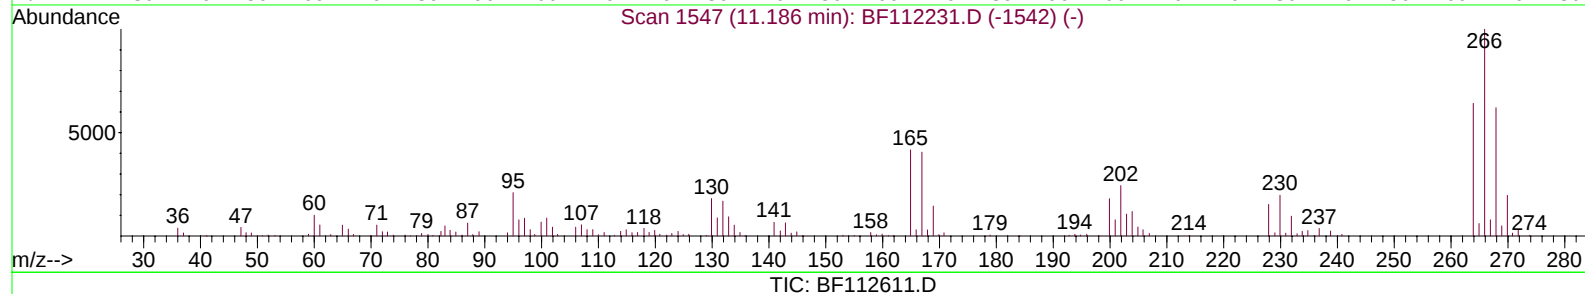
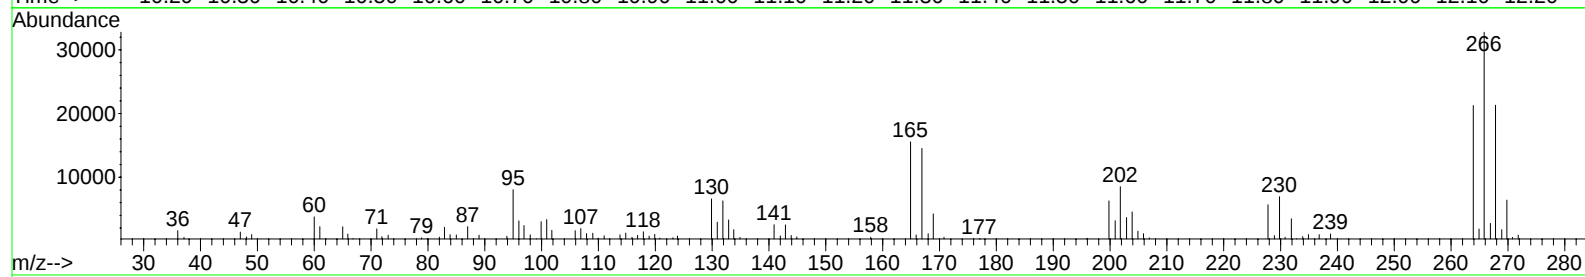


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021919\
Data File : BF112611.D
Acq On : 19 Feb 2019 10:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 17:48:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

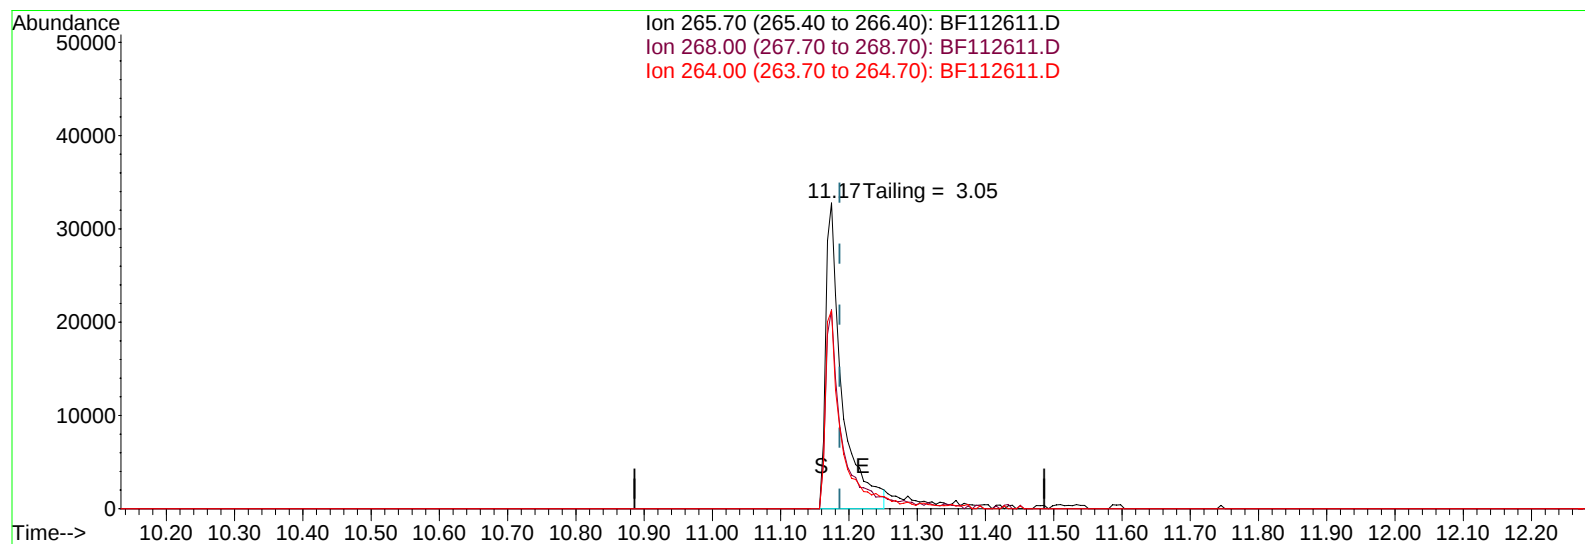

(70) Pentachlorophenol (C)




11.175min (-0.012) 33931.66ng

response 56312

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	65.05
264.00	63.60	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021919\
Data File : BF112611.D
Acq On : 19 Feb 2019 10:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 17:48:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

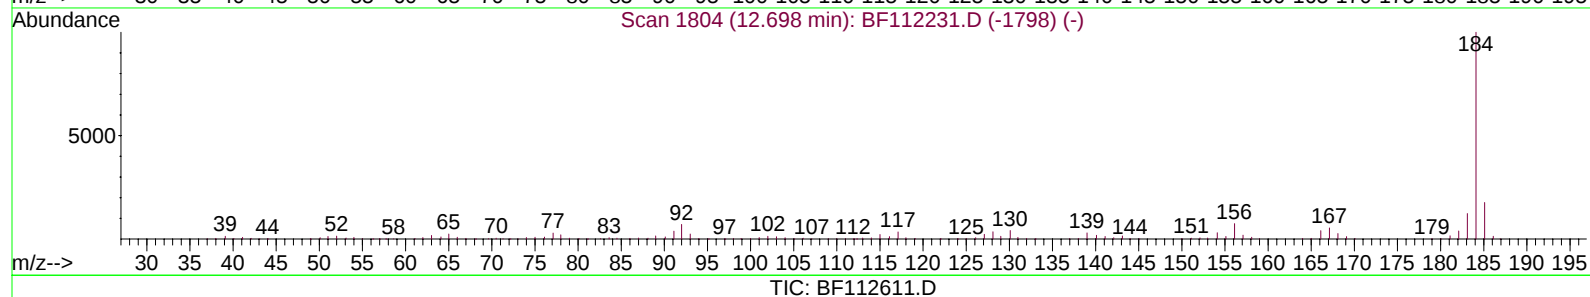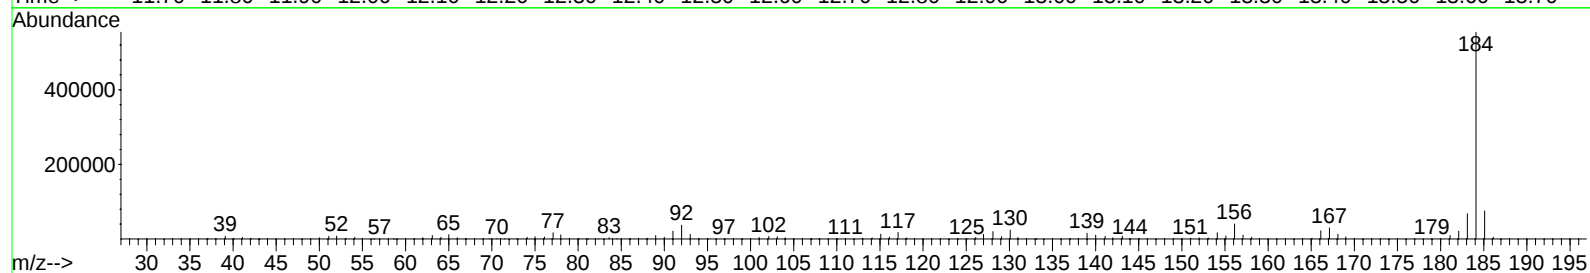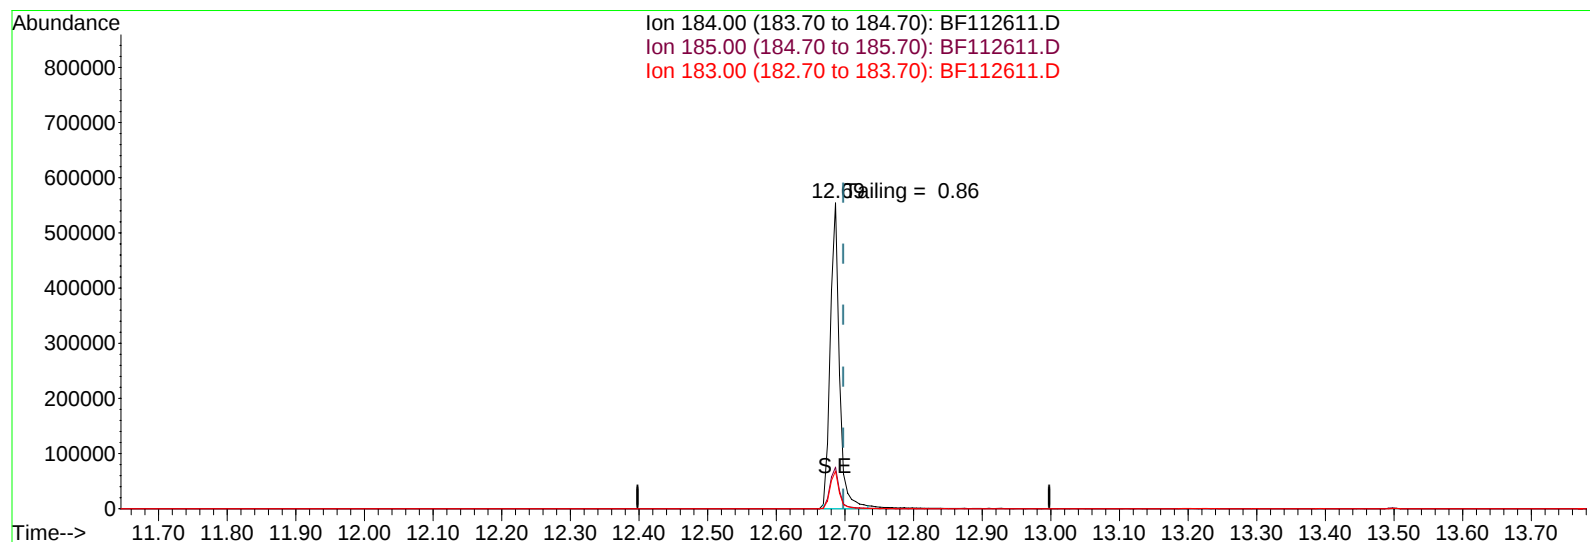

(77) Benzidine

12.686min (-0.012) 0.00ng

response 523389

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	13.61#
183.00	12.50	12.31
0.00	0.00	0.00