

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021919\
 Data File : BF112624.D
 Acq On : 19 Feb 2019 16:43
 Operator : JU/SJ
 Sample : K1515-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TS-11

Quant Time: Feb 20 03:24:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 28 10:38:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	80219	20.00	ng	-0.02
21) Naphthalene-d8	8.10	136	311610	20.00	ng	-0.02
39) Acenaphthene-d10	9.86	164	151482	20.00	ng	-0.03
64) Phenanthrene-d10	11.35	188	296796	20.00	ng	-0.02
76) Chrysene-d12	14.00	240	213323	20.00	ng	-0.01
87) Perylene-d12	15.47	264	185958	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	623843	165.18	ng	-0.02
7) Phenol-d6	6.47	99	766399	146.04	ng	-0.02
23) Nitrobenzene-d5	7.39	82	487452	90.13	ng	-0.02
42) 2,4,6-Tribromophenol	10.66	330	251307	142.53	ng	-0.02
45) 2-Fluorobiphenyl	9.17	172	959341	89.57	ng	-0.03
79) Terphenyl-d14	12.93	244	1024260	90.43	ng	-0.02
Target Compounds						
10) Phenol	6.49	94	22950	3.986	ng	93
50) Dimethylphthalate	9.57	163	55055	4.678	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021919\
Data File : BF112624.D
Acq On : 19 Feb 2019 16:43
Operator : JU/SJ
Sample : K1515-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TS-11

Quant Time: Feb 20 03:24:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

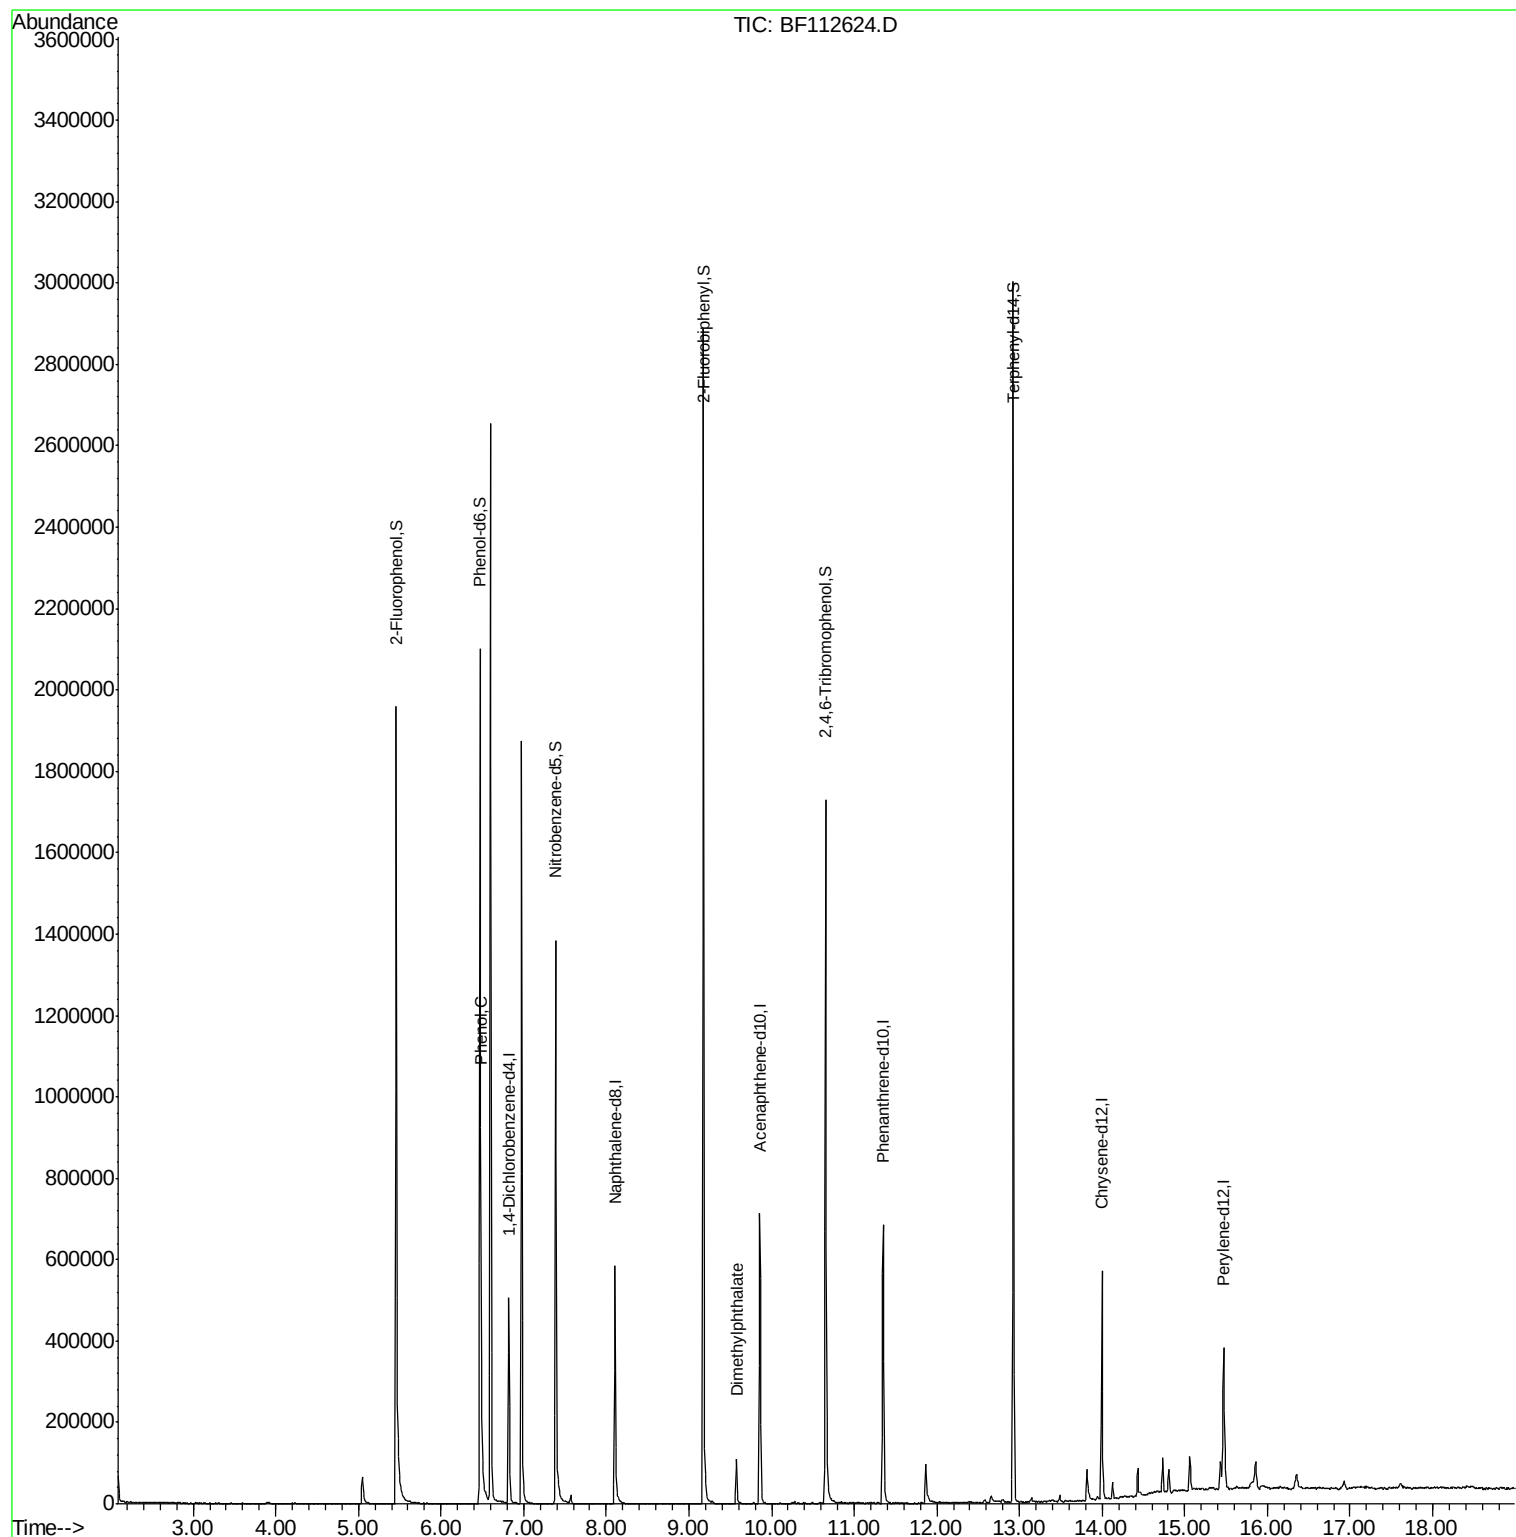

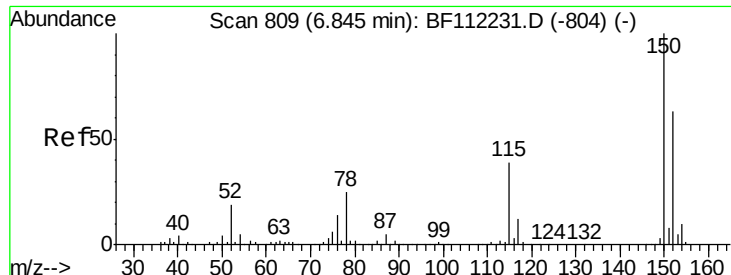


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. -0.02 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Instrument :
BNA_F
ClientSampleId :
TS-11

Tot Ion:152 Resp: 80219
Ion Ratio Lower Upper
152 100
150 151.2 127.4 191.0
115 59.8 45.5 68.3

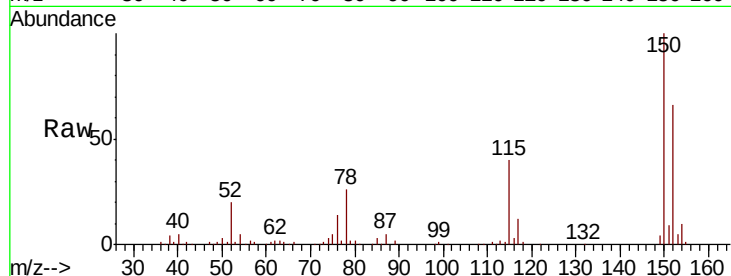


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

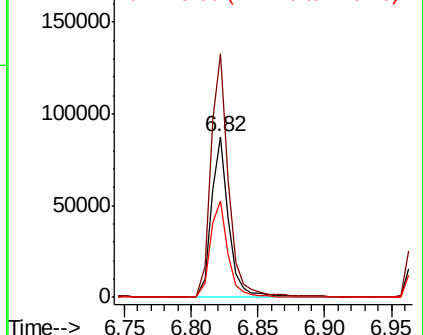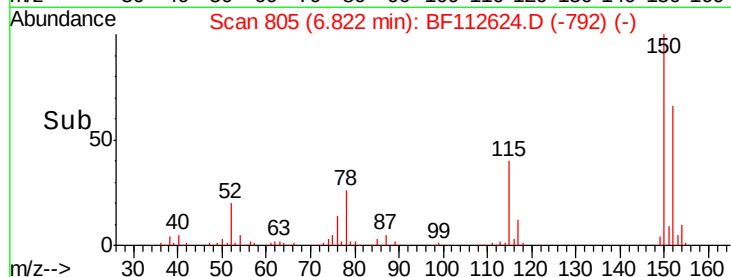



#5


2-Fluorophenol
Concen: 165.183 ng
RT: 5.46 min Scan# 573
Delta R.T. -0.02 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Tgt Ion:112 Resp: 623843
Ion Ratio Lower Upper
112 100
64 55.8 45.7 68.5
63 30.5 23.6 35.4



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

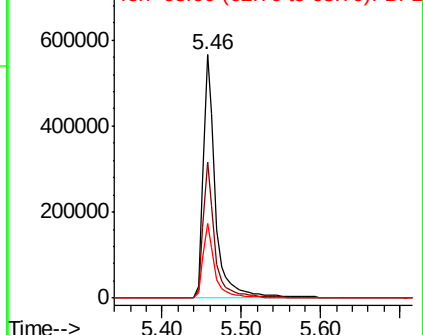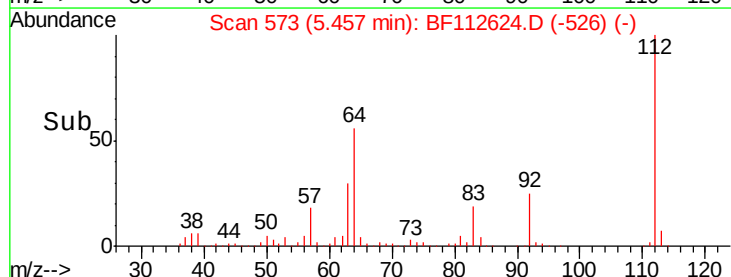

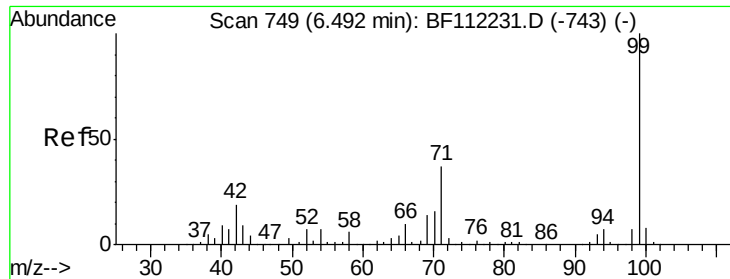

#7

Phenol-d6

Concen: 146.040 ng

RT: 6.47 min Scan# 746

Delta R.T. -0.02 min

Lab File: BF112624.D

Acq: 19 Feb 2019 16:43

Instrument :

BNA_F

ClientSampled :

TS-11


Tot Ion: 99 Resp: 766399

Ion Ratio Lower Upper




99 100

42 19.4 15.1 22.7

71 38.0 26.9 40.3

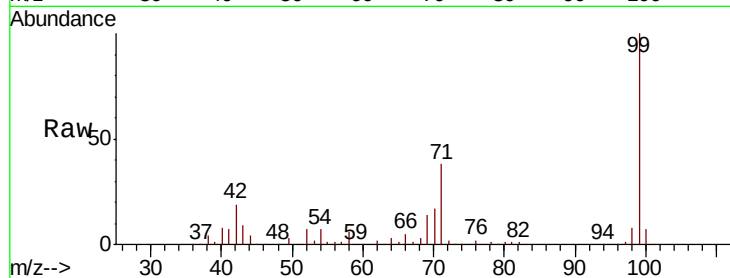

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

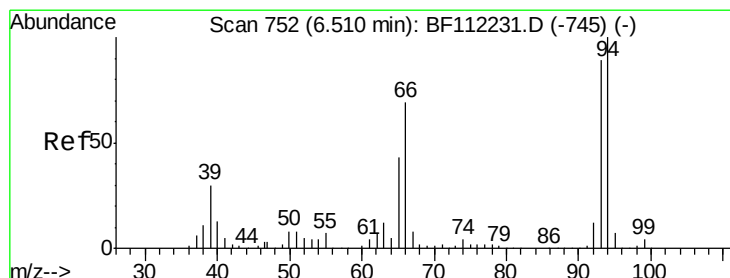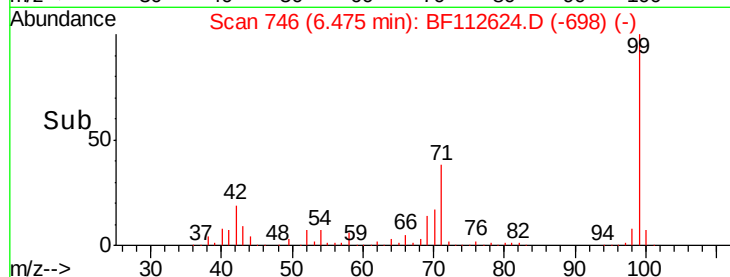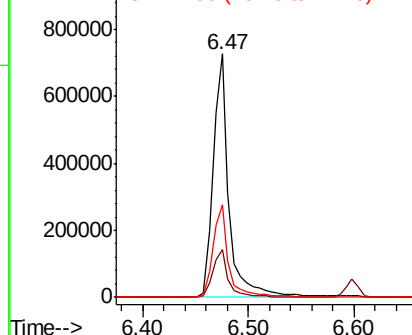

#10

Phenol

Concen: 3.986 ng

RT: 6.49 min Scan# 748

Delta R.T. -0.02 min

Lab File: BF112624.D

Acq: 19 Feb 2019 16:43


Tgt Ion: 94 Resp: 22950

Ion Ratio Lower Upper



94 100


65 32.9 20.3 60.3

66 66.0 42.4 82.4

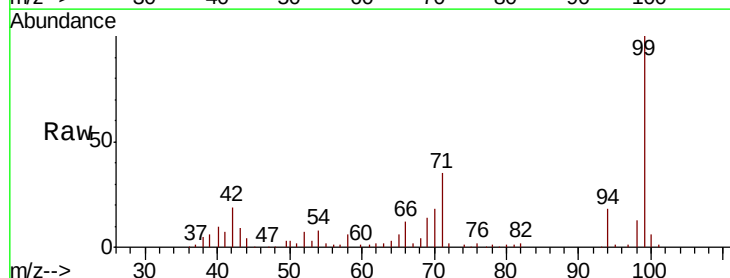

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1



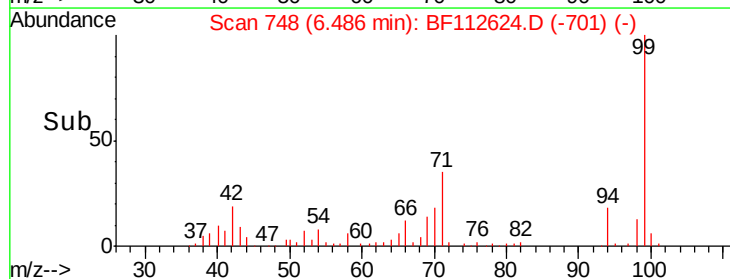
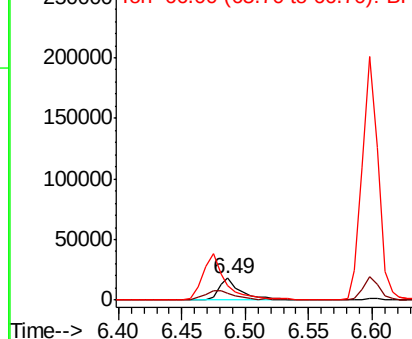


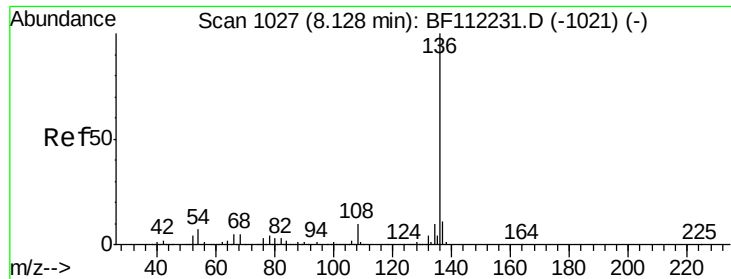

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.10 min Scan# 1023
Delta R.T. -0.02 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43




Instrument :
BNA_F
ClientSampleId :
TS-11


Tot Ion:136	Resp:	311610
Ion	Ratio	Lower Upper
136	100	
137	11.2	9.1 13.7
54	6.3	5.9 8.9
68	4.6	5.1 7.7#

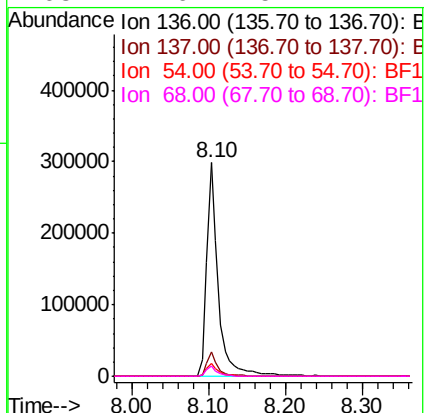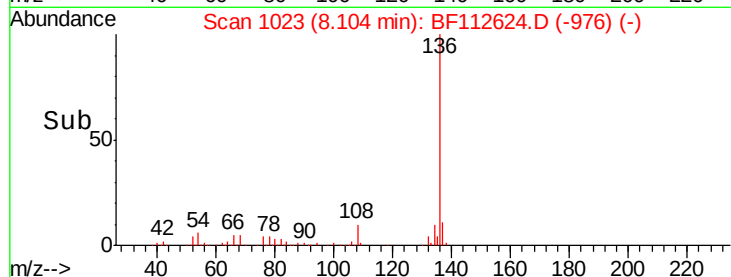

#23
Nitrobenzene-d5
Concen: 90.135 ng
RT: 7.39 min Scan# 901
Delta R.T. -0.02 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Tgt Ion: 82	Resp:	487452
Ion	Ratio	Lower Upper
82	100	
128	46.2	37.8 56.8
54	49.6	39.7 59.5

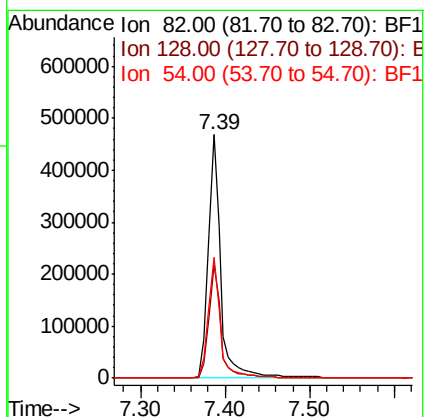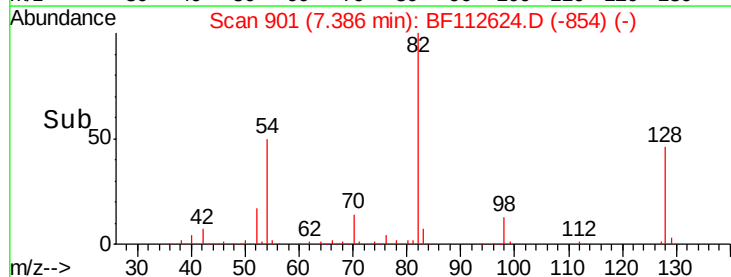


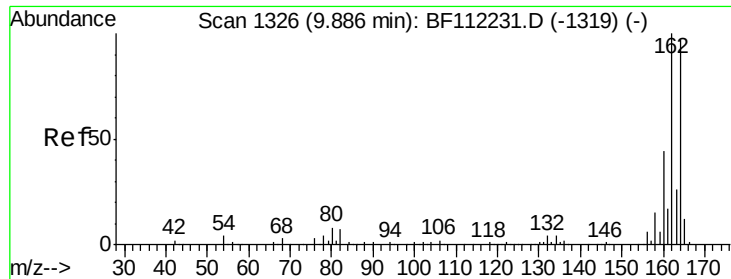




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.86 min Scan# 1321
Delta R.T. -0.03 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Instrument :
BNA_F
ClientSampleId :
TS-11

Tot Ion:164 Resp: 151482
Ion Ratio Lower Upper
164 100
162 100.3 82.2 123.4
160 43.9 36.2 54.4

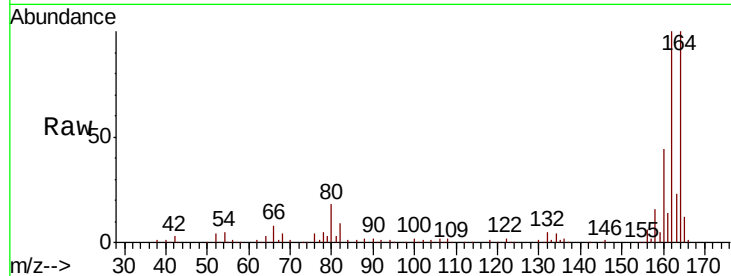


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

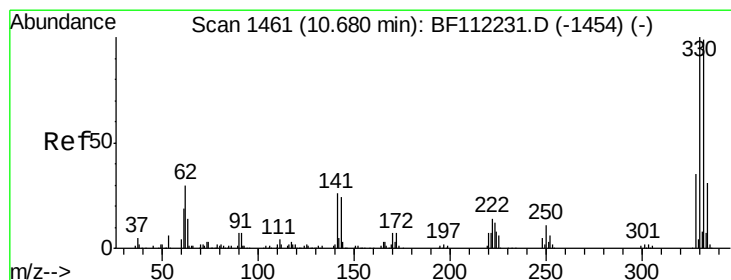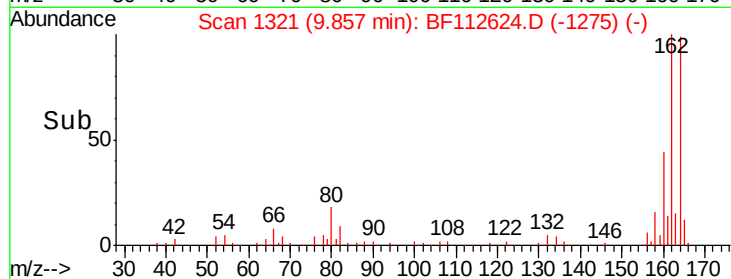
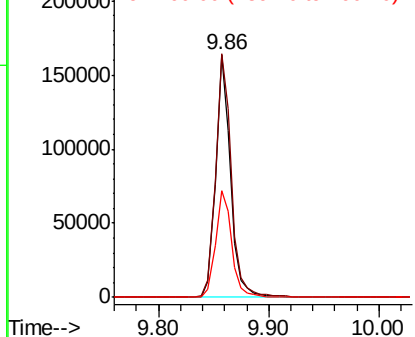



#42
2,4,6-Tribromophenol
Concen: 142.528 ng
RT: 10.66 min Scan# 1457
Delta R.T. -0.02 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Tgt Ion:330 Resp: 251307
Ion Ratio Lower Upper
330 100
332 95.1 76.6 114.8
141 34.0 24.3 36.5



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

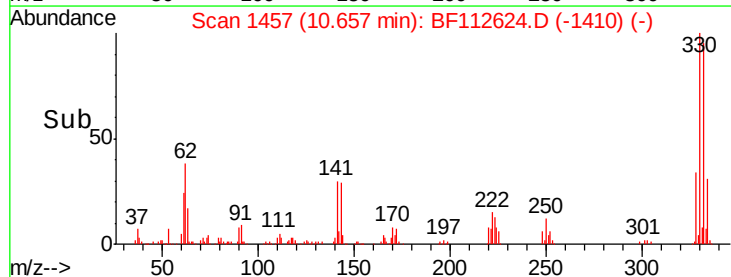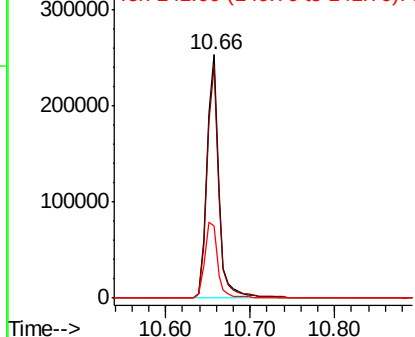


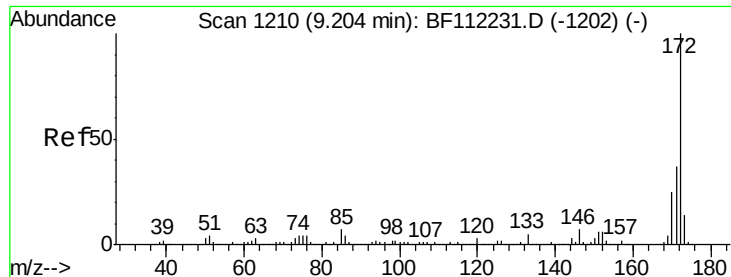




#45
2-Fluorobiphenyl
Concen: 89.570 ng
RT: 9.17 min Scan# 1205
Delta R.T. -0.03 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Instrument :
BNA_F
ClientSampleId :
TS-11

Tot Ion:172 Resp: 959341
Ion Ratio Lower Upper
172 100
171 36.5 30.5 45.7
170 23.5 20.2 30.4

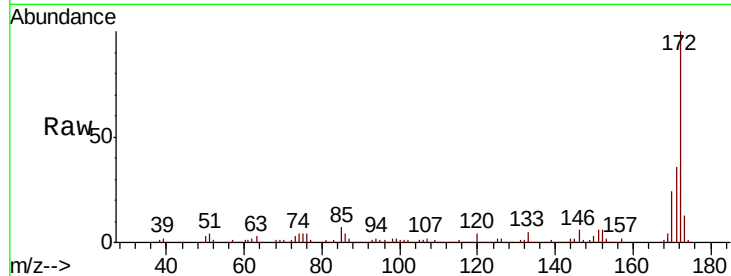


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

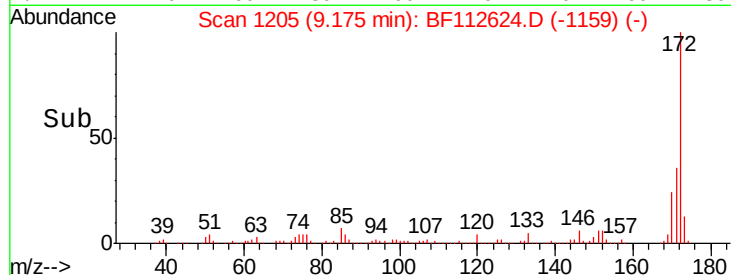
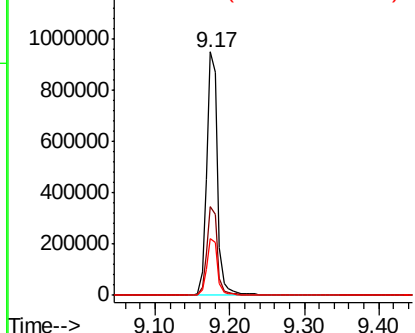



#50
Dimethylphthalate
Concen: 4.678 ng
RT: 9.57 min Scan# 1273
Delta R.T. -0.03 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Tgt Ion:163 Resp: 55055
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.8 8.5 12.7



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

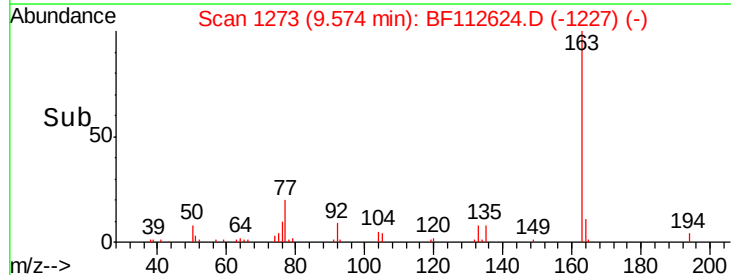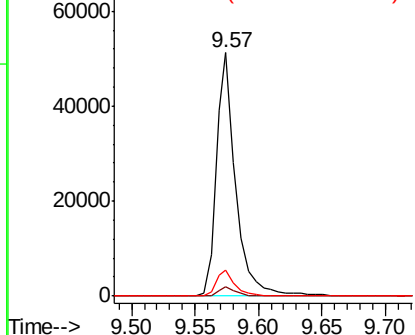


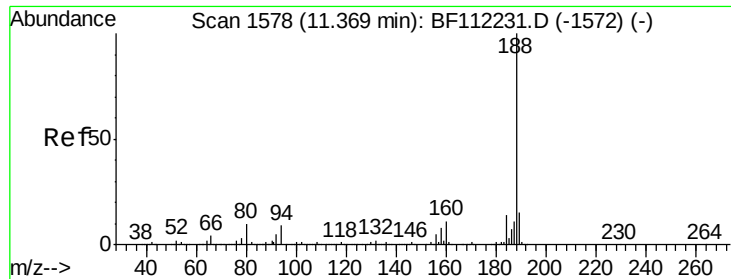




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.35 min Scan# 1575
Delta R.T. -0.02 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Instrument :
BNA_F
ClientSampleId :
TS-11

Tot Ion:188 Resp: 296796
Ion Ratio Lower Upper
188 100
94 7.6 8.2 12.2#
80 8.7 8.9 13.3#

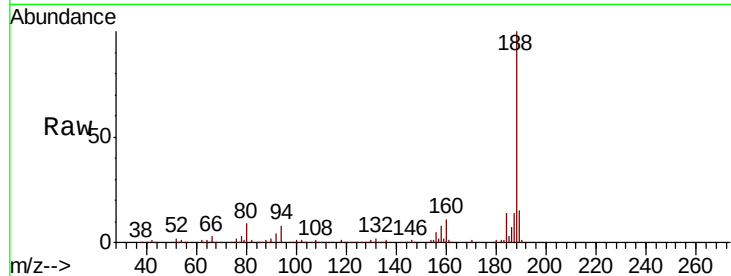


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

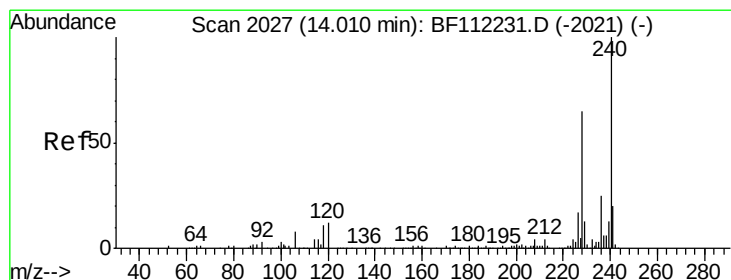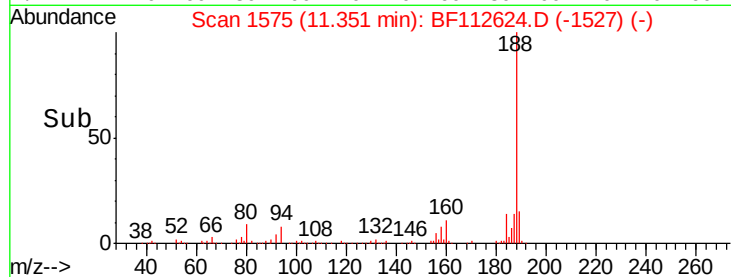
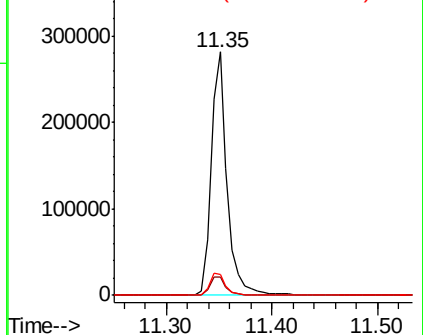



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2025
Delta R.T. -0.01 min
Lab File: BF112624.D
Acq: 19 Feb 2019 16:43

Tgt Ion:240 Resp: 213323
Ion Ratio Lower Upper
240 100
120 9.8 9.0 13.6
236 24.8 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



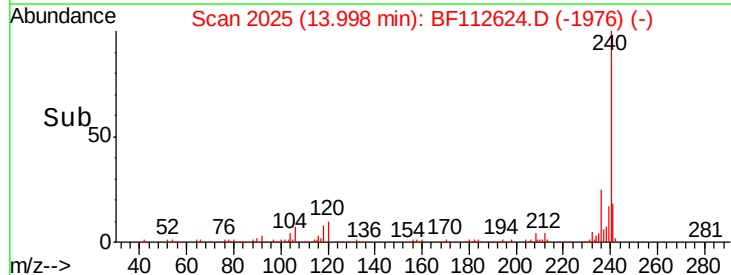
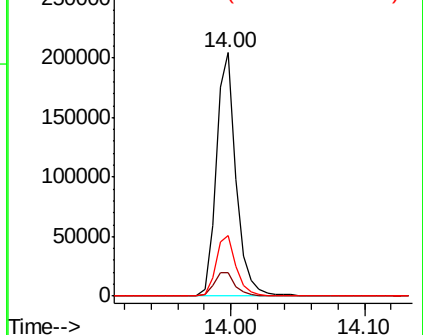


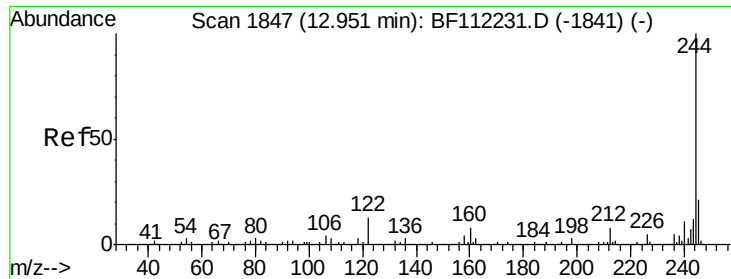

#79
 Terphenyl-d14
 Concen: 90.433 ng
 RT: 12.93 min Scan# 1843
 Delta R.T. -0.02 min
 Lab File: BF112624.D
 Acq: 19 Feb 2019 16:43

Instrument :
 BNA_F
 ClientSampled :
 TS-11

Tot Ion:244 Resp: 1024260
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.9 8.9
 122 11.9 9.8 14.6

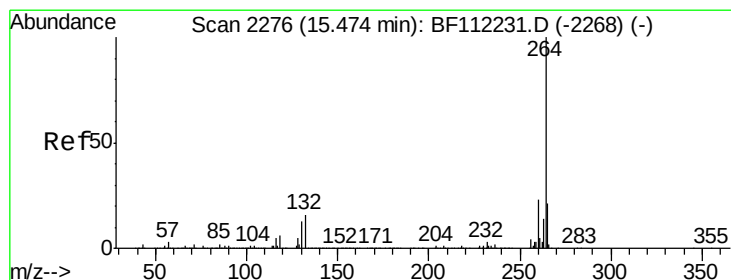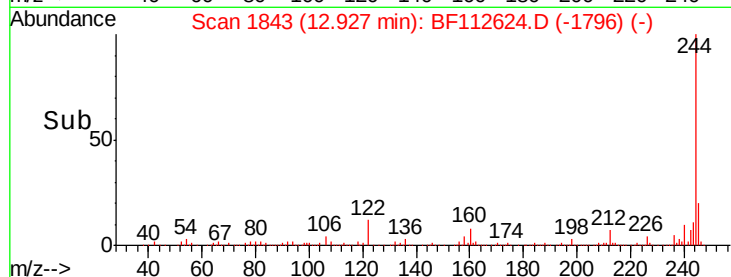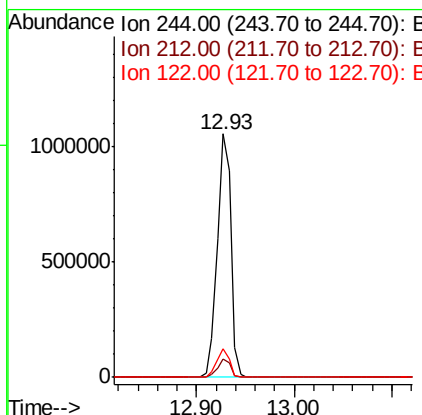

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.47 min Scan# 2275
 Delta R.T. -0.01 min
 Lab File: BF112624.D
 Acq: 19 Feb 2019 16:43

Tgt Ion:264 Resp: 185958
 Ion Ratio Lower Upper
 264 100
 260 22.4 18.2 27.2
 265 20.2 17.0 25.4

