
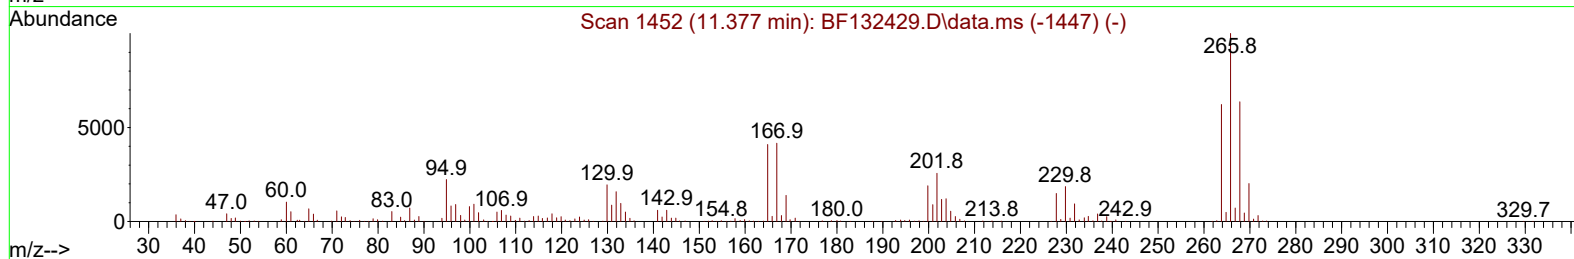
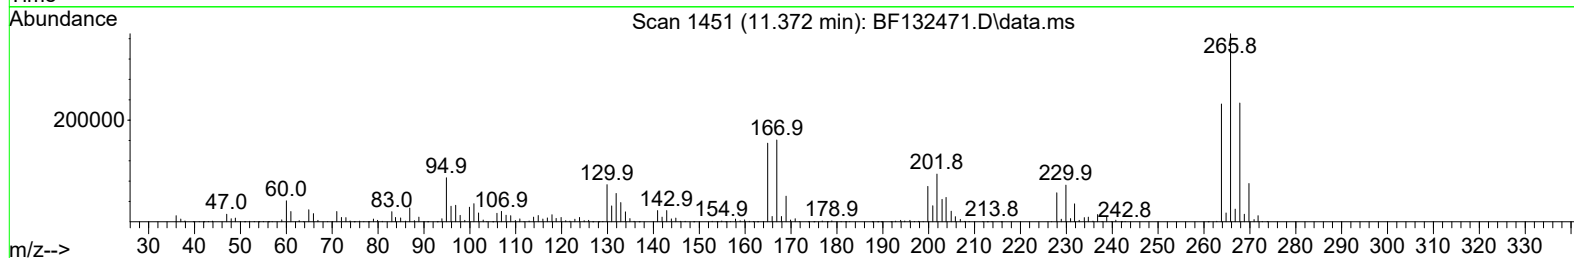


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022023\
Data File : BF132471.D
Acq On : 20 Feb 2023 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 04:15:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 20 13:34:28 2023
Response via : Initial Calibration

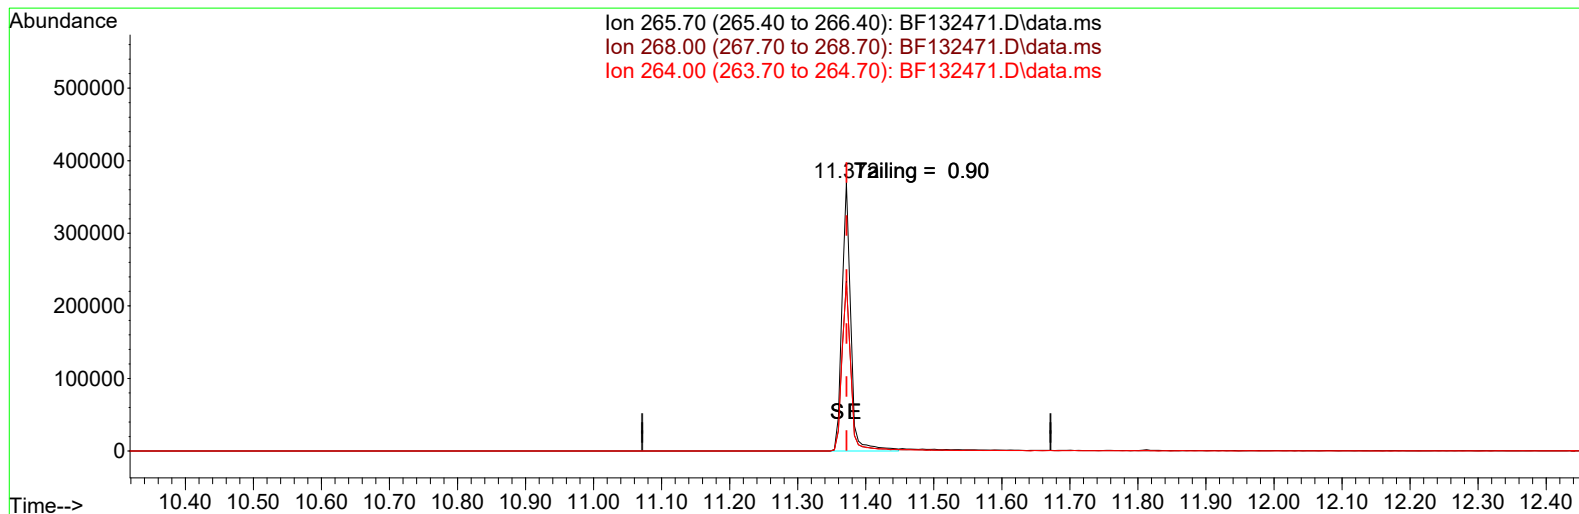

TIC: BF132471.D\data.ms

(70) Pentachlorophenol (C)




11.372min (+ 0.000) 623646.65 ng

response 333159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.21
264.00	62.20	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022023\
Data File : BF132471.D
Acq On : 20 Feb 2023 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 04:15:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 20 13:34:28 2023
Response via : Initial Calibration

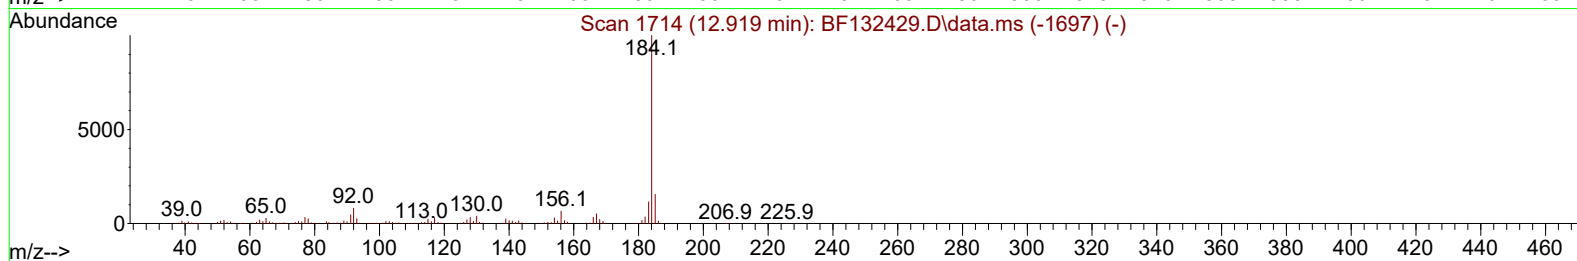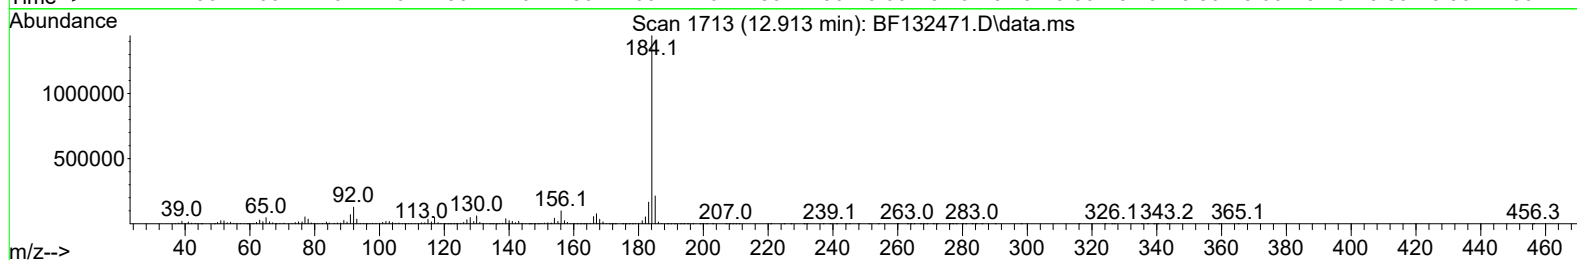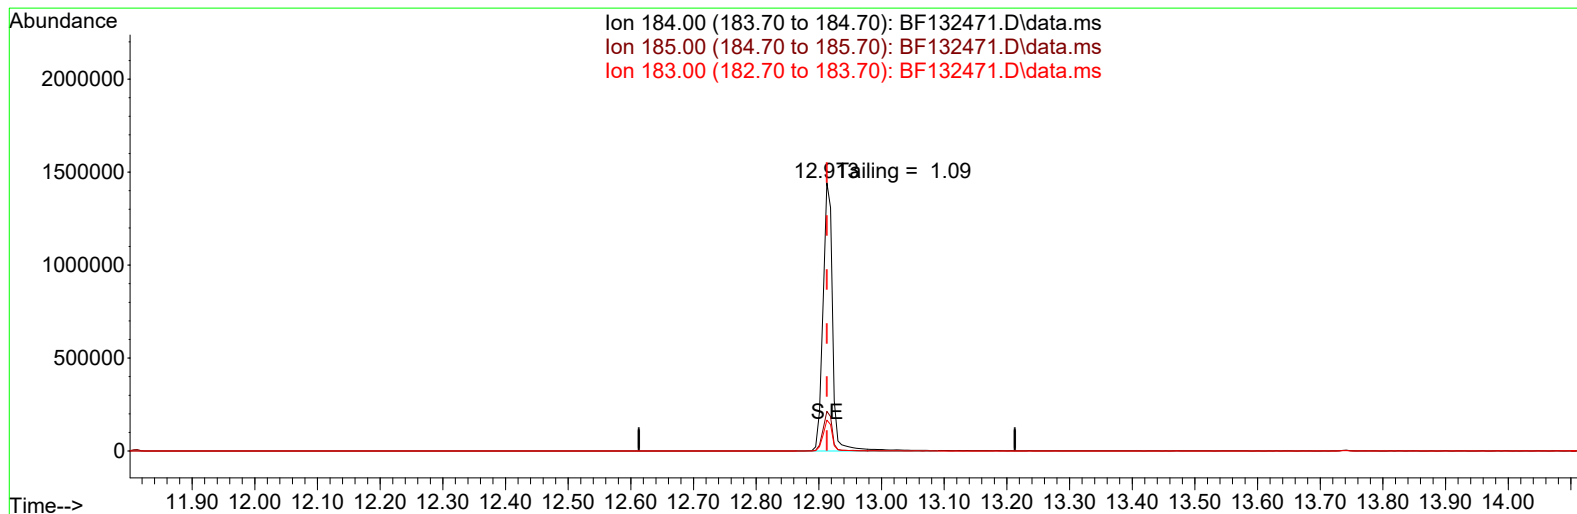

TIC: BF132471.D\data.ms

(77) Benzidine**12.913min (+ 0.000) 134010.93 ng****response 1549508**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.79
183.00	11.50	11.53
0.00	0.00	0.00