
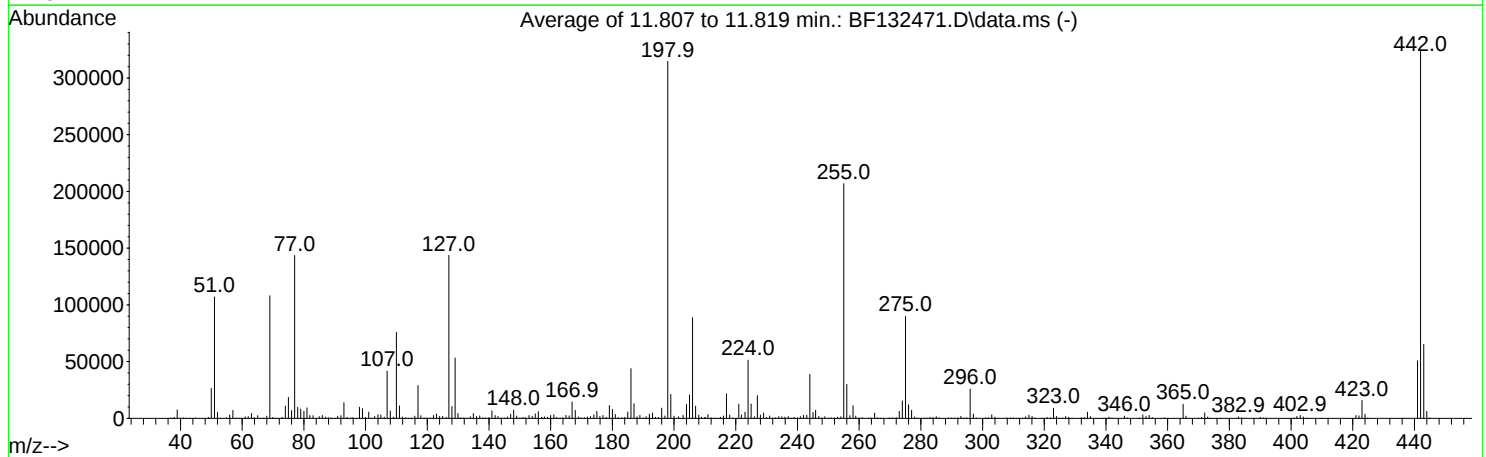


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022023\
 Data File : BF132471.D
 Acq On : 20 Feb 2023 10:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 20 13:34:28 2023

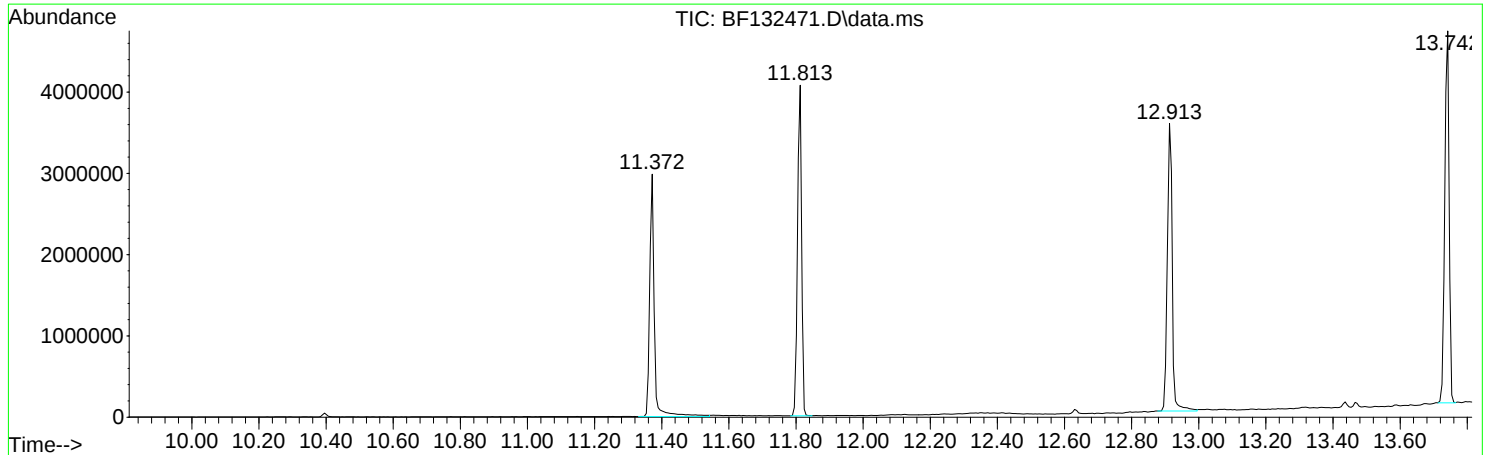




AutoFind: Scans 1525, 1526, 1527; Background Corrected with Scan 1519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	106981	PASS
68	69	0.00	2	1.8	1900	PASS
69	198	0.00	100	34.3	107989	PASS
70	69	0.00	2	0.7	750	PASS
127	198	10	80	45.7	143672	PASS
197	198	0.00	2	0.6	1993	PASS
198	198	100	100	100.0	314645	PASS
199	198	5	9	6.7	21131	PASS
275	198	10	60	28.6	89971	PASS
365	198	1	100	3.9	12289	PASS
441	198	0.01	100	16.1	50773	PASS
442	442	50	100	100.0	324331	PASS
443	442	15	24	20.1	65048	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022023\
Data File : BF132471.D
Acq On : 20 Feb 2023 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 21 04:15:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 20 13:34:28 2023
Response via : Initial Calibration

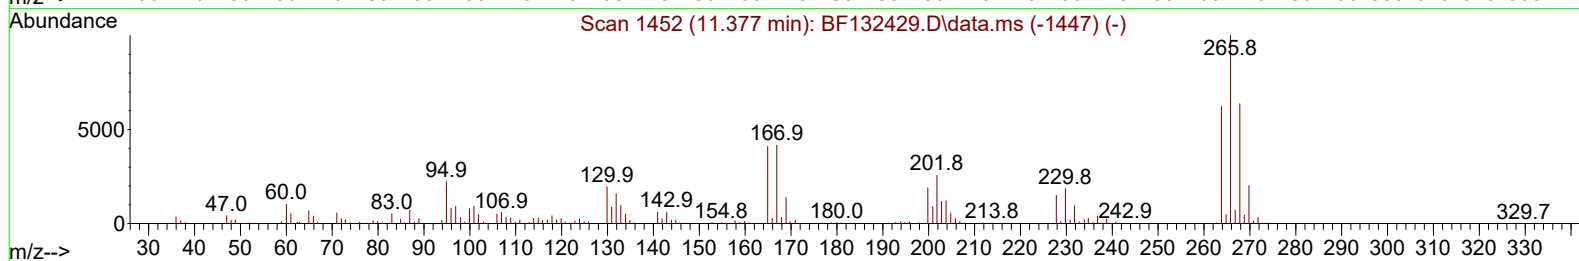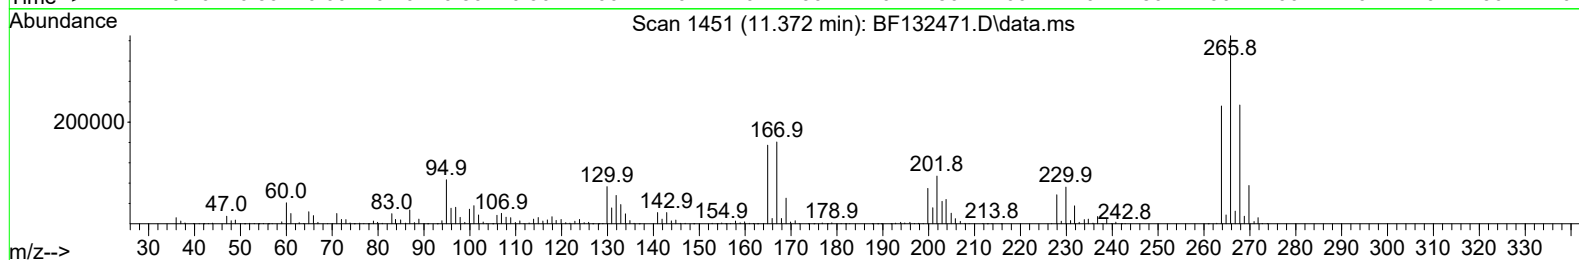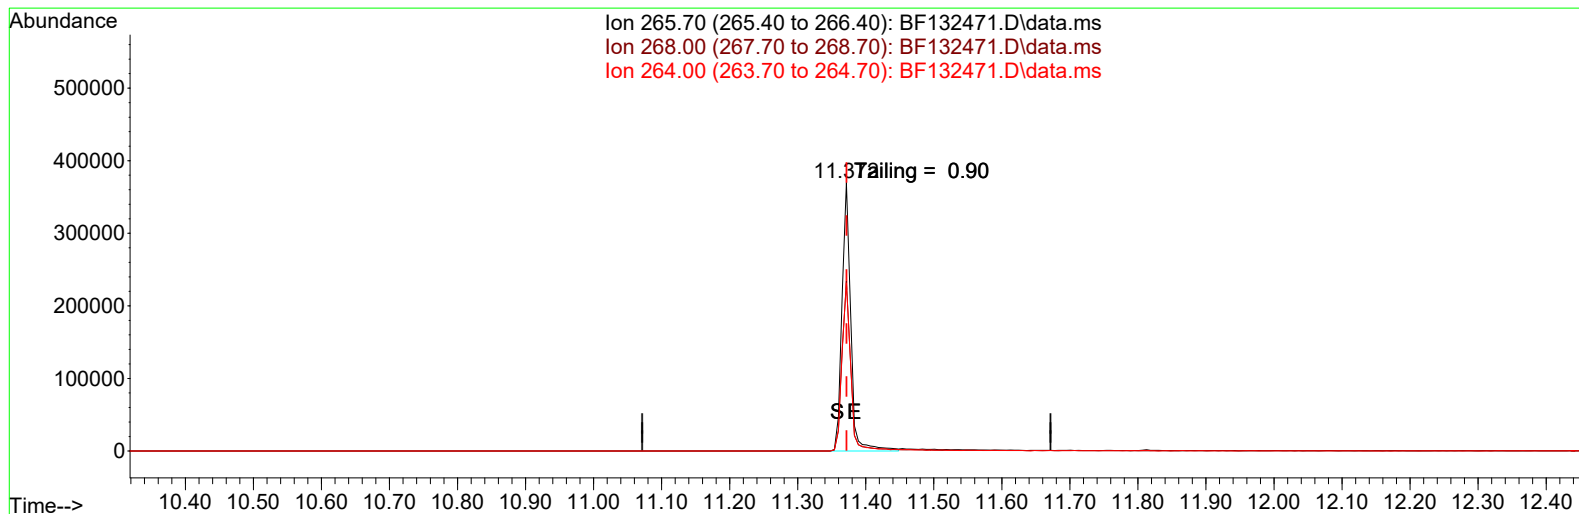

TIC: BF132471.D\data.ms

(70) Pentachlorophenol (C)

11.372min (+ 0.000) 623646.65 ng




response 333159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.21
264.00	62.20	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022023\
 Data File : BF132471.D
 Acq On : 20 Feb 2023 10:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 21 04:15:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 20 13:34:28 2023
 Response via : Initial Calibration

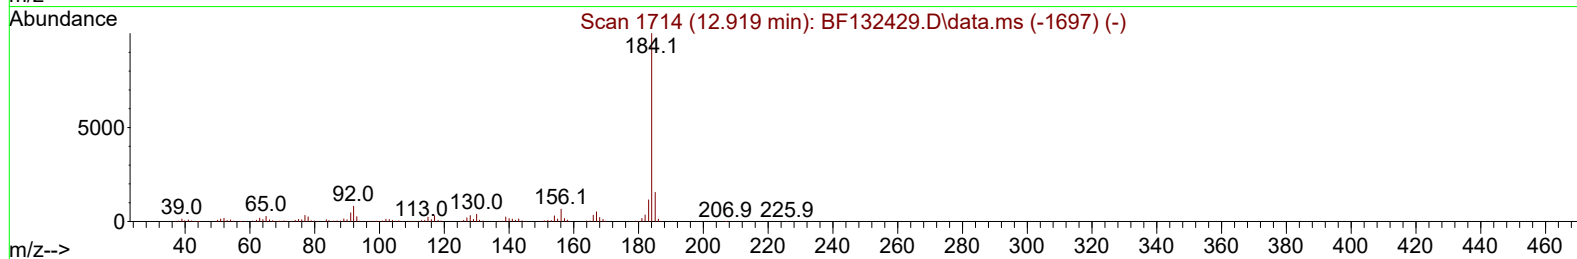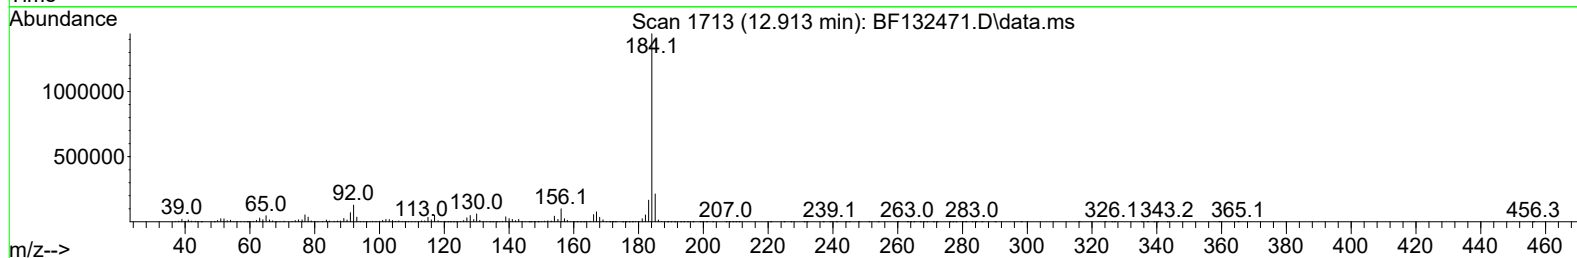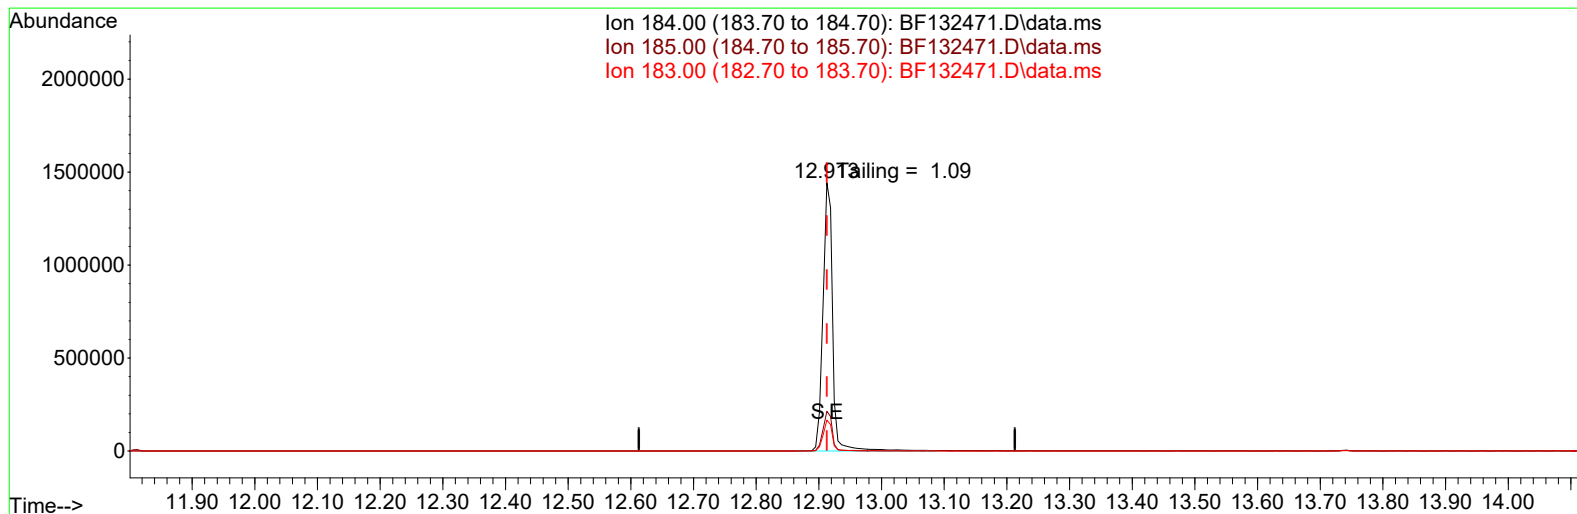

TIC: BF132471.D\data.ms

(77) Benzidine

12.913min (+ 0.000) 134010.93 ng

response 1549508

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.79
183.00	11.50	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/20/2023	BNA_F	<u>BF132471.D</u>
Compound Name	Response	Retention Time
DDT	860145	13.742
DDD	23562	13.436
DDE	760	13.095
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24322	884467	2.75

Instrument :
BNA_F
ClientSampleId :
DFTPP