
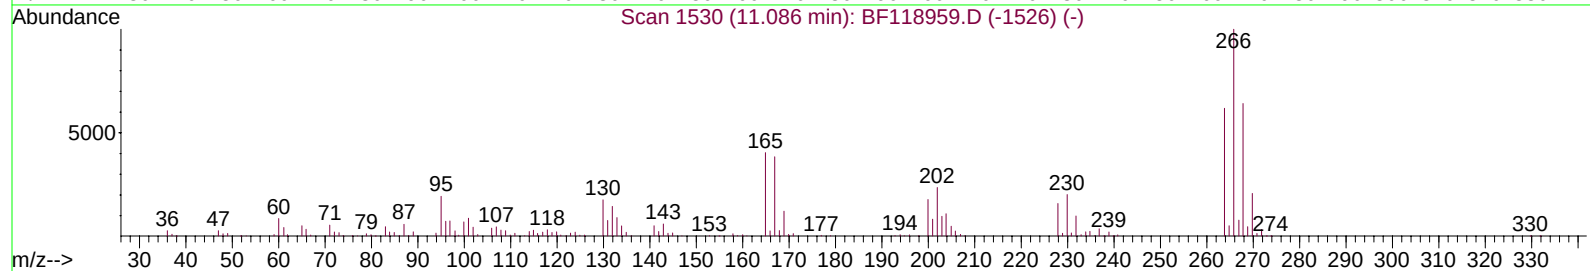
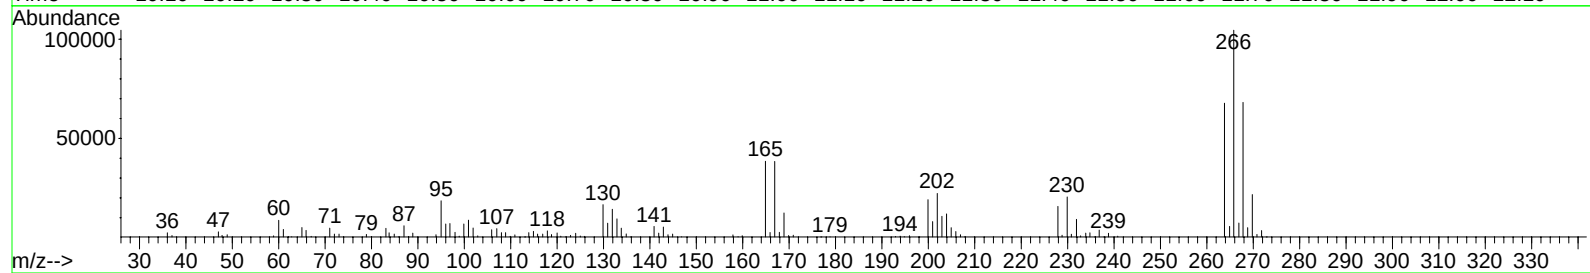


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022120\  
Data File   : BF118989.D  
Acq On      : 21 Feb 2020   12:35  
Operator    : CG/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Feb 21 17:36:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 20 17:40:17 2020
Response via : Initial Calibration

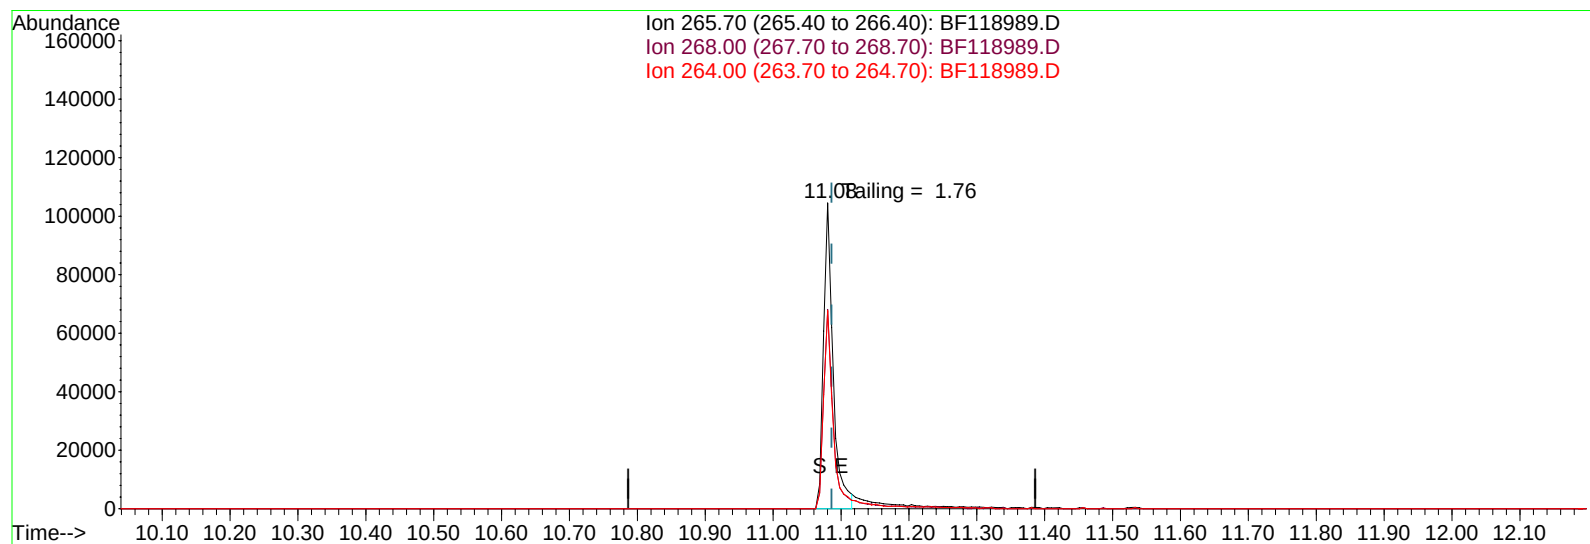

TIC: BF118989.D

(70) Pentachlorophenol (C)




11.080min (-0.006) 36358.62ng

```
response 113011
```

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	65.21
264.00	61.90	64.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022120\
 Data File : BF118989.D
 Acq On : 21 Feb 2020 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:36:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 20 17:40:17 2020
 Response via : Initial Calibration

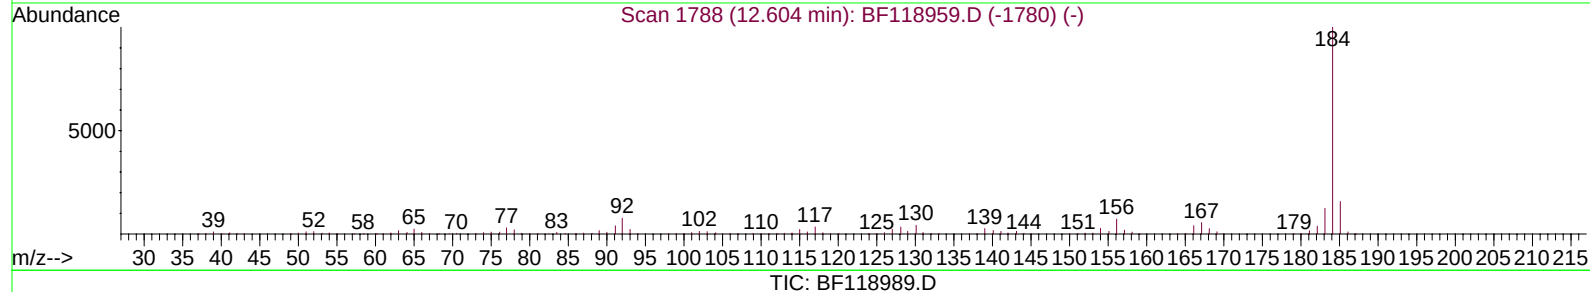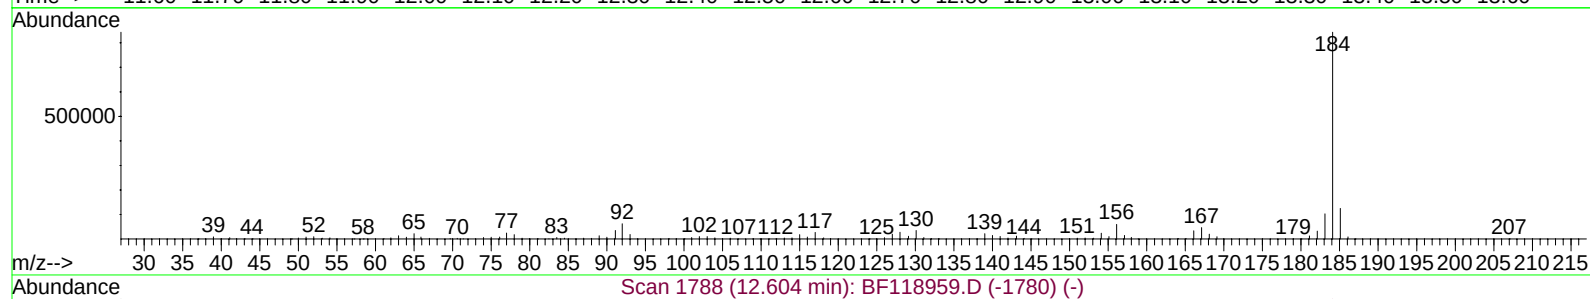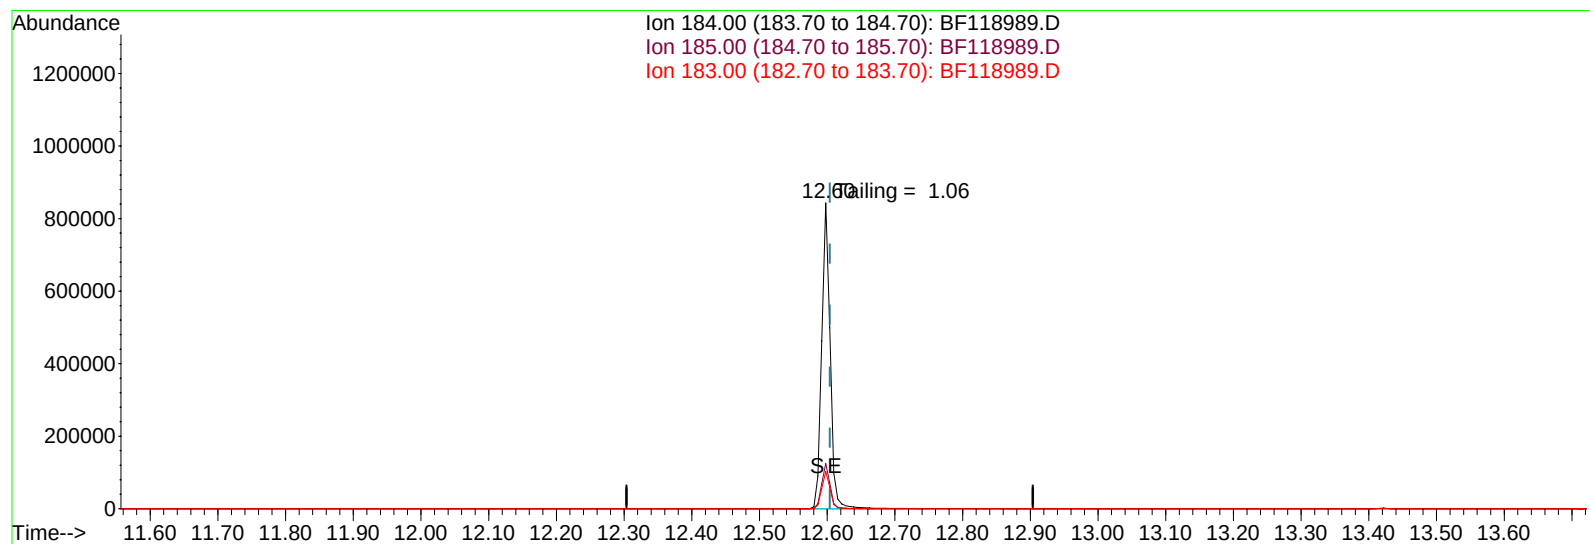

(77) Benzidine

12.598min (-0.006) 0.00ng

response 734900

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.82
183.00	12.40	12.16
0.00	0.00	0.00