

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022120\
 Data File : BF119005.D
 Acq On : 21 Feb 2020 21:15
 Operator : CG/JU
 Sample : L1631-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-D-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	556	560	578	rBV	2827983	2692927	87.58%	11.231%
2	6.398	728	733	750	rBV	2501992	2599089	84.53%	10.840%
3	6.751	790	793	803	rVB	921696	874624	28.44%	3.648%
4	6.910	816	820	824	rBV	2717094	2347359	76.34%	9.790%
5	7.316	884	889	892	rBV	1861012	1668213	54.25%	6.958%
6	8.033	1007	1011	1018	rBV	1196455	1054934	34.31%	4.400%
7	9.110	1189	1194	1197	rBV	3632357	3074879	100.00%	12.824%
8	9.504	1257	1261	1270	rVB	343717	300746	9.78%	1.254%
9	9.786	1305	1309	1313	rBV	1316946	1094372	35.59%	4.564%
10	10.574	1439	1443	1457	rBV	1962421	1731144	56.30%	7.220%
11	11.269	1557	1561	1568	rBV	1201355	1018271	33.12%	4.247%
12	11.798	1648	1651	1659	rBV2	71137	93181	3.03%	0.389%
13	12.851	1826	1830	1833	rBV	3275990	2876850	93.56%	11.998%
14	13.757	1980	1984	1996	rBV	185167	345020	11.22%	1.439%
15	13.904	2004	2009	2013	rBV	1183759	1092625	35.53%	4.557%
16	14.374	2086	2089	2091	rBV	38996	37196	1.21%	0.155%
17	14.674	2137	2140	2143	rBV	47508	44160	1.44%	0.184%
18	14.992	2191	2194	2198	rVB	47683	54661	1.78%	0.228%
19	15.333	2247	2252	2260	rVB	769672	976713	31.76%	4.074%


Sum of corrected areas: 23976964

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022120\
Data File : BF119005.D
Acq On : 21 Feb 2020 21:15
Operator : CG/JU
Sample : L1631-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-D-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

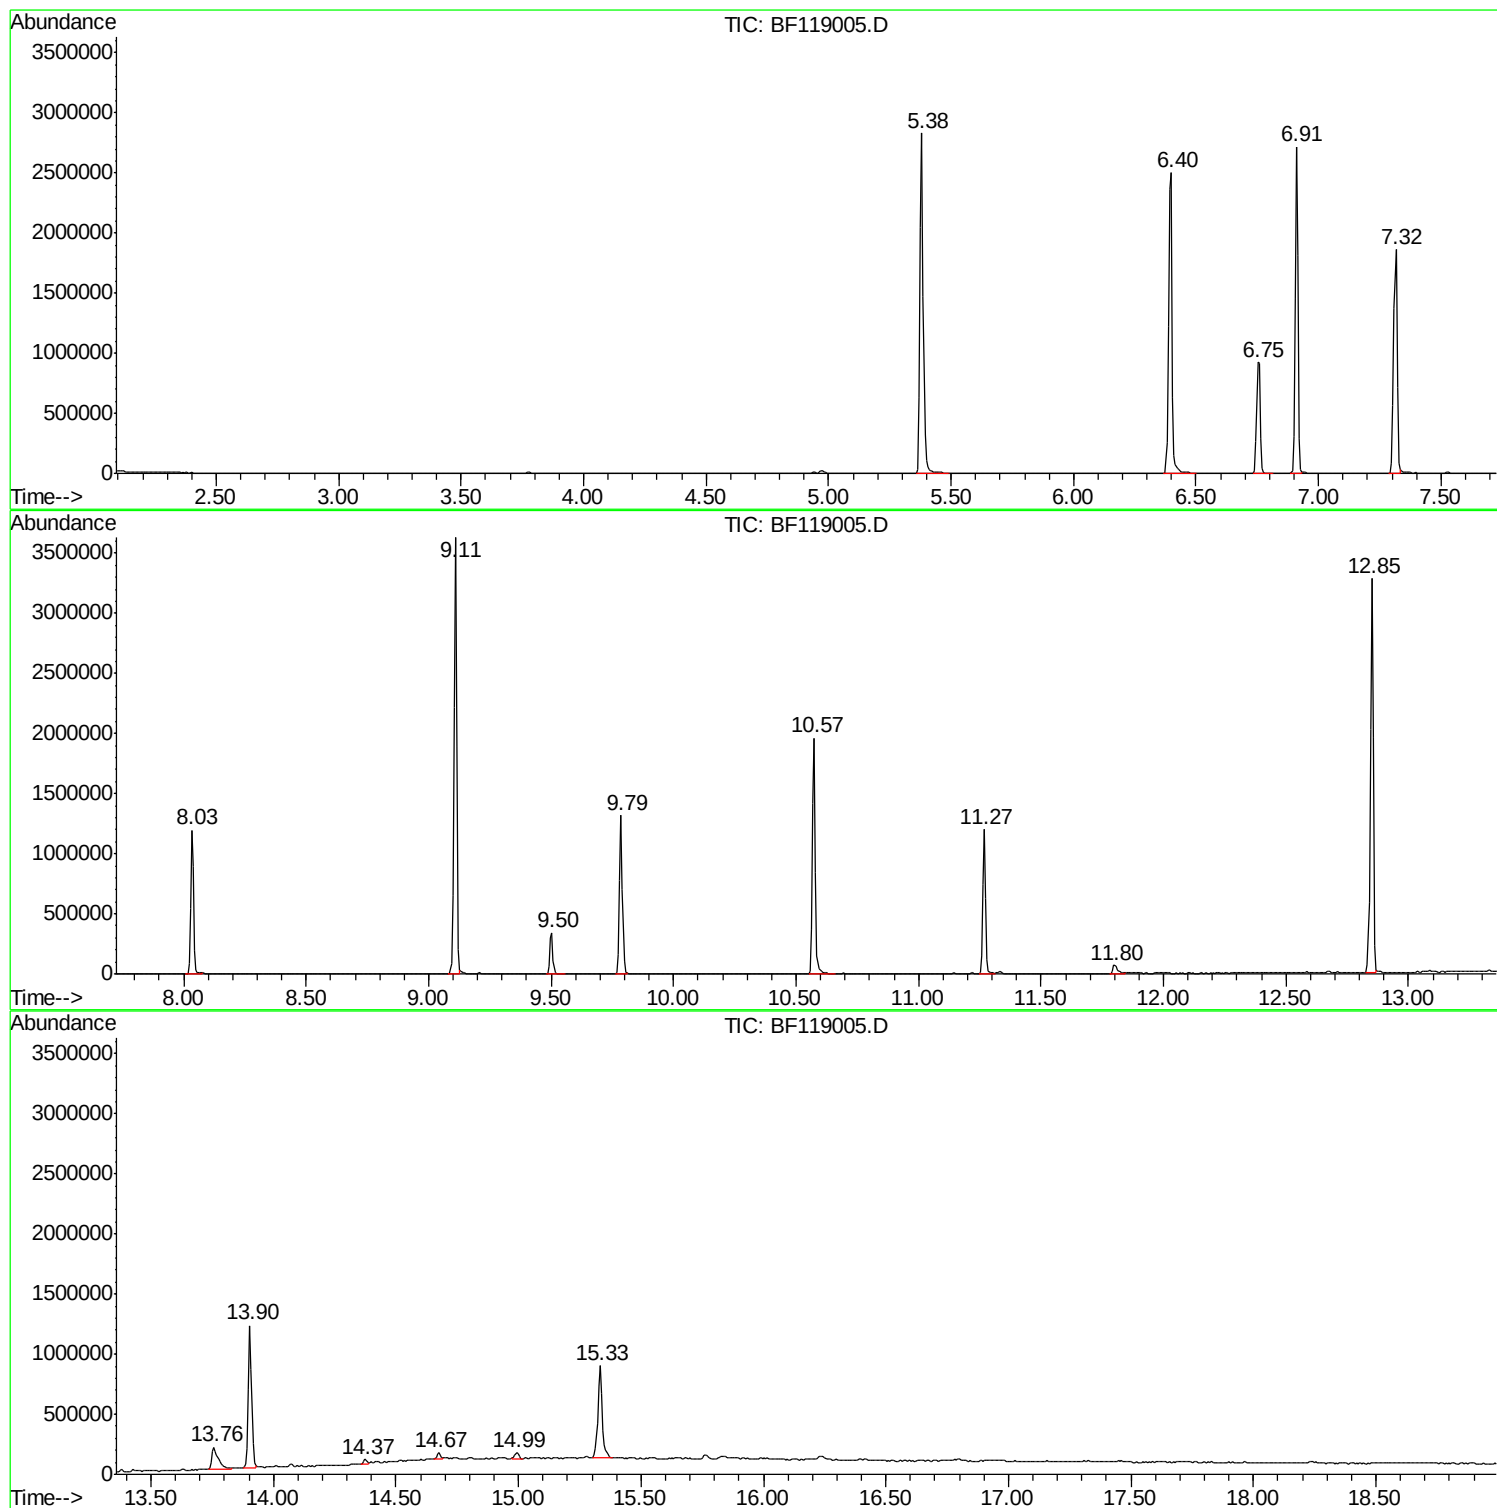

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022120\
Data File : BF119005.D
Acq On : 21 Feb 2020 21:15
Operator : CG/JU
Sample : L1631-11
Misc :
ALS Vial : 17 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
TP-D-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dichloroacetic acid, heptad... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.		
13.76	6.32 ng	345020	Chrysene-d12	13.90		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
2		n-Nonadecanol-1	284	C19H40O	001454-84-8	93
3		17-Pentatriacontene	491	C35H70	006971-40-0	91
4		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	91
5		Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91

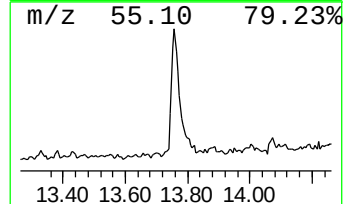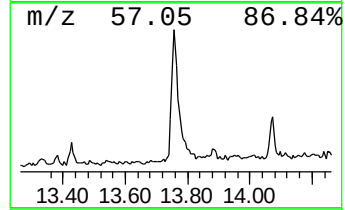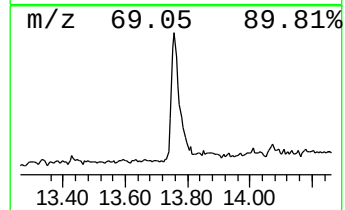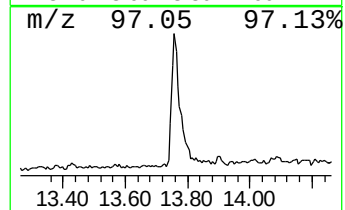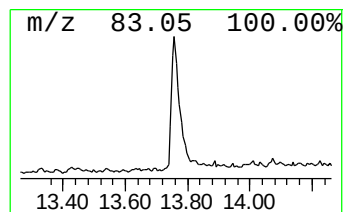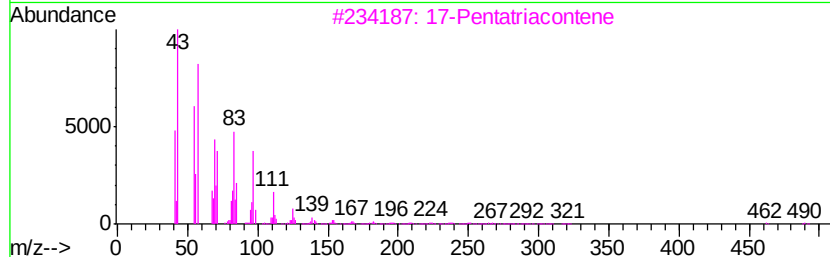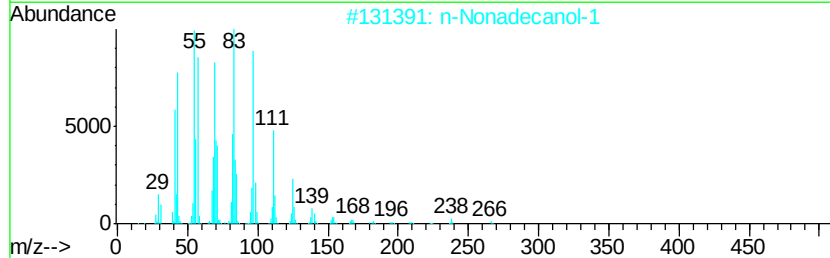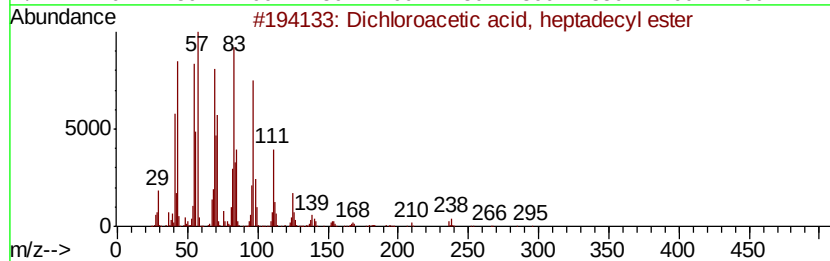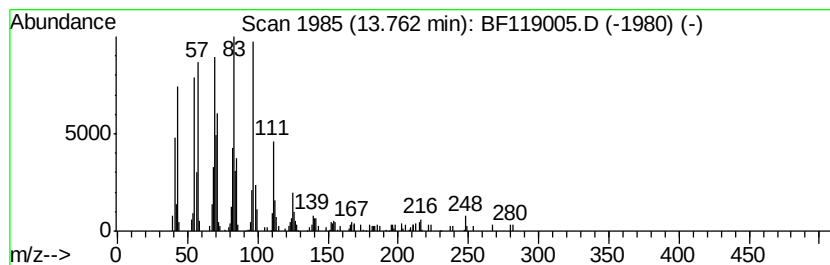

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022120\
Data File : BF119005.D
Acq On : 21 Feb 2020 21:15
Operator : CG/JU
Sample : L1631-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-D-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ac...	13.76	6.3	ng	345020	5	13.90	1092630	20.0