


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022120\
 Data File : BF118989.D
 Acq On : 21 Feb 2020 12:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 20 17:40:17 2020

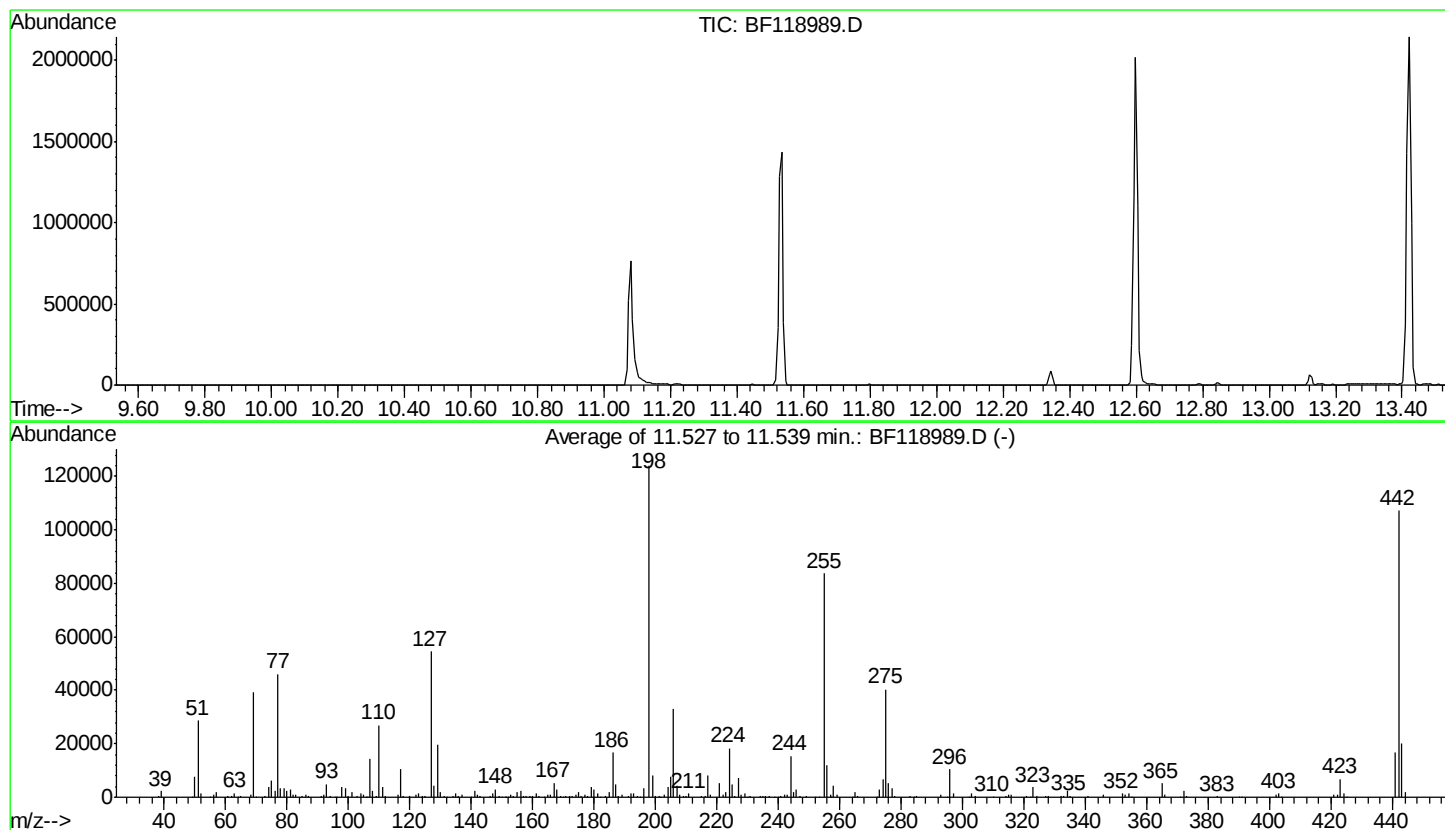

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	28679	PASS
68	69	0.00	2	2.0	782	PASS
69	198	0.00	100	31.7	39284	PASS
70	69	0.00	2	0.3	121	PASS
127	198	10	80	43.9	54399	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	123976	PASS
199	198	5	9	6.7	8258	PASS
275	198	10	60	32.6	40405	PASS
365	198	1	100	4.1	5111	PASS
441	198	0.01	100	13.4	16555	PASS
442	198	50	100	86.3	107026	PASS
443	442	15	24	18.7	20003	PASS