
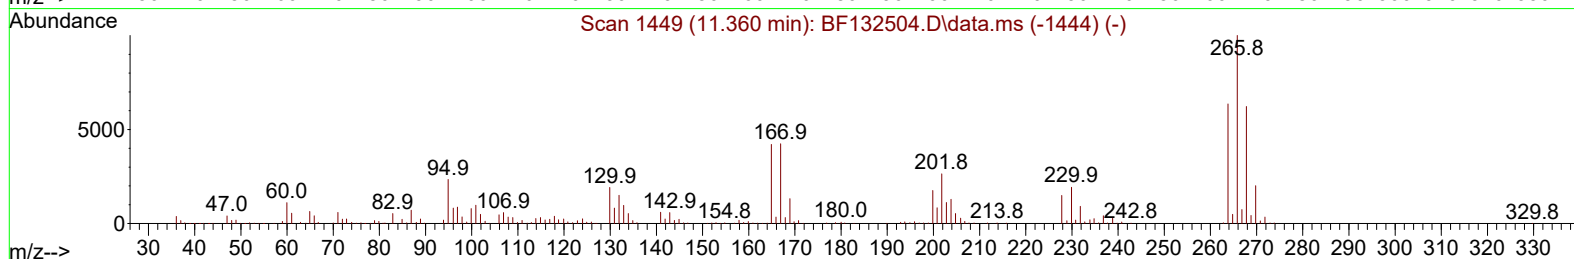
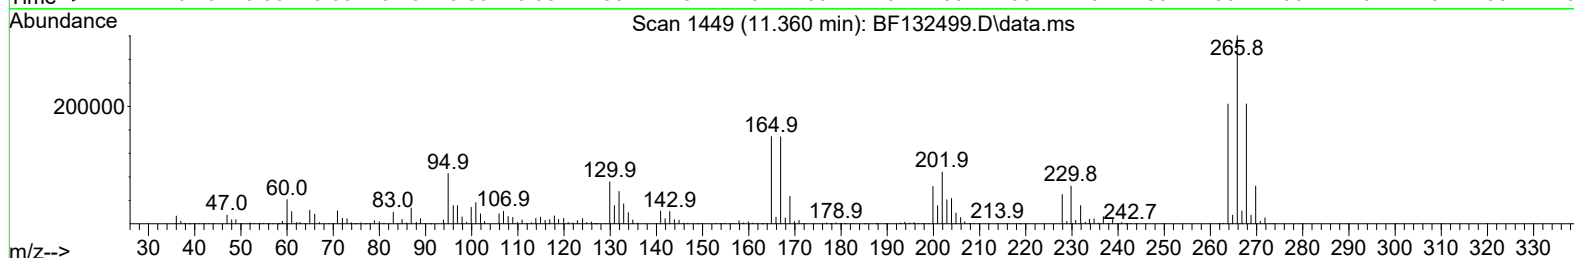


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022223\
Data File : BF132499.D
Acq On : 22 Feb 2023 11:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 04:15:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 00:59:42 2023
Response via : Initial Calibration

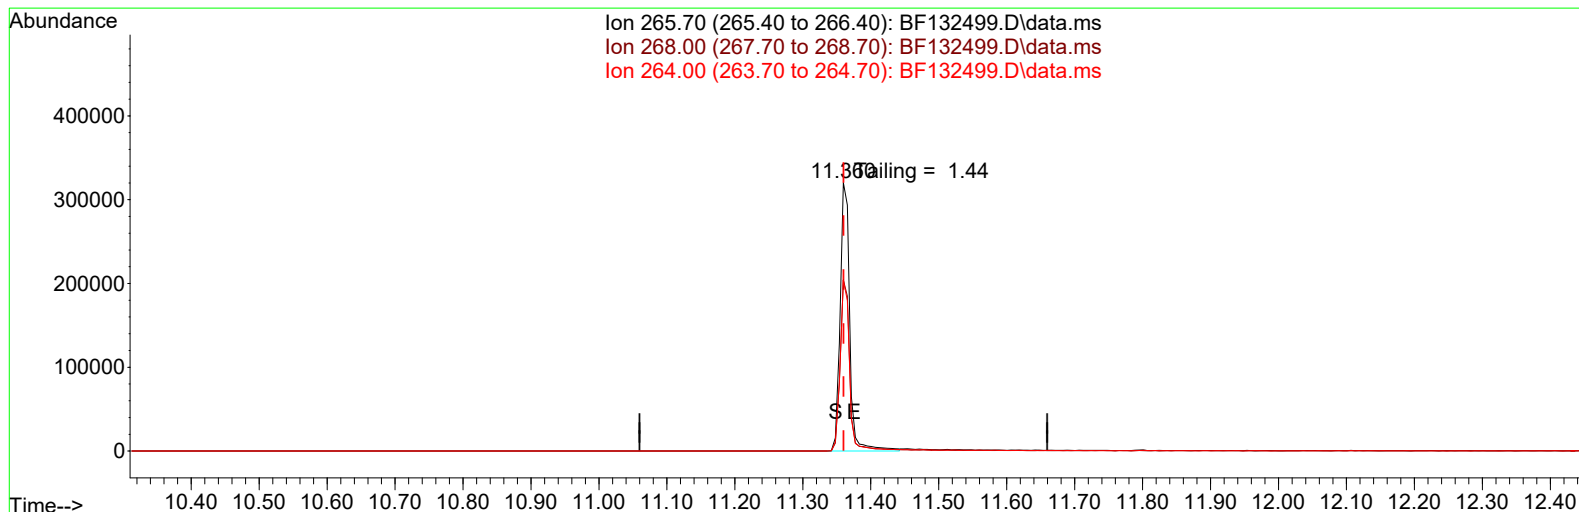

TIC: BF132499.D\data.ms

(70) Pentachlorophenol (C)




11.360min (-0.000) 286384.36 ng

response 314345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.76
264.00	63.60	63.64
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022223\  
Data File : BF132499.D  
Acq On    : 22 Feb 2023  11:39  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Feb 23 04:15:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 00:59:42 2023
Response via : Initial Calibration

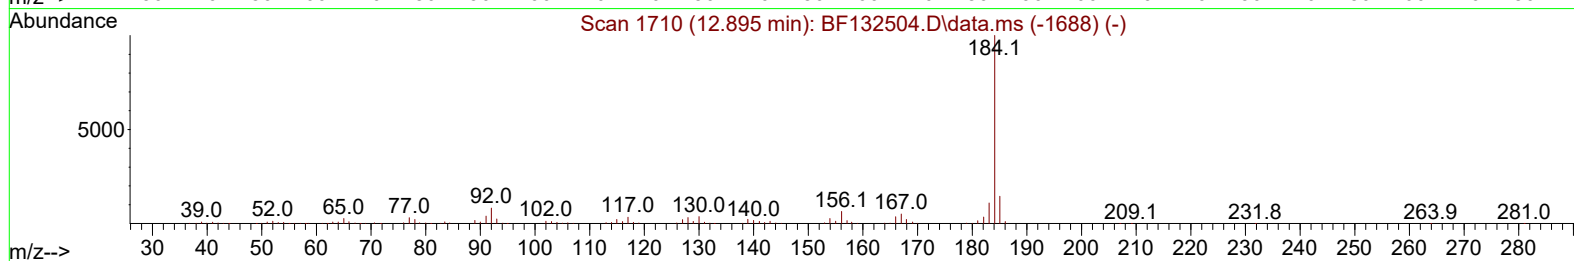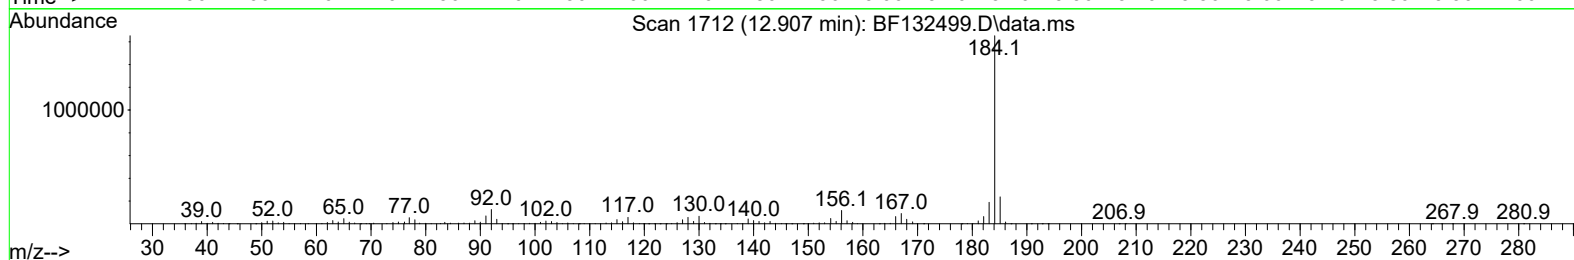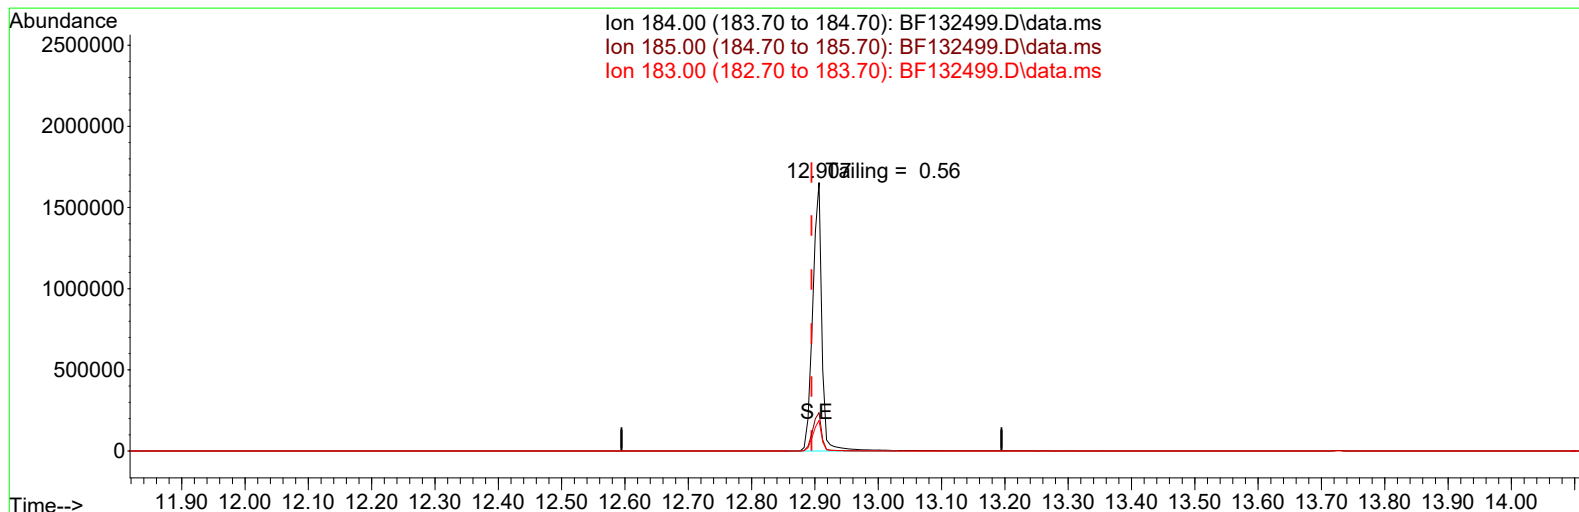

TIC: BF132499.D\data.ms

(77) Benzidine

12.907min (+ 0.012) 1095704.25 ng

response **1680372**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.34
183.00	10.90	11.42
0.00	0.00	0.00