


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022223\
 Data File : BF132499.D
 Acq On : 22 Feb 2023 11:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 23 00:59:42 2023

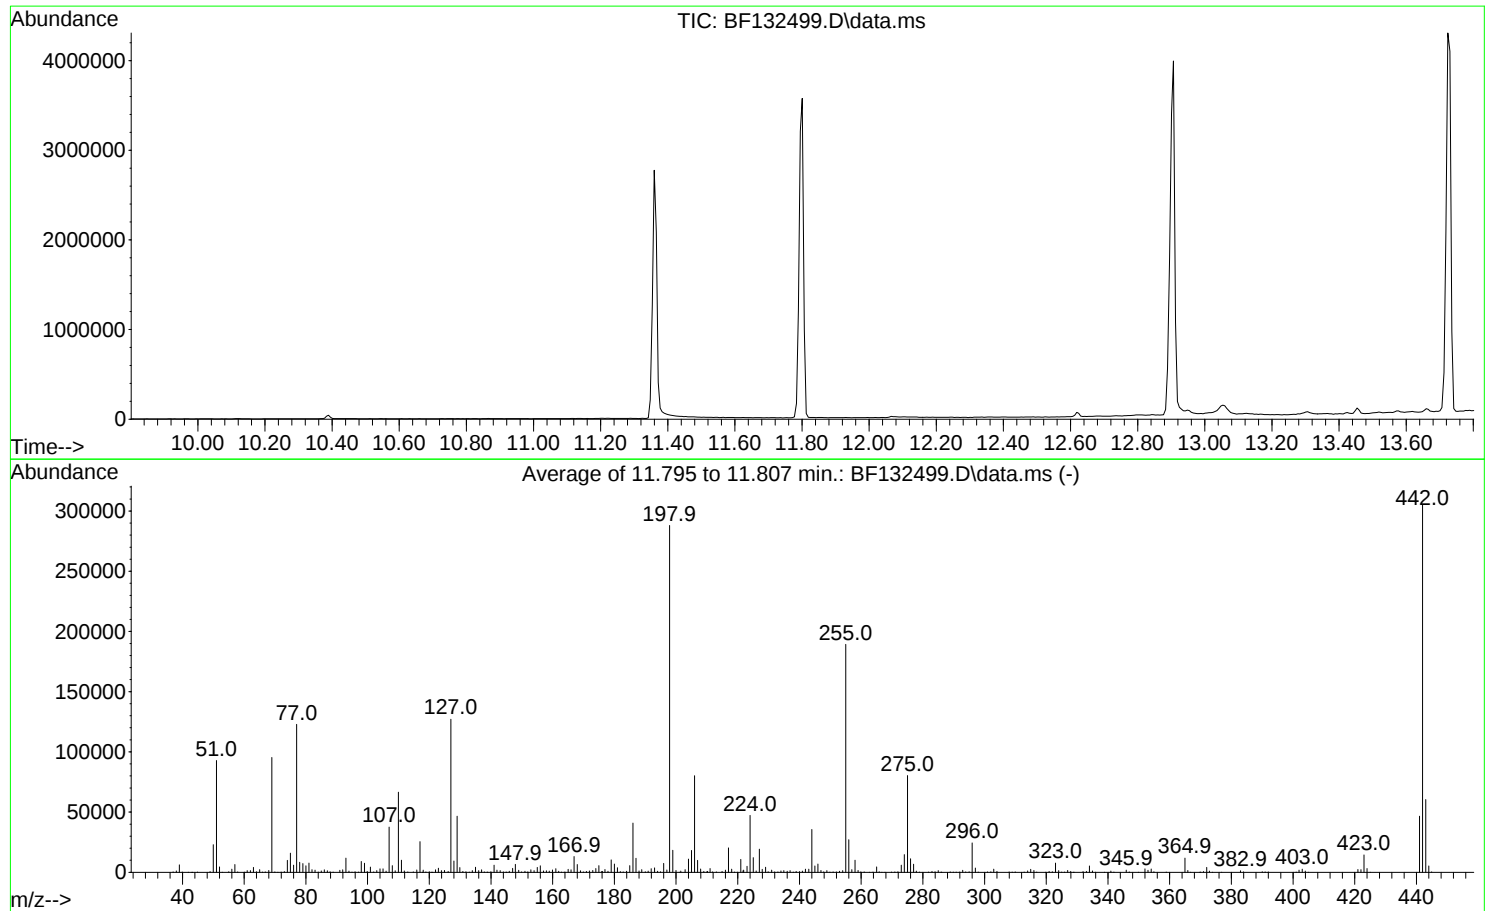




AutoFind: Scans 1523, 1524, 1525; Background Corrected with Scan 1517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	92859	PASS
68	69	0.00	2	1.6	1533	PASS
69	198	0.00	100	33.1	95355	PASS
70	69	0.00	2	0.4	411	PASS
127	198	10	80	44.1	127131	PASS
197	198	0.00	2	0.7	1879	PASS
198	198	100	100	100.0	287997	PASS
199	198	5	9	6.4	18303	PASS
275	198	10	60	27.9	80357	PASS
365	198	1	100	4.1	11723	PASS
441	198	0.01	100	16.2	46619	PASS
442	442	50	100	100.0	305493	PASS
443	442	15	24	19.8	60461	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022223\
Data File : BF132499.D
Acq On : 22 Feb 2023 11:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 23 04:15:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 00:59:42 2023
Response via : Initial Calibration

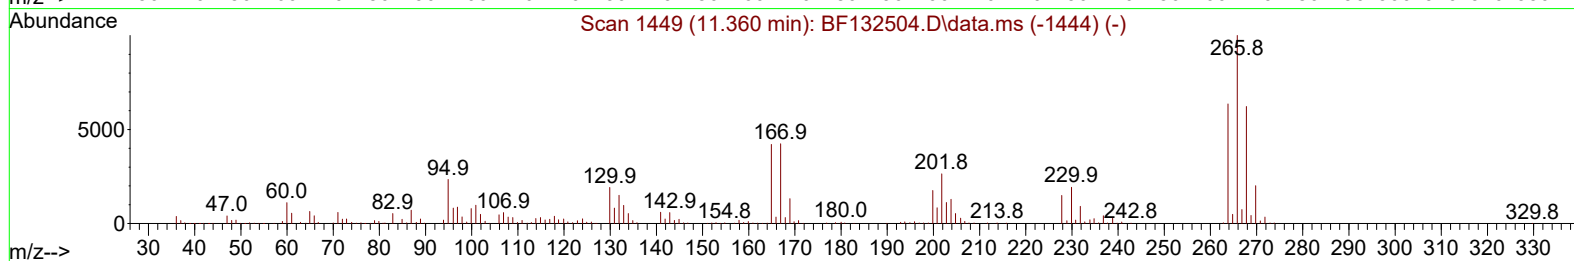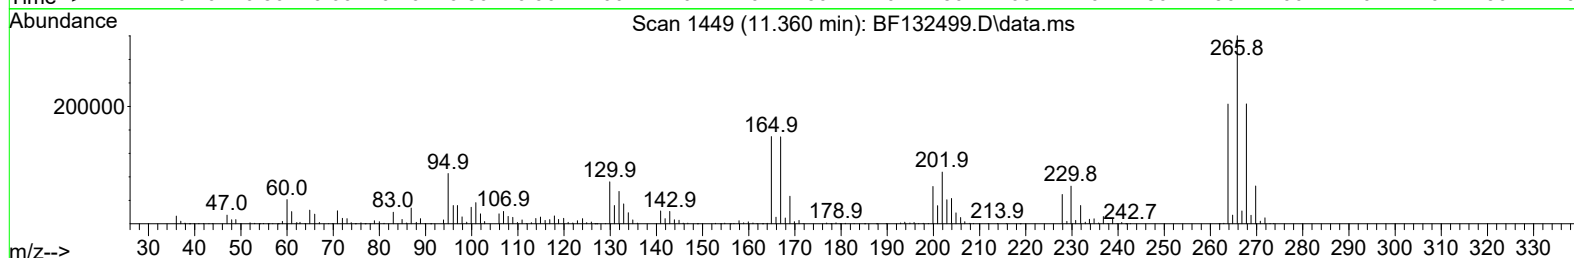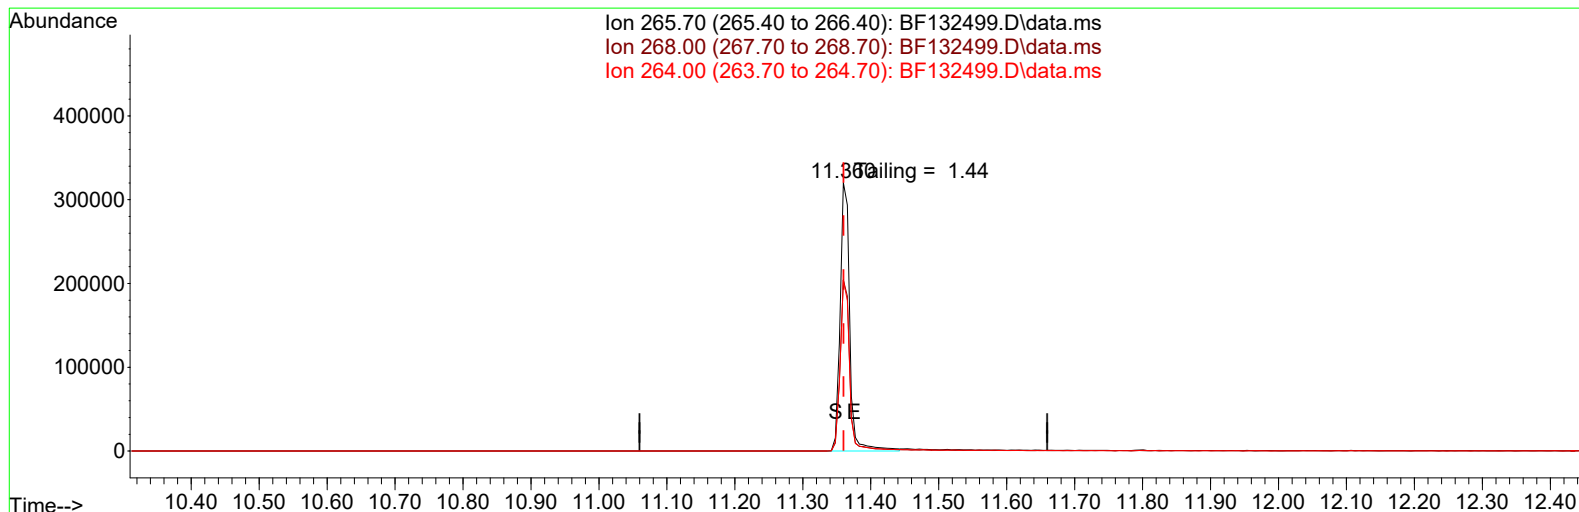

TIC: BF132499.D\data.ms

(70) Pentachlorophenol (C)

11.360min (-0.000) 286384.36 ng




response 314345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.76
264.00	63.60	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022223\
Data File : BF132499.D
Acq On : 22 Feb 2023 11:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 23 04:15:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 00:59:42 2023
Response via : Initial Calibration

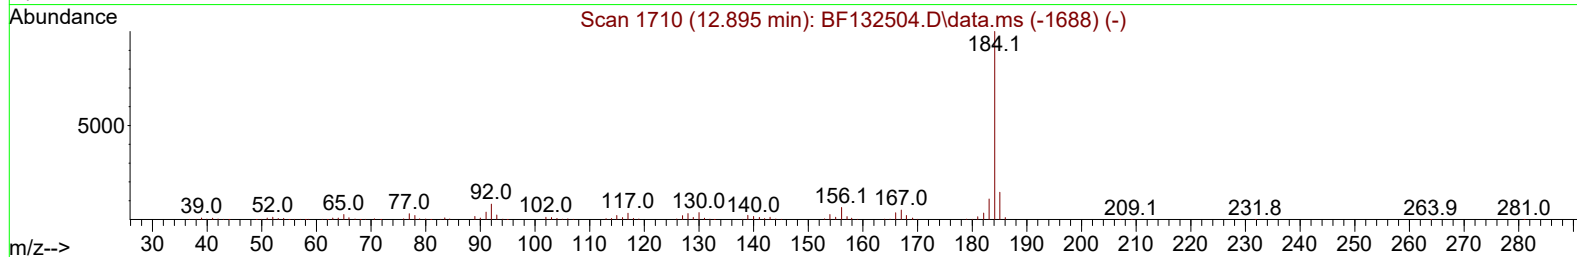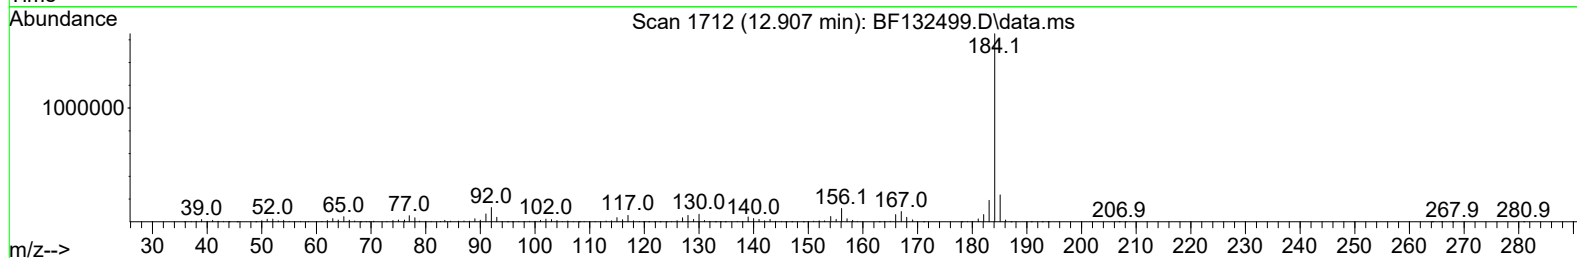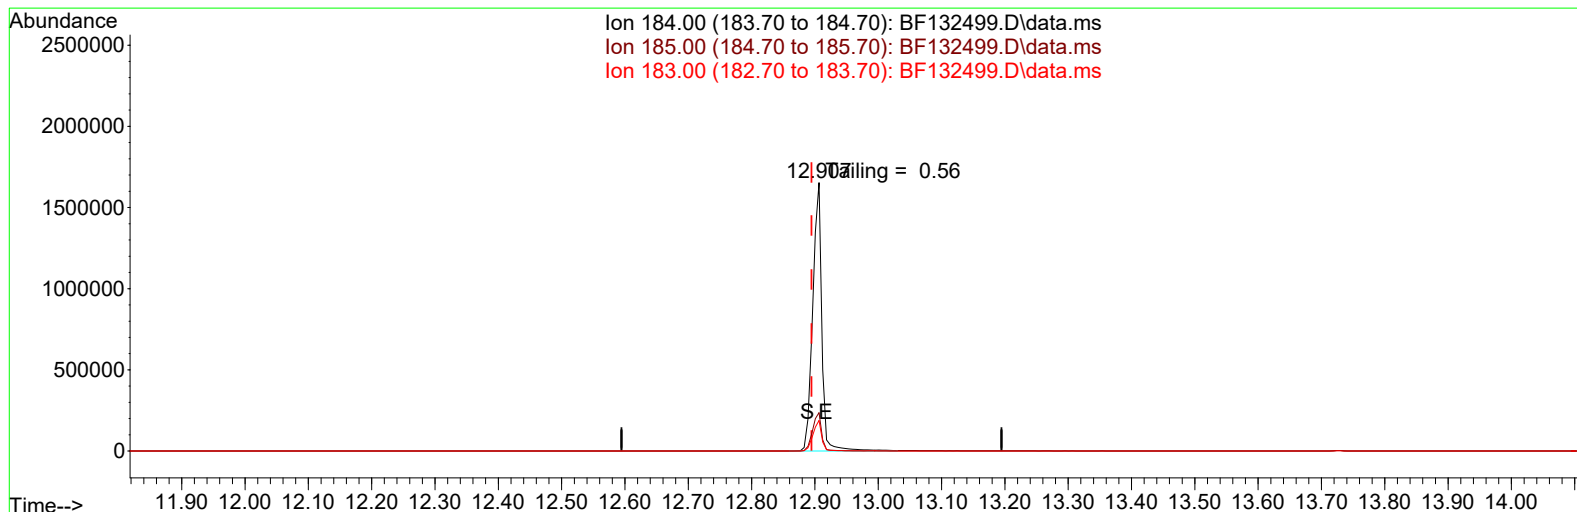

TIC: BF132499.D\data.ms

(77) Benzidine

12.907min (+ 0.012) 1095704.25 ng

response 1680372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.34
183.00	10.90	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/22/2023	BNA_F	<u>BF132499.D</u>
Compound Name	Response	Retention Time
DDT	846683	13.73
DDD	11997	13.454
DDE	319	13.083
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12316	858999	1.43

Instrument :
BNA_F
ClientSampleId :
DFTPP