


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022521\
 Data File : BF123296.D
 Acq On : 25 Feb 2021 12:51
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

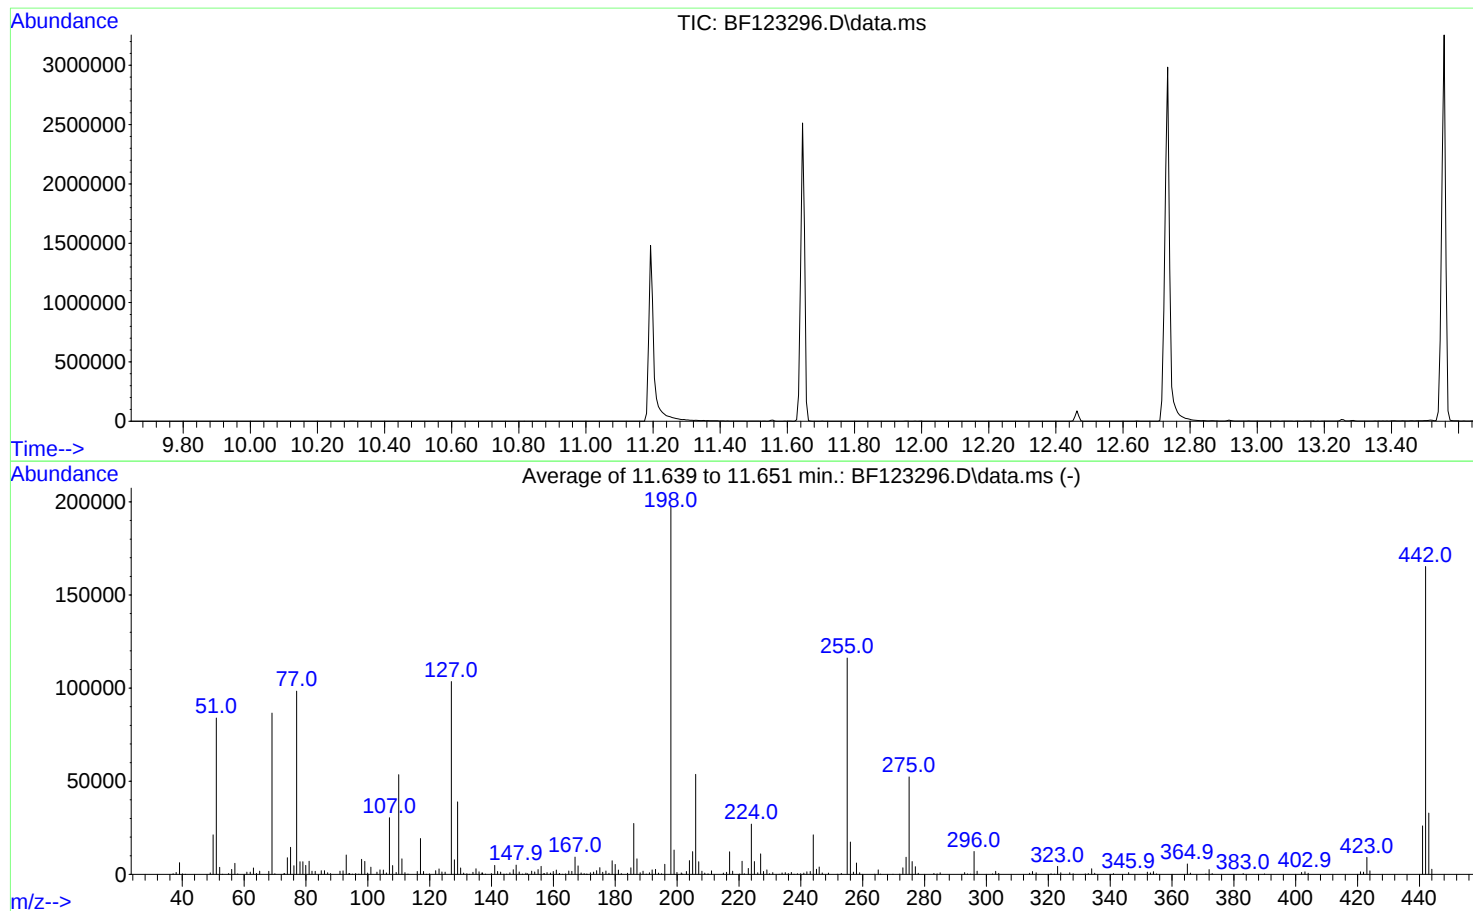




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	83939	PASS
68	69	0.00	2	1.9	1673	PASS
69	198	0.00	100	43.9	86629	PASS
70	69	0.00	2	0.4	309	PASS
127	198	10	80	52.4	103528	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	197504	PASS
199	198	5	9	6.6	13081	PASS
275	198	10	60	26.5	52293	PASS
365	198	1	100	2.8	5602	PASS
441	198	0.01	100	13.2	26045	PASS
442	442	50	100	100.0	165312	PASS
443	442	15	24	19.9	32944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022521\
Data File : BF123296.D
Acq On : 25 Feb 2021 12:51
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 25 14:18:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 16:08:53 2021
Response via : Initial Calibration

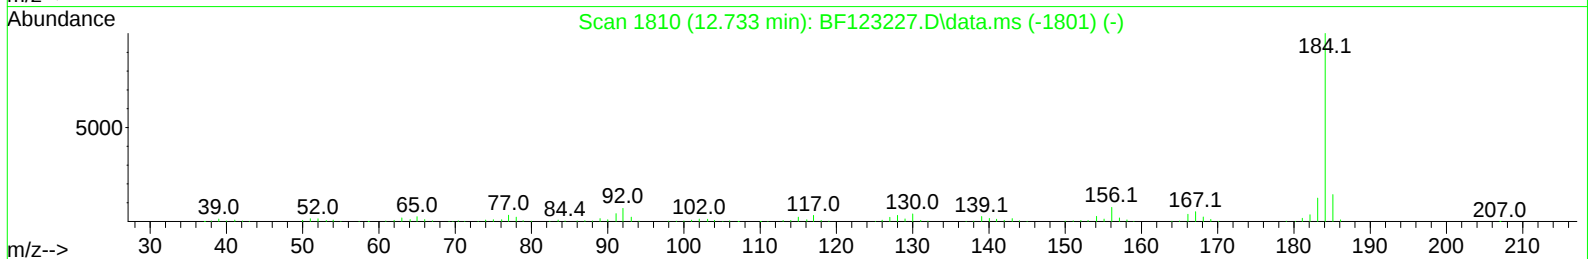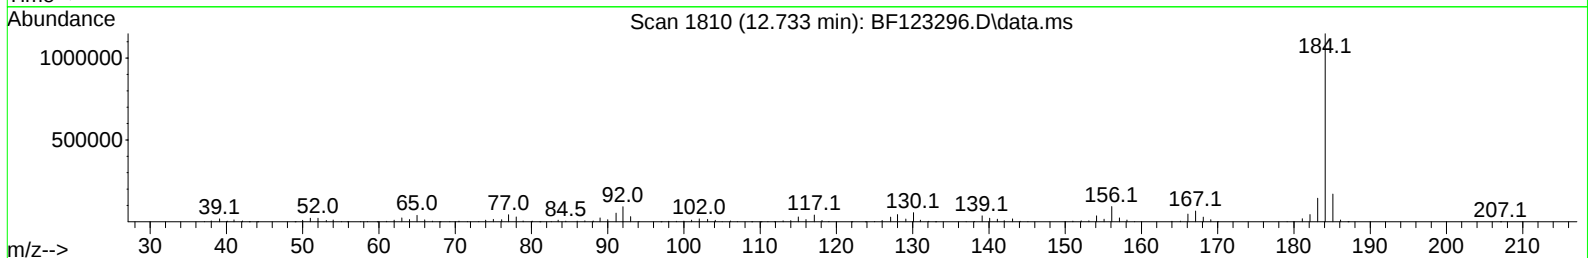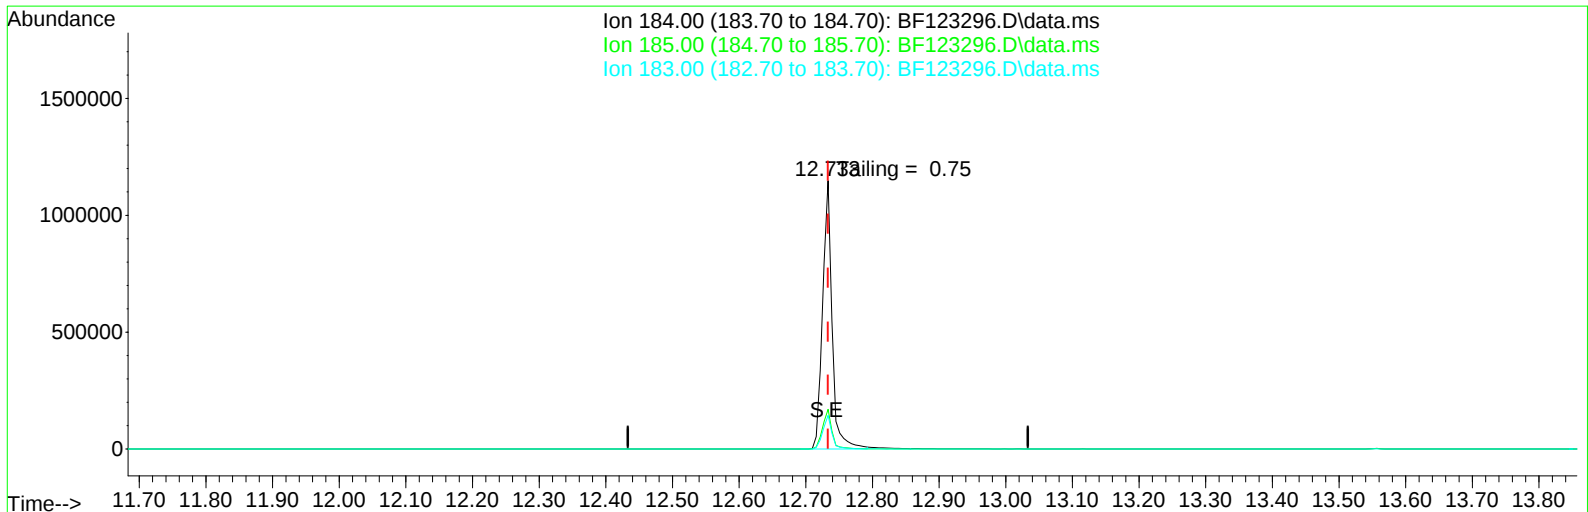

TIC: BF123296.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng

response 1152613

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.80
183.00	12.10	12.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/25/2021	BNA_F	BF123296.D
Compound Name	Response	Retention Time
DDT	496971	13.55
DDD	3505	13.25
DDE	1591	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5096	502067	1.02

Instrument :
BNA_F
ClientSampleId :
DFTPP