

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022620\
 Data File : BF119092.D
 Acq On : 26 Feb 2020 13:55
 Operator : CG/JU
 Sample : L1681-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Feb 26 16:11:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 26 16:03:05 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	152993	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	591870	20.00	ng	-0.01
39) Acenaphthene-d10	9.77	164	324679	20.00	ng	-0.01
64) Phenanthrene-d10	11.26	188	606943	20.00	ng	0.00
76) Chrysene-d12	13.89	240	430597	20.00	ng	-0.01
87) Perylene-d12	15.32	264	337965	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	773168	84.45	ng	0.00
7) Phenol-d6	6.39	99	940198	84.44	ng	-0.02
23) Nitrobenzene-d5	7.30	82	612585	54.65	ng	-0.02
42) 2,4,6-Tribromophenol	10.56	330	342311	80.59	ng	-0.01
45) 2-Fluorobiphenyl	9.10	172	1180373	53.56	ng	-0.01
79) Terphenyl-d14	12.84	244	1357274	54.27	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.30	70	84389	13.007	ng	# 74
25) Isophorone	7.30	82	612579	31.466	ng	# 63
50) Dimethylphthalate	9.49	163	64383	2.593	ng	99
51) 2,6-Dinitrotoluene	9.77	165	41103	7.452	ng	# 33
57) 2,4-Dinitrotoluene	9.77	165	41103	5.749	ng	# 21
67) 4-Bromophenyl-phenylether	10.56	248	22609	2.850	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF022620\
Data File : BF119092.D
Acq On : 26 Feb 2020 13:55
Operator : CG/JU
Sample : L1681-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Feb 26 16:11:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 26 16:03:05 2020
Response via : Initial Calibration

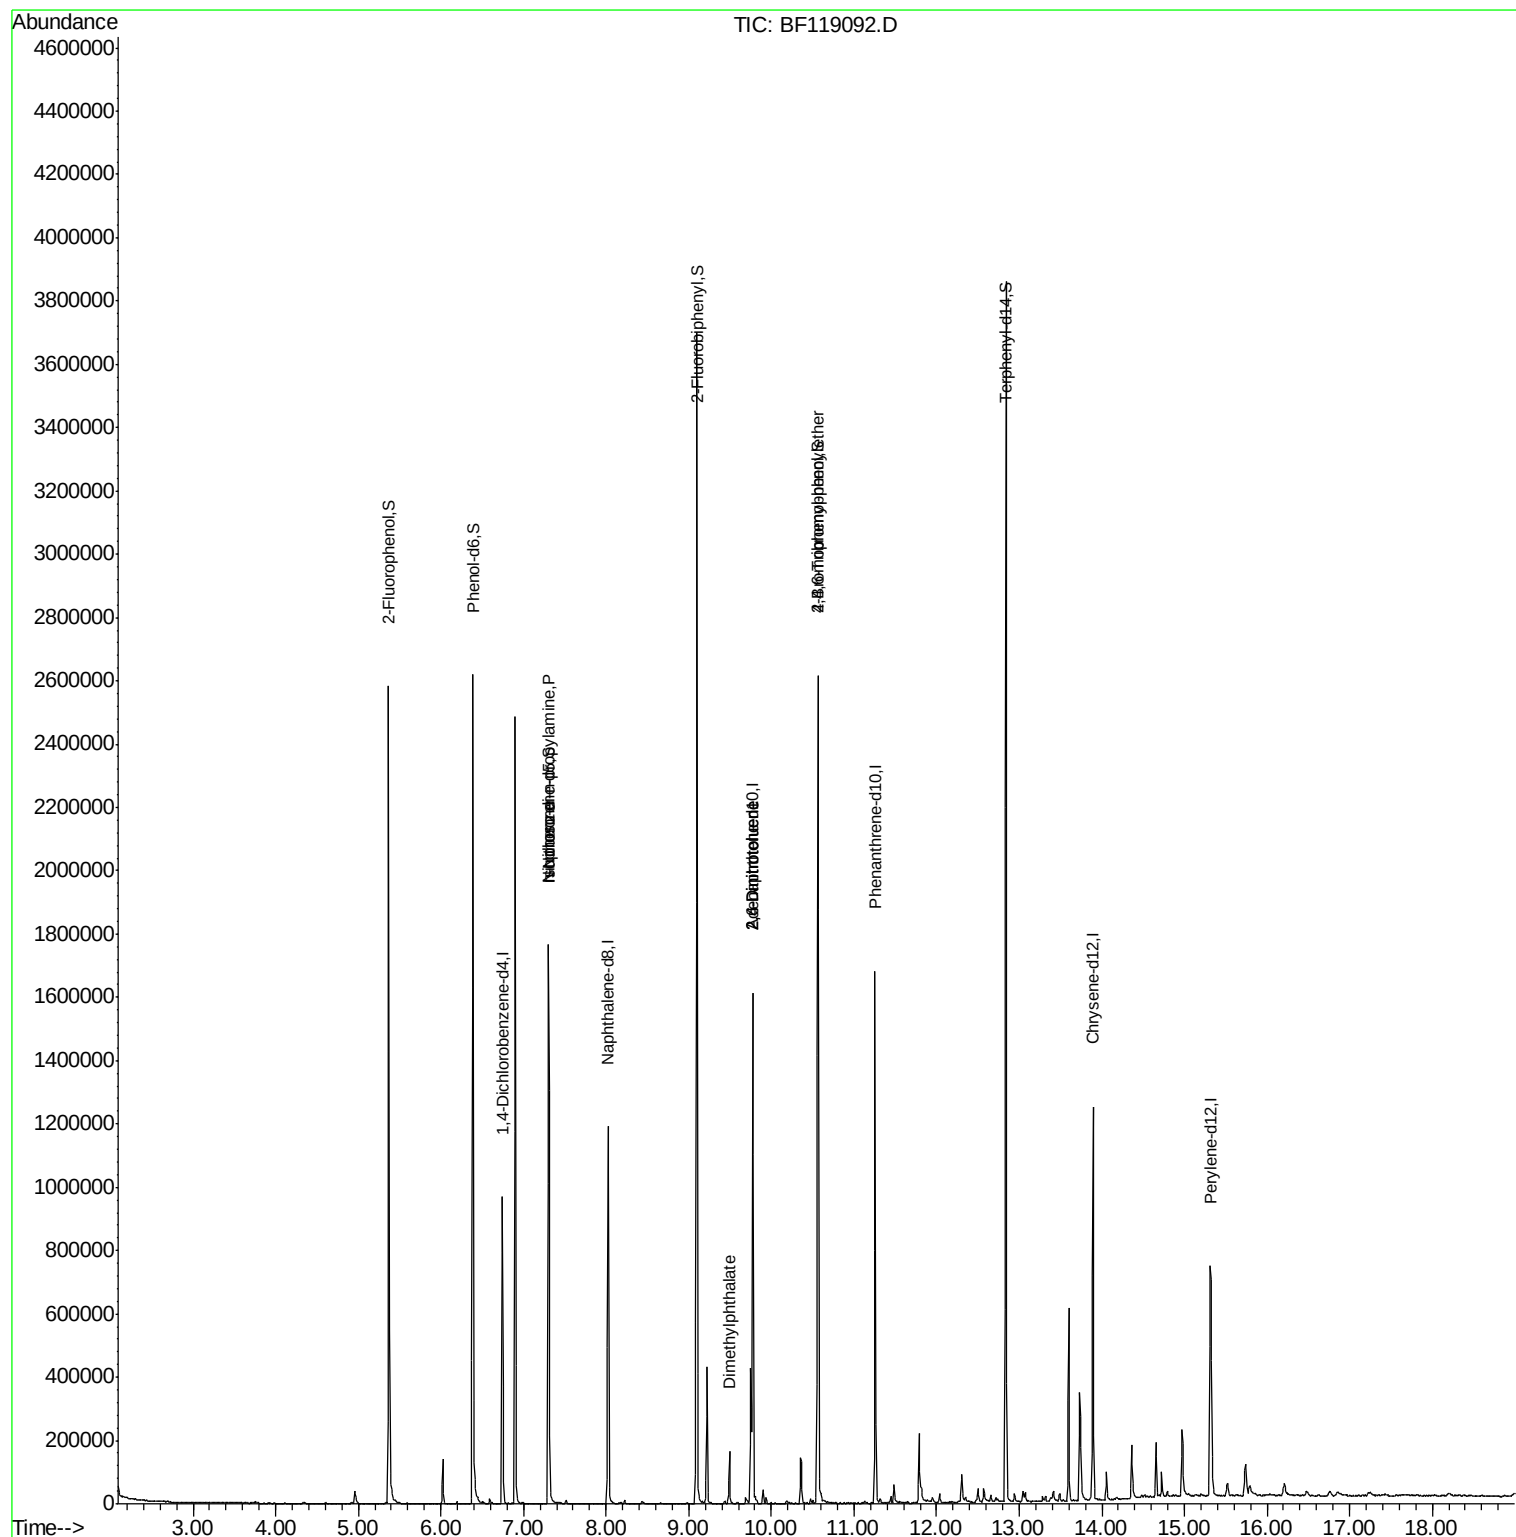

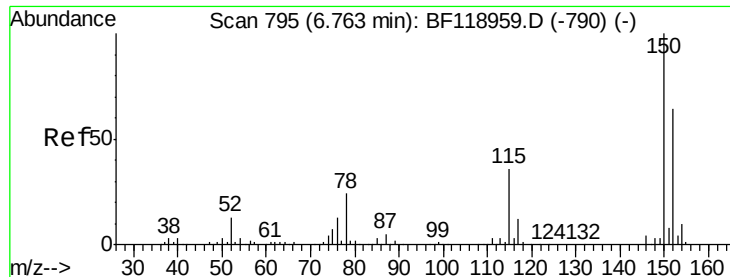


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 792
Delta R.T. -0.00 min
Lab File: BF119092.D
Acq: 26 Feb 2020 13:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.7	123.0	184.6
115	58.0	49.5	74.3

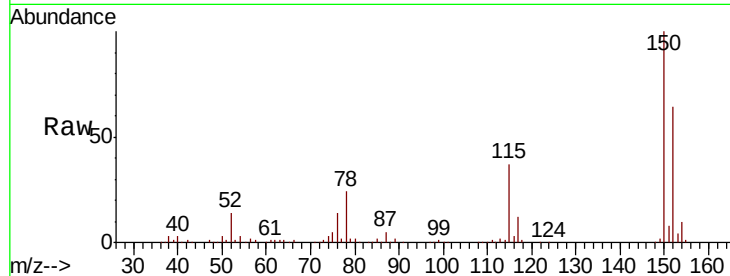


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

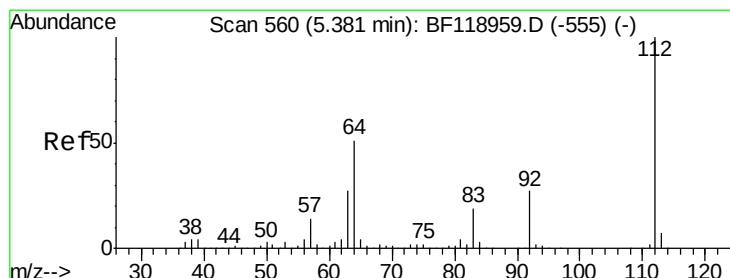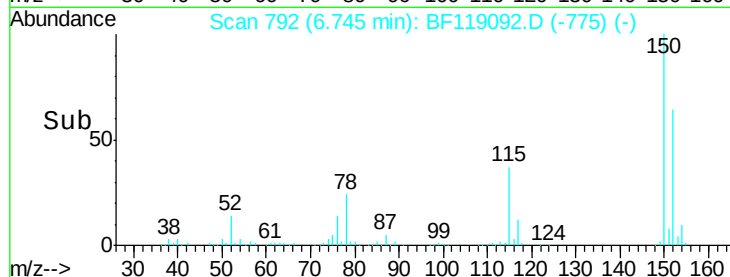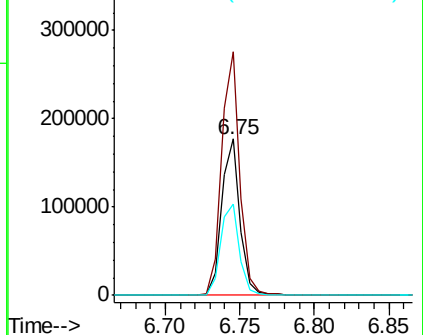



#5


2-Fluorophenol
Concen: 84.455 ng
RT: 5.37 min Scan# 558
Delta R.T. -0.00 min
Lab File: BF119092.D
Acq: 26 Feb 2020 13:55

Tgt Ion	Ratio	Lower	Upper
112	100		
64	55.1	45.0	67.4
63	29.7	24.2	36.4

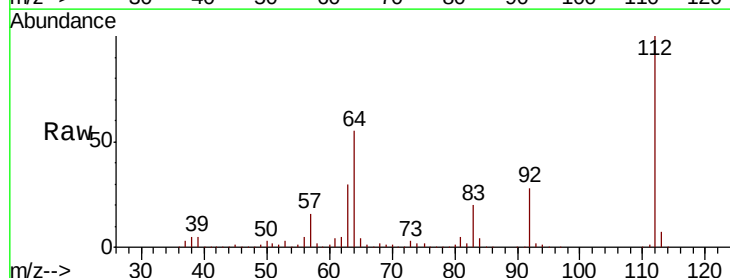

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

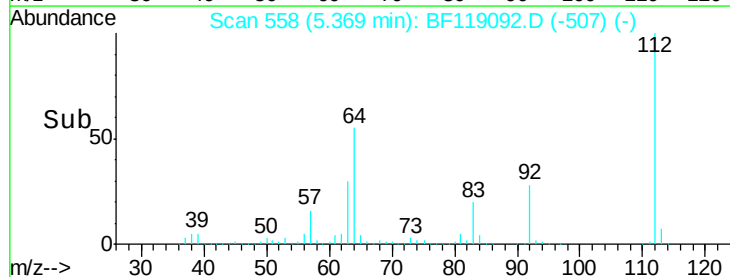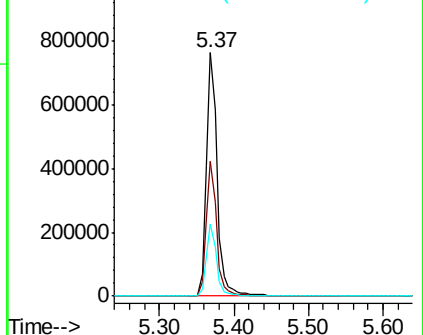

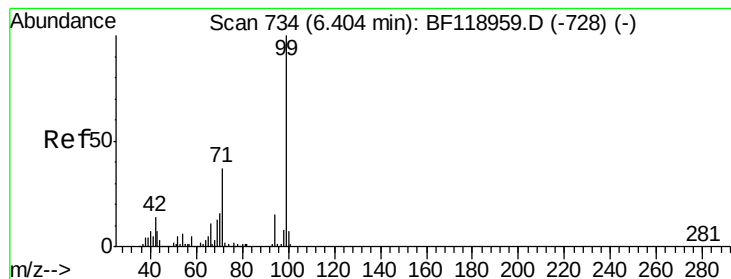

#7

Phenol-d6

Concen: 84.444 ng

RT: 6.39 min Scan# 731

Delta R.T. -0.02 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 940198

Ion Ratio Lower Upper

99 100

42 15.0 12.6 18.8

71 38.6 31.0 46.4

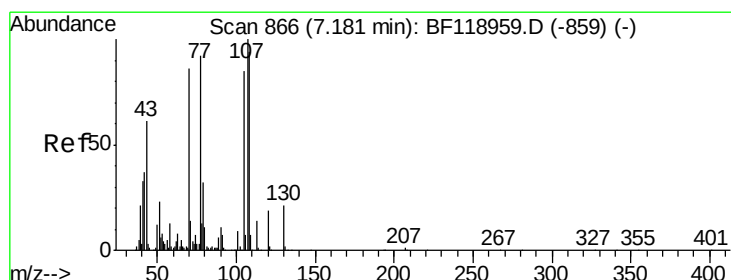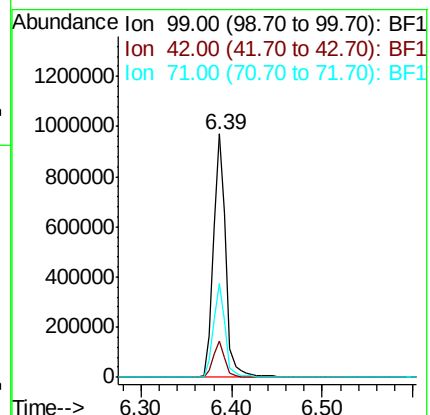

#19

n-Nitroso-di-n-propylamine

Concen: 13.007 ng

RT: 7.30 min Scan# 887

Delta R.T. 0.13 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55

Tgt Ion: 70 Resp: 84389




Ion Ratio Lower Upper


70 100

42 36.2 38.0 57.0#

101 0.0 8.2 12.4#

130 2.1 18.2 27.4#

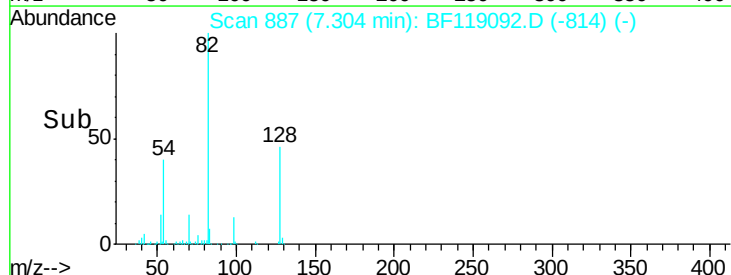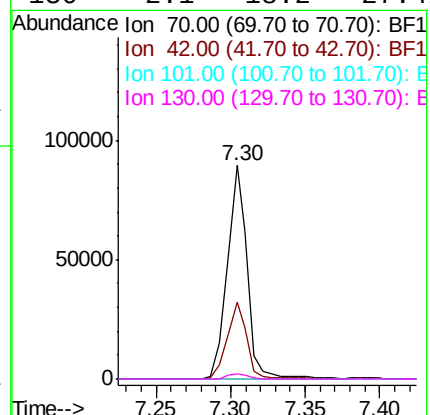



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1009

Delta R.T. -0.01 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 591870


Ion Ratio Lower Upper

136 100

137 11.2 8.8 13.2

54 5.2 3.8 5.6

68 5.5 3.9 5.9



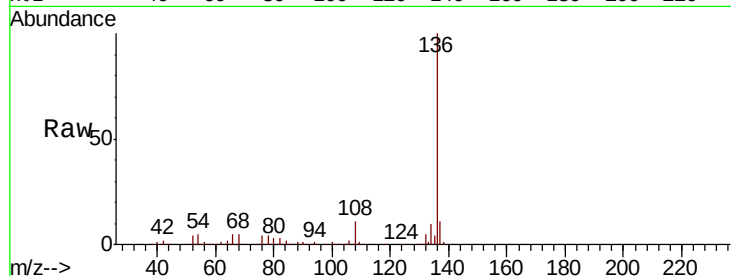


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

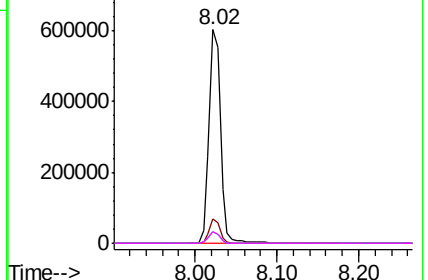

#23

Nitrobenzene-d5

Concen: 54.648 ng

RT: 7.30 min Scan# 887

Delta R.T. -0.02 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55


Tgt Ion: 82 Resp: 612585

Ion Ratio Lower Upper

82 100

128 46.3 37.9 56.9



54 40.0 33.4 50.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

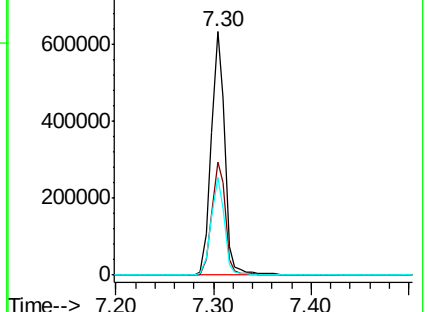

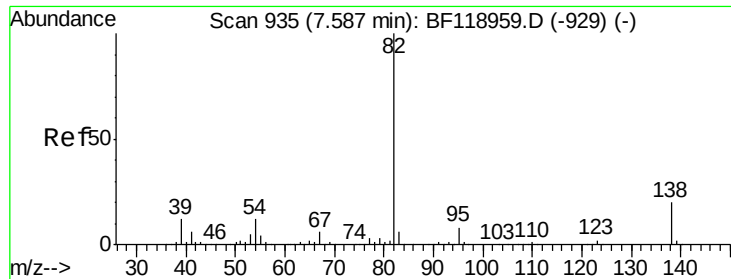

#25

Isophorone

Concen: 31.466 ng

RT: 7.30 min Scan# 887

Delta R.T. -0.28 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 612579

Ion Ratio Lower Upper

82 100

95 0.0 6.4 9.6#




138 0.0 15.7 23.5#

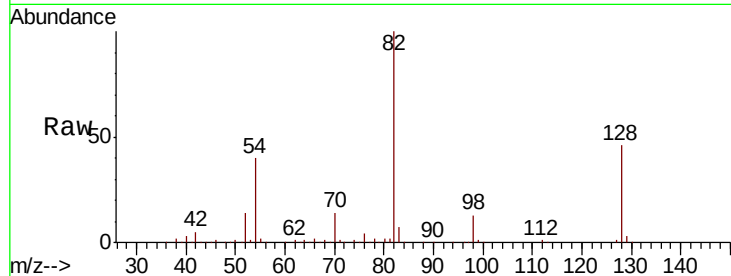

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

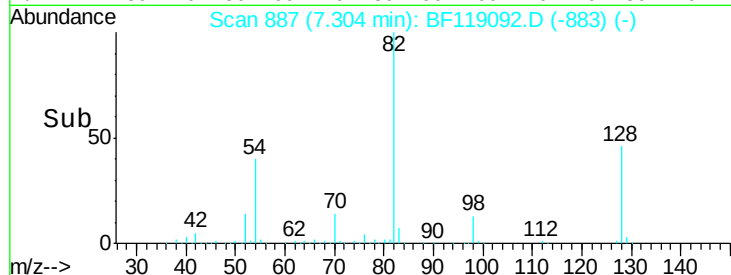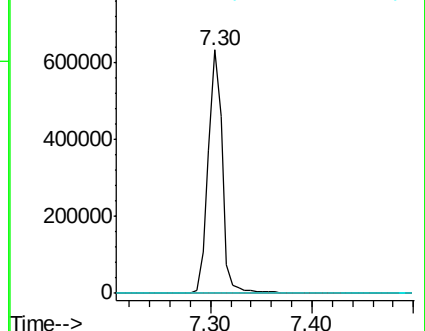

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.77 min Scan# 1307

Delta R.T. -0.01 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55


Tgt Ion:164 Resp: 324679

Ion Ratio Lower Upper

164 100

162 101.8 81.8 122.8



160 44.0 36.0 54.0




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

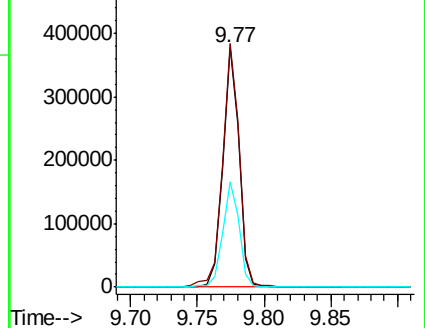

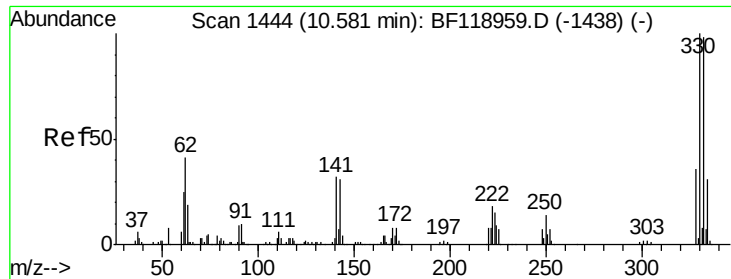

#42

2,4,6-Tribromophenol

Concen: 80.594 ng

RT: 10.56 min Scan# 1441

Delta R.T. -0.01 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55

Instrument :

BNA_F

ClientSampleId :


Tot Ion:330 Resp: 342311

Ion Ratio Lower Upper




330 100

332 97.2 76.0 114.0

141 29.9 22.9 34.3



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

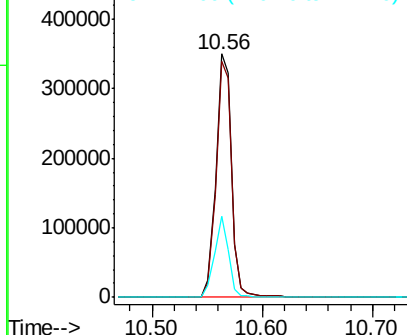

#45

2-Fluorobiphenyl

Concen: 53.557 ng

RT: 9.10 min Scan# 1192

Delta R.T. -0.01 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55


Tgt Ion:172 Resp: 1180373

Ion Ratio Lower Upper



172 100


171 35.9 30.6 45.8

170 24.1 20.2 30.2



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

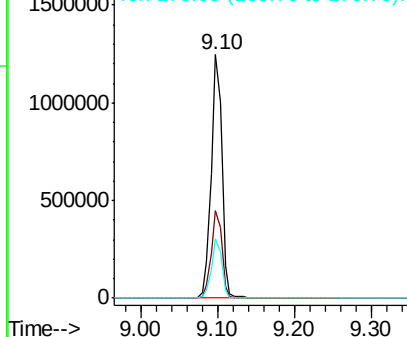







#50
Dimethylphthalate
Concen: 2.593 ng
RT: 9.49 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BF119092.D
Acq: 26 Feb 2020 13:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 64383
Ion Ratio Lower Upper
163 100
194 4.3 3.5 5.3
164 10.0 8.4 12.6

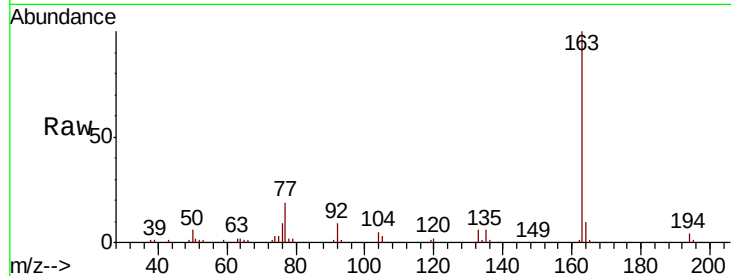


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

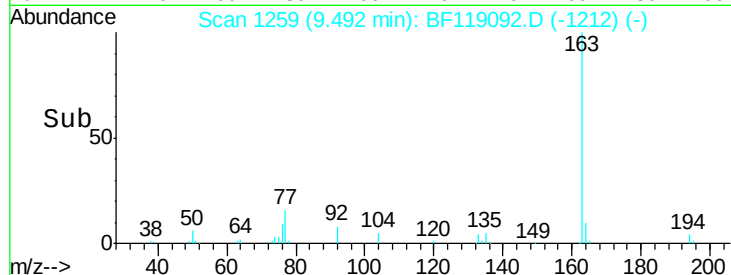
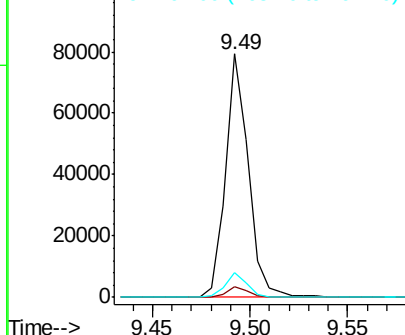



#51
2,6-Dinitrotoluene
Concen: 7.452 ng
RT: 9.77 min Scan# 1307
Delta R.T. 0.19 min
Lab File: BF119092.D
Acq: 26 Feb 2020 13:55

Tgt Ion:165 Resp: 41103
Ion Ratio Lower Upper
165 100
63 1.3 34.3 51.5#
89 1.4 38.3 57.5#

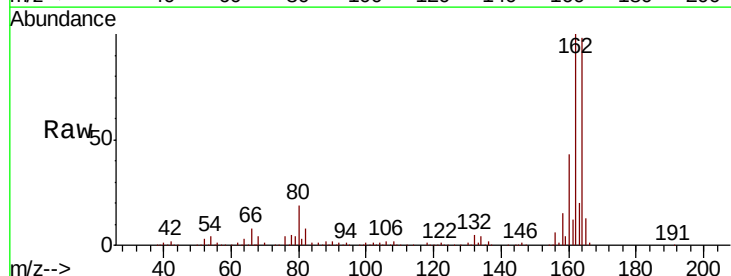

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

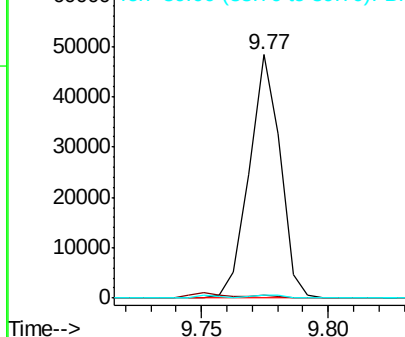




#57
 2,4-Dinitrotoluene
 Concen: 5.749 ng
 RT: 9.77 min Scan# 1307
 Delta R.T. -0.21 min
 Lab File: BF119092.D
 Acq: 26 Feb 2020 13:55

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.3	42.3	63.5#
89	1.4	60.2	90.4#
182	0.0	2.3	3.5#



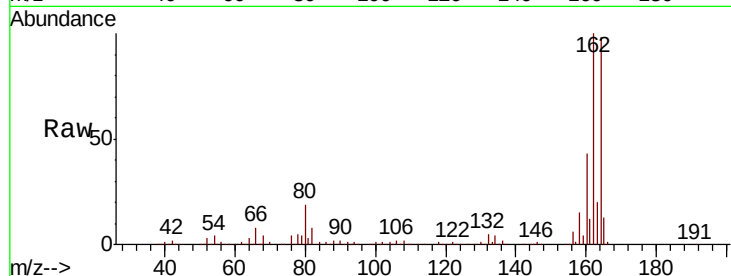


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

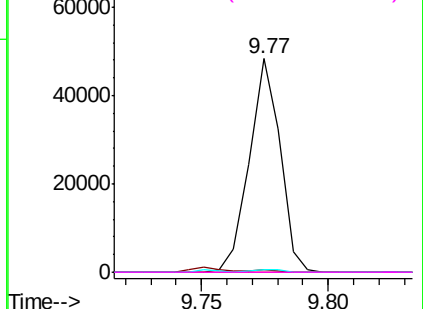

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.26 min Scan# 1559
 Delta R.T. -0.01 min
 Lab File: BF119092.D
 Acq: 26 Feb 2020 13:55



Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.9	7.1	10.7
80	9.8	7.8	11.8

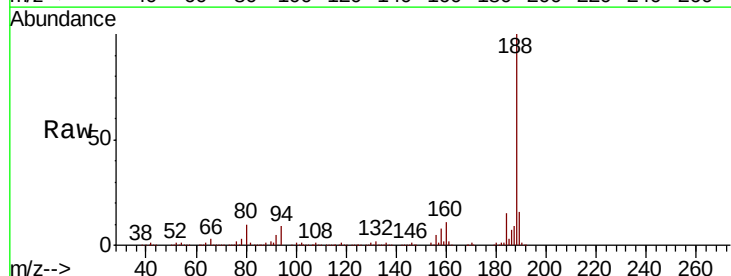


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

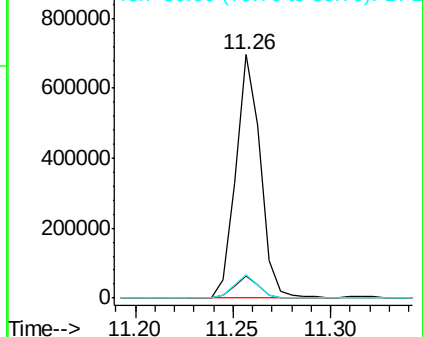


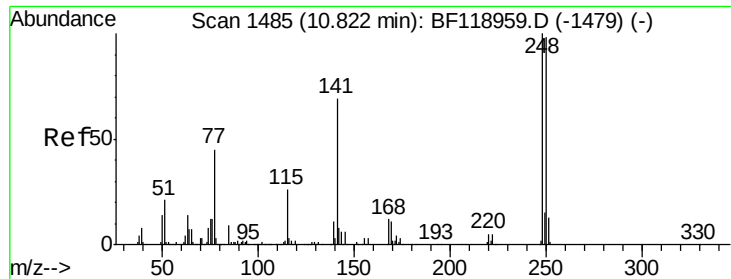




#67
4-Bromophenyl-phenylether
Concen: 2.850 ng
RT: 10.56 min Scan# 1441
Delta R.T. -0.25 min
Lab File: BF119092.D
Acq: 26 Feb 2020 13:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 22609
Ion Ratio Lower Upper
248 100
250 198.4 76.7 115.1#
141 469.6 60.7 91.1#




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

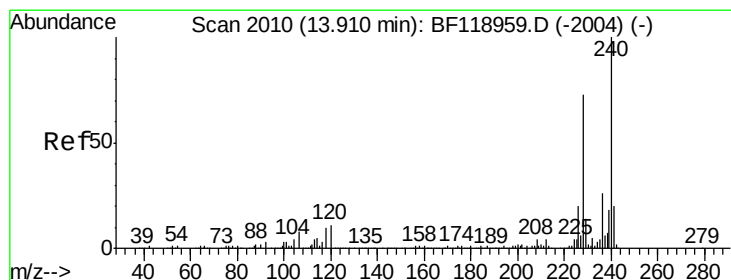
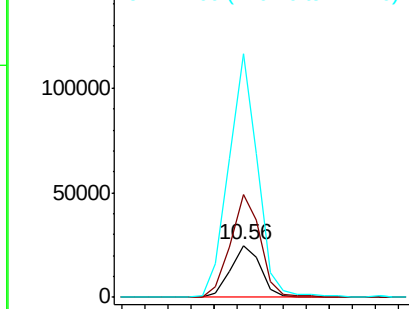



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.89 min Scan# 2007
Delta R.T. -0.01 min
Lab File: BF119092.D
Acq: 26 Feb 2020 13:55

Tgt Ion:240 Resp: 430597
Ion Ratio Lower Upper
240 100
120 10.3 8.4 12.6
236 25.8 21.0 31.4

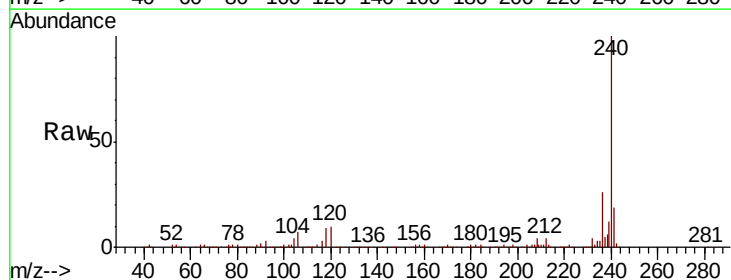

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

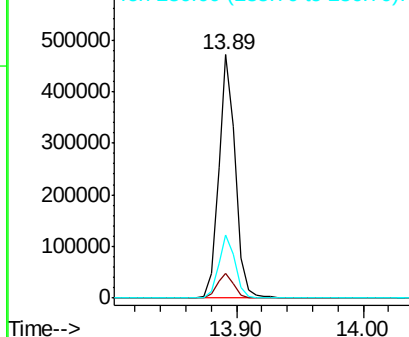

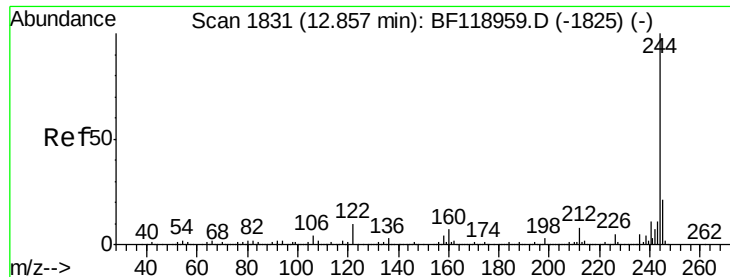

#79

Terphenyl-d14

Concen: 54.268 ng

RT: 12.84 min Scan# 1828

Delta R.T. -0.01 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1357274

Ion Ratio Lower Upper

244 100

212 7.4 6.6 10.0




122 10.1 8.2 12.2

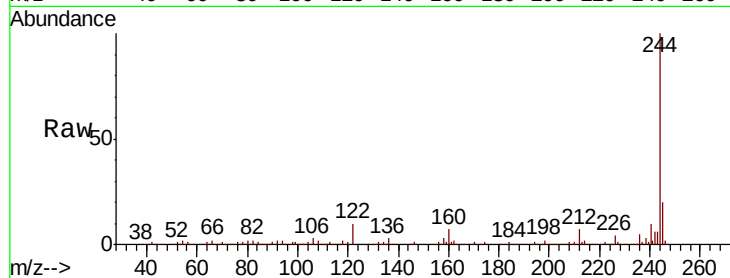

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

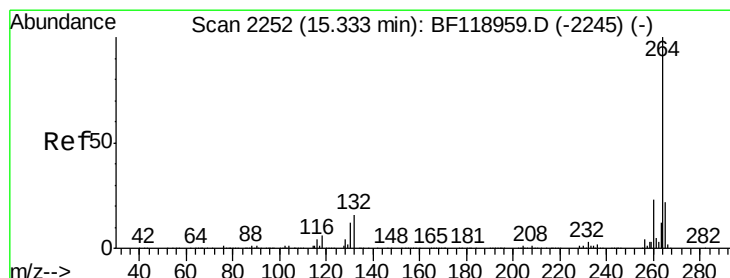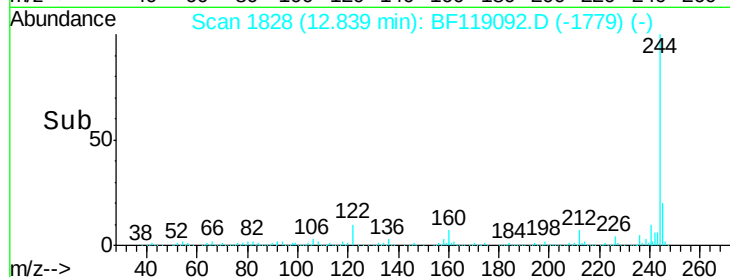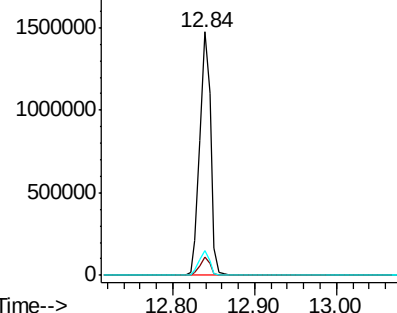

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.32 min Scan# 2249

Delta R.T. -0.01 min

Lab File: BF119092.D

Acq: 26 Feb 2020 13:55


Tgt Ion:264 Resp: 337965

Ion Ratio Lower Upper

264 100

260 23.9 19.4 29.2

265 21.4 17.7 26.5

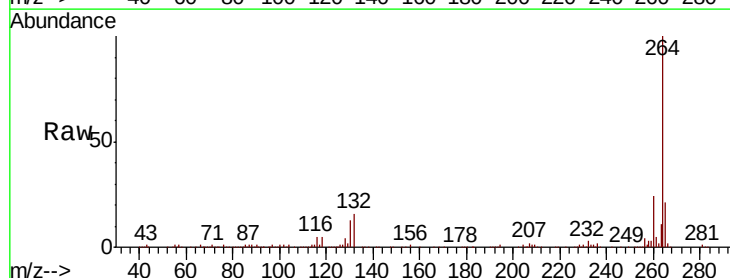

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

