
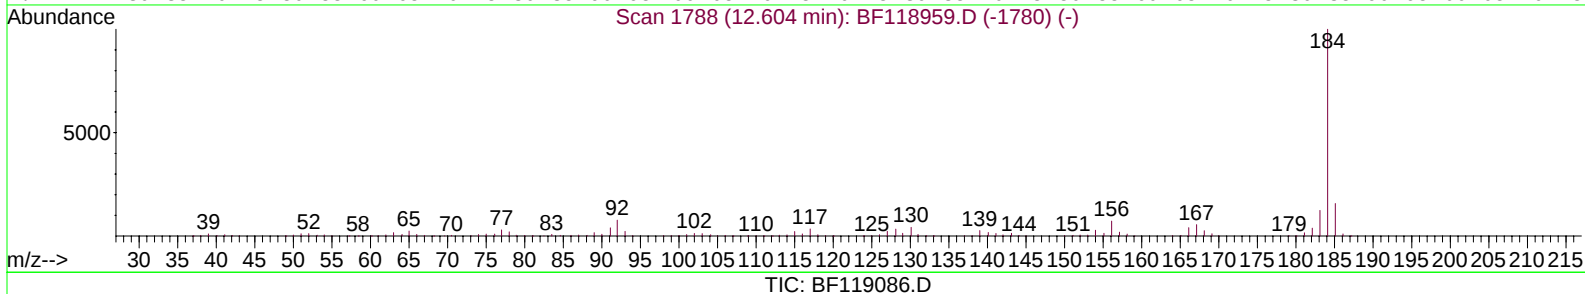
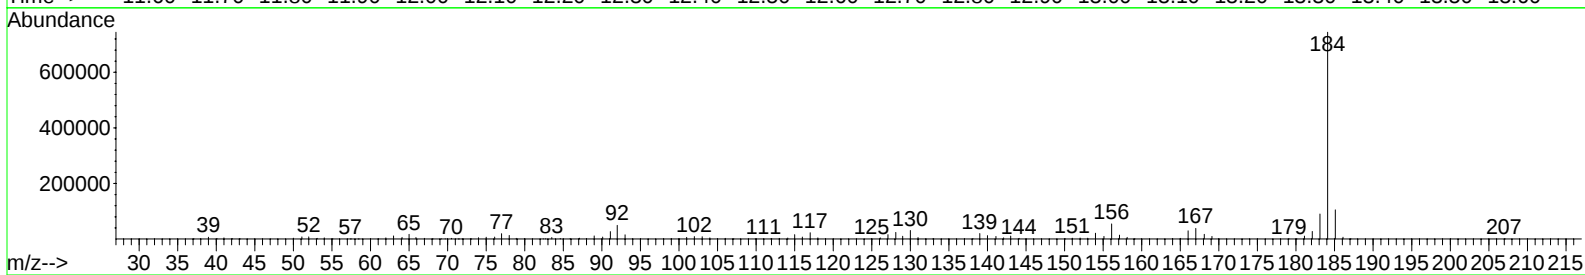


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022620\
Data File : BF119086.D
Acq On : 26 Feb 2020 10:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 17:52:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 26 16:03:05 2020
Response via : Initial Calibration

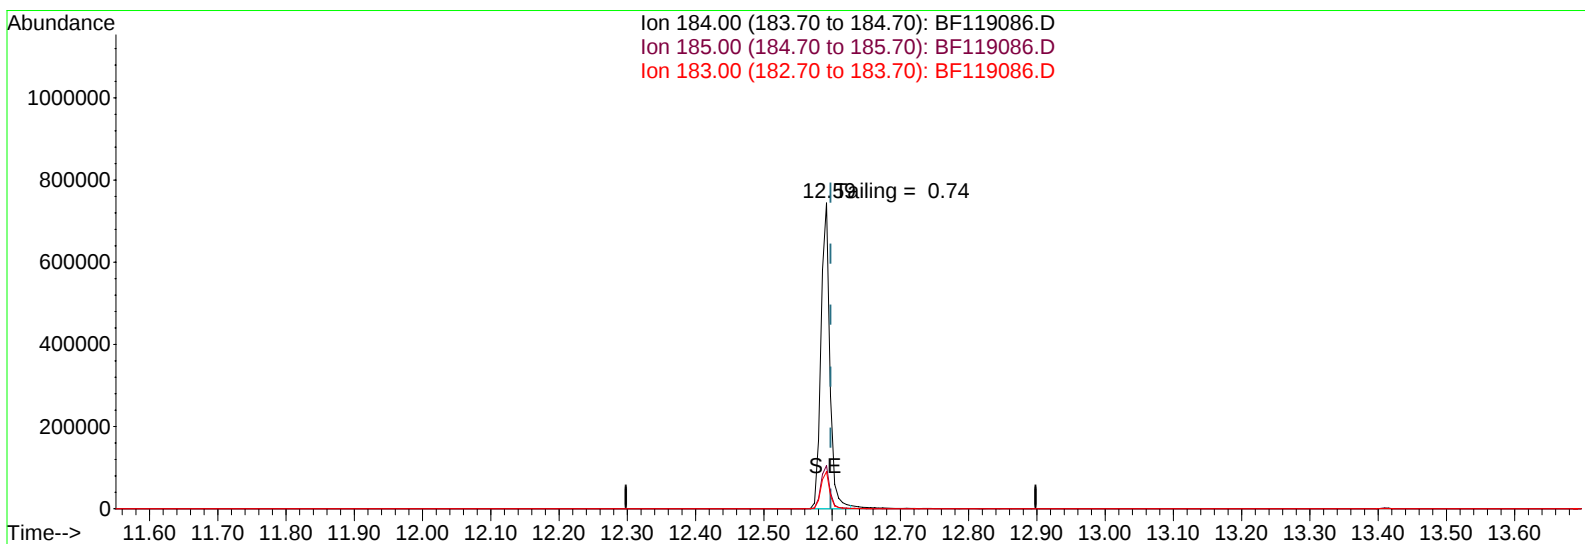

(77) Benzidine




12.592min (-0.006) 0.00ng

response 680953

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.14
183.00	12.40	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022620\
 Data File : BF119086.D
 Acq On : 26 Feb 2020 10:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 17:52:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 26 16:03:05 2020
 Response via : Initial Calibration

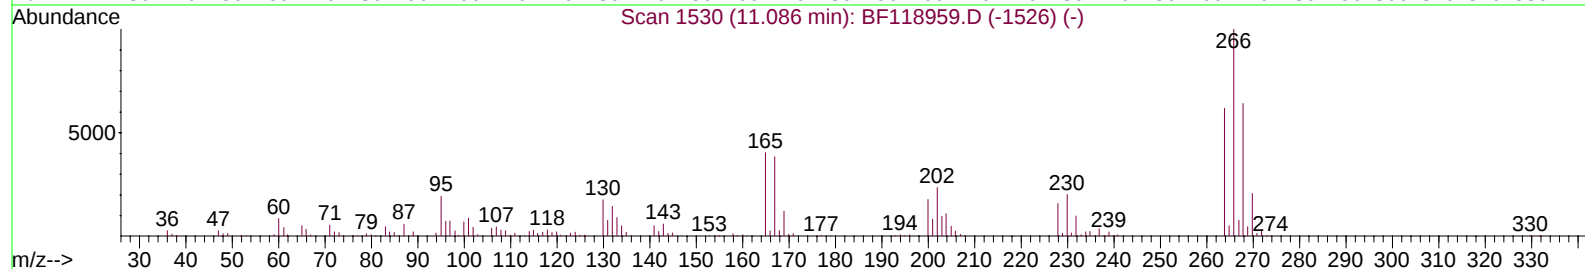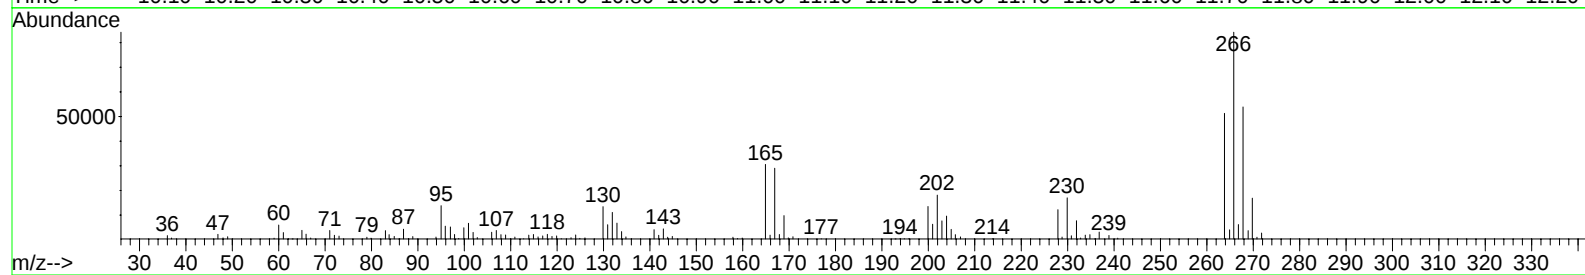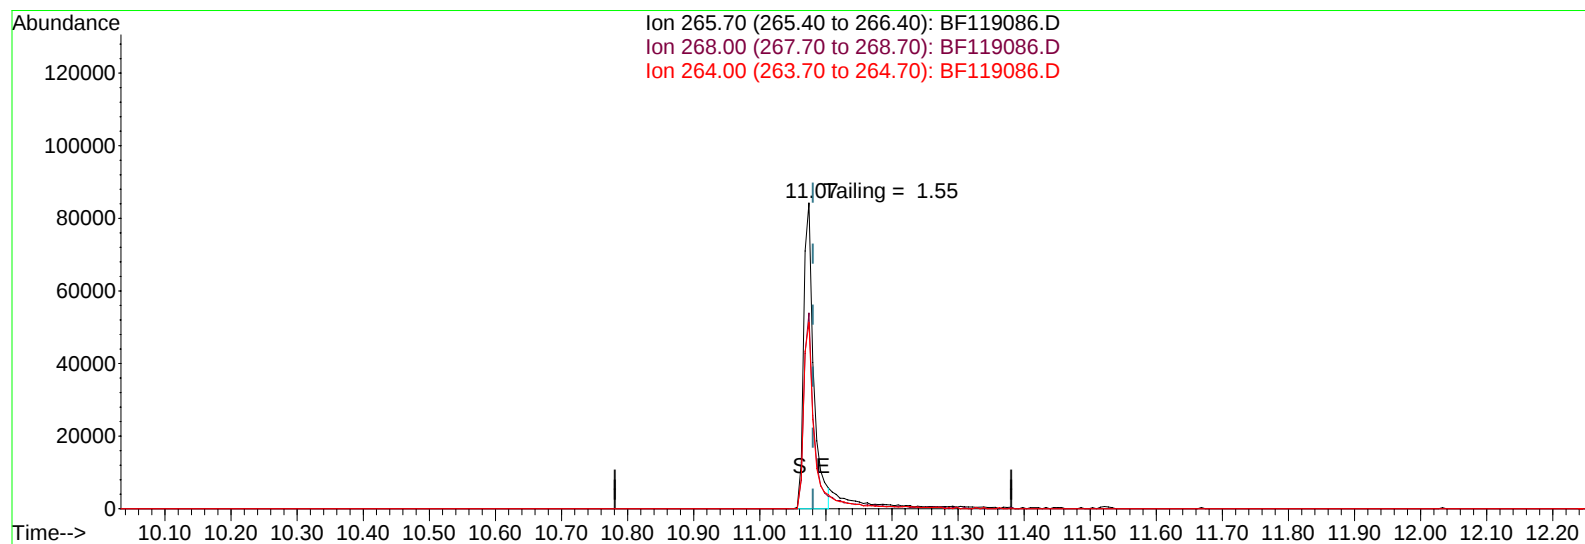

TIC: BF119086.D

(70) Pentachlorophenol (C)

11.074min (-0.006) 28130.73ng

response 102465

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	64.01
264.00	63.70	60.93
0.00	0.00	0.00