


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF022620\
 Data File : BF119086.D
 Acq On : 26 Feb 2020 10:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 26 16:03:05 2020

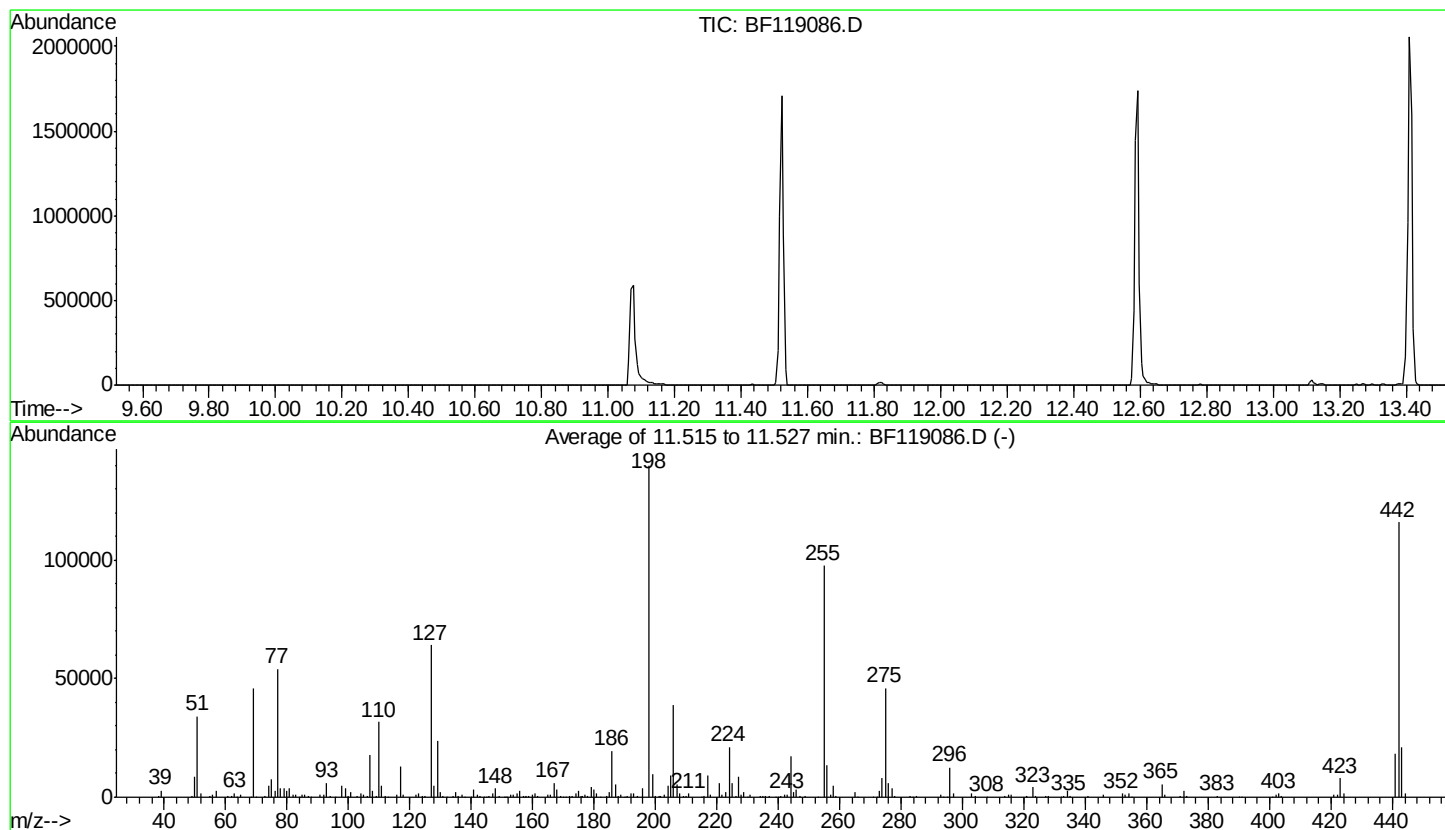

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	34148	PASS
68	69	0.00	2	0.5	235	PASS
69	198	0.00	100	32.8	45821	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	45.9	64093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139776	PASS
199	198	5	9	6.8	9569	PASS
275	198	10	60	32.8	45896	PASS
365	198	1	100	4.1	5681	PASS
441	198	0.01	100	13.2	18440	PASS
442	198	50	100	82.8	115768	PASS
443	442	15	24	18.0	20870	PASS