
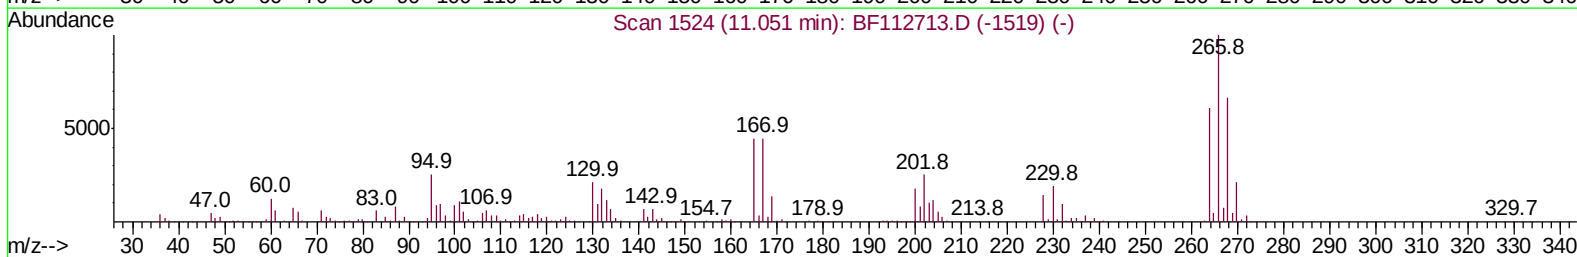
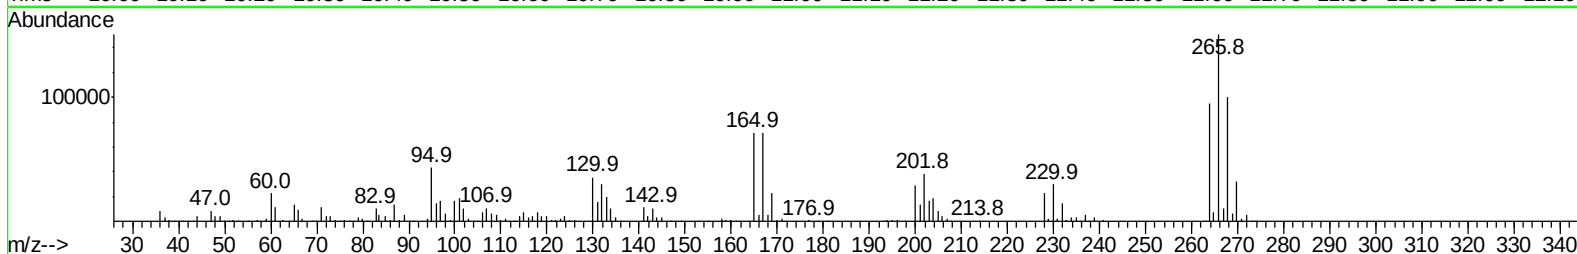


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022719\
Data File : BF112709.D
Acq On : 27 Feb 2019 9:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:01:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 27 16:08:50 2019
Response via : Initial Calibration

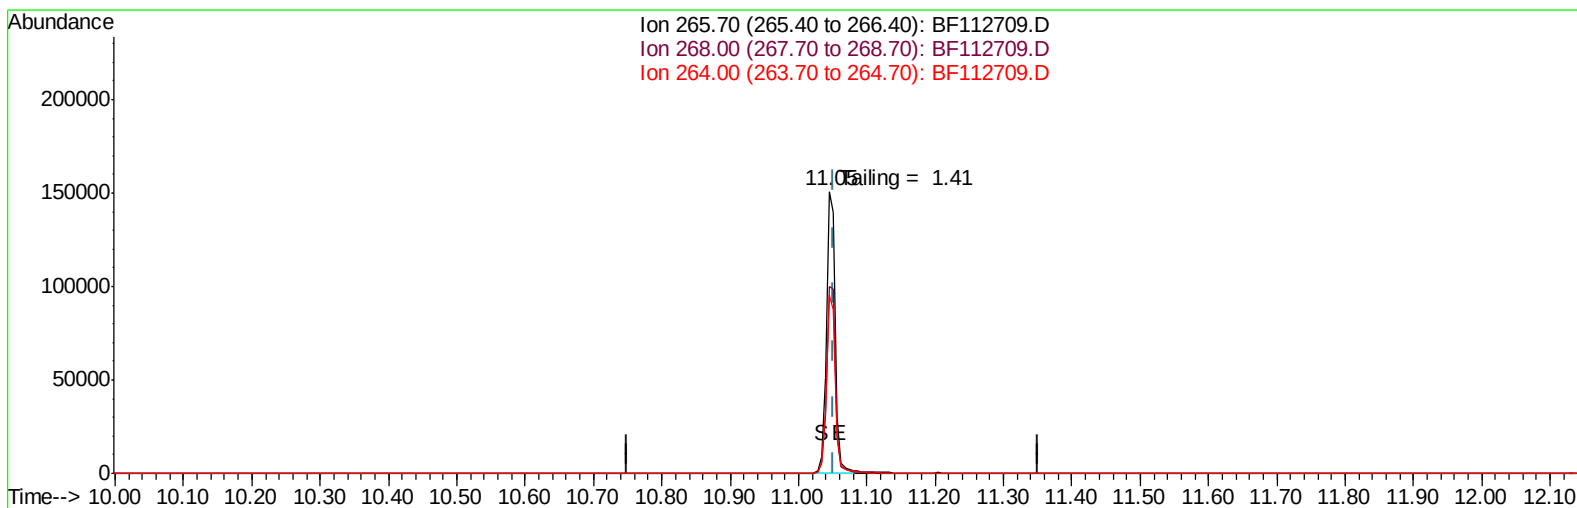

TIC: BF112709.D

(70) Pentachlorophenol (C)




11.045min (-0.006) 35373.92ng

response 141155

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.21
264.00	61.10	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF022719\
 Data File : BF112709.D
 Acq On : 27 Feb 2019 9:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 08:01:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 27 16:08:50 2019
 Response via : Initial Calibration

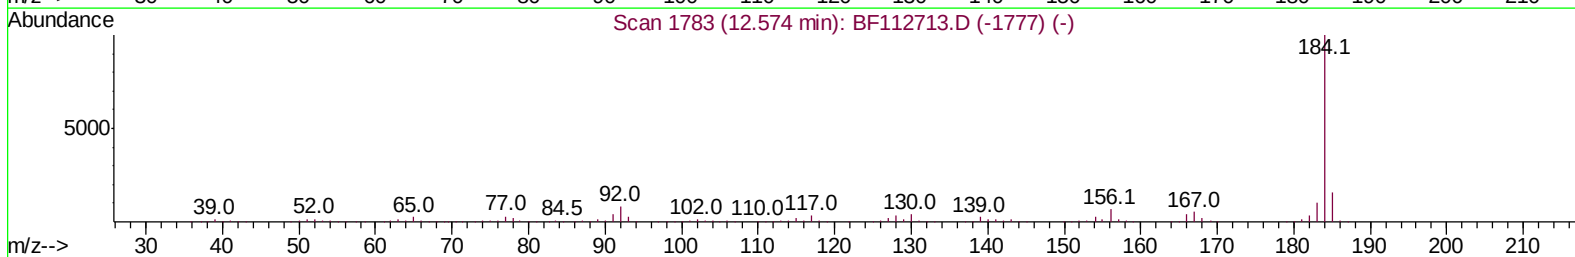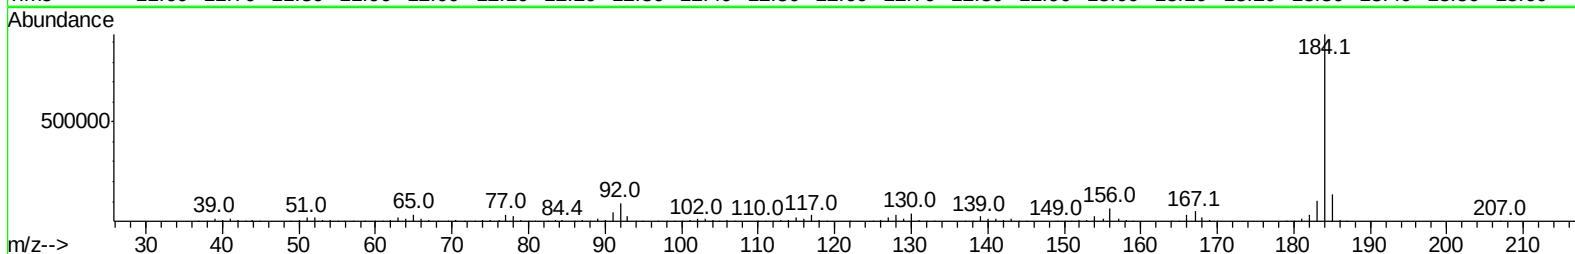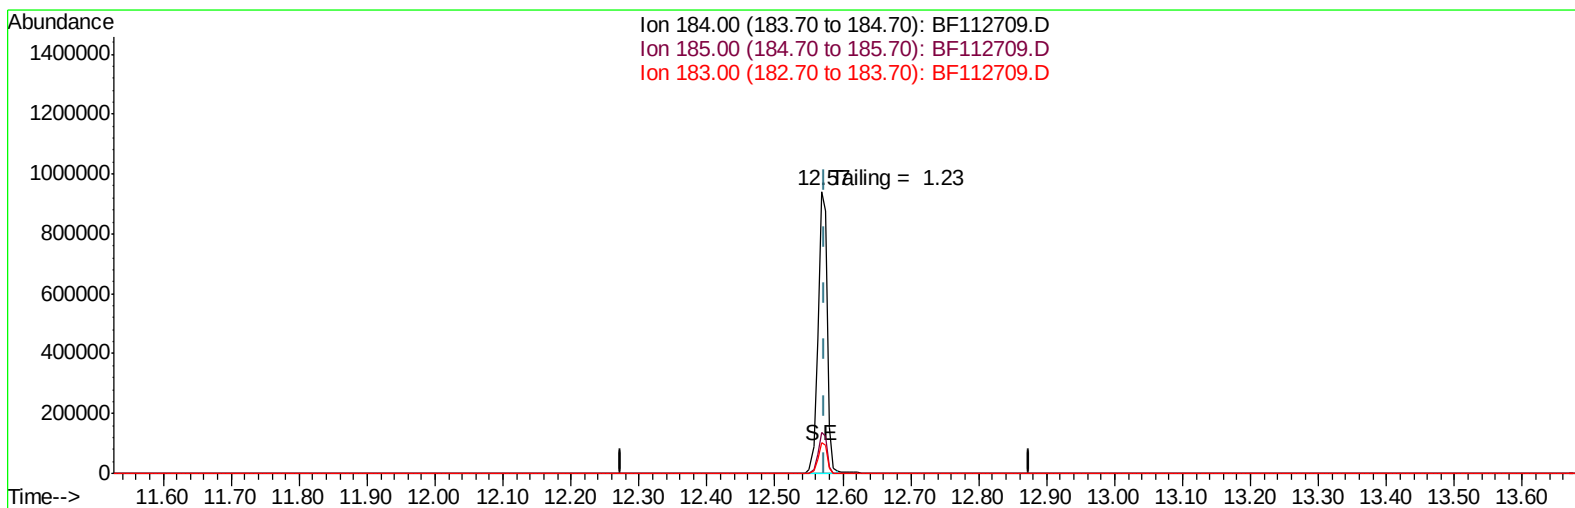

TIC: BF112709.D

(77) Benzidine

12.568min (-0.006) 18596.40ng

response 908854

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.75
183.00	10.70	10.71
0.00	0.00	0.00